

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
 Data File : PL053115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 18:30
 Operator : SG\AJ
 Sample : K5213-04MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-2(5-10)MSD

Manual Integrations
 APPROVED

Ankita
 10/8/2019 2:17:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 05:37:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.048	171.6E6	46966209	17.255	17.491
28)	SA Decachlor...	8.338	9.126	153.0E6	48315522	15.280	16.469
Target Compounds							
8)	B Heptachlo...	5.281	5.916	123.1E6	46300550	9.445	13.815 #
13)	MA Dieldrin	5.881	6.529	130.5E6	58200552	10.109	17.842 #
14)	MA Endrin	6.122	6.746	72106408	25838582	6.330	9.305m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
Data File : PL053115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 18:30
Operator : SG\AJ
Sample : K5213-04MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
S-2(5-10)MSD


Manual Integrations
APPROVED

Ankita
10/8/2019 2:17:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 05:37:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

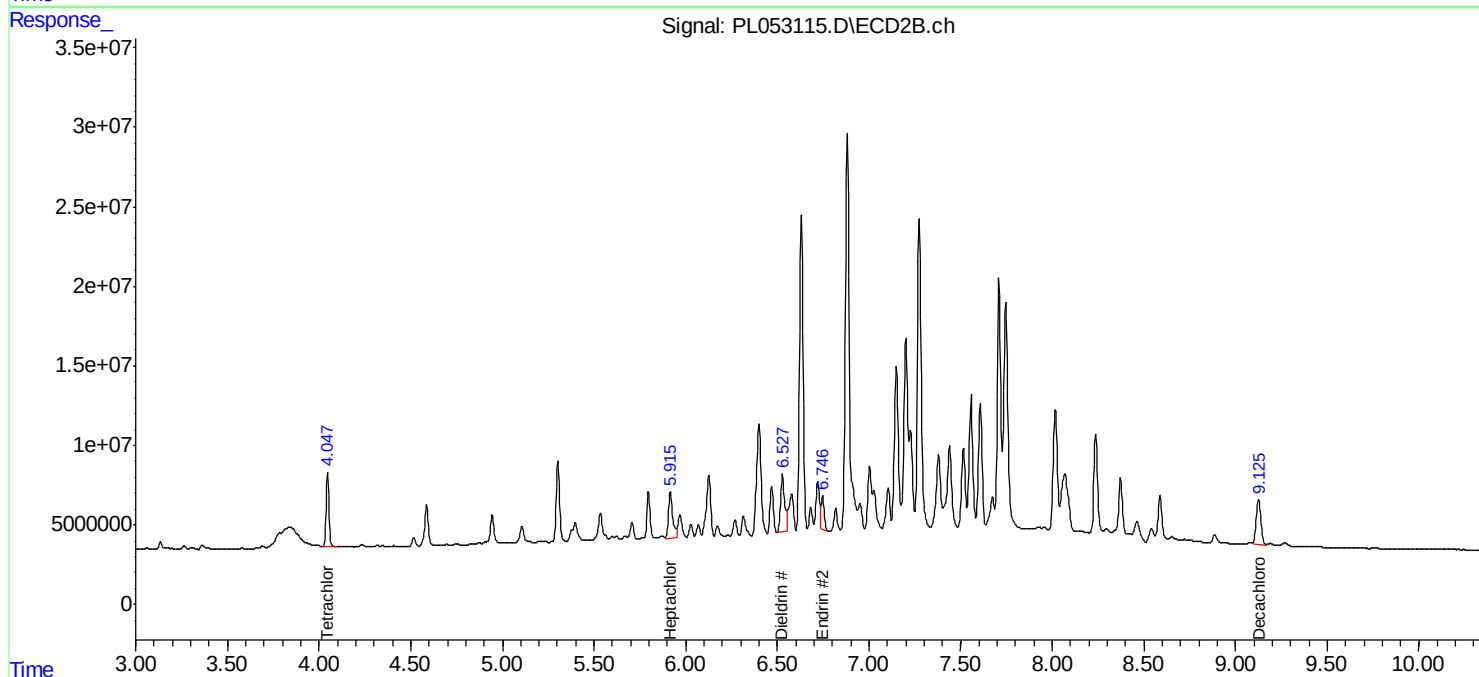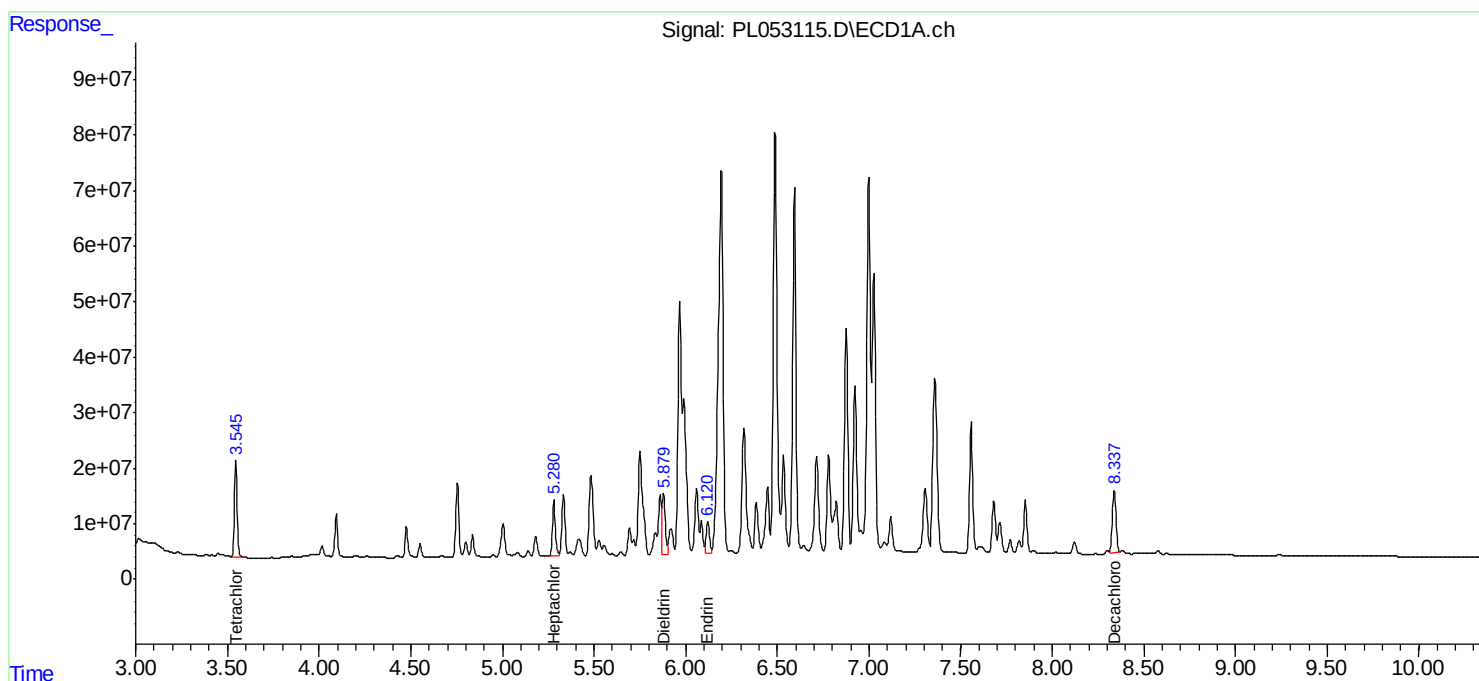

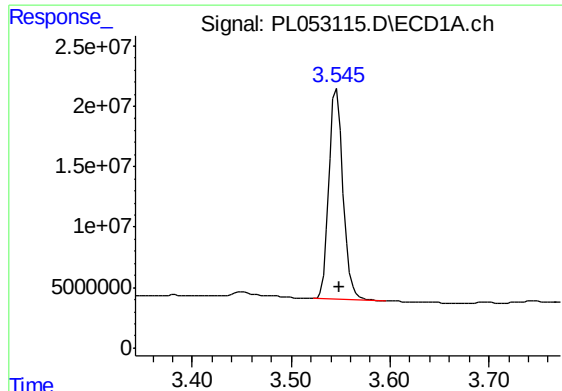


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 171635295
Conc: 17.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2(5-10)MSD


Manual Integrations
APPROVED

Ankita
10/8/2019 2:17:33 PM

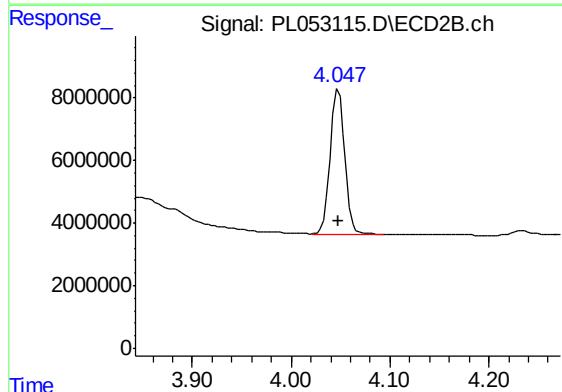


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 46966209
Conc: 17.49 ng/ml

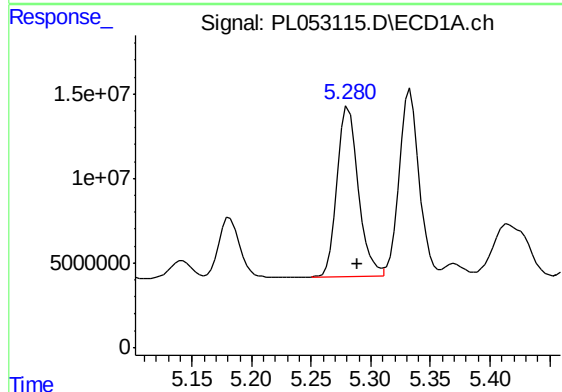


#8 Heptachlor epoxide

R.T.: 5.281 min
Delta R.T.: -0.008 min
Response: 123079943
Conc: 9.45 ng/ml

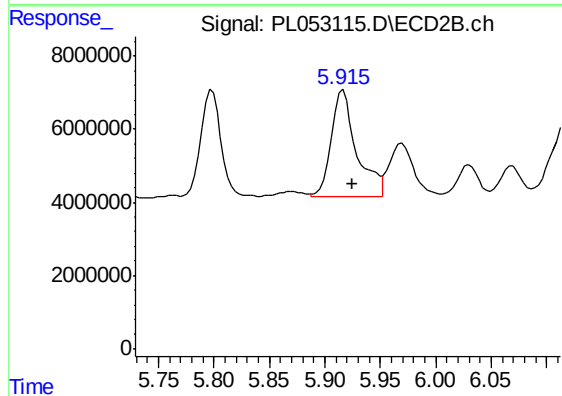

#8 Heptachlor epoxide

R.T.: 5.916 min
Delta R.T.: -0.009 min
Response: 46300550
Conc: 13.81 ng/ml

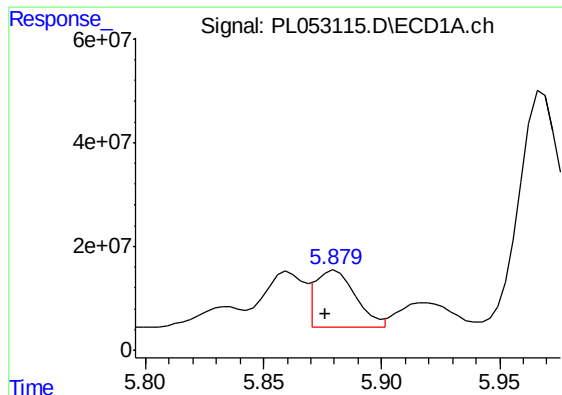


#13 Dieldrin

R.T.: 5.881 min
Delta R.T.: 0.004 min
Response: 130490193
Conc: 10.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2(5-10)MSD


Manual Integrations
APPROVED

Ankita
10/8/2019 2:17:33 PM

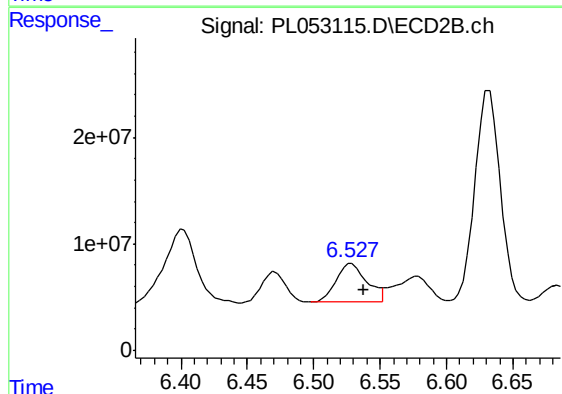


#13 Dieldrin

R.T.: 6.529 min
Delta R.T.: -0.009 min
Response: 58200552
Conc: 17.84 ng/ml

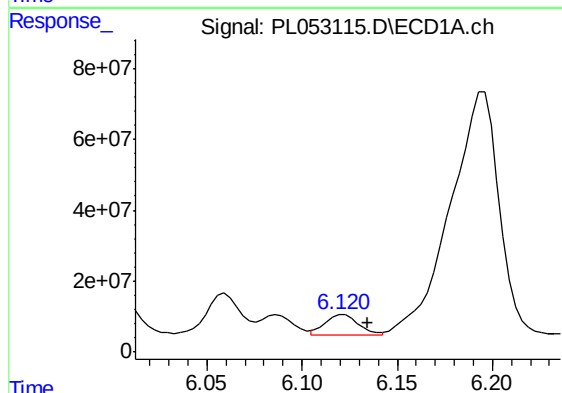


#14 Endrin

R.T.: 6.122 min
Delta R.T.: -0.013 min
Response: 72106408
Conc: 6.33 ng/ml

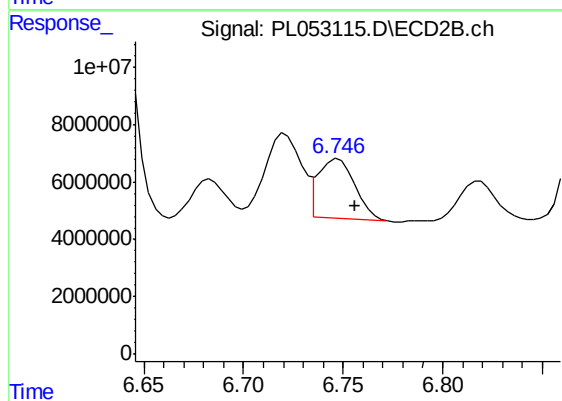

#14 Endrin

R.T.: 6.746 min
Delta R.T.: -0.010 min
Response: 25838582
Conc: 9.30 ng/ml m

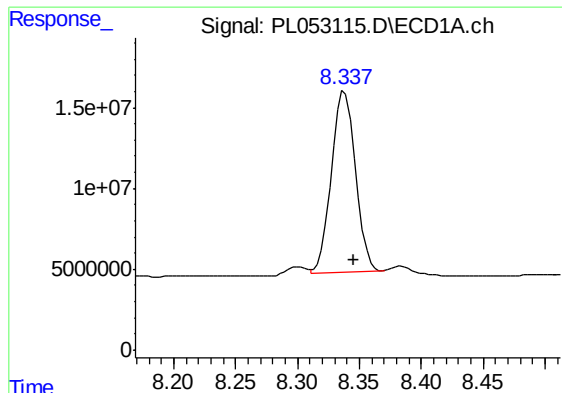


#28 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.007 min
Response: 153045186
Conc: 15.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2(5-10)MSD

Manual Integrations
APPROVED

Ankita
10/8/2019 2:17:33 PM

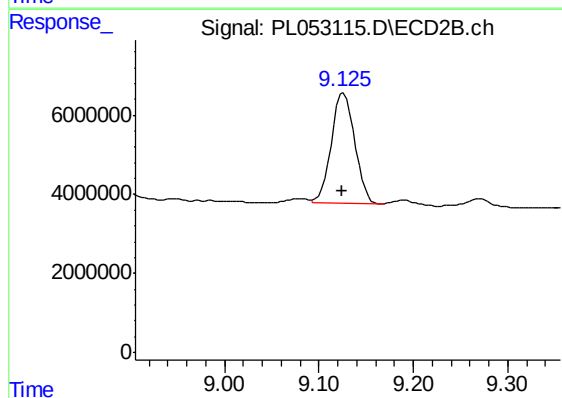

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 48315522
Conc: 16.47 ng/ml