

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100722\
 Data File : PL078191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 17:11
 Operator : AR\AJ
 Sample : N4749-08 (Sig #1); N4749-07 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8Q3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/07/2022
 Supervised By : Ankita Jodhani 10/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 10:53:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	2.622	29681261	55078567	16.827	16.371
2)	SA Decachlor...	8.901	7.716	31101758	50679516	20.519	18.716
Target Compounds							
13)	MA Dieldrin	6.222	5.169	4176252	6985213	2.245m	1.796

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100722\
Data File : PL078191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 17:11
Operator : AR\AJ
Sample : N4749-08 (Sig #1); N4749-07 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 10:53:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

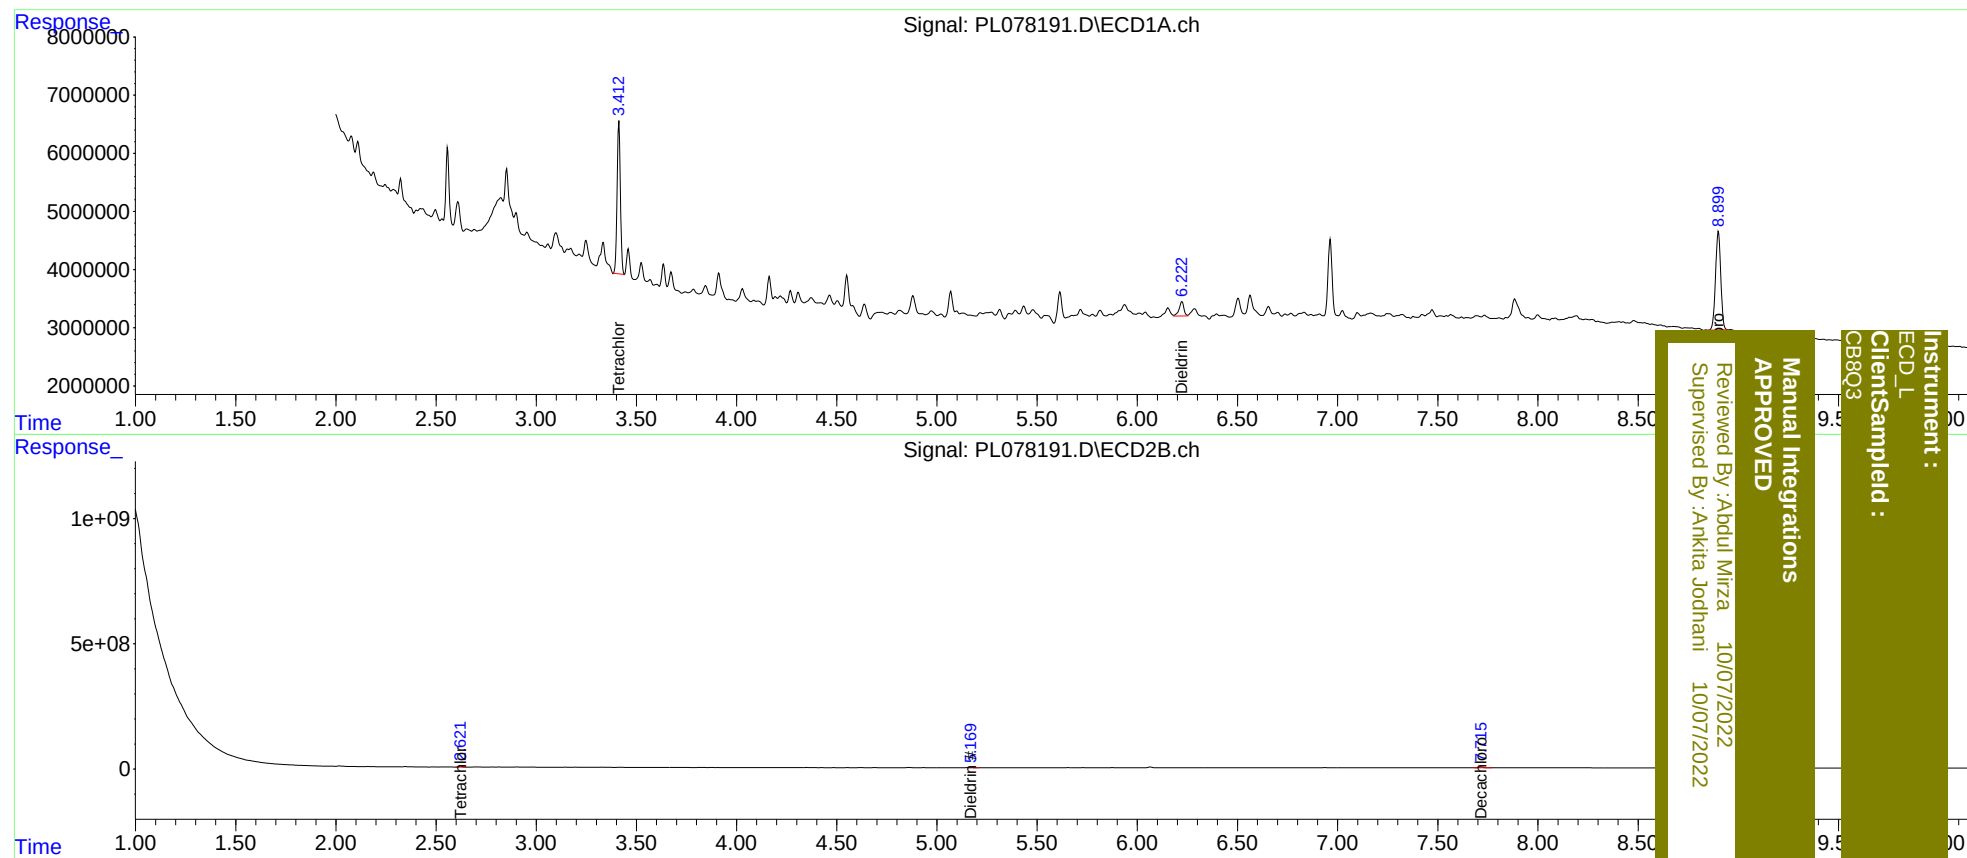

Reviewed By: Abdul Mirza 10/07/2022
Supervised By: Ankita Jodhani 10/07/2022

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
CB803