

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100722\
 Data File : PL078192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 17:25
 Operator : AR\AJ
 Sample : N4956-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8S9

Manual Integrations
 APPROVED

Reviewed By :Abdul
 Mirza

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 00:38:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

10/07/2022
 Supervised By :Ankita
 Jodhani

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	10/07/2022
----------	------	------	--------	--------	-------	-------	------------

System Monitoring Compounds

1) SA Tetrachlo...	3.413	2.621	34009632	53186903	19.281	15.808
27) SA Decachlor...	8.900	7.716	42636376	71131037	28.129	26.269

Target Compounds


2) A alpha-BHC	3.877	3.113	113.1E6	206.0E6	44.999	41.039
3) MA gamma-BHC...	4.213	3.437	107.1E6	198.6E6	44.369	43.370
4) MA Heptachlor	4.788	3.768	113.3E6	184.7E6	46.989	40.197
5) MB Aldrin	5.128	4.042	102.6E6	188.6E6	47.011	42.286
6) B beta-BHC	4.426	3.737	53855725	81028299	45.783	40.813
7) B delta-BHC	4.670	3.959	33786449	76750436	13.830	16.327
8) B Heptachlo...	5.562	4.541	90858796	174.4E6	42.944	44.195
9) A Endosulfan I	5.948	4.906	86269368	154.8E6	48.561	42.828
10) B trans-Chl...	5.818	4.790	89800896	164.7E6	45.984	40.754
11) B cis-Chlor...	5.895	4.852	90649844	164.1E6	48.047	42.539
12) B 4,4'-DDE	6.074	5.047	170.1E6	320.8E6	90.767	85.447
13) MA Dieldrin	6.224	5.169	186.3E6	317.9E6	100.143m	81.744
14) MA Endrin	6.457	5.441	161.5E6	308.7E6	100.163	95.734
15) B Endosulfa...	6.686	5.737	152.4E6	283.2E6	94.489	89.566
16) A 4,4'-DDD	6.599	5.598	136.3E6	262.3E6	100.461	86.846
17) MA 4,4'-DDT	6.908	5.847	135.7E6	277.0E6	93.262	91.689
18) B Endrin al...	6.817	5.916	117.9E6	215.9E6	87.599	83.506
19) B Endosulfa...	7.049	6.139	115.3E6	227.9E6	77.678	73.505
20) A Methoxychlor	7.391	6.424	359.8E6	644.3E6	479.742	432.934
21) B Endrin ke...	7.538	6.638	157.8E6	303.0E6	98.192	91.192

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100722\
Data File : PL078192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 17:25
Operator : AR\AJ
Sample : N4956-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 00:38:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

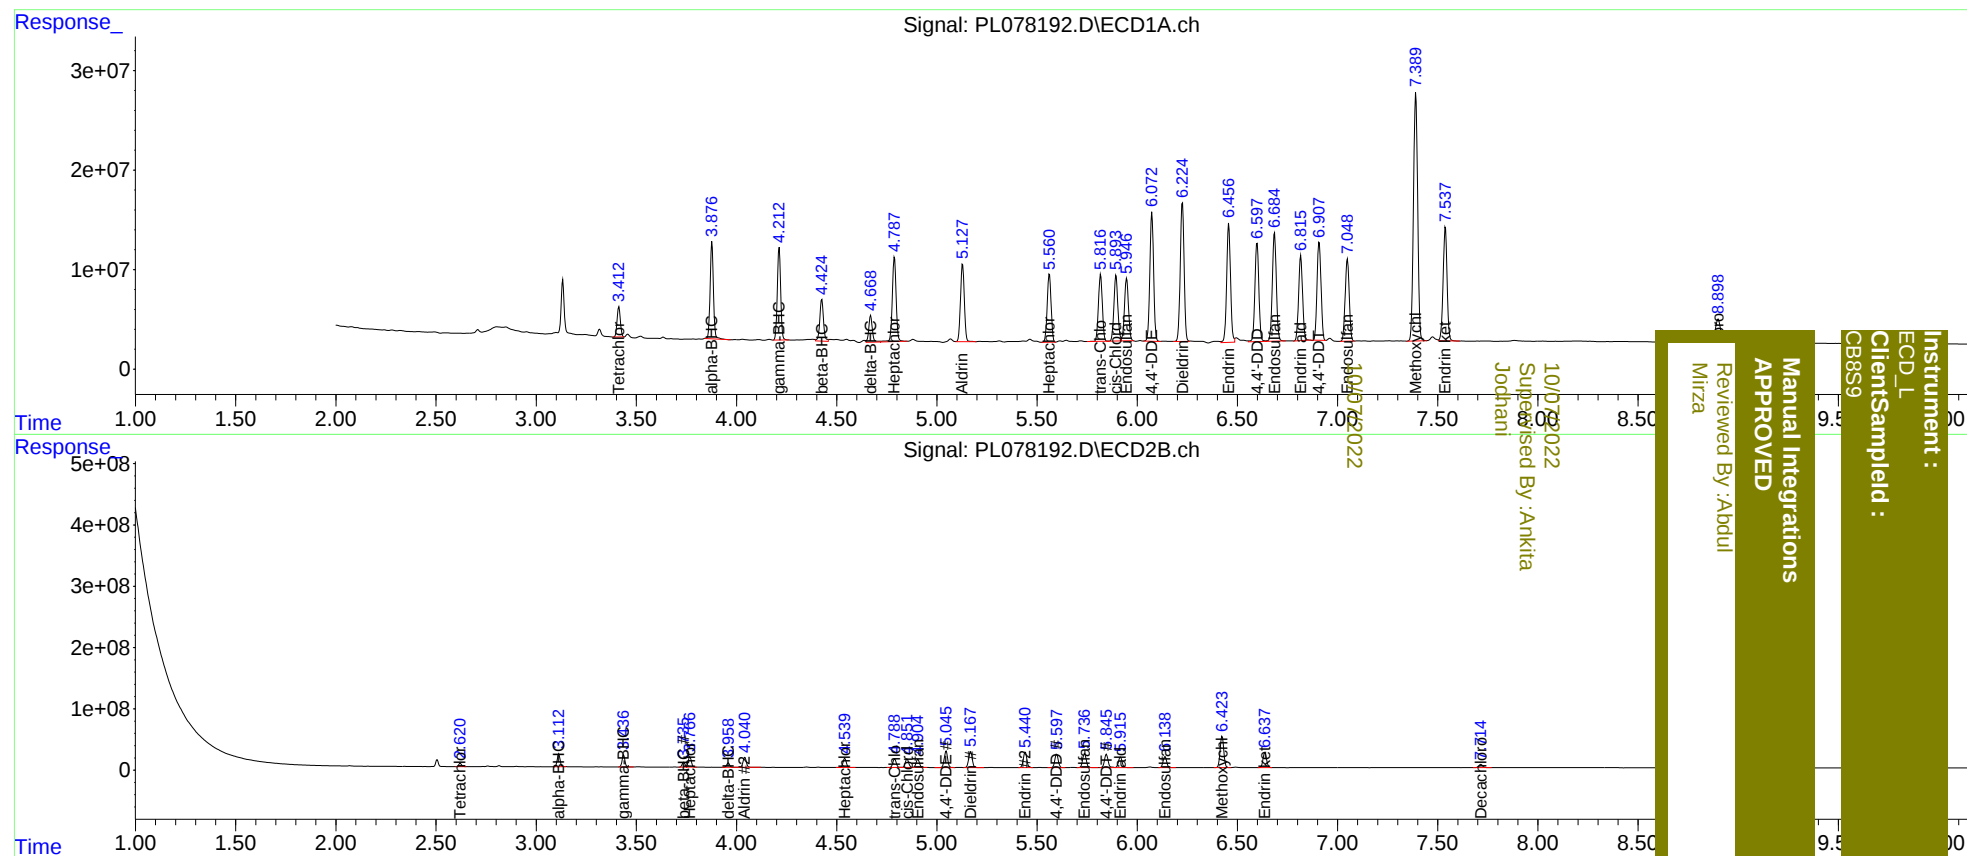

868.894
Reviewed By: Abdul
Mirza

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
CB8S9

10/07/2022
Supervised By: Ankita
Jochani