

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100724\
 Data File : PL092246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2024 17:14
 Operator : AR\AJ
 Sample : P4288-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-03-100324

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/07/2024
 Supervised By : Ankita Jodhani 10/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 23:38:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.779	20828325	28293069	9.362m	11.281m
28) SA Decachlor...	9.055	7.918	19745977	23203318	12.053m	9.274m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100724\
Data File : PL092246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2024 17:14
Operator : AR\AJ
Sample : P4288-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-03-100324


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/07/2024
Supervised By : Ankita Jodhani 10/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 23:38:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

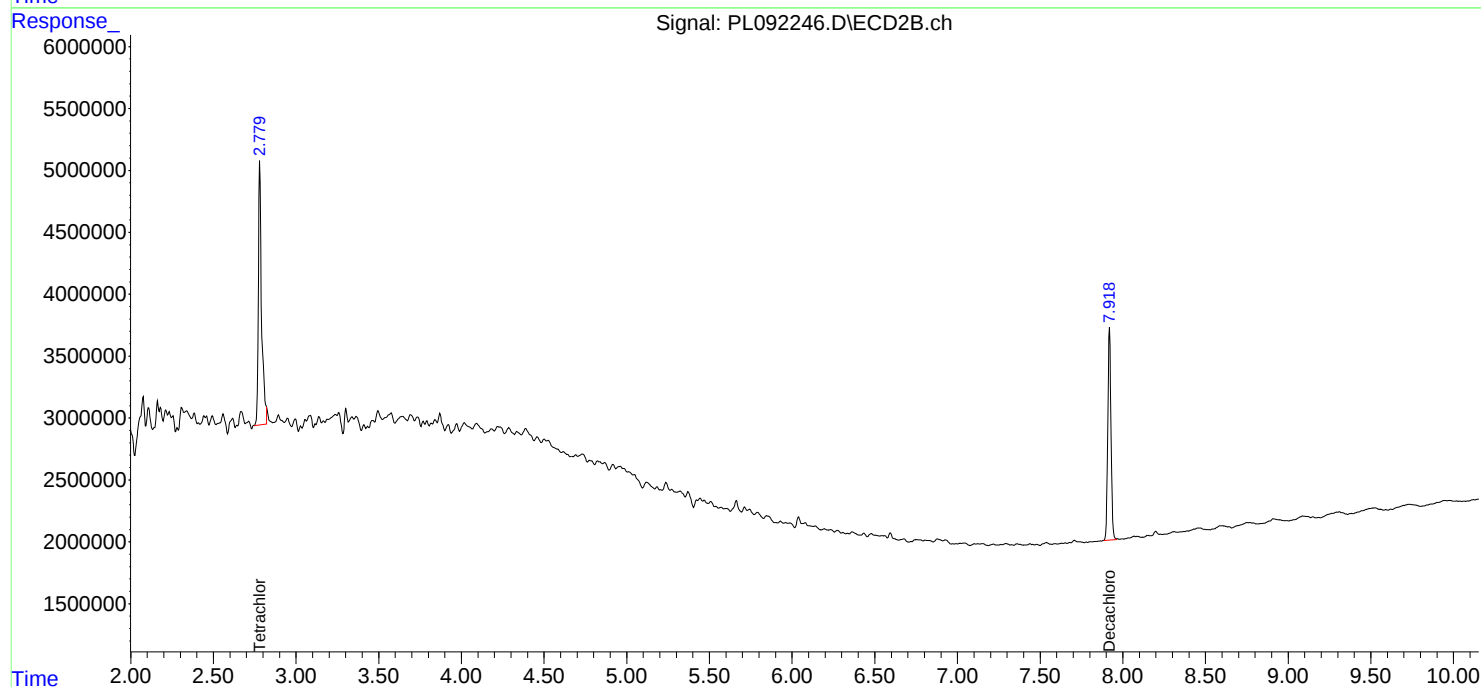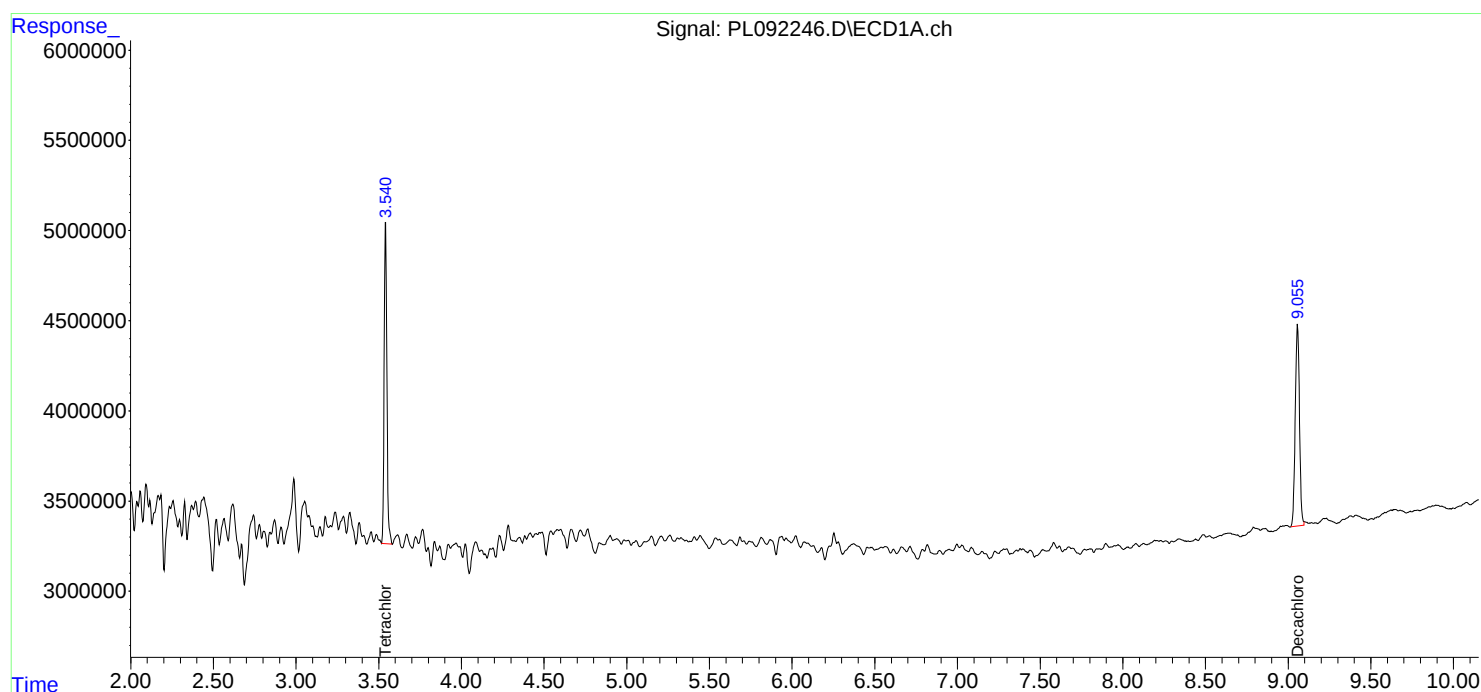

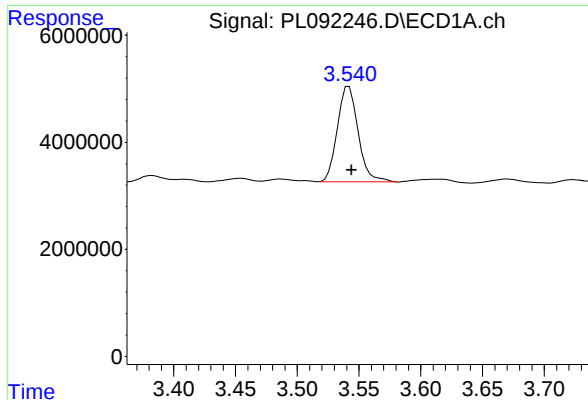


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 20828325
Conc: 9.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-03-100324


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/07/2024
Supervised By :Ankita Jodhani 10/07/2024

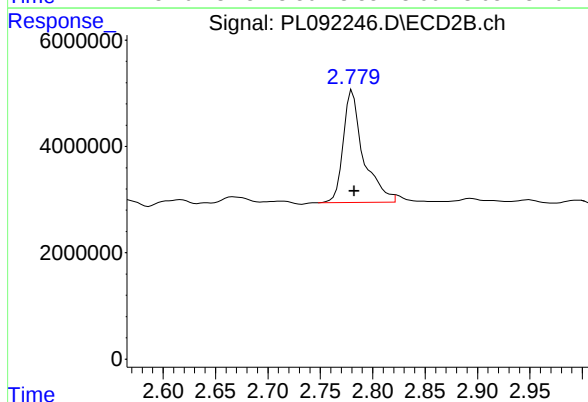


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: -0.003 min
Response: 28293069
Conc: 11.28 ng/ml m

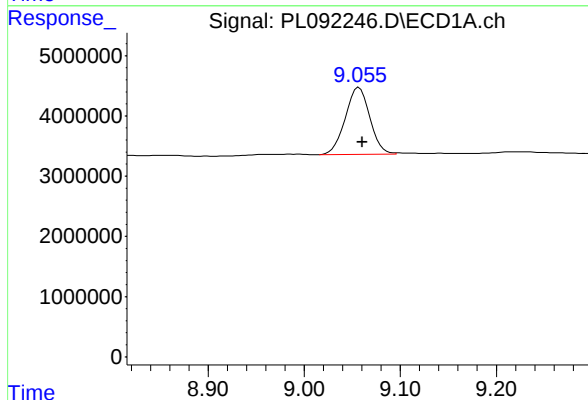

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: -0.005 min
Response: 19745977
Conc: 12.05 ng/ml m

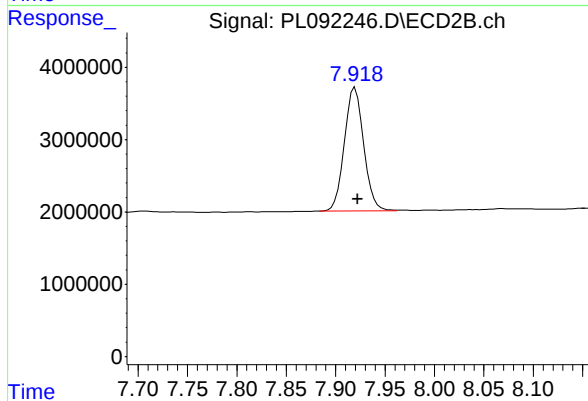

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: -0.004 min
Response: 23203318
Conc: 9.27 ng/ml m