

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
 Data File : PL097532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2025 12:52
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 13:31:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 13:26:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.523	2.820	270.6E6	526.6E6	75.150	74.388
28)	SA Decachlor...	8.995	7.980	190.6E6	337.2E6	74.224	74.307
Target Compounds							
23)	Chlordane-1	4.676	3.829	148.7E6	186.5E6	757.068	746.202
24)	Chlordane-2	5.199	4.407	168.3E6	203.6E6	759.276	746.304
25)	Chlordane-3	5.902	5.040	613.8E6	647.9E6	747.037	742.856
26)	Chlordane-4	5.986	5.104	738.3E6	578.5E6	744.750	746.963
27)	Chlordane-5	6.823	5.998	125.8E6	217.6E6	750.009	741.513



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
Data File : PL097532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2025 12:52
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 13:31:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 13:26:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

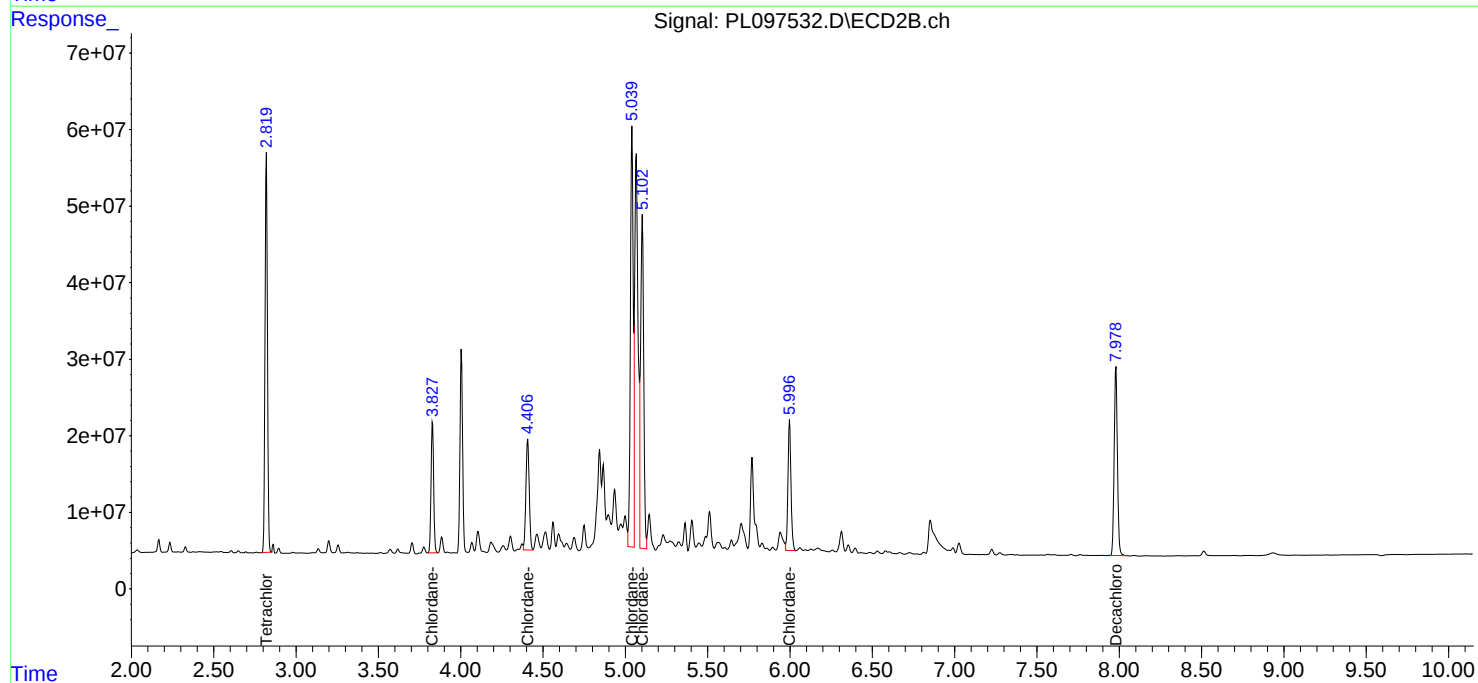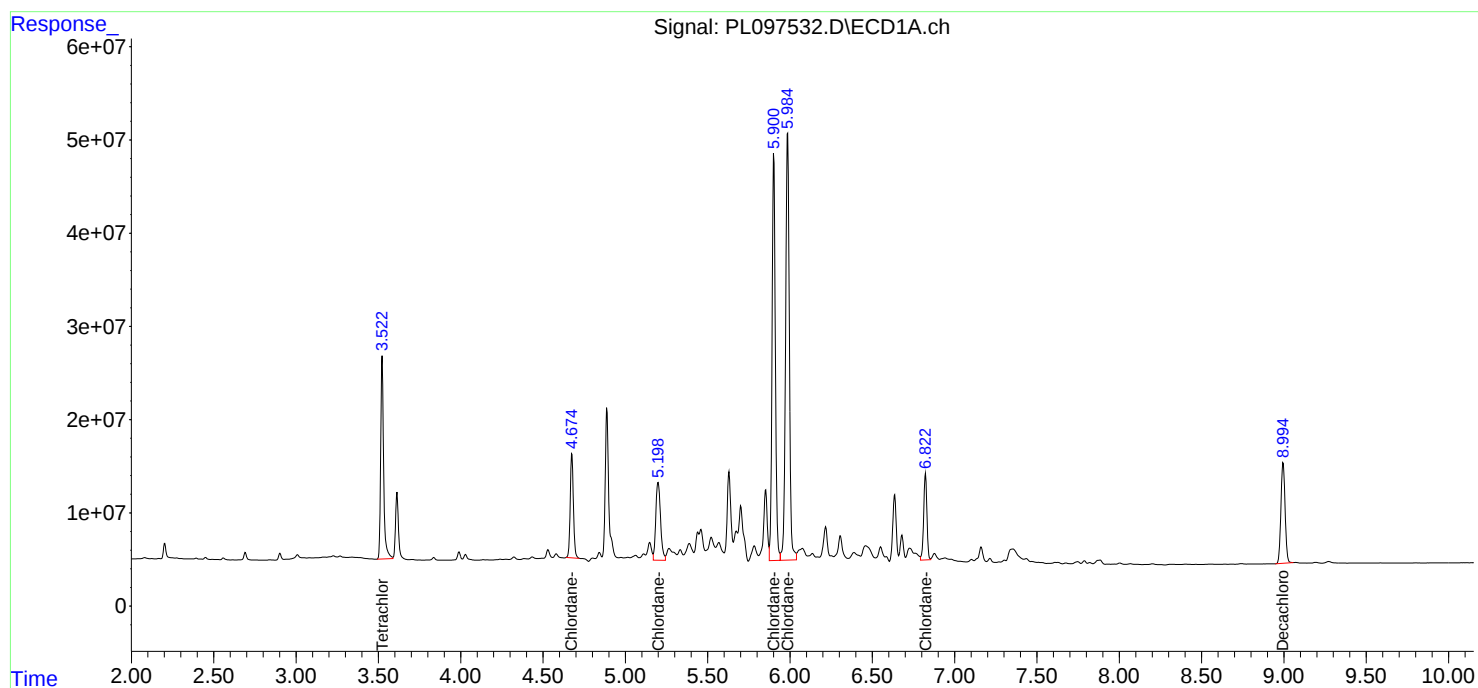


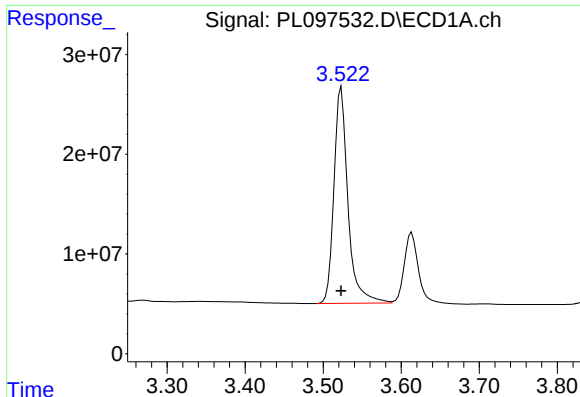

#1 Tetrachloro-m-xylene


R.T.: 3.523 min
Delta R.T.: 0.000 min
Response: 270581594
Conc: 75.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

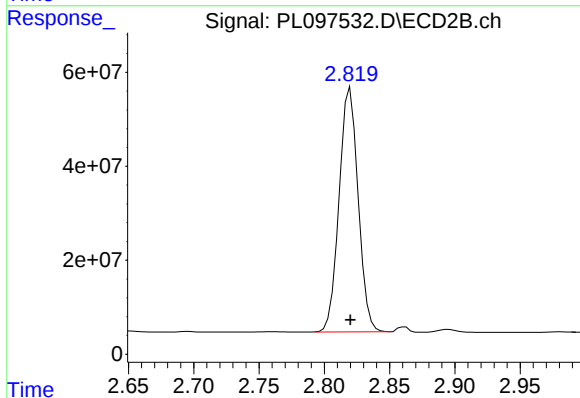


#1 Tetrachloro-m-xylene

R.T.: 2.820 min
Delta R.T.: 0.000 min
Response: 526636034
Conc: 74.39 ng/ml

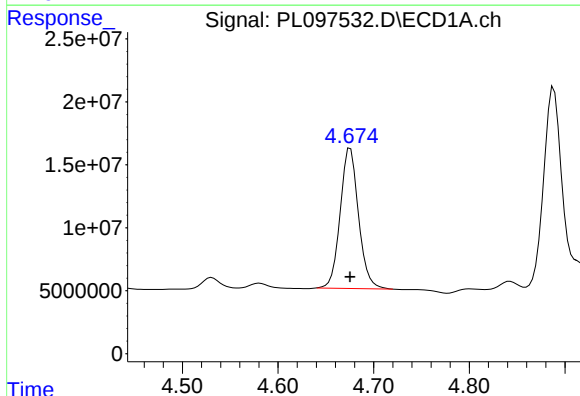


#23 Chlordane-1

R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 148730261
Conc: 757.07 ng/ml

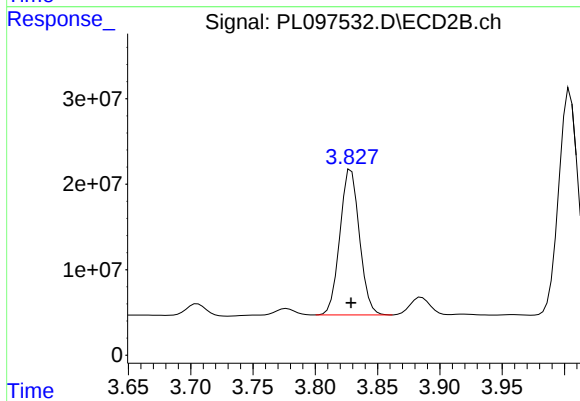

#23 Chlordane-1


R.T.: 3.829 min
Delta R.T.: 0.000 min
Response: 186505232
Conc: 746.20 ng/ml

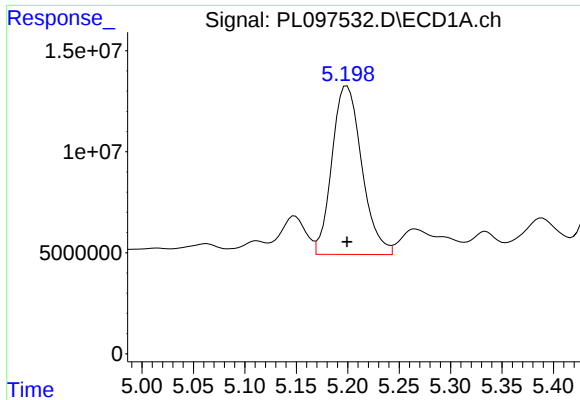

#24 Chlordane-2


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 168344494
Conc: 759.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

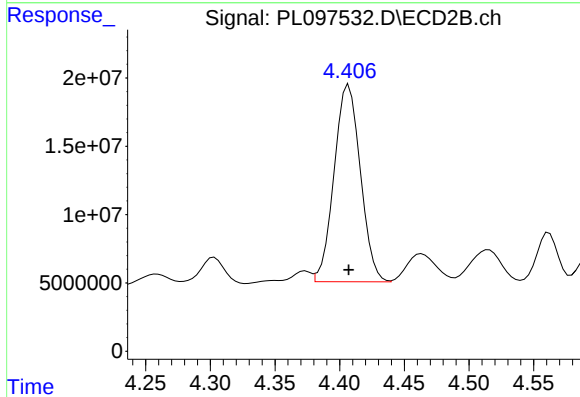


#24 Chlordane-2

R.T.: 4.407 min
Delta R.T.: 0.000 min
Response: 203596034
Conc: 746.30 ng/ml

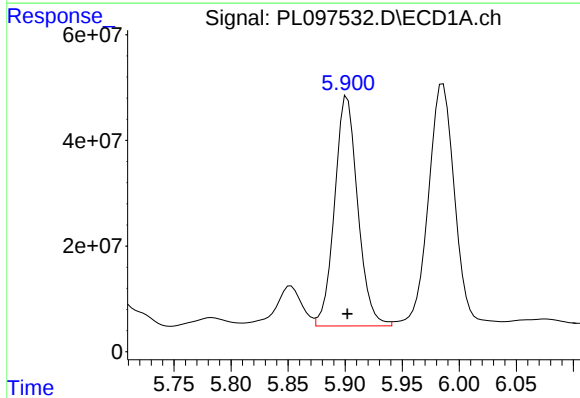


#25 Chlordane-3

R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 613826017
Conc: 747.04 ng/ml

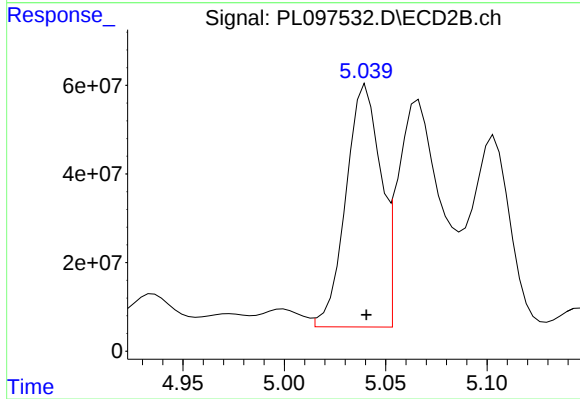

#25 Chlordane-3


R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 647934625
Conc: 742.86 ng/ml

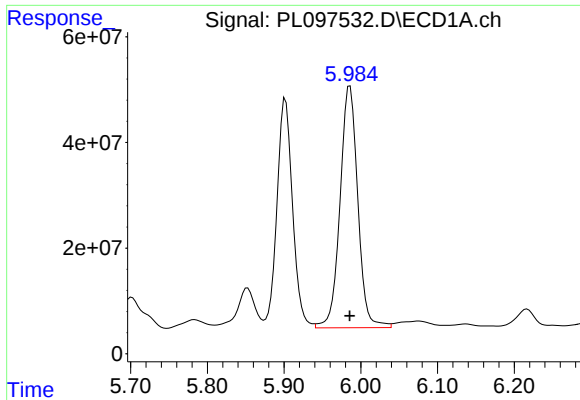

#26 Chlordane-4


R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 738261583
Conc: 744.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

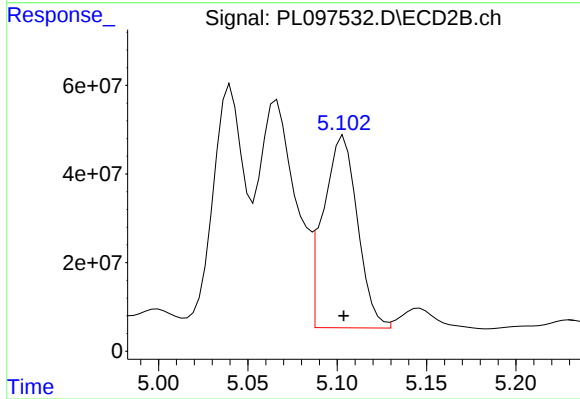


#26 Chlordane-4

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 578530693
Conc: 746.96 ng/ml

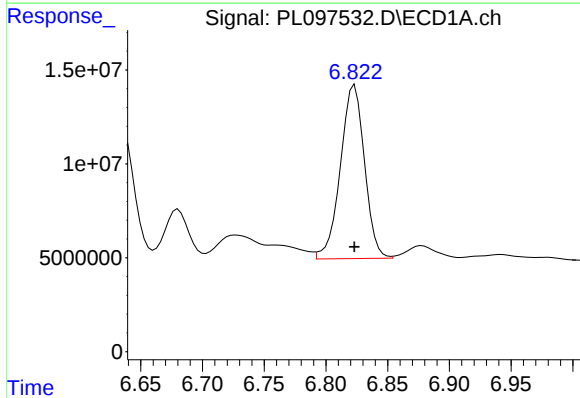


#27 Chlordane-5

R.T.: 6.823 min
Delta R.T.: 0.000 min
Response: 125832419
Conc: 750.01 ng/ml

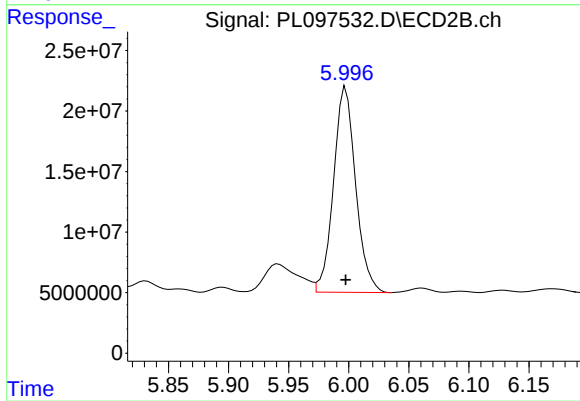

#27 Chlordane-5


R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 217637551
Conc: 741.51 ng/ml

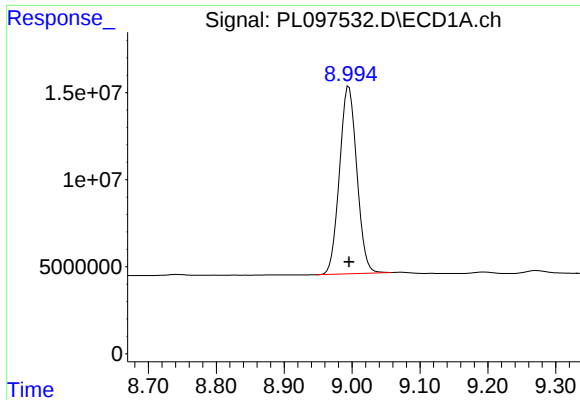

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.000 min
Response: 190646188
Conc: 74.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

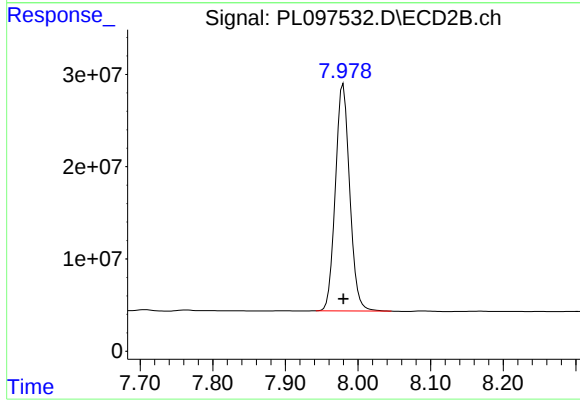

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 337200689
Conc: 74.31 ng/ml