

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
 Data File : PL097535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2025 13:32
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 13:54:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 13:54:22 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.822	19490052	36334304	5.325	5.131
28)	SA Decachlor...	8.996	7.980	15057042	28981270	5.637	5.967
Target Compounds							
23)	Chlordane-1	4.676	3.830	10736217	13670957	53.708	53.812
24)	Chlordane-2	5.200	4.409	12122119	24468542	53.704	84.682 #
25)	Chlordane-3	5.903	5.041	50957385	58350465	62.307	64.013
26)	Chlordane-4	5.986	5.105	56300708	50978214	54.888	65.488
27)	Chlordane-5	6.824	5.998	10144406	15690043	59.946	52.986


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
Data File : PL097535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2025 13:32
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 13:54:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 13:54:22 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

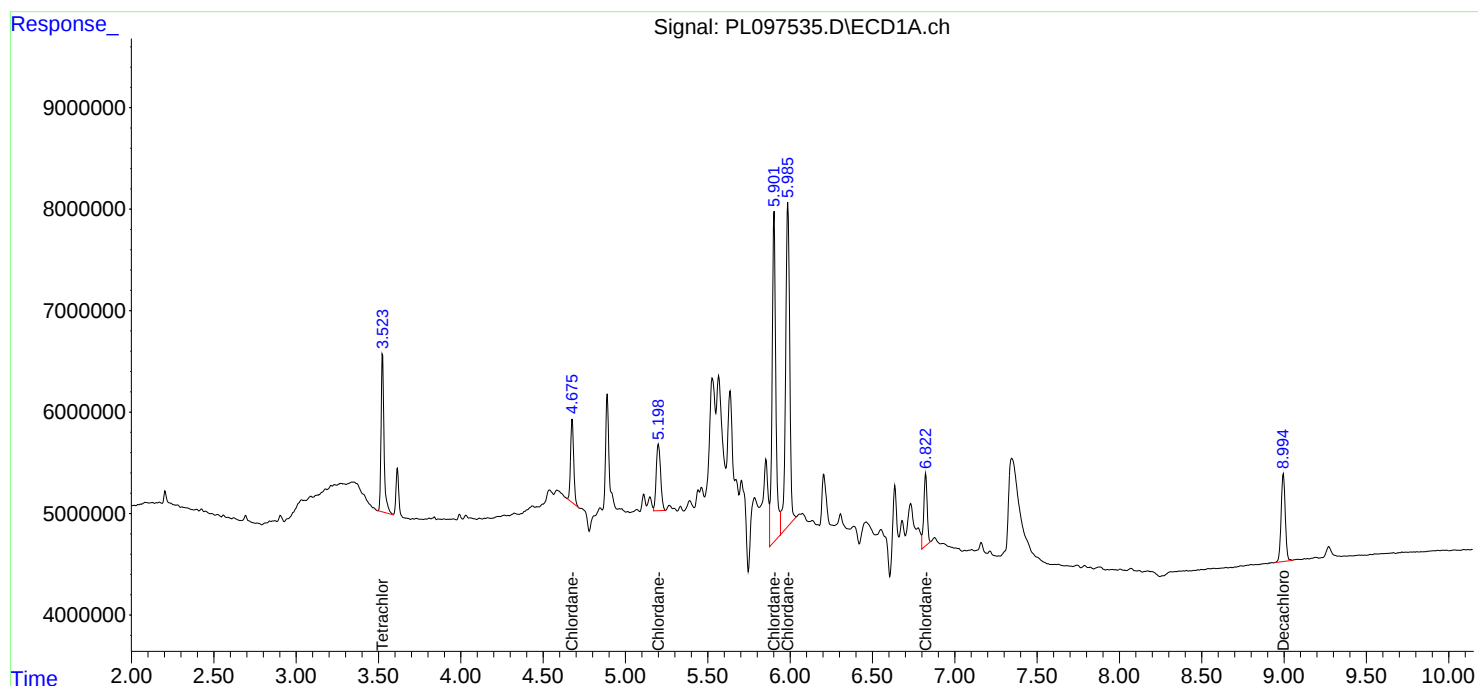


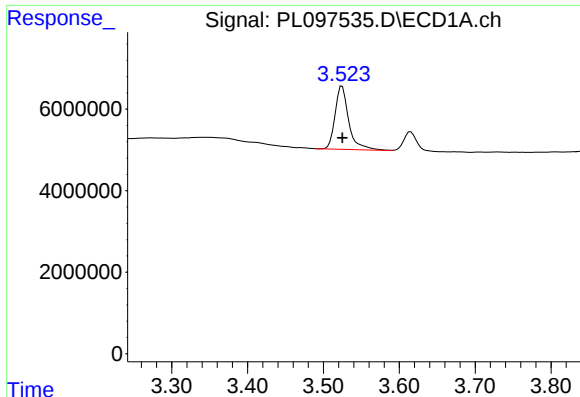

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 19490052
Conc: 5.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

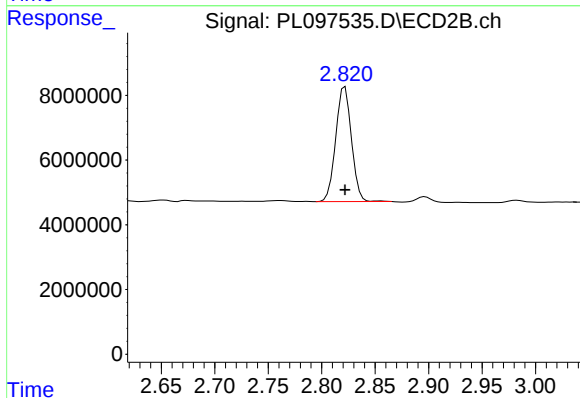


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 36334304
Conc: 5.13 ng/ml

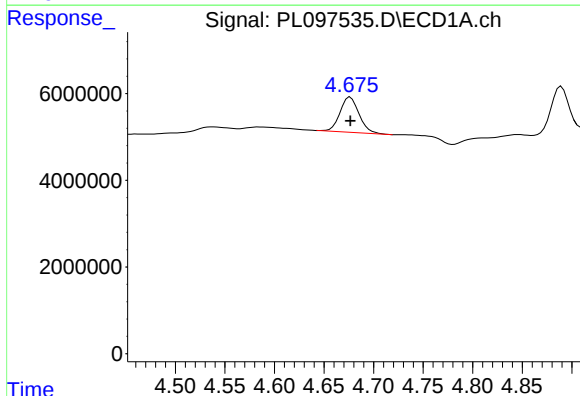


#23 Chlordane-1

R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 10736217
Conc: 53.71 ng/ml

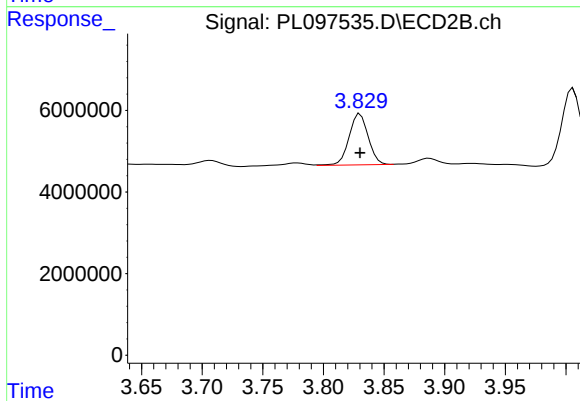

#23 Chlordane-1


R.T.: 3.830 min
Delta R.T.: 0.000 min
Response: 13670957
Conc: 53.81 ng/ml

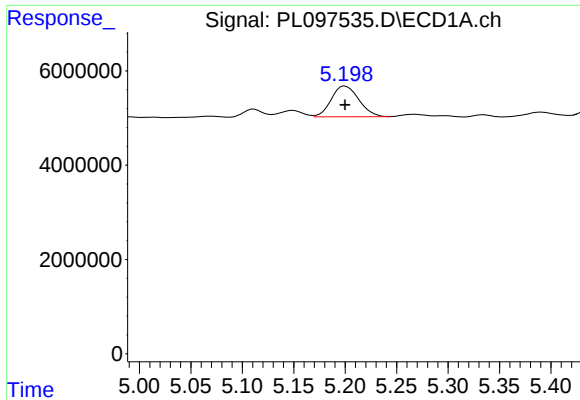

#24 Chlordane-2


R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 12122119
Conc: 53.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

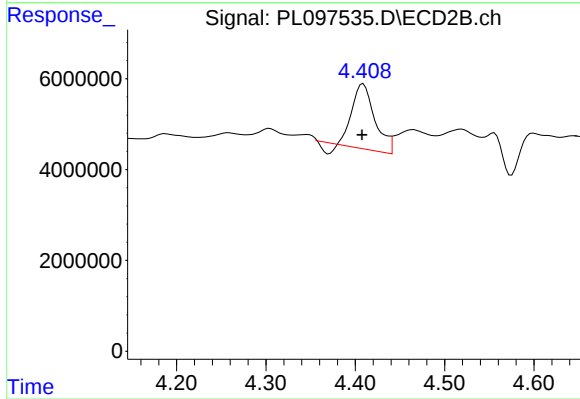


#24 Chlordane-2

R.T.: 4.409 min
Delta R.T.: 0.001 min
Response: 24468542
Conc: 84.68 ng/ml

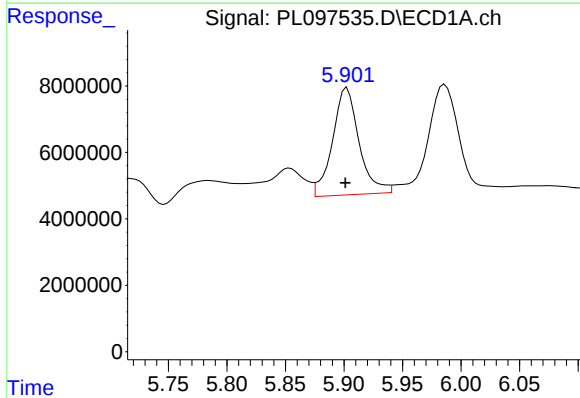


#25 Chlordane-3

R.T.: 5.903 min
Delta R.T.: 0.001 min
Response: 50957385
Conc: 62.31 ng/ml

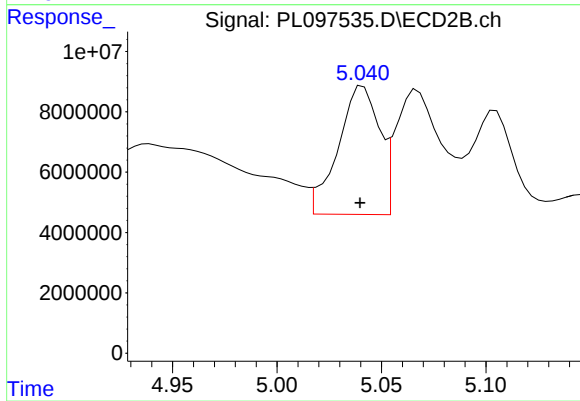

#25 Chlordane-3


R.T.: 5.041 min
Delta R.T.: 0.001 min
Response: 58350465
Conc: 64.01 ng/ml

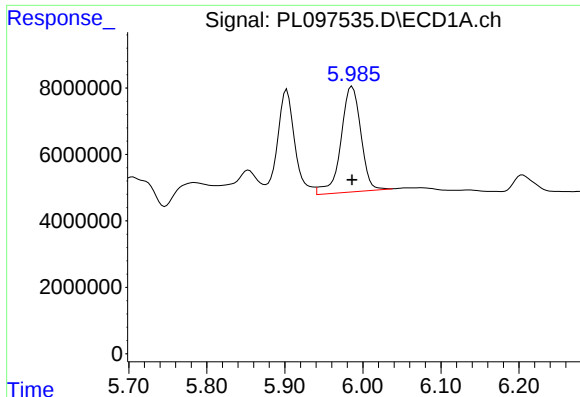

#26 Chlordane-4


R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 56300708
Conc: 54.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

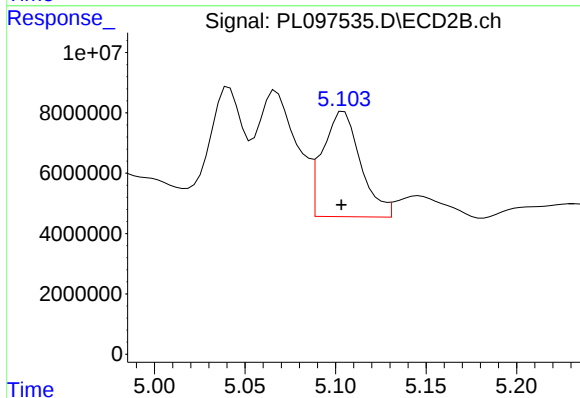


#26 Chlordane-4

R.T.: 5.105 min
Delta R.T.: 0.001 min
Response: 50978214
Conc: 65.49 ng/ml

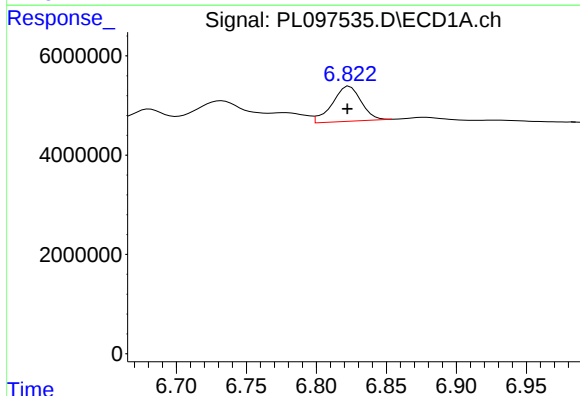


#27 Chlordane-5

R.T.: 6.824 min
Delta R.T.: 0.001 min
Response: 10144406
Conc: 59.95 ng/ml

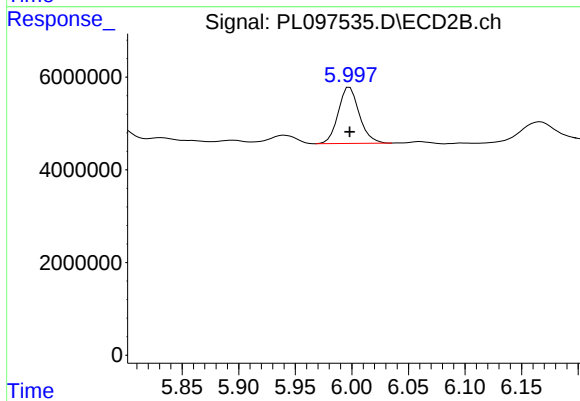

#27 Chlordane-5


R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 15690043
Conc: 52.99 ng/ml

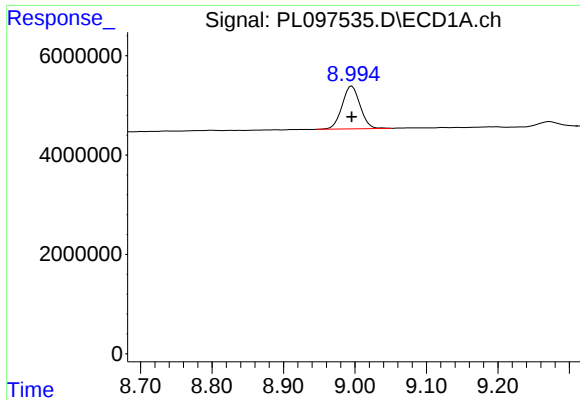

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 15057042
Conc: 5.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

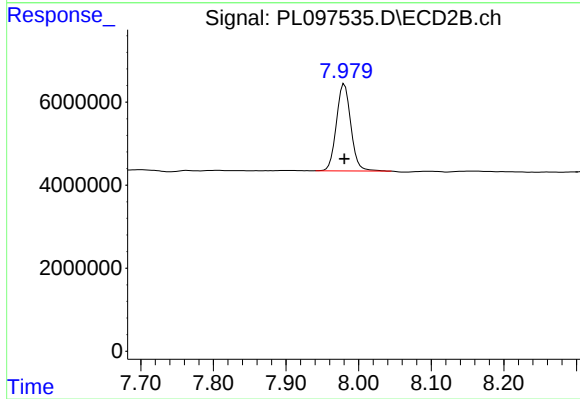

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 28981270
Conc: 5.97 ng/ml