

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
 Data File : PL097558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2025 19:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 03:07:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 16:47:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.526	2.823	77055926	116.4E6	18.901	19.125
28)	SA Decachlor...	8.997	7.981	60537430	80666053	20.358	15.545
Target Compounds							
14)	MA Endrin	0.000	5.709	0	17396229	N.D.	2.350 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
Data File : PL097558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2025 19:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 03:07:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 16:47:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

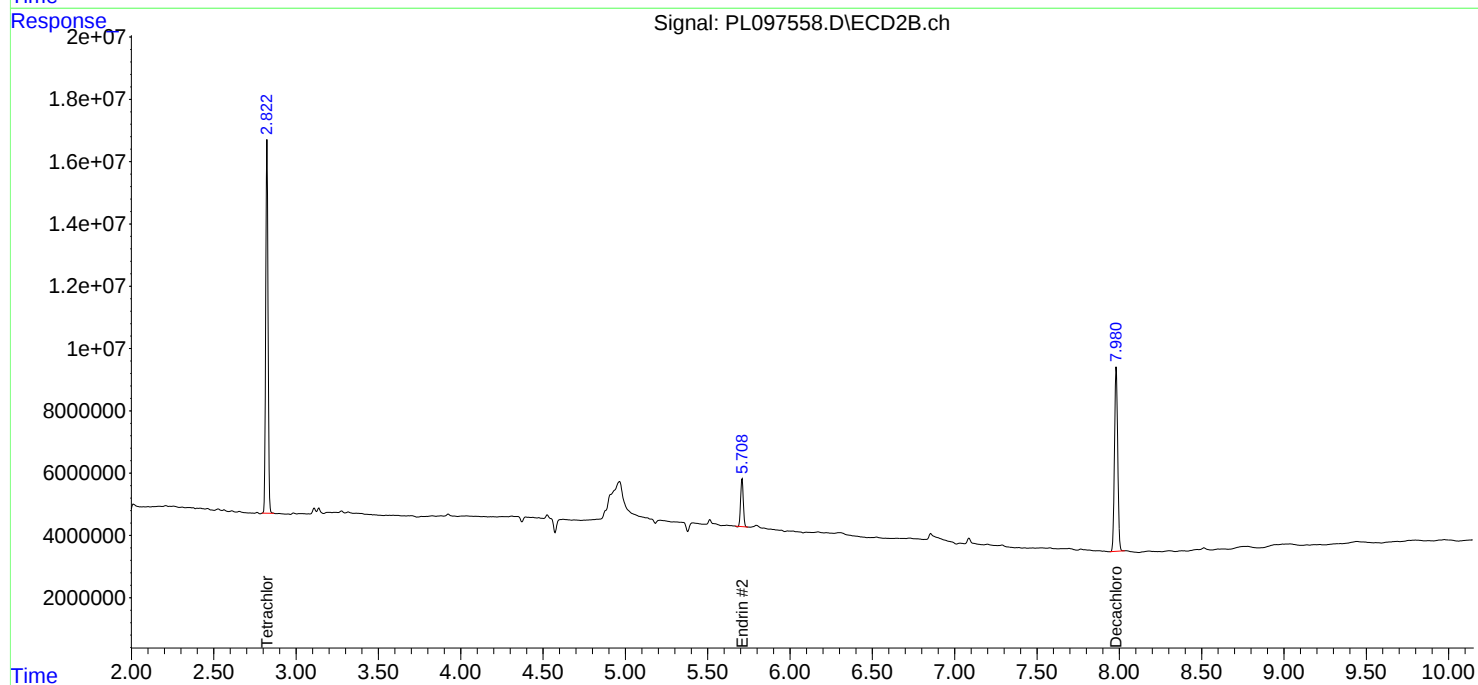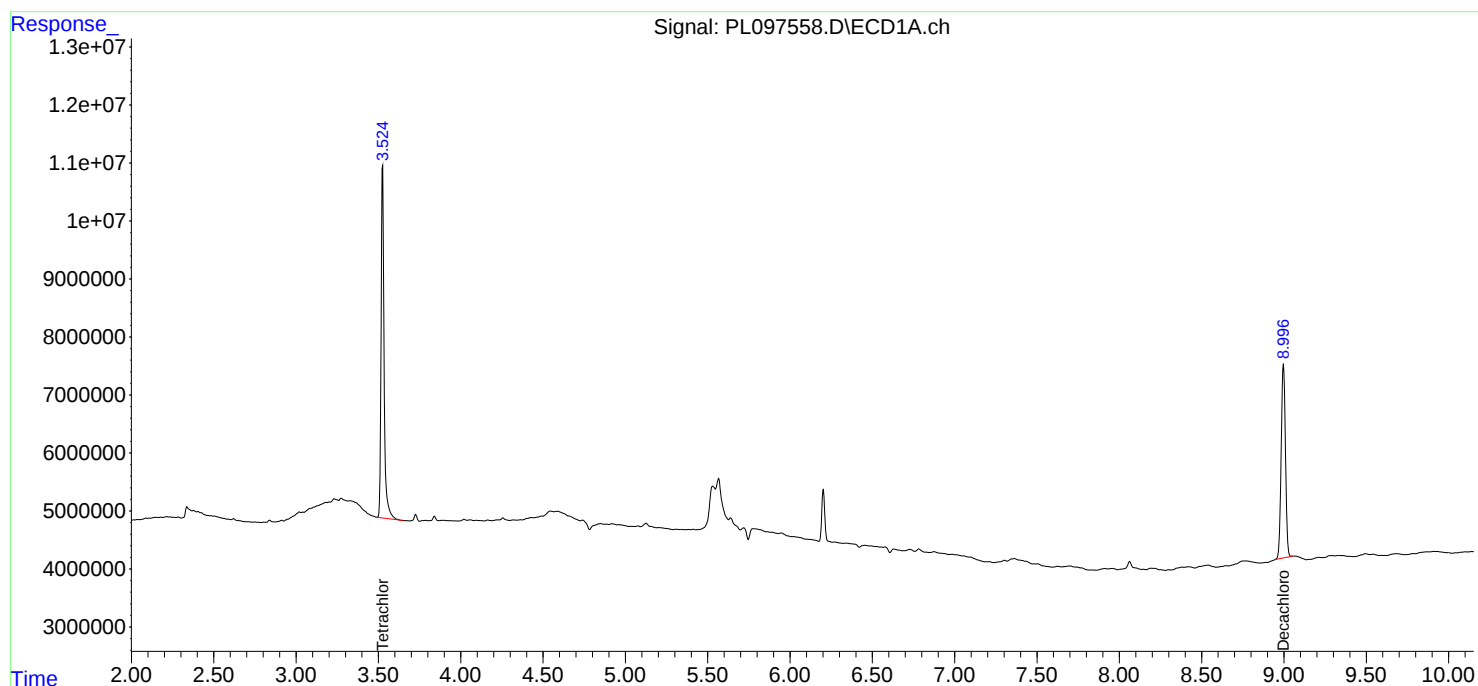


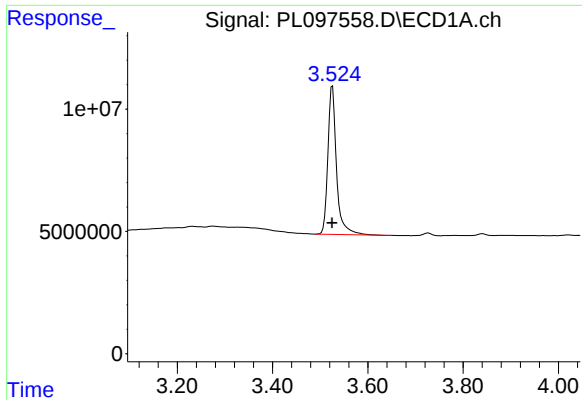

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 77055926
Conc: 18.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

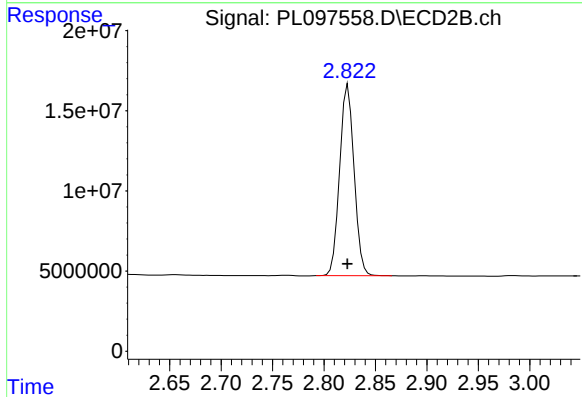


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 116399924
Conc: 19.12 ng/ml

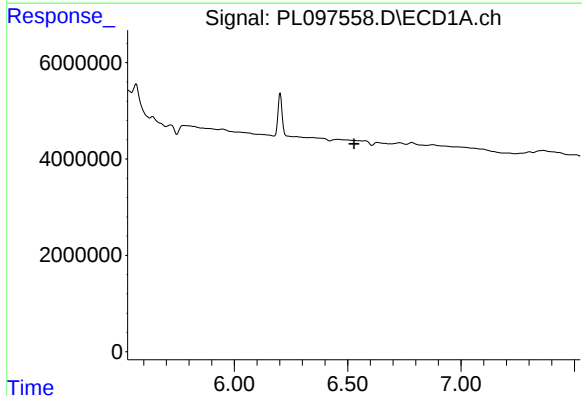


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.528 min
Response: 0
Conc: N.D.

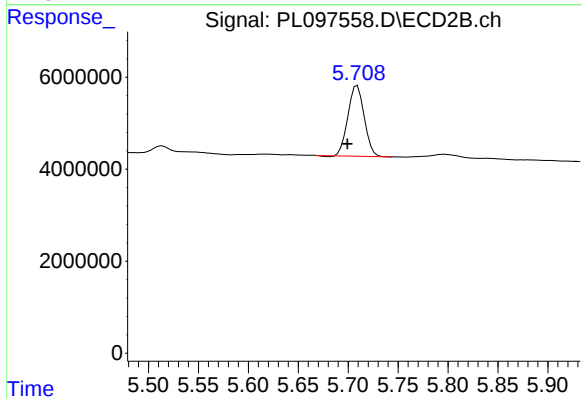

#14 Endrin


R.T.: 5.709 min
Delta R.T.: 0.010 min
Response: 17396229
Conc: 2.35 ng/ml

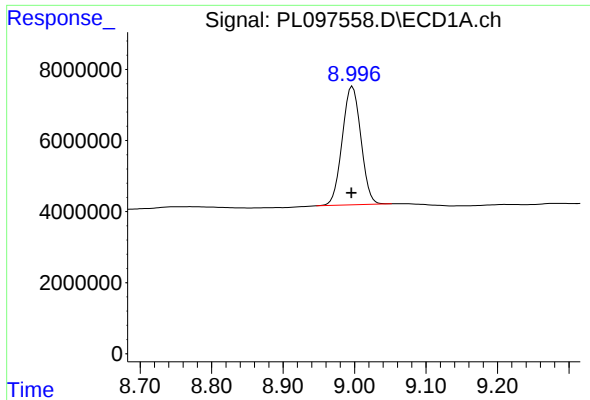

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.002 min
Response: 60537430
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

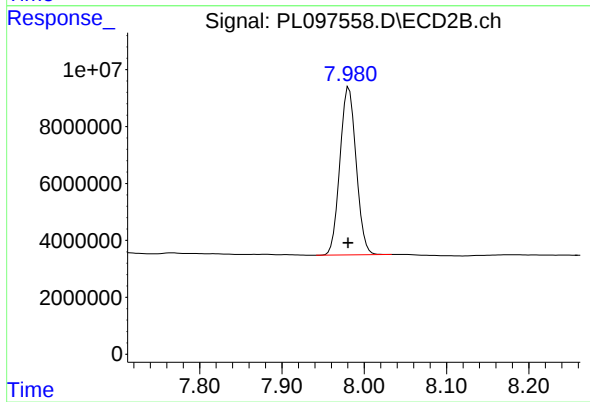

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.001 min
Response: 80666053
Conc: 15.55 ng/ml