

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
 Data File : PL097531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2025 12:38
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 13:29:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 13:26:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.523	2.817	358.5E6	717.7E6	99.662	100.963
28)	SA Decachlor...	8.999	7.981	256.7E6	448.2E6	99.410	98.306
Target Compounds							
23)	Chlordane-1	4.676	3.827	193.2E6	251.5E6	988.211	1003.531
24)	Chlordane-2	5.201	4.406	215.7E6	268.7E6	978.748	982.524
25)	Chlordane-3	5.904	5.039	821.7E6	868.7E6	998.044	991.255
26)	Chlordane-4	5.987	5.102	989.7E6	770.2E6	994.882	992.400
27)	Chlordane-5	6.825	5.997	163.5E6	298.6E6	974.694	1011.541



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
Data File : PL097531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2025 12:38
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 13:29:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 13:26:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

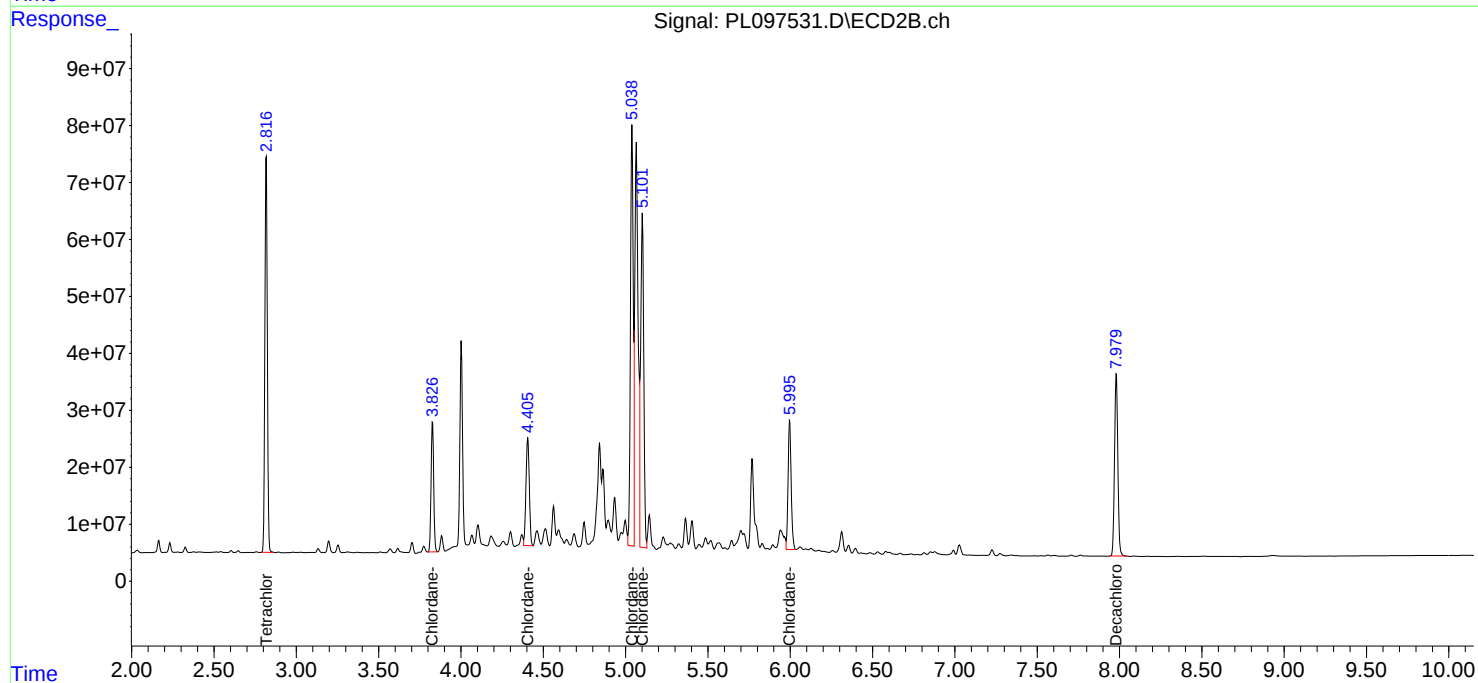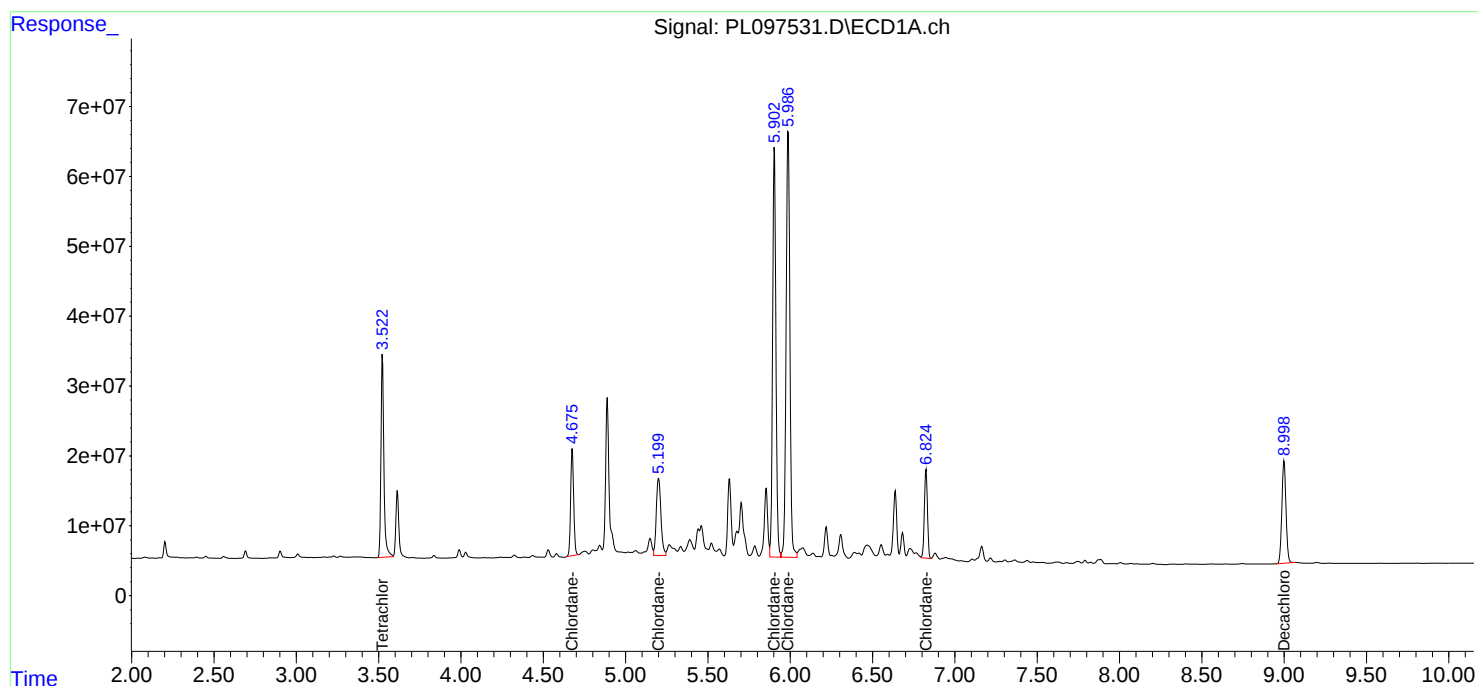


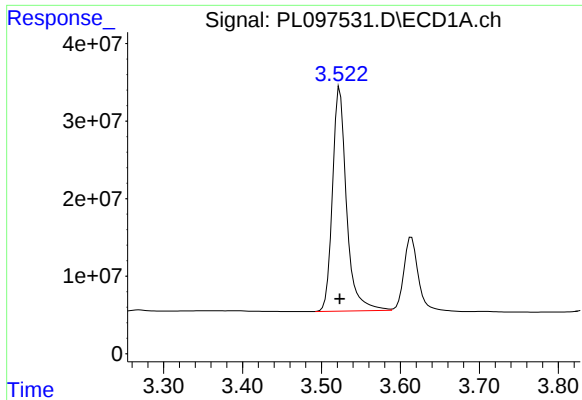

#1 Tetrachloro-m-xylene


R.T.: 3.523 min
Delta R.T.: 0.000 min
Response: 358483603
Conc: 99.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

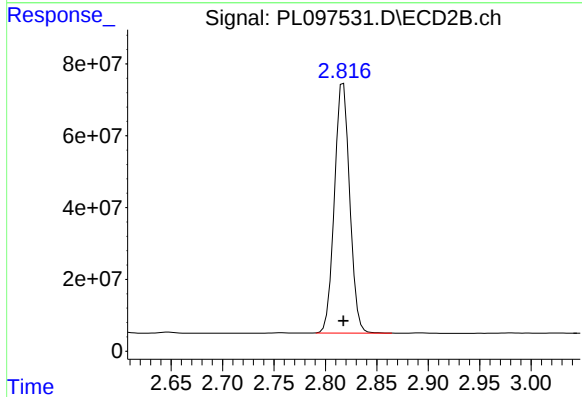


#1 Tetrachloro-m-xylene

R.T.: 2.817 min
Delta R.T.: 0.000 min
Response: 717695306
Conc: 100.96 ng/ml

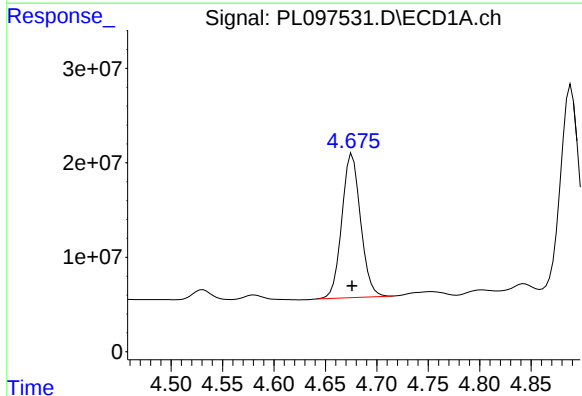


#23 Chlordane-1

R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 193224787
Conc: 988.21 ng/ml

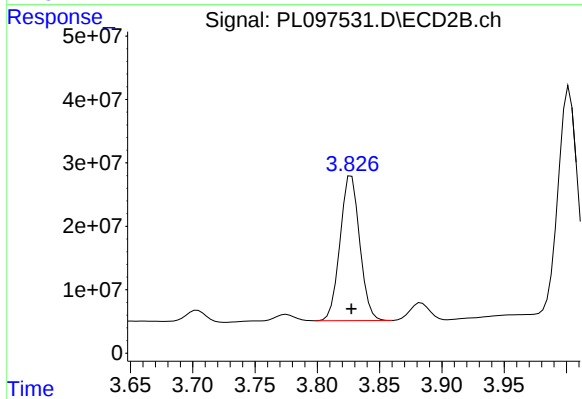

#23 Chlordane-1


R.T.: 3.827 min
Delta R.T.: 0.000 min
Response: 251456835
Conc: 1003.53 ng/ml

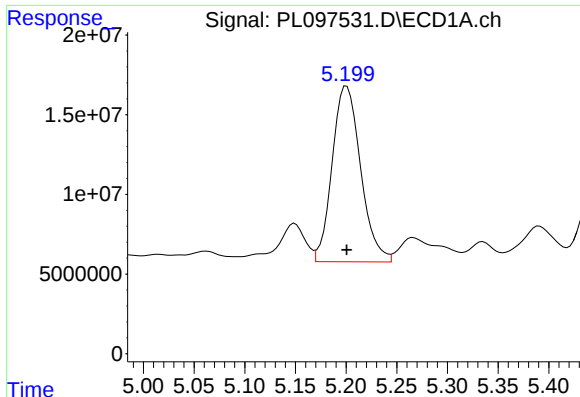

#24 Chlordane-2


R.T.: 5.201 min
Delta R.T.: 0.000 min
Response: 215663133
Conc: 978.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

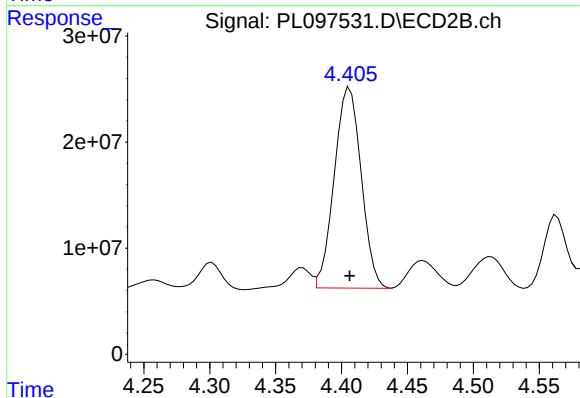


#24 Chlordane-2

R.T.: 4.406 min
Delta R.T.: 0.000 min
Response: 268698978
Conc: 982.52 ng/ml

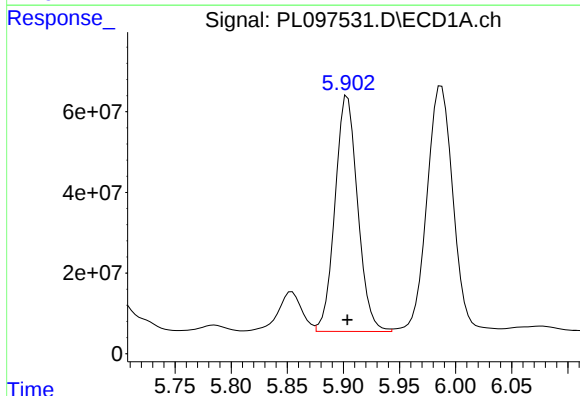


#25 Chlordane-3

R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 821693638
Conc: 998.04 ng/ml

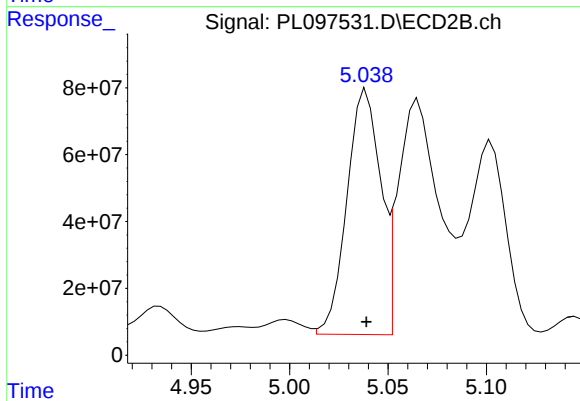

#25 Chlordane-3


R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 868711336
Conc: 991.26 ng/ml

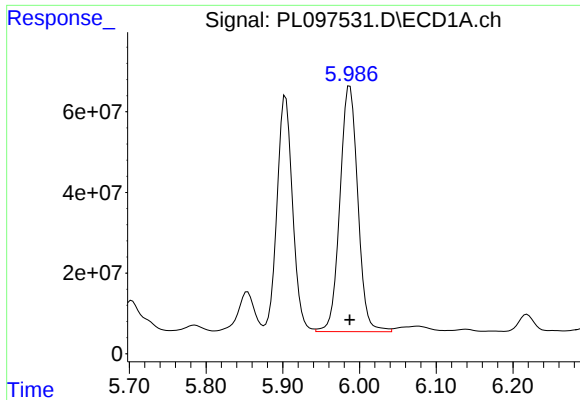

#26 Chlordane-4


R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 989666040
Conc: 994.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

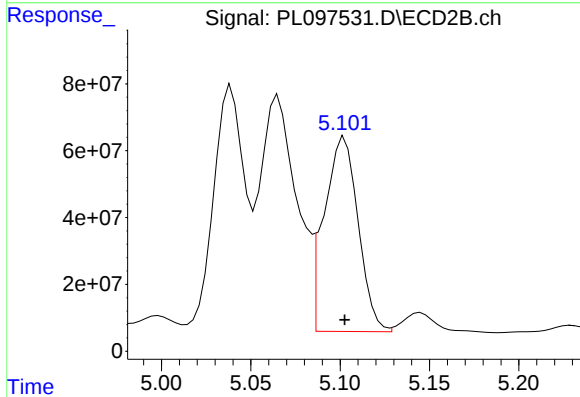


#26 Chlordane-4

R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 770181417
Conc: 992.40 ng/ml

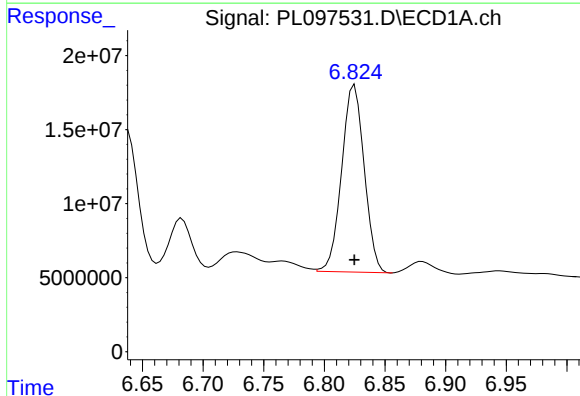


#27 Chlordane-5

R.T.: 6.825 min
Delta R.T.: 0.000 min
Response: 163527701
Conc: 974.69 ng/ml

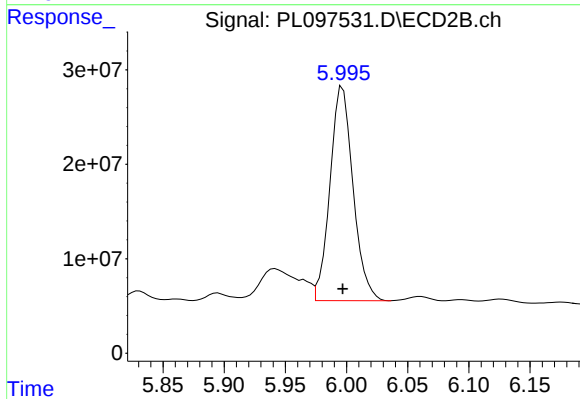

#27 Chlordane-5


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 298571865
Conc: 1011.54 ng/ml

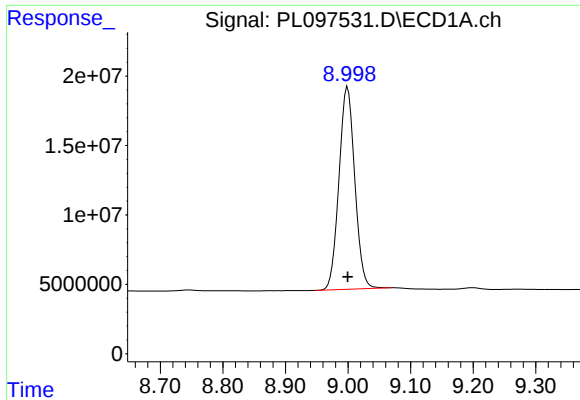

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 256658293
Conc: 99.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

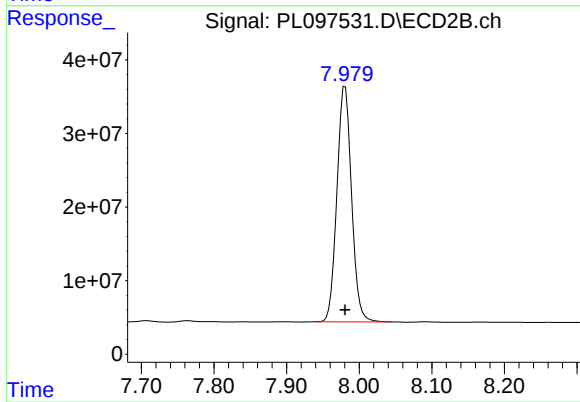

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 448169914
Conc: 98.31 ng/ml