

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
 Data File : PL097557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2025 19:39
 Operator : AR\AJ
 Sample : Q3297-11
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/08/2025
 Supervised By :mohammad ahmed 10/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 03:07:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 16:47:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.524	2.824	58784891	87141472	14.420m	14.317
28) SA Decachlor...	8.996	7.982	40265744	54386767	13.541	10.481

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100725\
Data File : PL097557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2025 19:39
Operator : AR\AJ
Sample : Q3297-11
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
TP2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/08/2025
Supervised By : mohammad ahmed 10/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 03:07:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 16:47:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

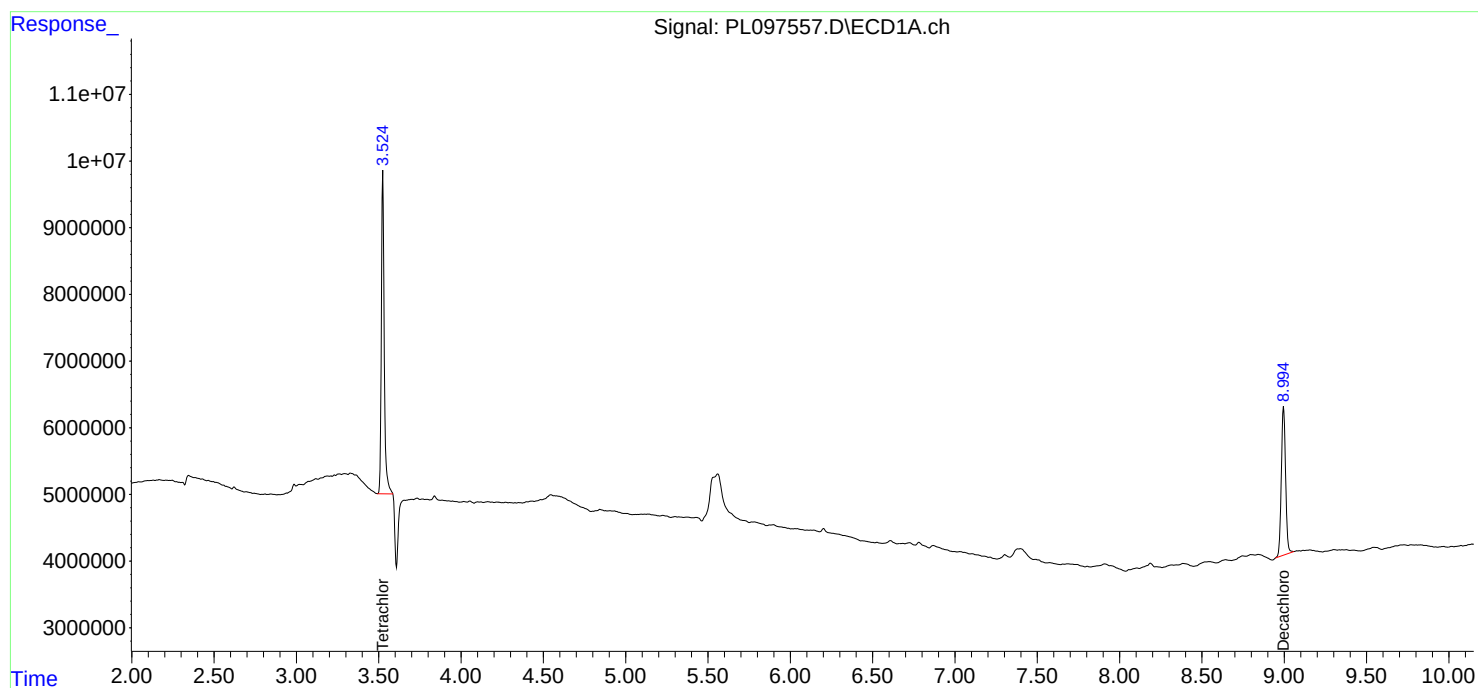

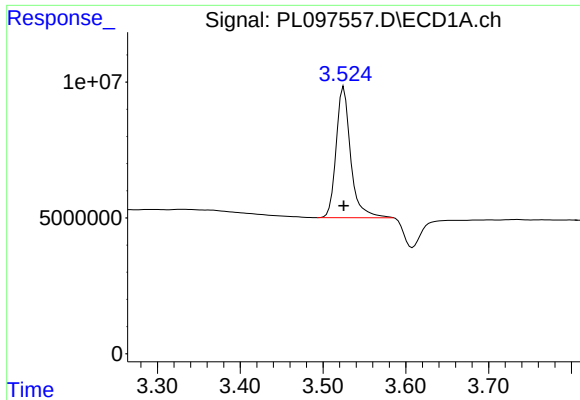


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.001 min
Response: 58784891
Conc: 14.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/08/2025
Supervised By :mohammad ahmed 10/09/2025

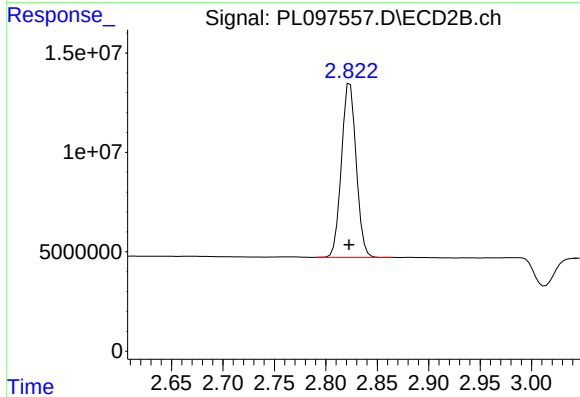


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 87141472
Conc: 14.32 ng/ml

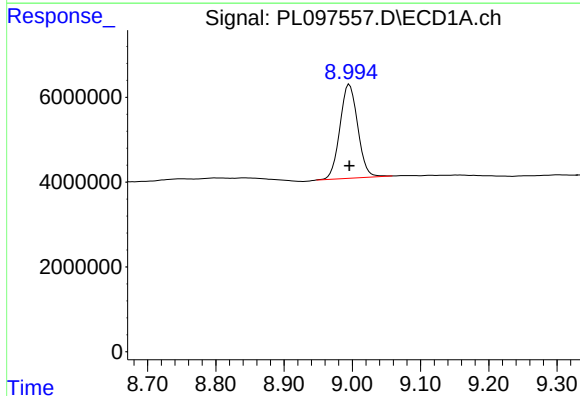

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 40265744
Conc: 13.54 ng/ml

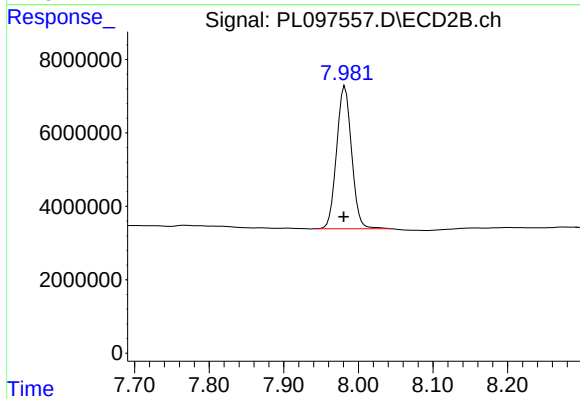

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.002 min
Response: 54386767
Conc: 10.48 ng/ml