

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100818\
 Data File : PL040785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2018 18:01
 Operator : AJ\SJ
 Sample : J5309-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 01:09:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 06 04:55:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.805	169.8E6	65003109	18.930	19.803
28)	SA Decachlor...	7.806	8.725	107.4E6	30789897	9.932	10.934
Target Compounds							
4)	MA Heptachlor	0.000	5.009f	0	4189355	N.D.	0.985 #
5)	MB Aldrin	4.386	0.000	7090350	0	0.573	N.D. #
7)	B delta-BHC	4.386f	4.844	7090350	2720731	0.543	0.664
8)	B Heptachlo...	4.903f	0.000	20814409	0	1.729	N.D. #
12)	B 4,4'-DDE	0.000	6.081	0	2268958	N.D.	0.631 #
16)	A 4,4'-DDD	5.781	0.000	33240316	0	3.460	N.D. #
19)	B Endosulfa...	6.327	0.000	18936081	0	1.743	N.D. #
23)	Chlordane-1	4.048	0.000	6299298	0	14.944	N.D. #
27)	Chlordane-5	0.000	6.675	0	8028974	N.D.	70.593 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100818\
Data File : PL040785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2018 18:01
Operator : AJ\SJ
Sample : J5309-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 01:09:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
Quant Title : GC Extractables
QLast Update : Sat Oct 06 04:55:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

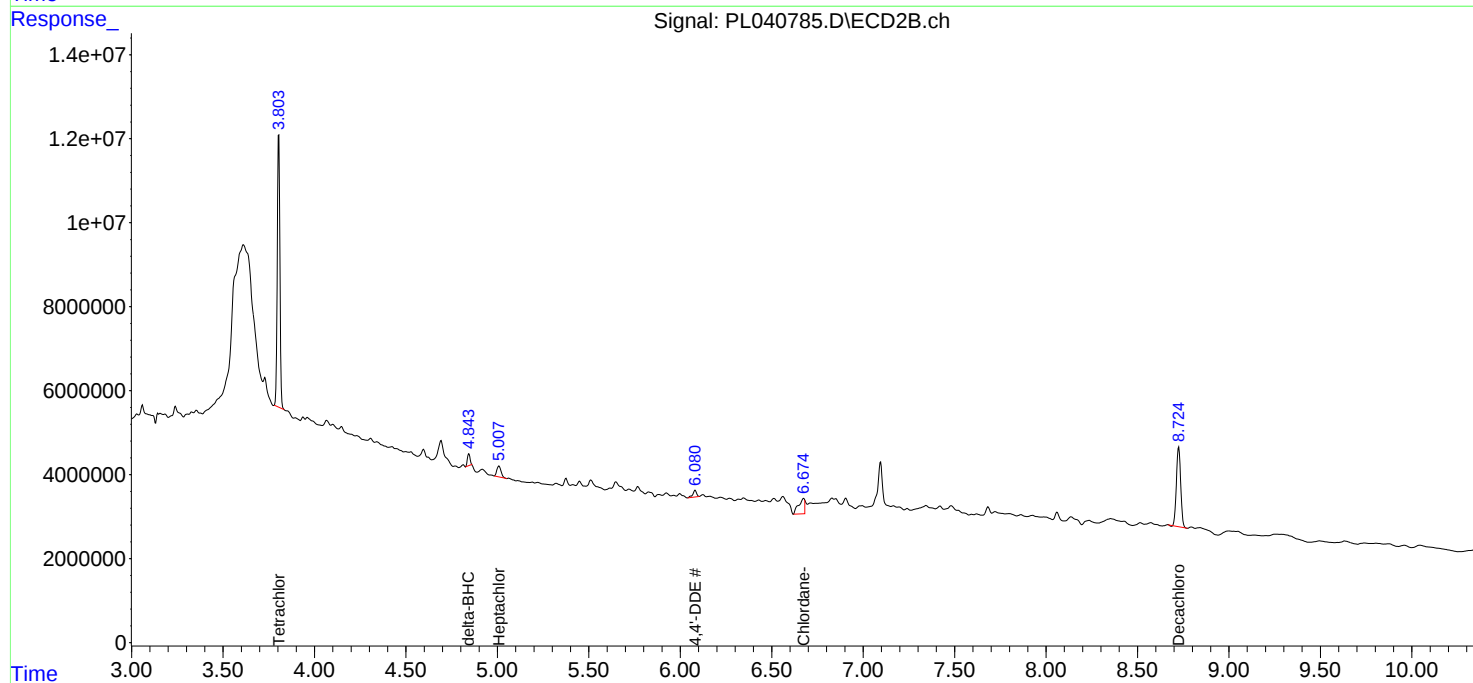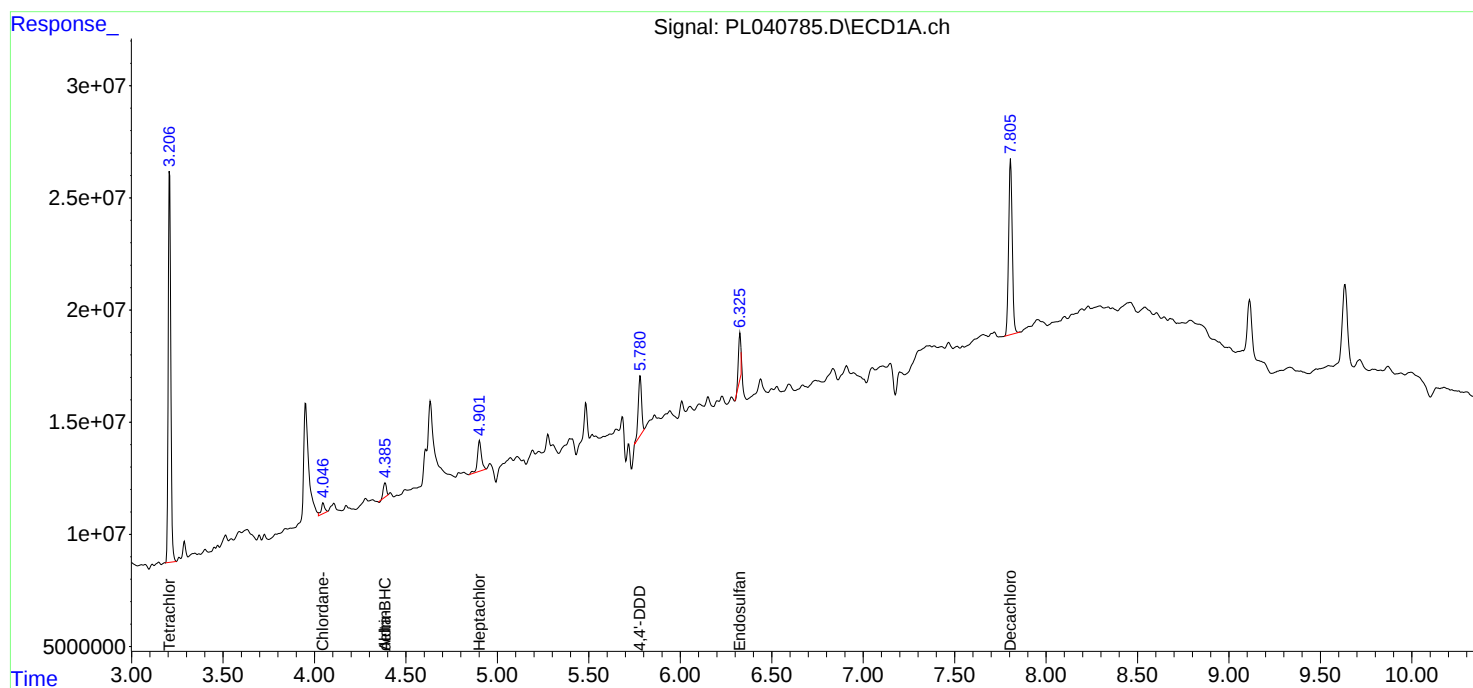


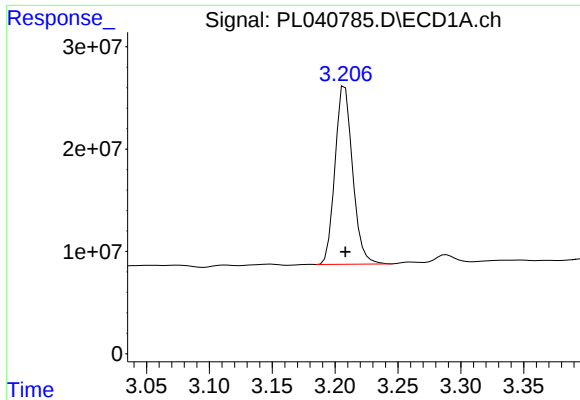

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 169828794
Conc: 18.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

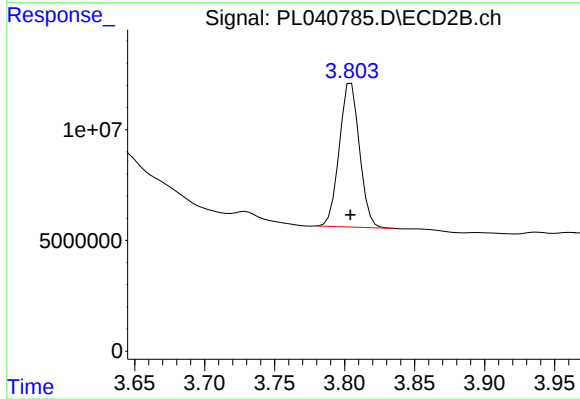


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 65003109
Conc: 19.80 ng/ml

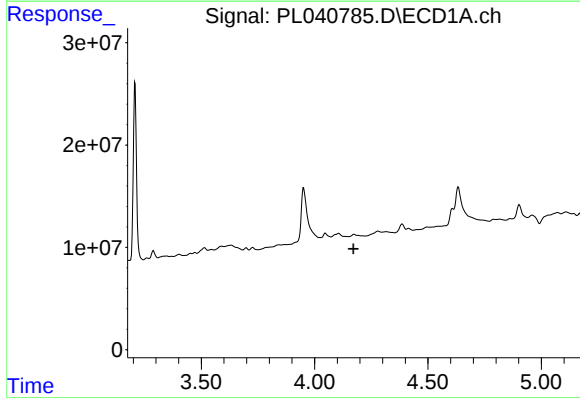


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.172 min
Response: 0
Conc: N.D.

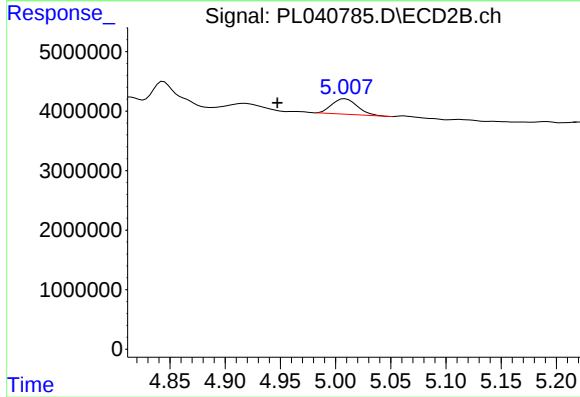

#4 Heptachlor


R.T.: 5.009 min
Delta R.T.: 0.061 min
Response: 4189355
Conc: 0.98 ng/ml

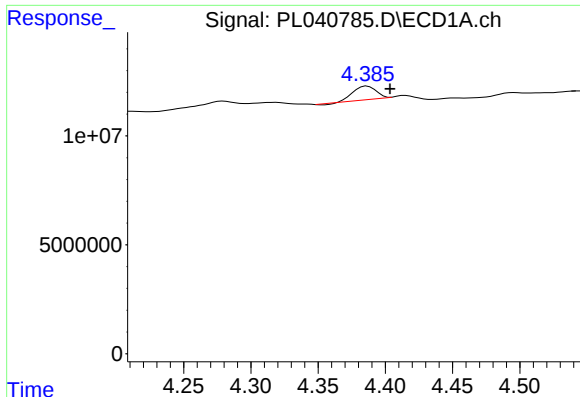

#5 Aldrin


R.T.: 4.386 min
Delta R.T.: -0.017 min
Response: 7090350
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

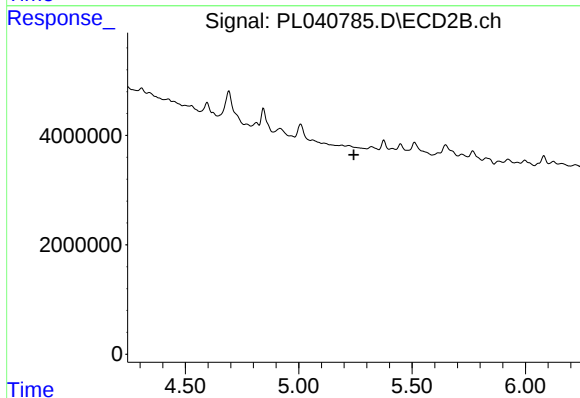


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.243 min
Response: 0
Conc: N.D.

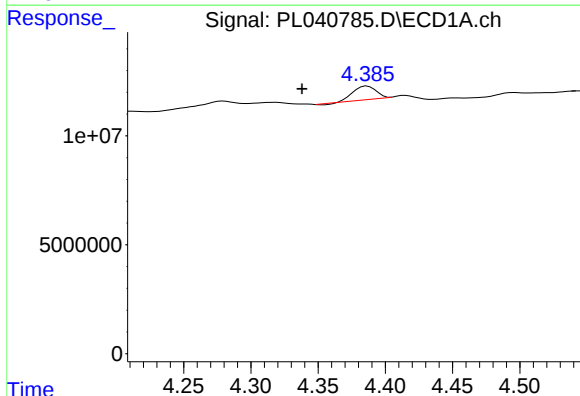


#7 delta-BHC

R.T.: 4.386 min
Delta R.T.: 0.048 min
Response: 7090350
Conc: 0.54 ng/ml

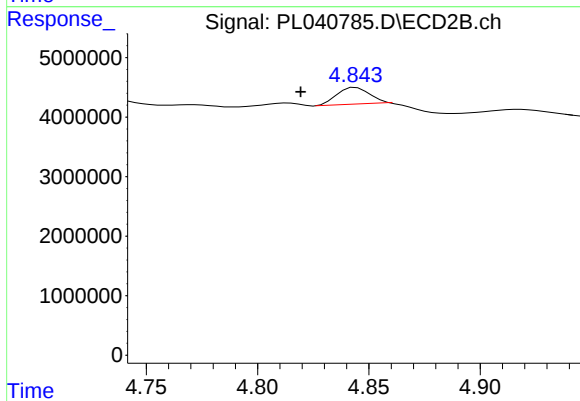

#7 delta-BHC


R.T.: 4.844 min
Delta R.T.: 0.025 min
Response: 2720731
Conc: 0.66 ng/ml

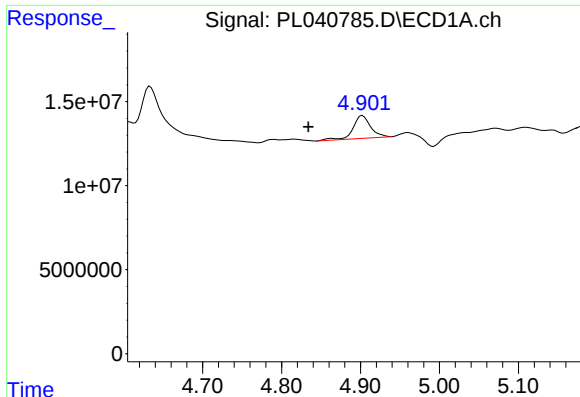

#8 Heptachlor epoxide


R.T.: 4.903 min
Delta R.T.: 0.069 min
Response: 20814409
Conc: 1.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

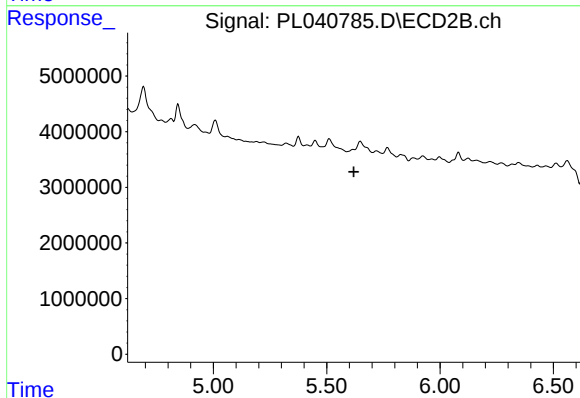


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.620 min
Response: 0
Conc: N.D.

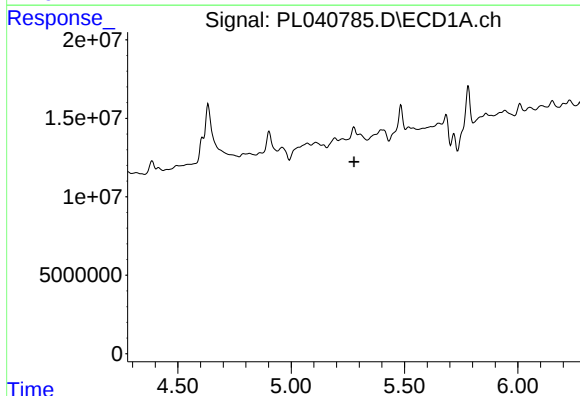


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

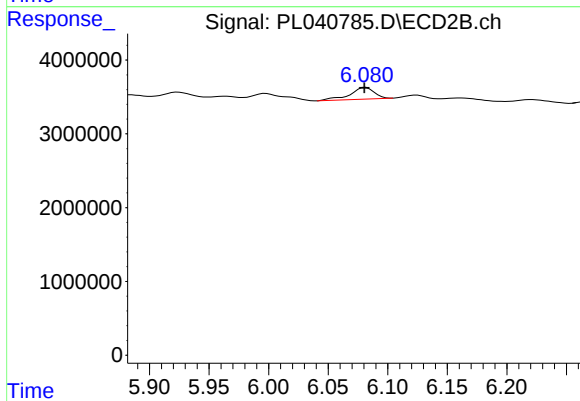

#12 4,4'-DDE


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 2268958
Conc: 0.63 ng/ml

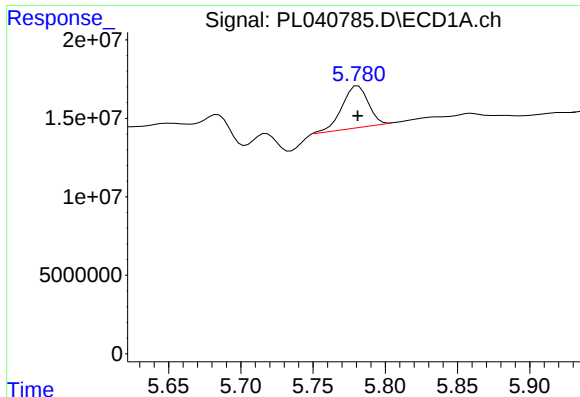

#16 4,4'-DDD


R.T.: 5.781 min
Delta R.T.: 0.000 min
Response: 33240316
Conc: 3.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

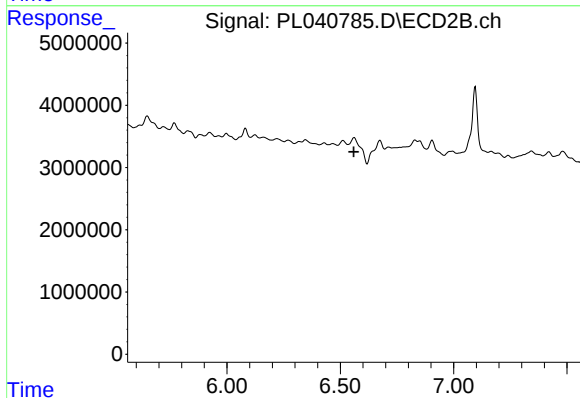


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

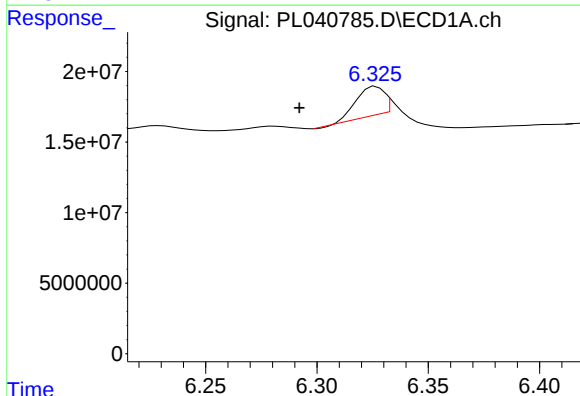


#19 Endosulfan Sulfate

R.T.: 6.327 min
Delta R.T.: 0.035 min
Response: 18936081
Conc: 1.74 ng/ml

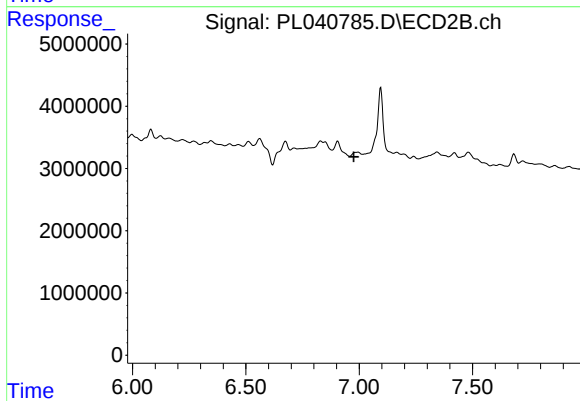

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.977 min
Response: 0
Conc: N.D.

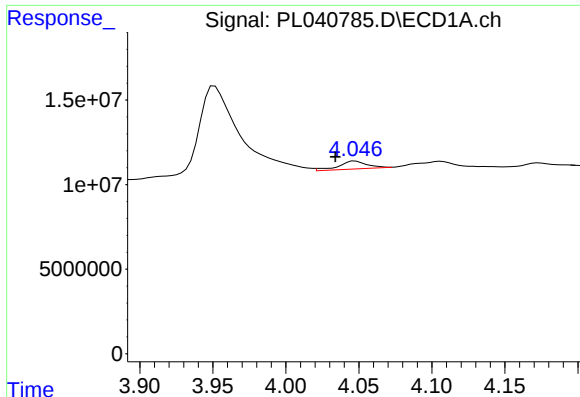

#23 Chlordane-1


R.T.: 4.048 min
Delta R.T.: 0.014 min
Response: 6299298
Conc: 14.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

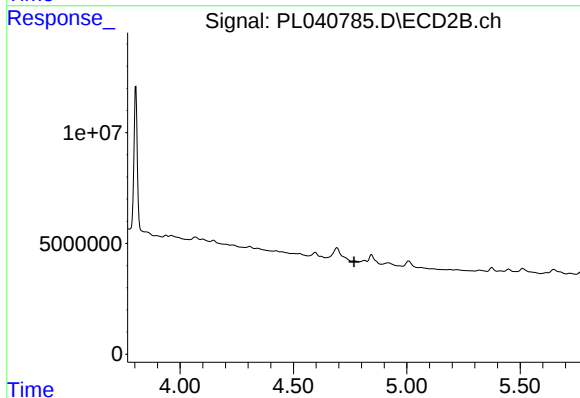


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.768 min
Response: 0
Conc: N.D.

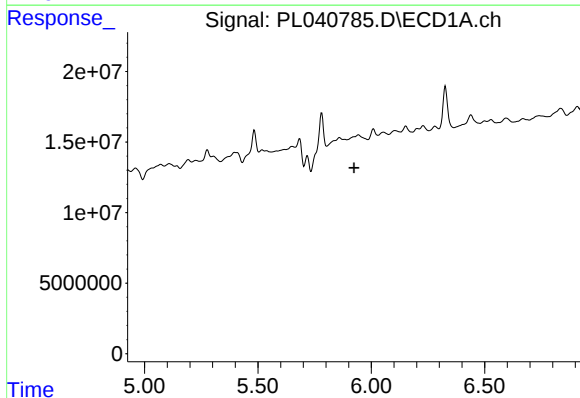


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.924 min
Response: 0
Conc: N.D.

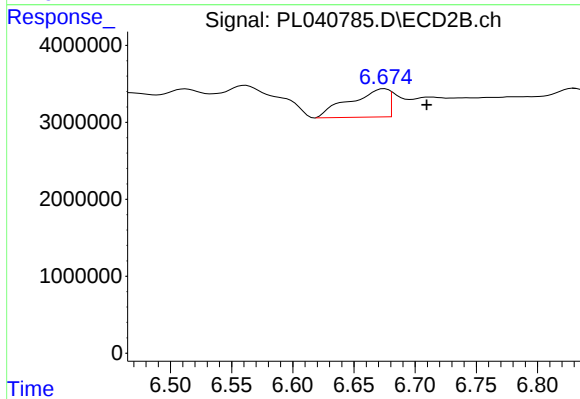

#27 Chlordane-5


R.T.: 6.675 min
Delta R.T.: -0.035 min
Response: 8028974
Conc: 70.59 ng/ml

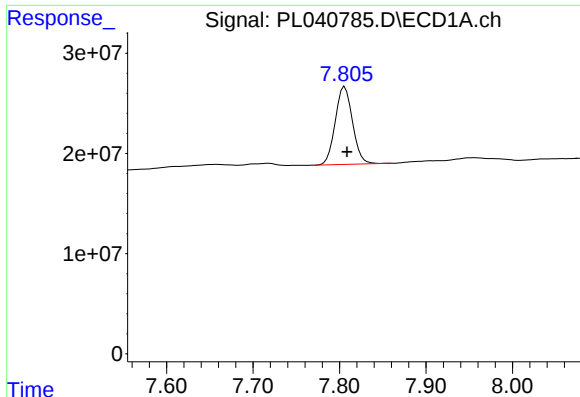

#28 Decachlorobiphenyl

R.T.: 7.806 min
Delta R.T.: -0.002 min
Response: 107405927
Conc: 9.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

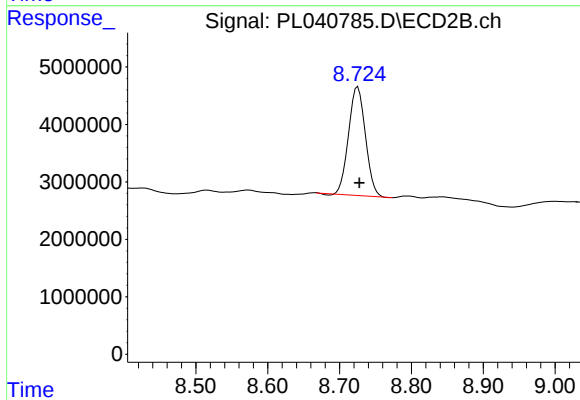

#28 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.002 min
Response: 30789897
Conc: 10.93 ng/ml