

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100818\
 Data File : PL040800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2018 23:42
 Operator : AJ\SJ
 Sample : J5309-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 02:17:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 06 04:55:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.804	153.5E6	59909347	17.110	18.251
28)	SA Decachlor...	7.806	8.725	72021310	24033491	6.660	8.535 #
Target Compounds							
2)	A alpha-BHC	3.585f	0.000	8224765	0	0.577	N.D. #
4)	MA Heptachlor	4.106f	0.000	10470268	0	0.730	N.D. #
6)	B beta-BHC	4.106f	0.000	10470268	0	2.230	N.D. #
7)	B delta-BHC	0.000	4.844f	0	4713501	N.D.	1.151 #
9)	A Endosulfan I	5.192	5.924f	13697351	2096903	1.168	0.621 #
11)	B alpha-Chl...	0.000	5.924	0	2096903	N.D.	0.584 #
17)	MA 4,4'-DDT	6.008	0.000	10745626	0	1.047	N.D. #
26)	Chlordane-4	0.000	5.924	0	2096903	N.D.	3.569 #
27)	Chlordane-5	0.000	6.671	0	4950549	N.D.	43.527 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100818\
Data File : PL040800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2018 23:42
Operator : AJ\SJ
Sample : J5309-25
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 02:17:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
Quant Title : GC Extractables
QLast Update : Sat Oct 06 04:55:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

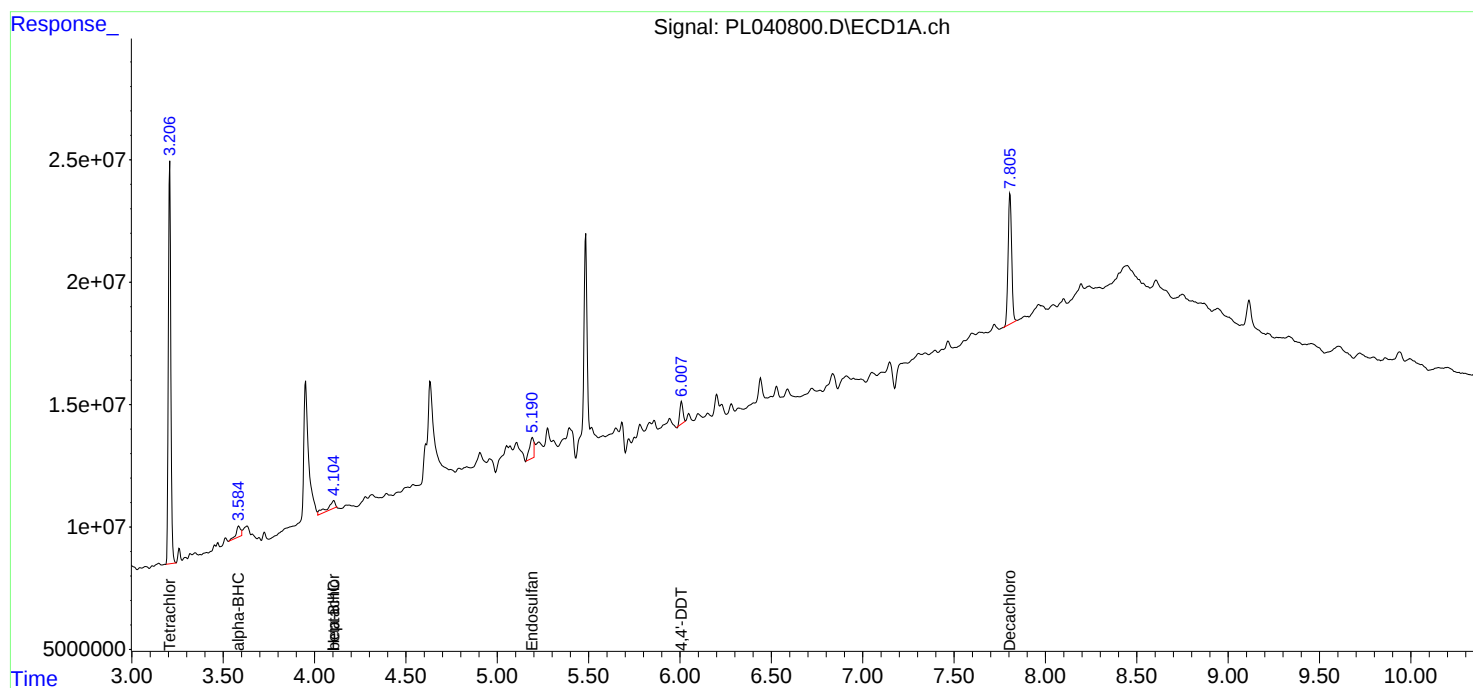


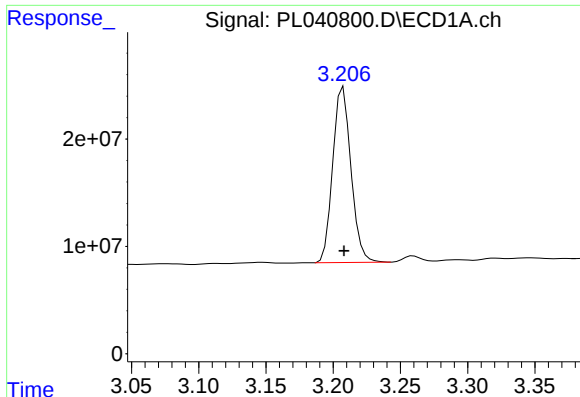

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 153502363
Conc: 17.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

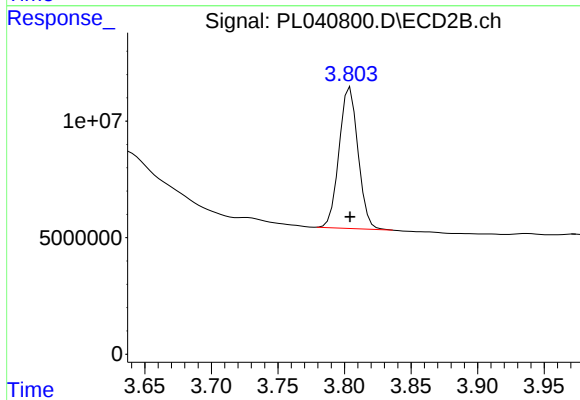


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 59909347
Conc: 18.25 ng/ml

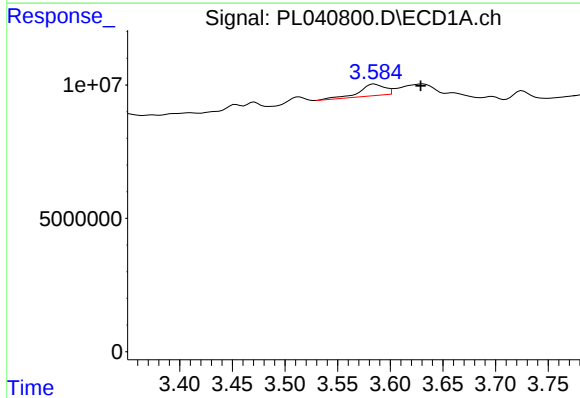


#2 alpha-BHC

R.T.: 3.585 min
Delta R.T.: -0.044 min
Response: 8224765
Conc: 0.58 ng/ml

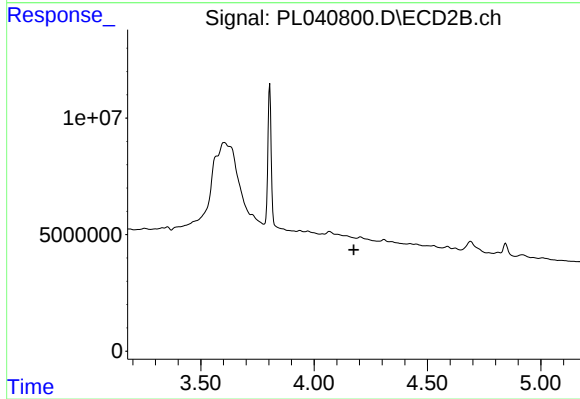

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.176 min
Response: 0
Conc: N.D.

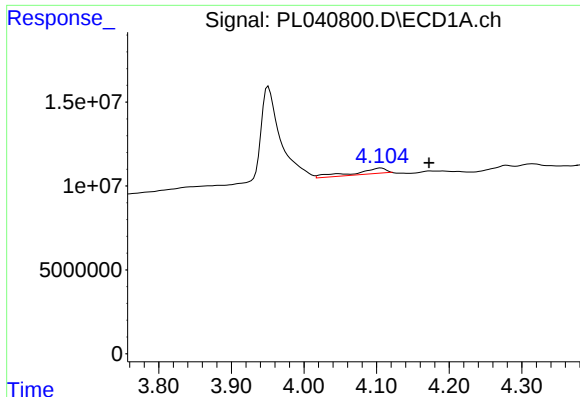

#4 Heptachlor


R.T.: 4.106 min
Delta R.T.: -0.066 min
Response: 10470268
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

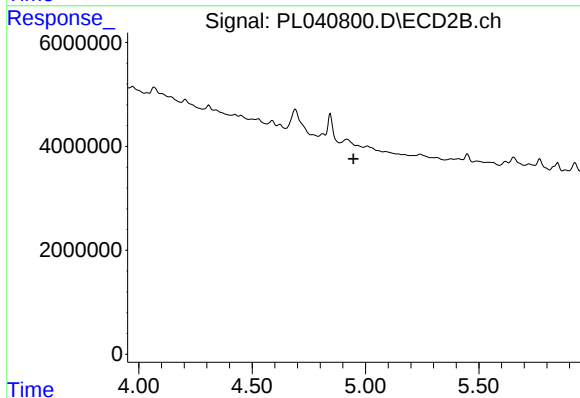


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.947 min
Response: 0
Conc: N.D.

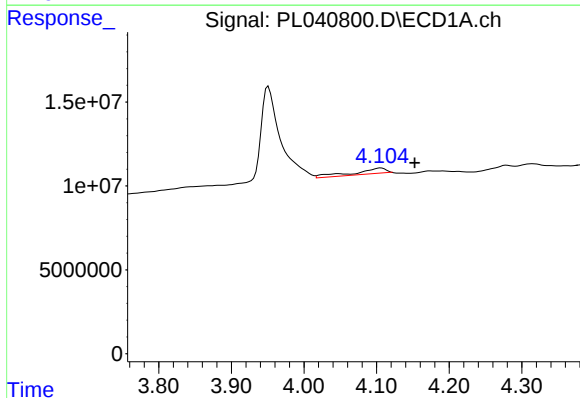


#6 beta-BHC

R.T.: 4.106 min
Delta R.T.: -0.047 min
Response: 10470268
Conc: 2.23 ng/ml

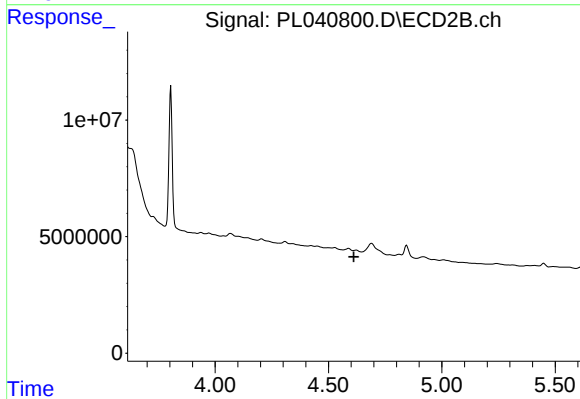

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

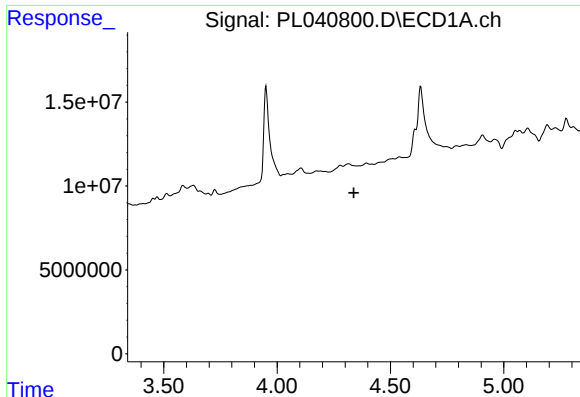

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

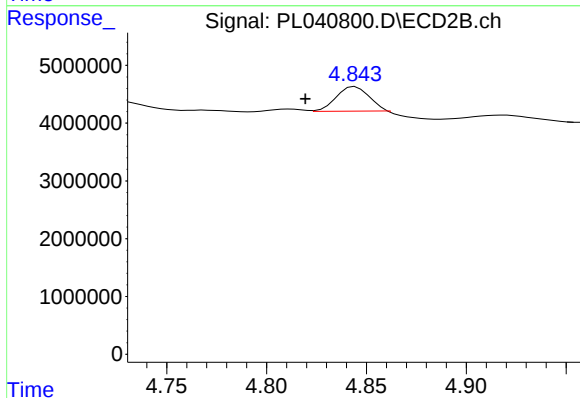


#7 delta-BHC

R.T.: 4.844 min
Delta R.T.: 0.025 min
Response: 4713501
Conc: 1.15 ng/ml

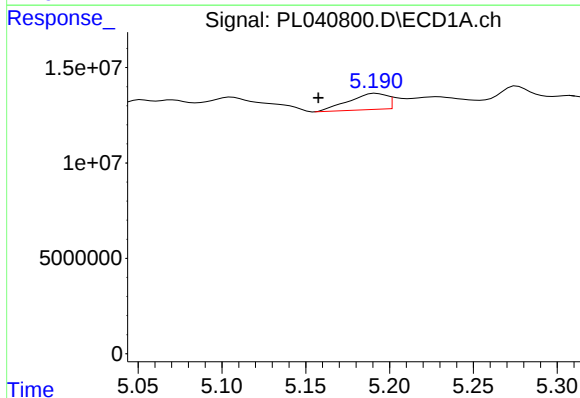


#9 Endosulfan I

R.T.: 5.192 min
Delta R.T.: 0.034 min
Response: 13697351
Conc: 1.17 ng/ml

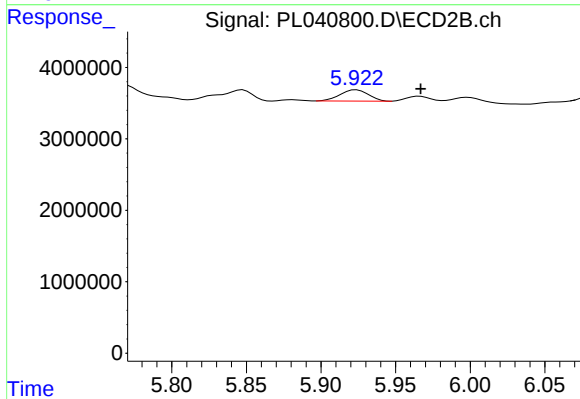

#9 Endosulfan I


R.T.: 5.924 min
Delta R.T.: -0.043 min
Response: 2096903
Conc: 0.62 ng/ml

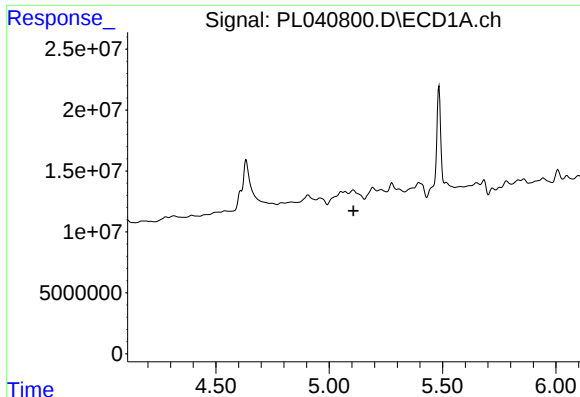

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

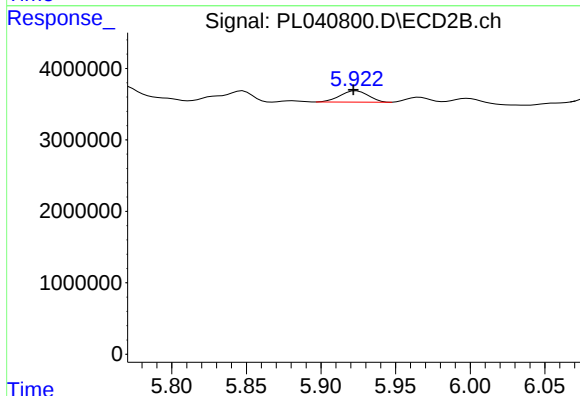


#11 alpha-Chlordane

R.T.: 5.924 min
Delta R.T.: 0.002 min
Response: 2096903
Conc: 0.58 ng/ml

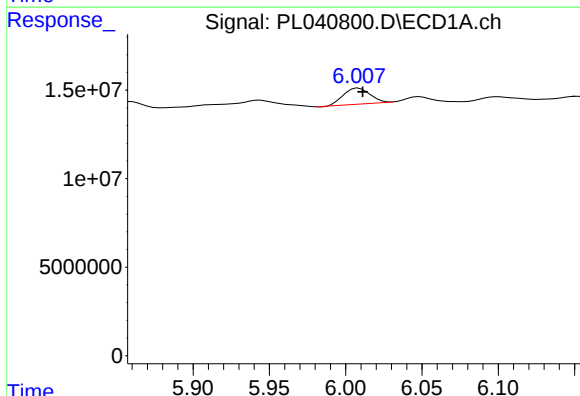


#17 4,4'-DDT

R.T.: 6.008 min
Delta R.T.: -0.003 min
Response: 10745626
Conc: 1.05 ng/ml

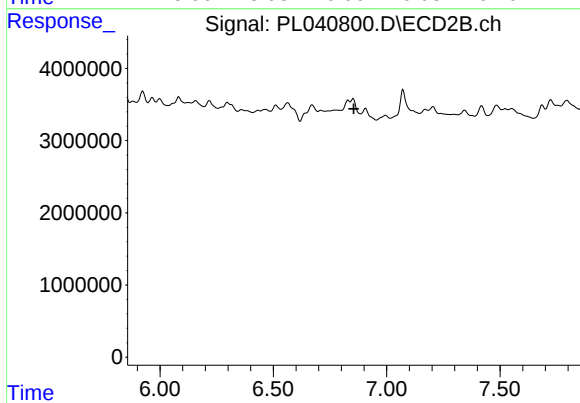

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.855 min
Response: 0
Conc: N.D.

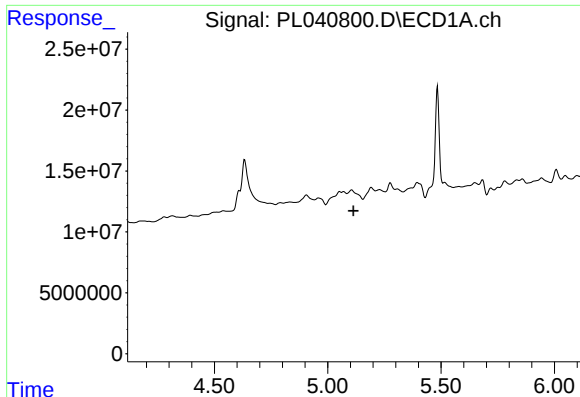

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

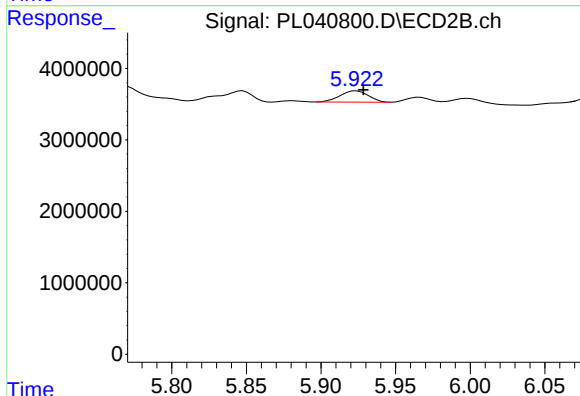


#26 Chlordane-4

R.T.: 5.924 min
Delta R.T.: -0.005 min
Response: 2096903
Conc: 3.57 ng/ml

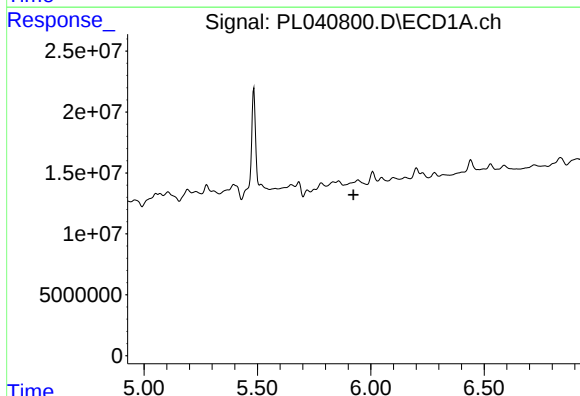


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.924 min
Response: 0
Conc: N.D.

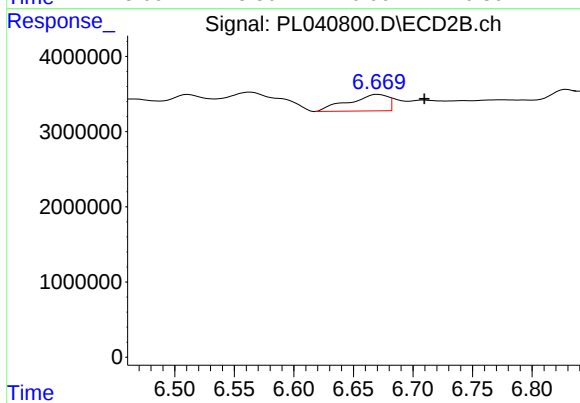

#27 Chlordane-5


R.T.: 6.671 min
Delta R.T.: -0.039 min
Response: 4950549
Conc: 43.53 ng/ml

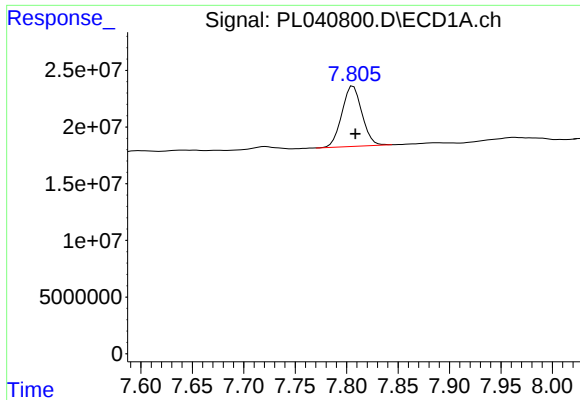

#28 Decachlorobiphenyl

R.T.: 7.806 min
Delta R.T.: -0.002 min
Response: 72021310
Conc: 6.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

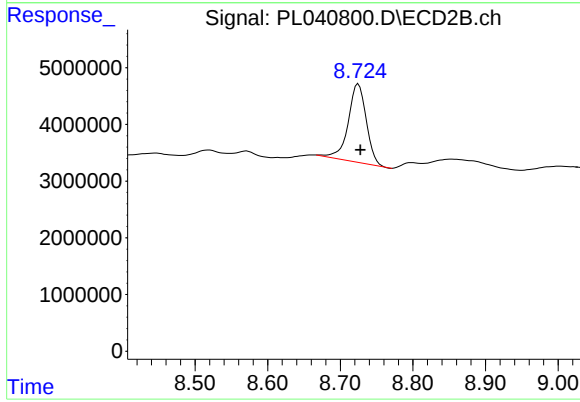

#28 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.003 min
Response: 24033491
Conc: 8.53 ng/ml