

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100819\
 Data File : PL053160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2019 18:36
 Operator : SG\AJ
 Sample : K5238-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 00:43:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.048	196.5E6	48705765	19.753	18.139
28)	SA Decachlor...	8.336	9.125	150.7E6	48984262	15.050	16.697
Target Compounds							
6)	B beta-BHC	4.505f	0.000	25364986	0	4.085	N.D. #
7)	B delta-BHC	0.000	5.085f	0	9323029	N.D.	2.576 #
12)	B 4,4'-DDE	0.000	6.368f	0	3781111	N.D.	1.158 #
19)	B Endosulfa...	0.000	7.311	0	5244753	N.D.	1.921 #
23)	Chlordane-1	0.000	5.054	0	1392634	N.D.	13.730 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100819\
Data File : PL053160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 18:36
Operator : SG\AJ
Sample : K5238-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 00:43:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

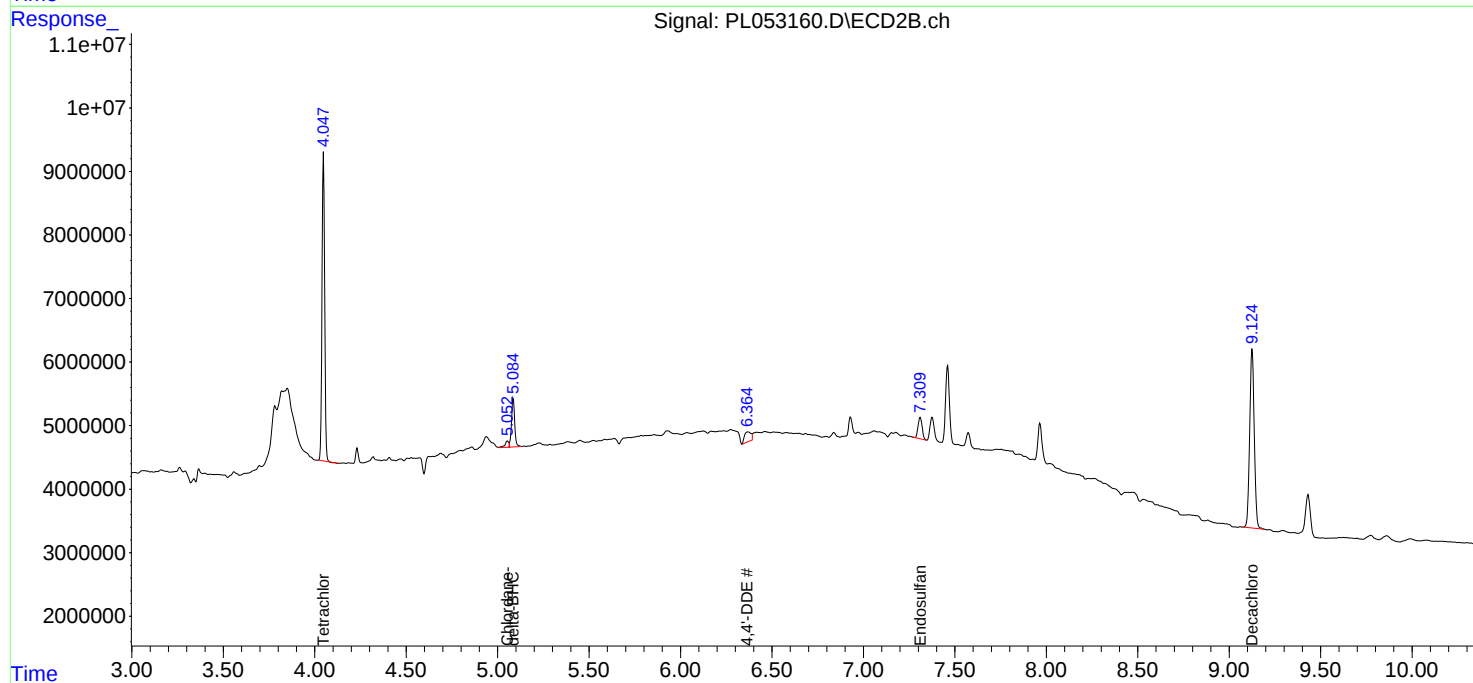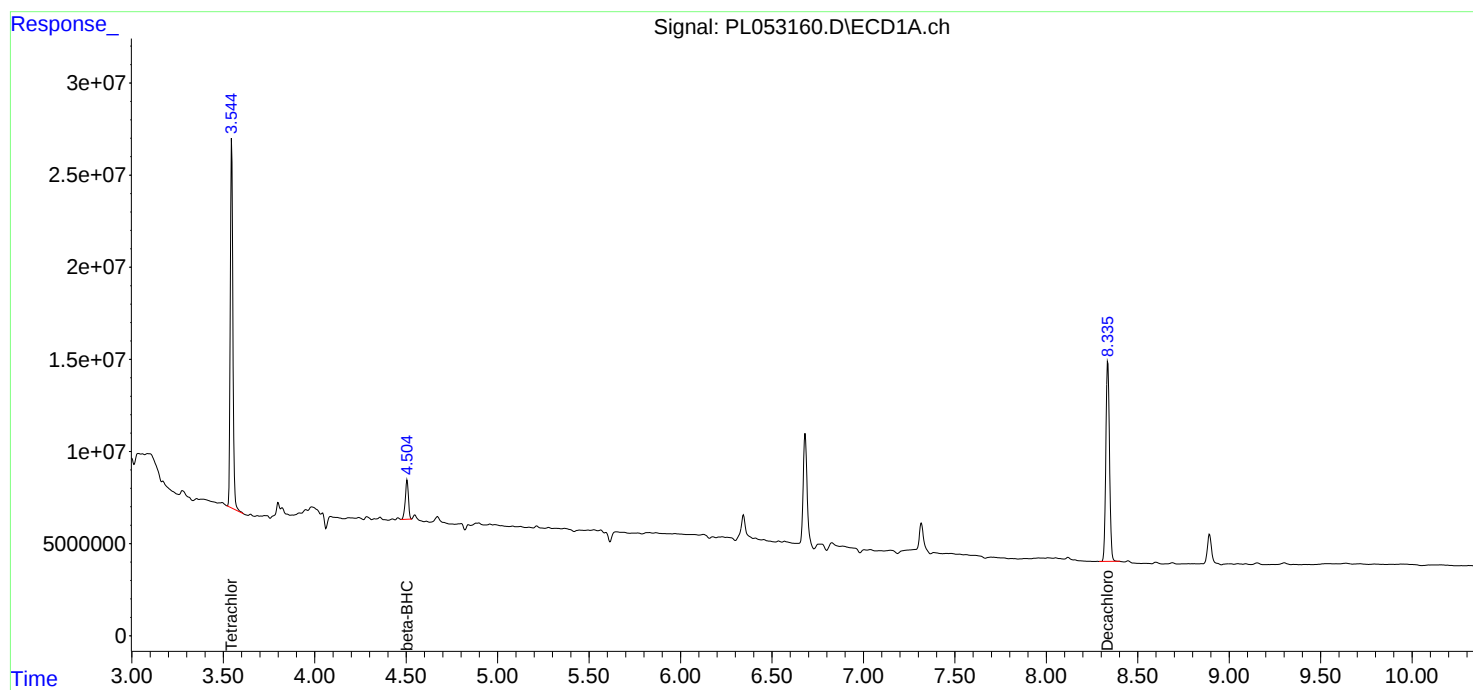


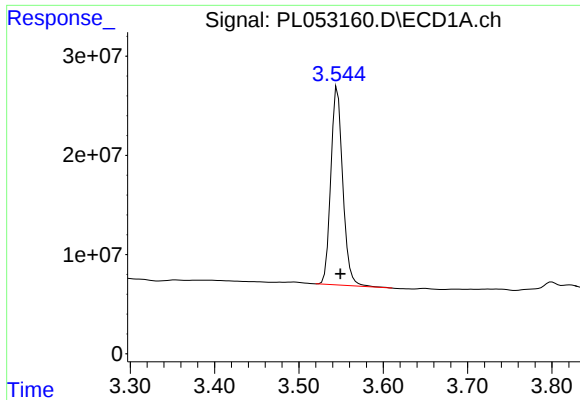

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 196477367
Conc: 19.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

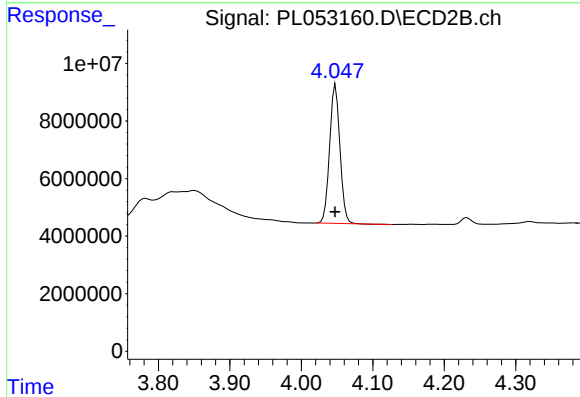


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 48705765
Conc: 18.14 ng/ml

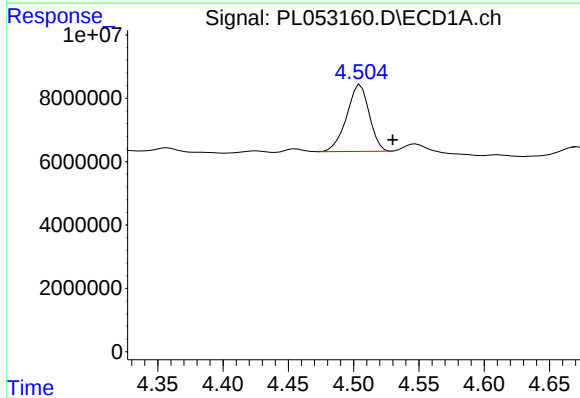


#6 beta-BHC

R.T.: 4.505 min
Delta R.T.: -0.025 min
Response: 25364986
Conc: 4.09 ng/ml

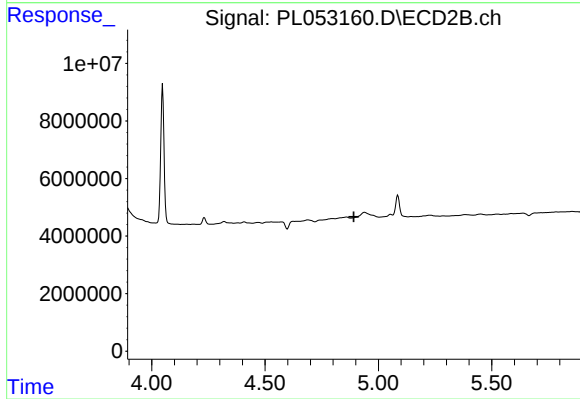

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

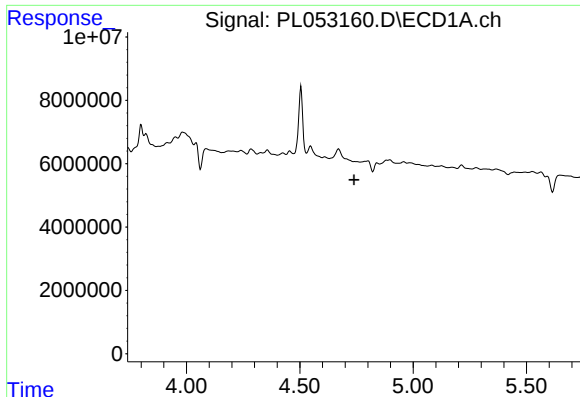

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

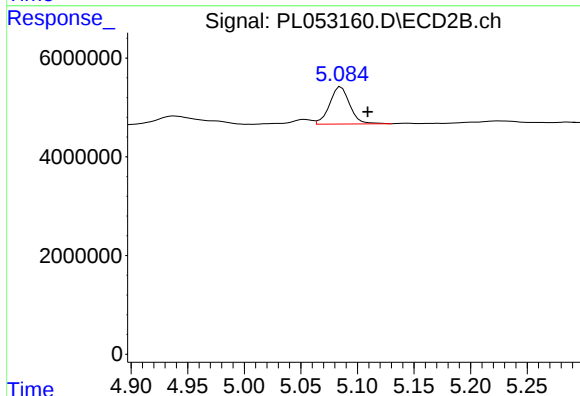


#7 delta-BHC

R.T.: 5.085 min
Delta R.T.: -0.024 min
Response: 9323029
Conc: 2.58 ng/ml

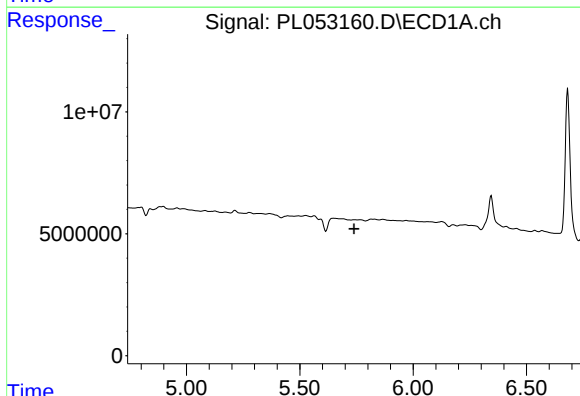


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

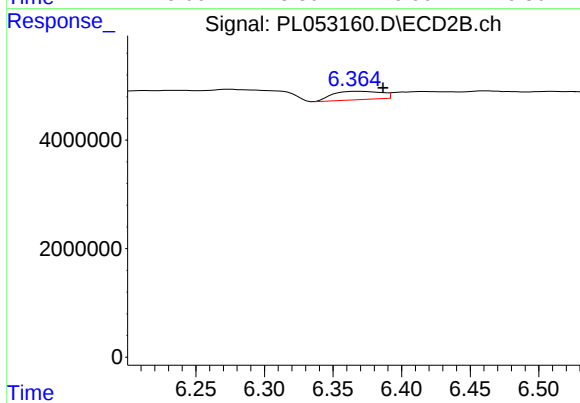

#12 4,4'-DDE


R.T.: 6.368 min
Delta R.T.: -0.019 min
Response: 3781111
Conc: 1.16 ng/ml

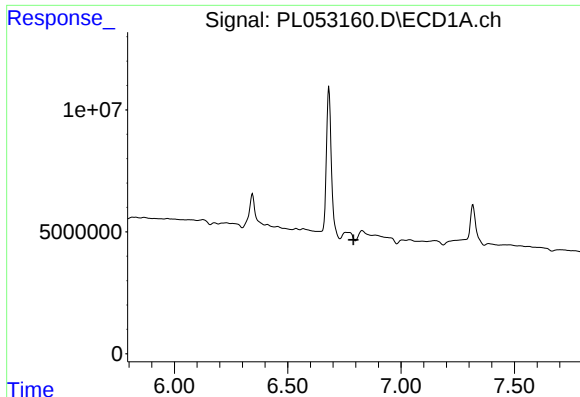

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

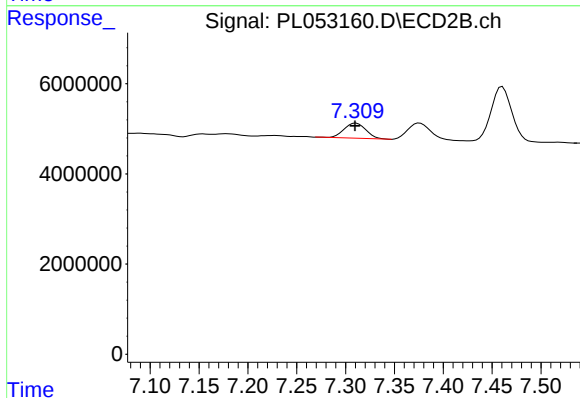


#19 Endosulfan Sulfate

R.T.: 7.311 min
Delta R.T.: 0.000 min
Response: 5244753
Conc: 1.92 ng/ml

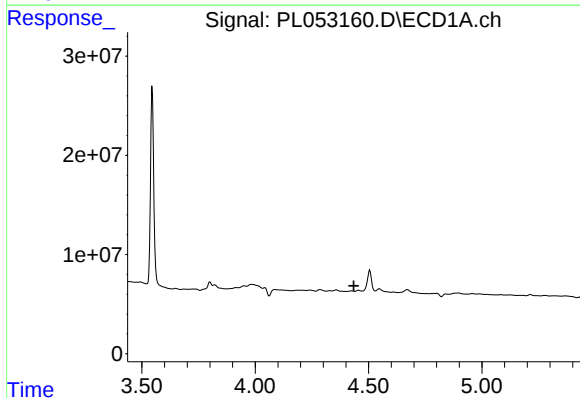


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.435 min
Response: 0
Conc: N.D.

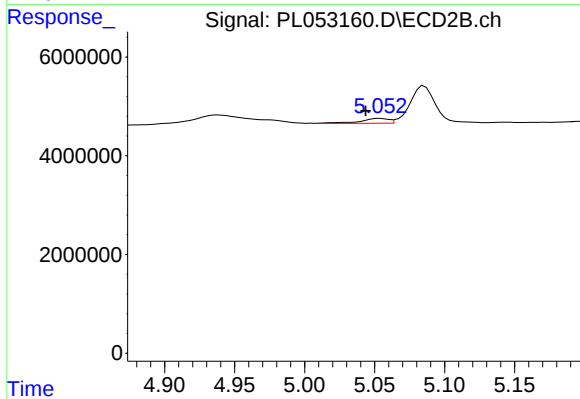

#23 Chlordane-1


R.T.: 5.054 min
Delta R.T.: 0.010 min
Response: 1392634
Conc: 13.73 ng/ml

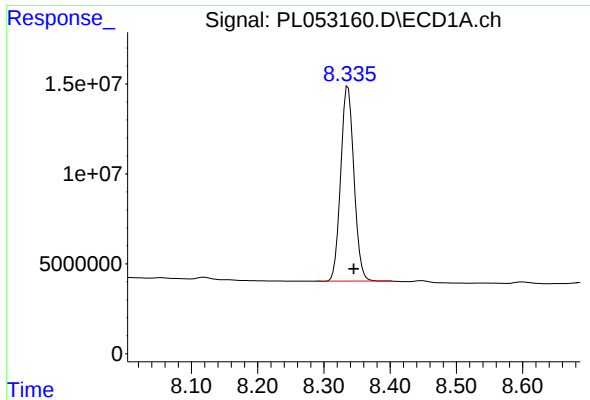

#28 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.009 min
Response: 150737393
Conc: 15.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

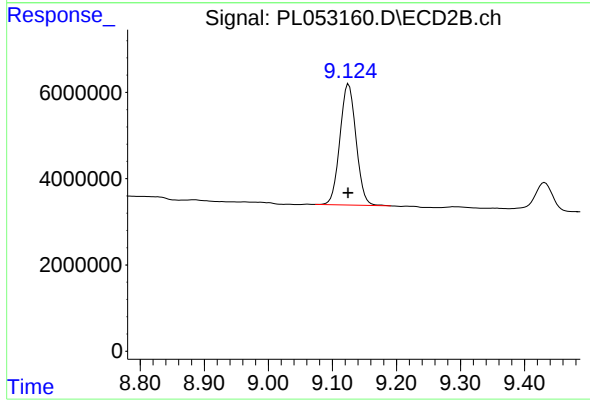

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.001 min
Response: 48984262
Conc: 16.70 ng/ml