

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100819\
 Data File : PL053161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2019 18:50
 Operator : SG\AJ
 Sample : K4230-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 00:43:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.048	189.8E6	45733530	19.078	17.032
28)	SA Decachlor...	8.335	9.125	155.4E6	49285139	15.511	16.800
Target Compounds							
4)	MA Heptachlor	0.000	5.235	0	1975883	N.D.	0.519 #
8)	B Heptachlo...	0.000	5.907f	0	3512606	N.D.	1.048 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100819\
Data File : PL053161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 18:50
Operator : SG\AJ
Sample : K4230-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 00:43:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

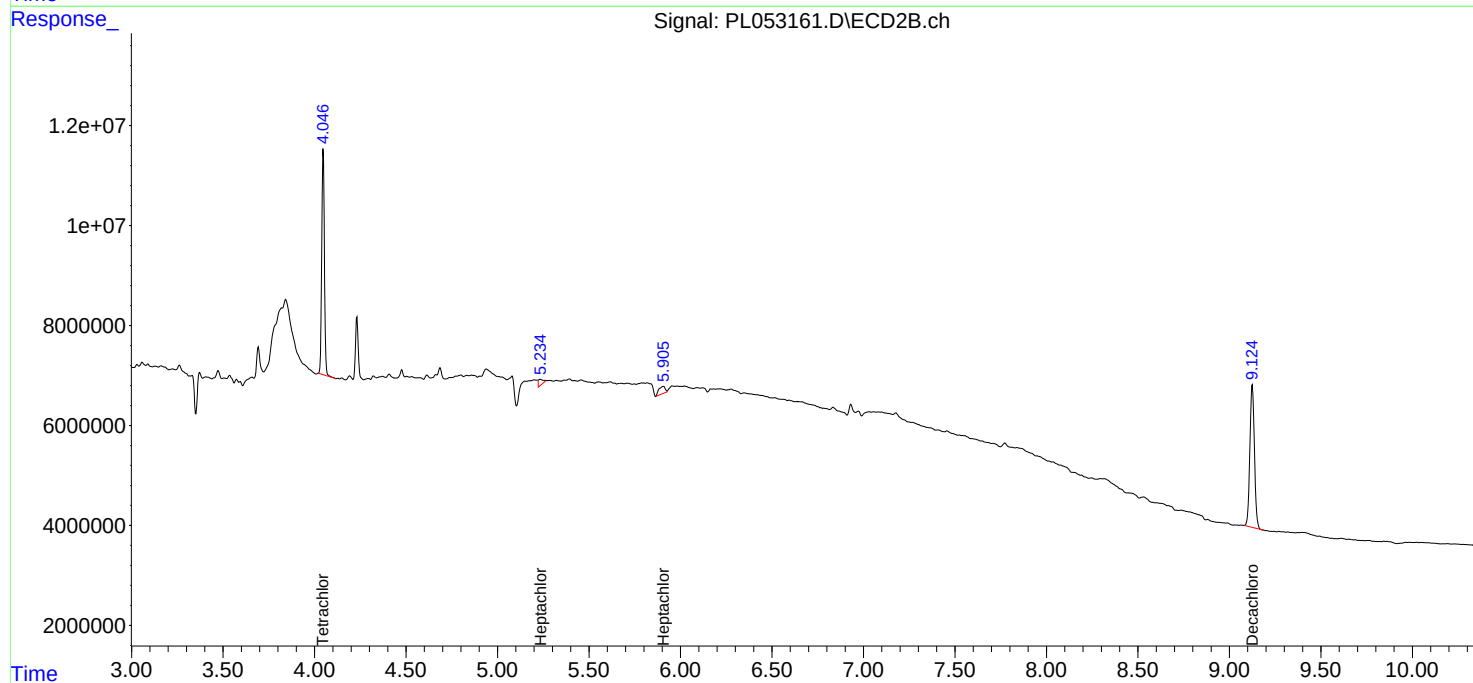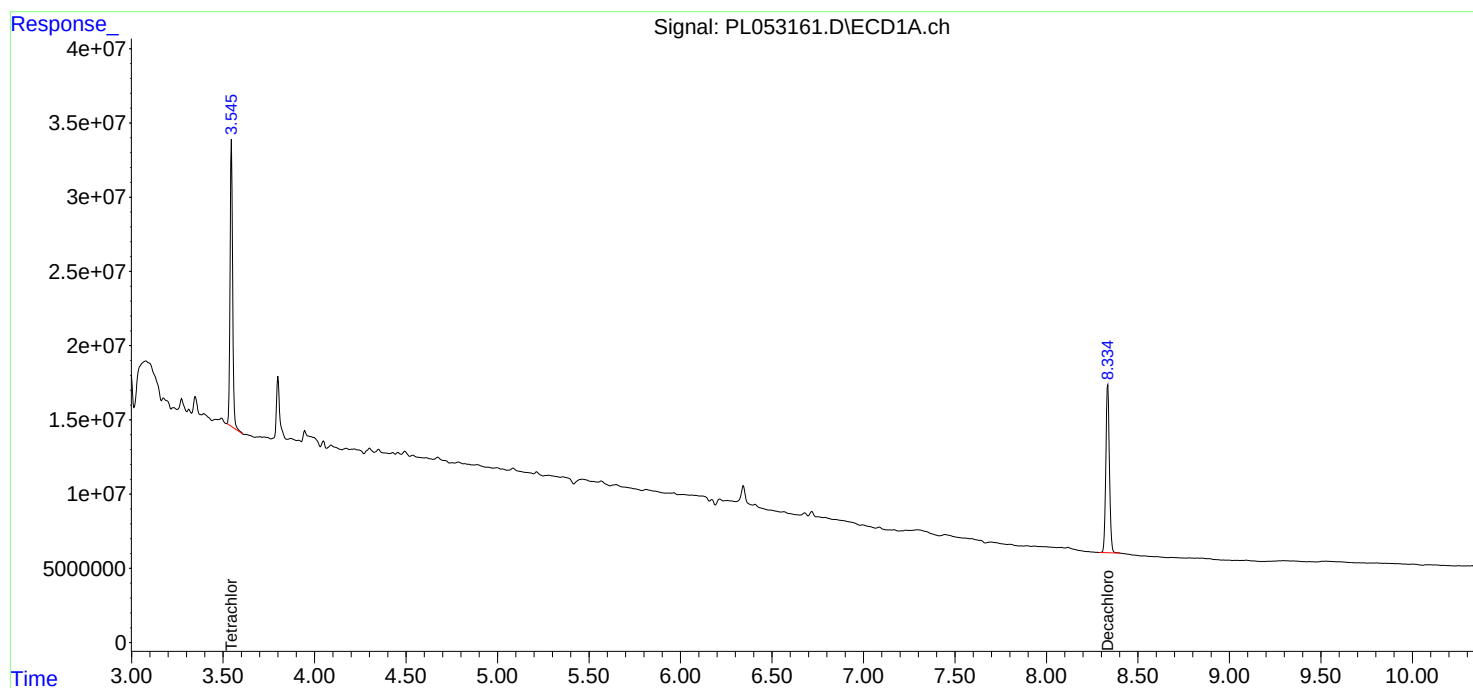


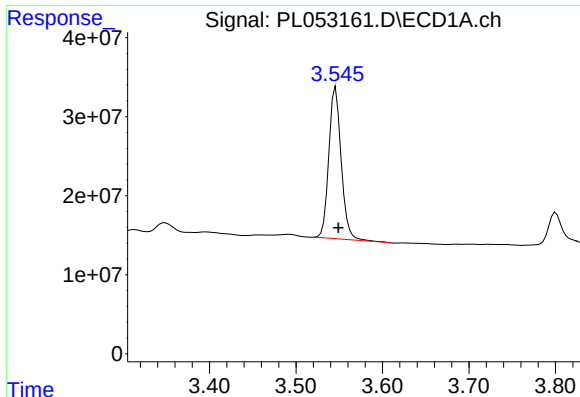

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 189761464
Conc: 19.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

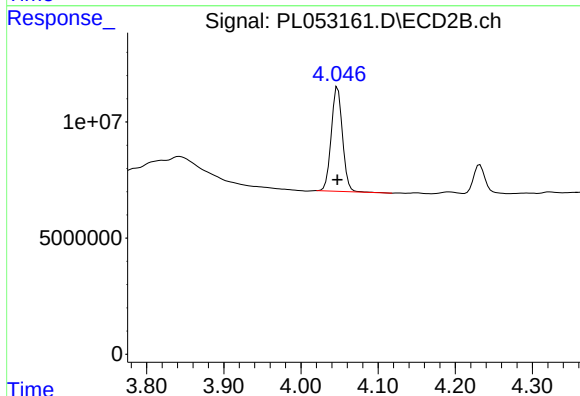


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 45733530
Conc: 17.03 ng/ml

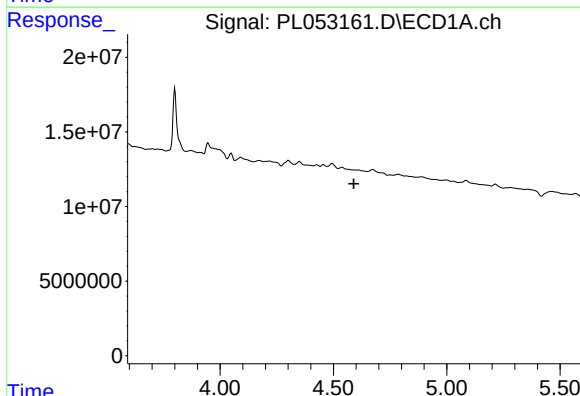


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

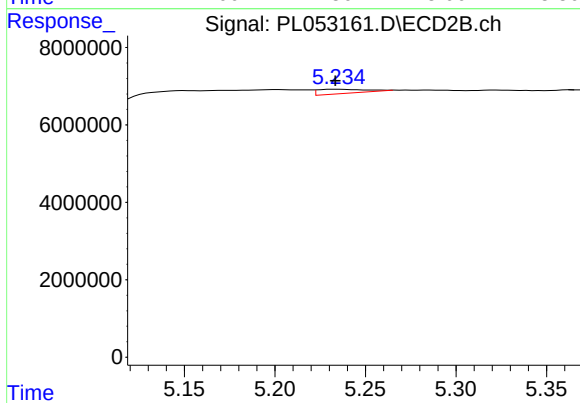

#4 Heptachlor


R.T.: 5.235 min
Delta R.T.: 0.001 min
Response: 1975883
Conc: 0.52 ng/ml

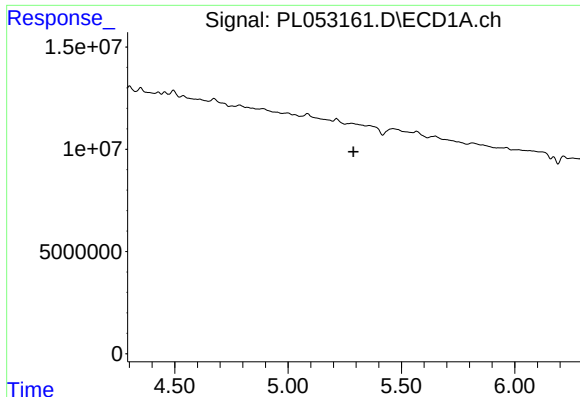

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

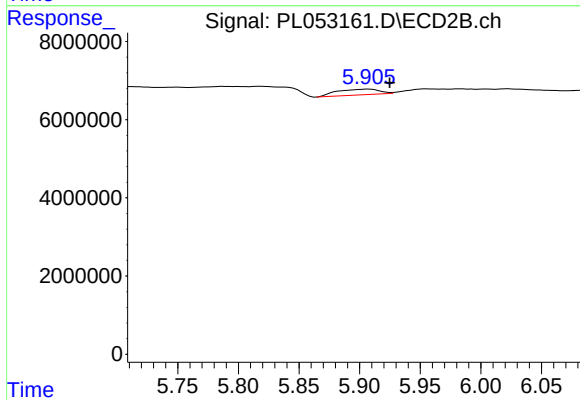


#8 Heptachlor epoxide

R.T.: 5.907 min
Delta R.T.: -0.018 min
Response: 3512606
Conc: 1.05 ng/ml

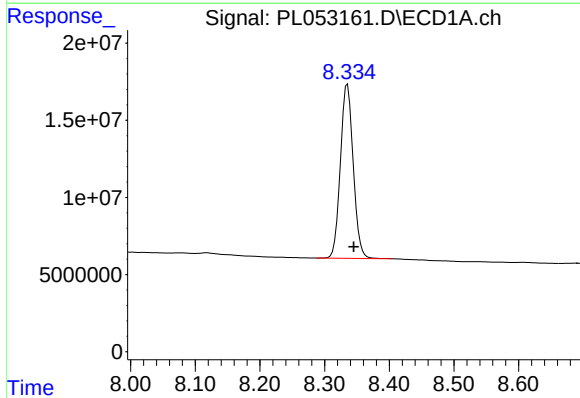

#28 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.010 min
Response: 155360363
Conc: 15.51 ng/ml

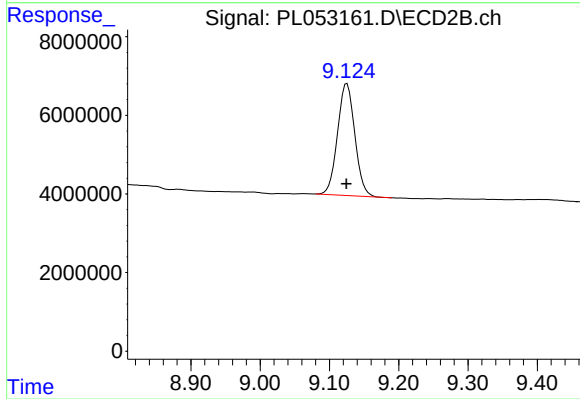

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.001 min
Response: 49285139
Conc: 16.80 ng/ml