

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100819\
 Data File : PL053162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2019 19:04
 Operator : SG\AJ
 Sample : K5238-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 00:43:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.048	180.5E6	44090728	18.146	16.420
28)	SA Decachlor...	8.336	9.126	149.2E6	47355435	14.895	16.142
Target Compounds							
2)	A alpha-BHC	0.000	4.408f	0	1524915	N.D.	0.397 #
7)	B delta-BHC	0.000	5.085f	0	2835809	N.D.	0.783 #
8)	B Heptachlo...	0.000	5.930	0	12299869	N.D.	3.670 #
11)	B alpha-Chl...	0.000	6.235	0	429896	N.D.	0.128 #
15)	B Endosulfa...	0.000	6.935f	0	3072004	N.D.	1.035 #
17)	MA 4,4'-DDT	0.000	7.178	0	2916871	N.D.	1.121 #
18)	B Endrin al...	0.000	7.100	0	341688	N.D.	0.139 #
26)	Chlordane-4	0.000	6.235	0	429896	N.D.	0.810 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100819\
Data File : PL053162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 19:04
Operator : SG\AJ
Sample : K5238-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 00:43:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

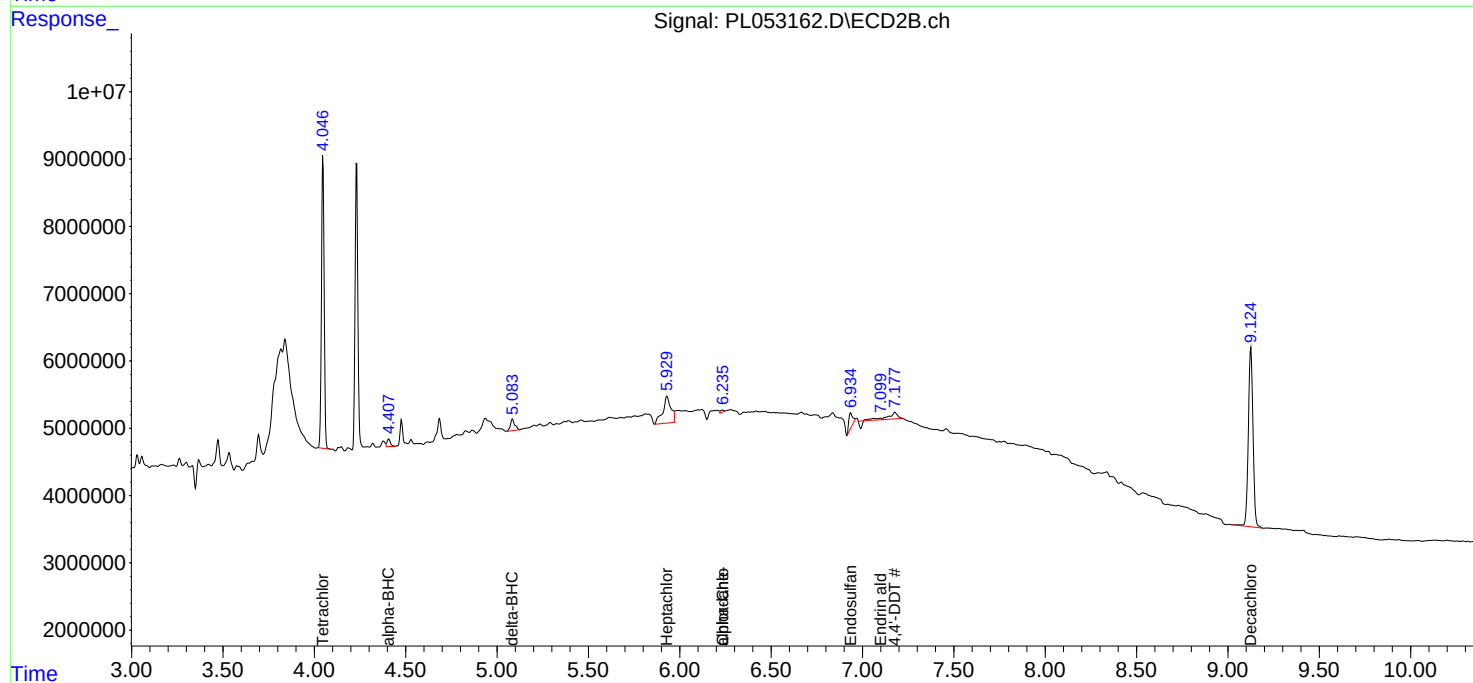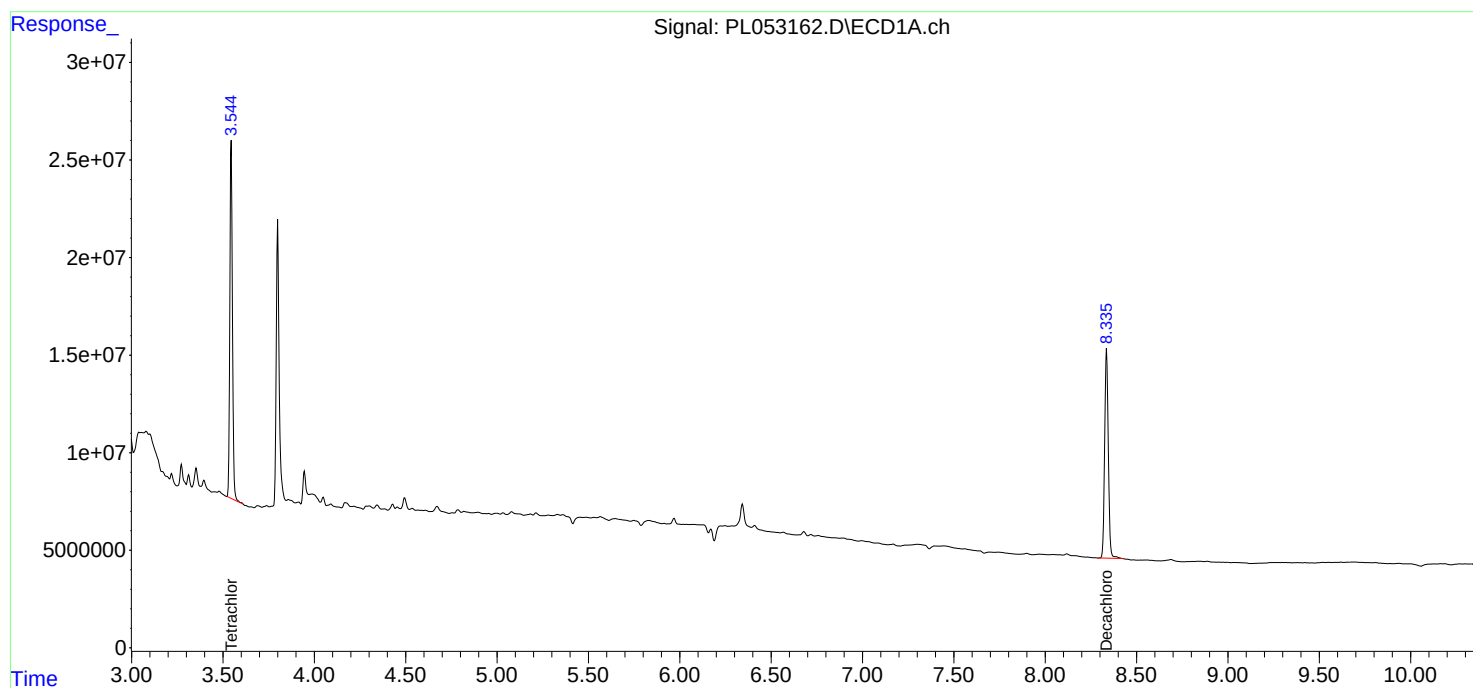


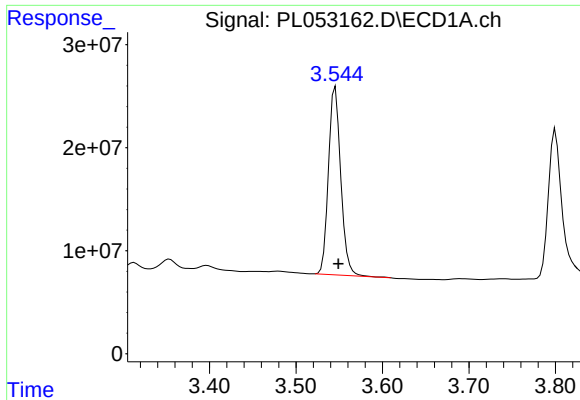

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 180490394
Conc: 18.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

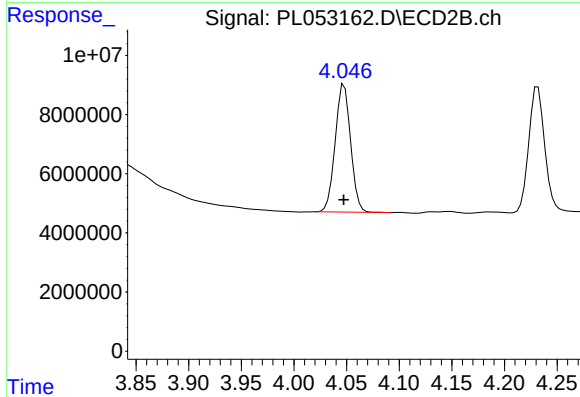


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 44090728
Conc: 16.42 ng/ml

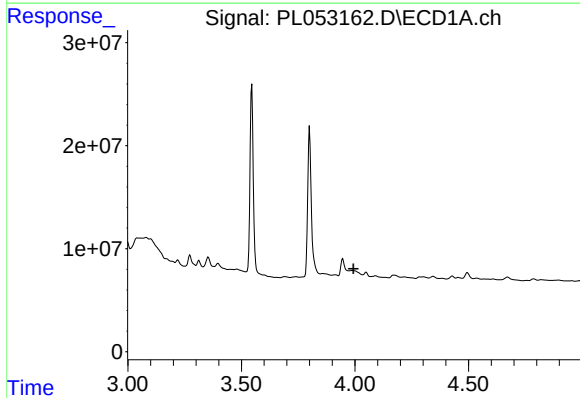


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.994 min
Response: 0
Conc: N.D.

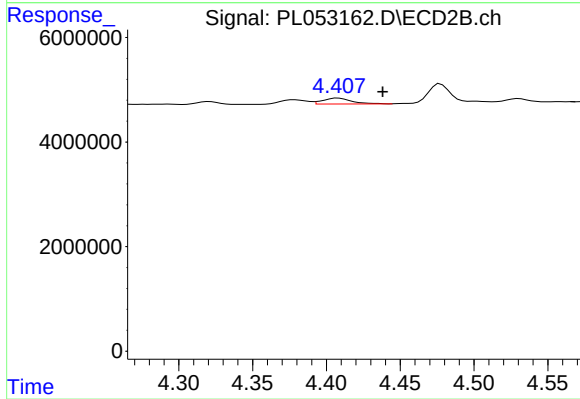

#2 alpha-BHC


R.T.: 4.408 min
Delta R.T.: -0.030 min
Response: 1524915
Conc: 0.40 ng/ml

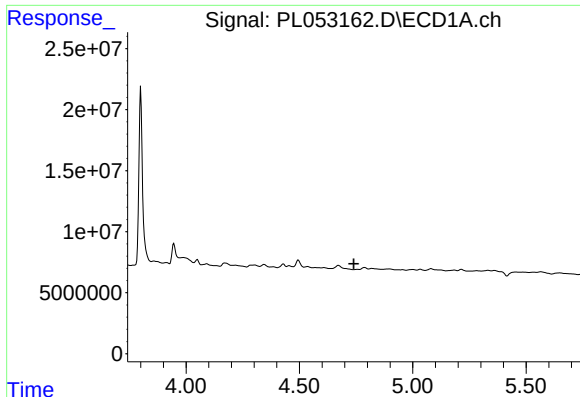

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

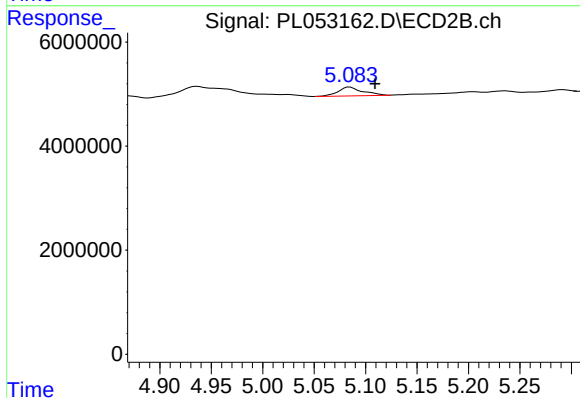


#7 delta-BHC

R.T.: 5.085 min
Delta R.T.: -0.025 min
Response: 2835809
Conc: 0.78 ng/ml

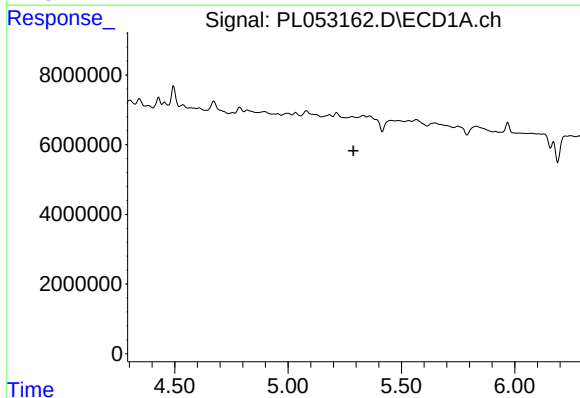


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

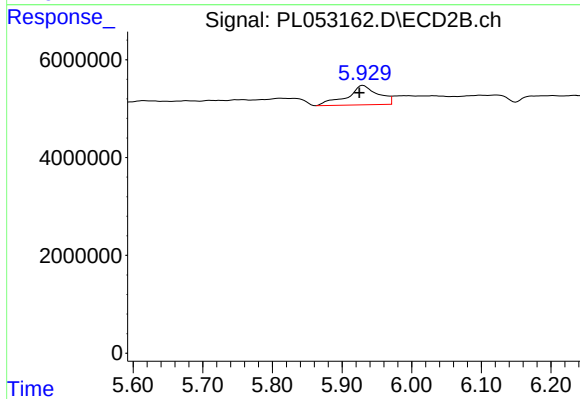

#8 Heptachlor epoxide


R.T.: 5.930 min
Delta R.T.: 0.005 min
Response: 12299869
Conc: 3.67 ng/ml

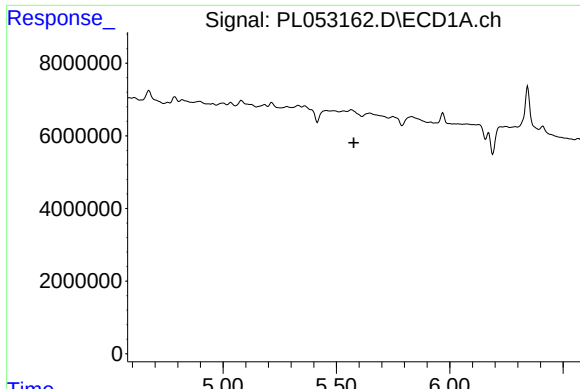

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

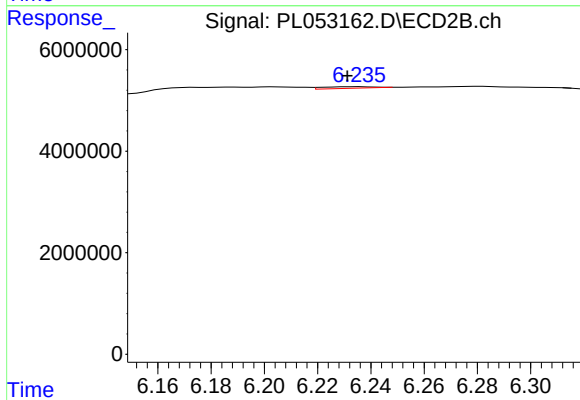


#11 alpha-Chlordane

R.T.: 6.235 min
Delta R.T.: 0.004 min
Response: 429896
Conc: 0.13 ng/ml

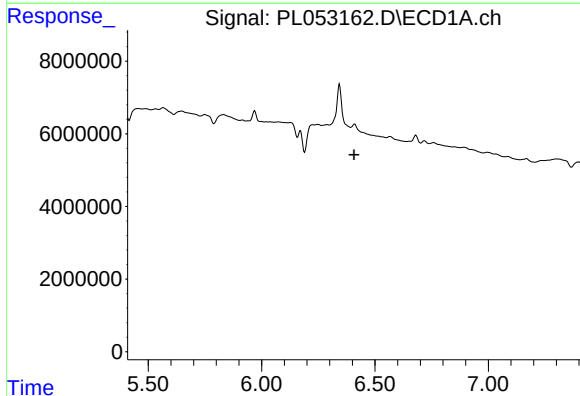


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

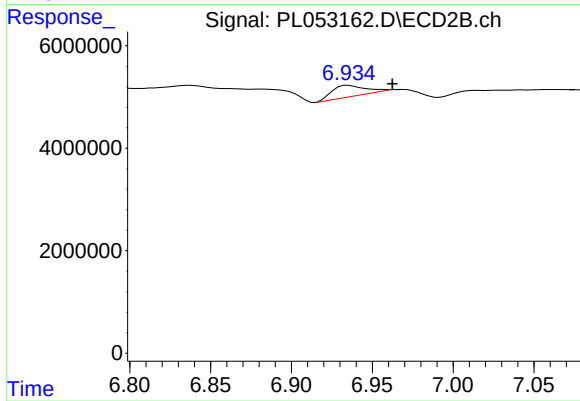

#15 Endosulfan II


R.T.: 6.935 min
Delta R.T.: -0.027 min
Response: 3072004
Conc: 1.04 ng/ml

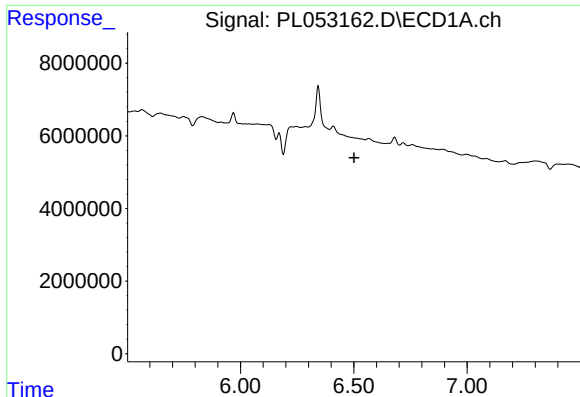

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

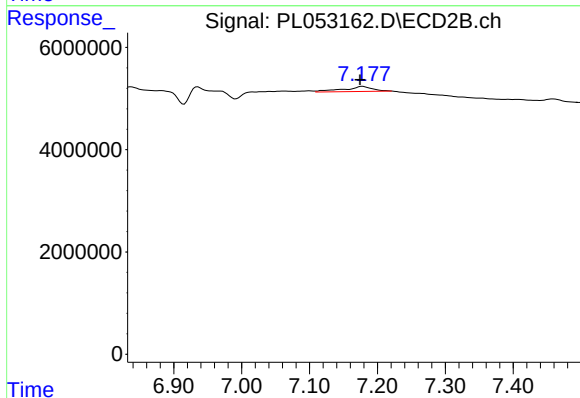


#17 4,4'-DDT

R.T.: 7.178 min
Delta R.T.: 0.004 min
Response: 2916871
Conc: 1.12 ng/ml

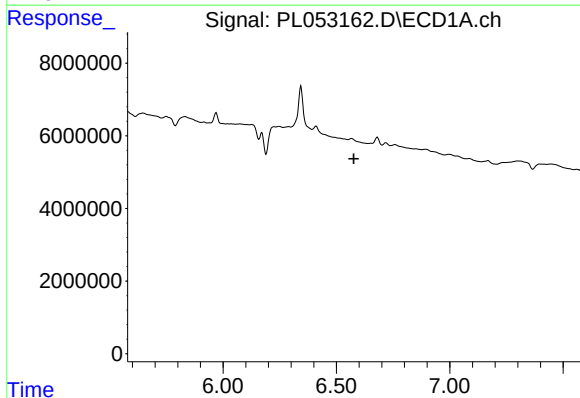


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.577 min
Response: 0
Conc: N.D.

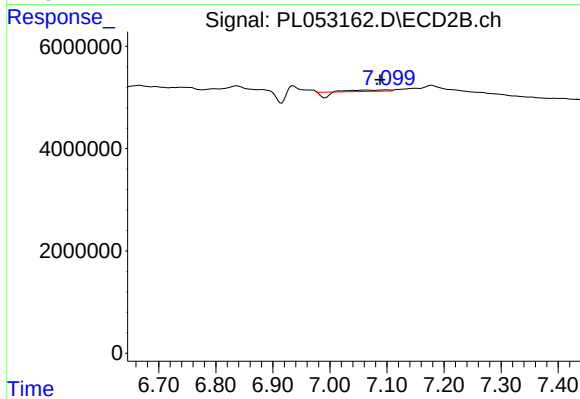

#18 Endrin aldehyde


R.T.: 7.100 min
Delta R.T.: 0.012 min
Response: 341688
Conc: 0.14 ng/ml

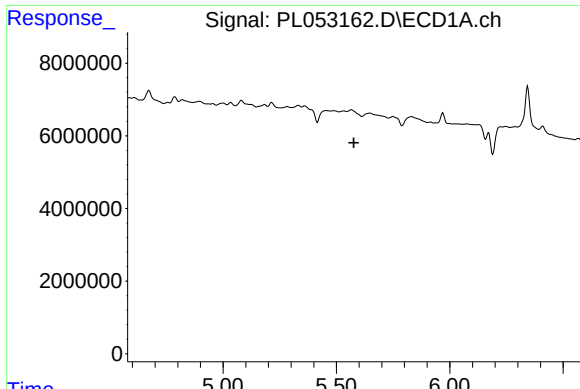

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

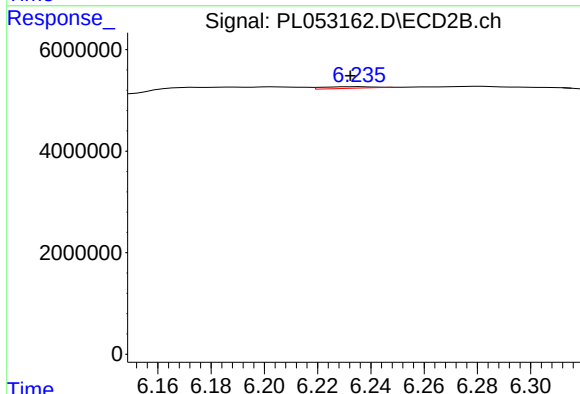


#26 Chlordane-4

R.T.: 6.235 min
Delta R.T.: 0.003 min
Response: 429896
Conc: 0.81 ng/ml

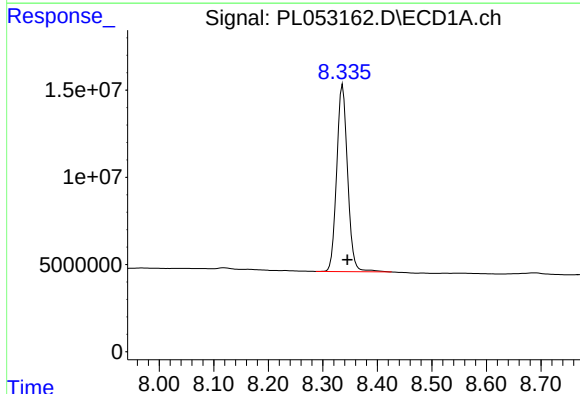

#28 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.009 min
Response: 149193132
Conc: 14.90 ng/ml

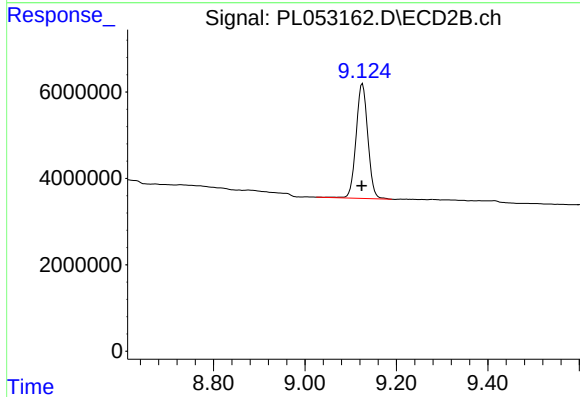

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 47355435
Conc: 16.14 ng/ml