

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100820\
 Data File : PL062116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 13:28
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 04:49:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100820CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 09 04:48:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	3.961	33161484	52934124	20.000	20.000
27)	SA Decachlor...	8.143	9.007	65819949	92966552	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.852	4.348	44068720	72729946	20.000	20.000
3)	MA gamma-BHC...	4.132	4.631	39786179	69929835	20.000	20.000
4)	MA Heptachlor	4.430	5.138	34656666	57881784	20.000	20.000
9)	A Endosulfan I	5.451	6.183	31238038	53548243	20.000	20.000
13)	MA Dieldrin	5.693	6.439	67264949	111.1E6	40.000	40.000
14)	MA Endrin	5.947	6.657	59440484	91743990	40.000	40.000
16)	A 4,4'-DDD	6.076	6.781	48126777	74745954	40.000	40.000
17)	MA 4,4'-DDT	6.316	7.080	46586589	86120612	40.000	40.000
20)	A Methoxychlor	6.860	7.539	149.2E6	222.3E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100820\
Data File : PL062116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 13:28
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 04:49:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100820CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 09 04:48:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

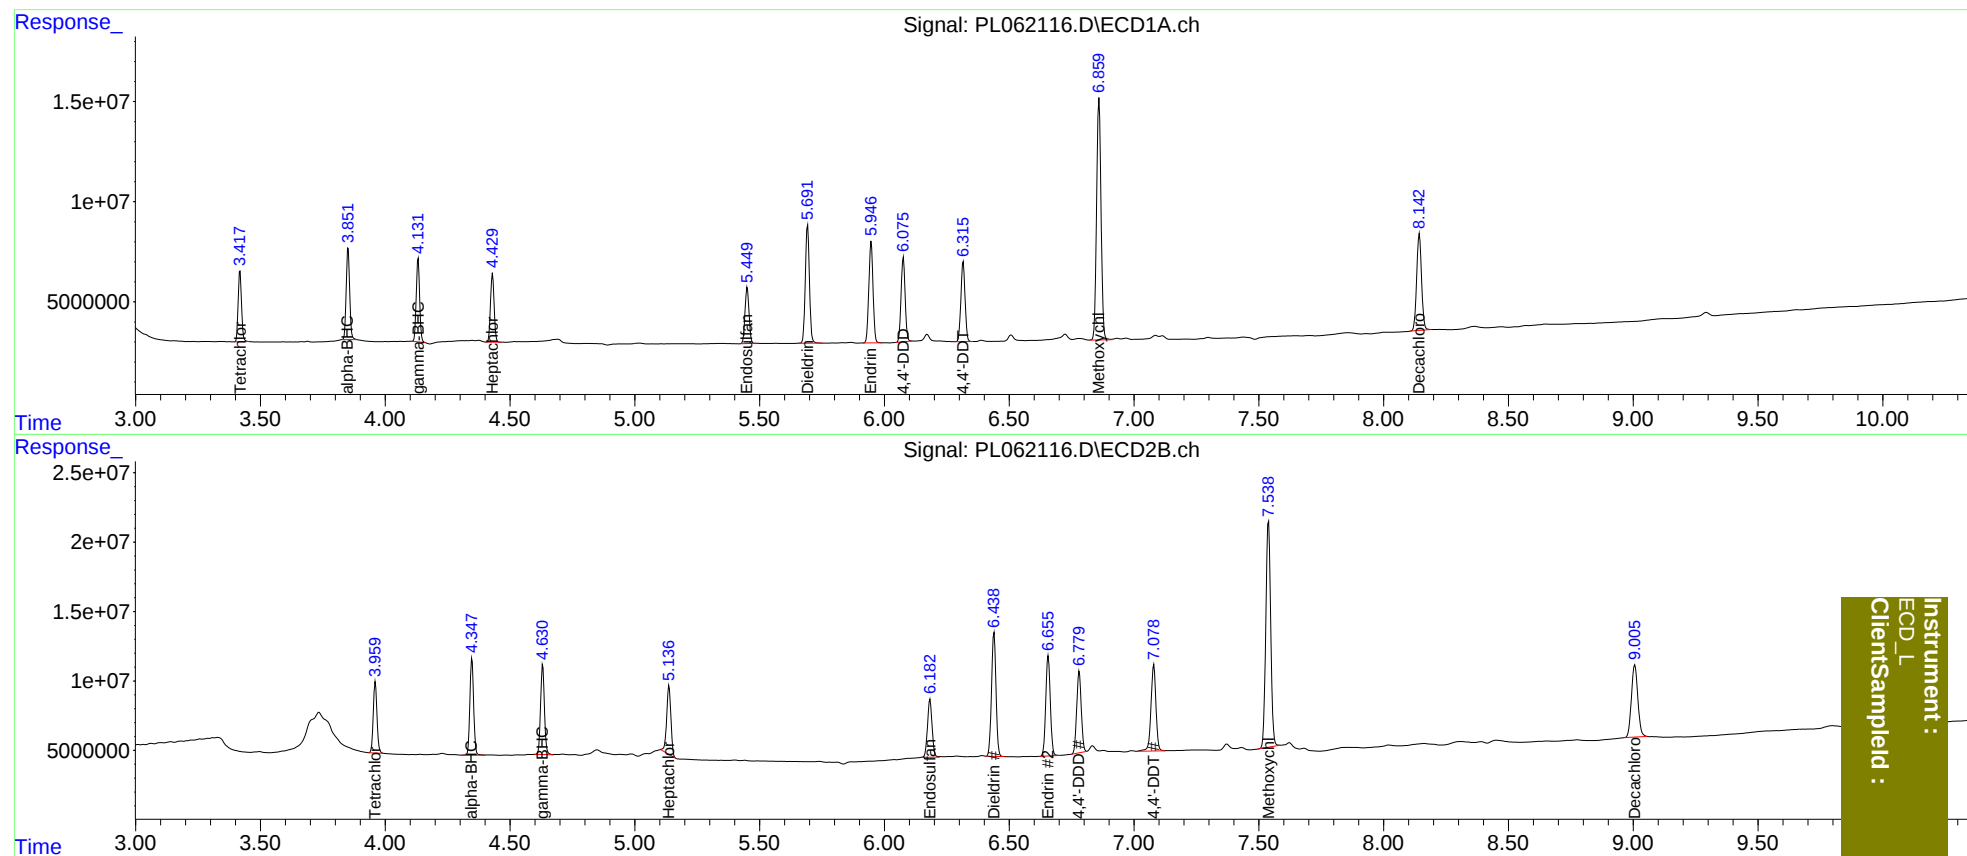


Instrument :
ECD_L
ClientSampled :

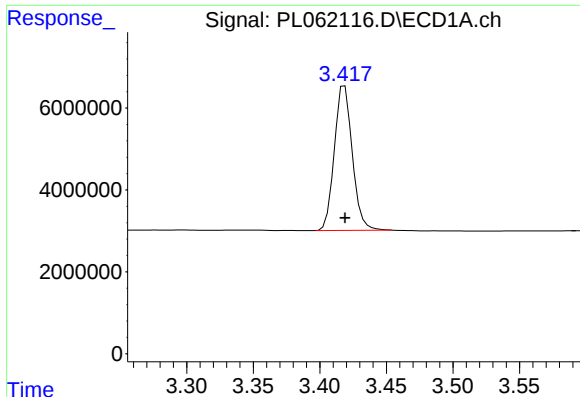

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 33161484
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

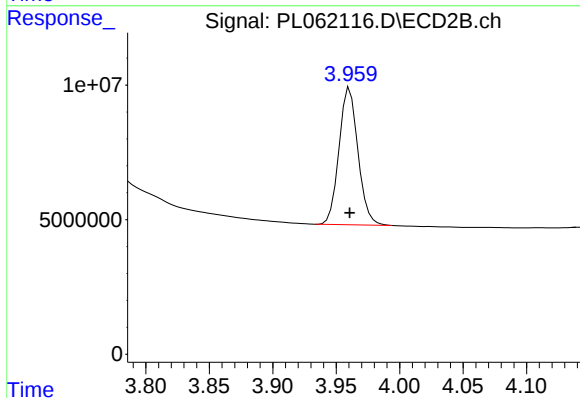


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 52934124
Conc: 20.00 ng/ml

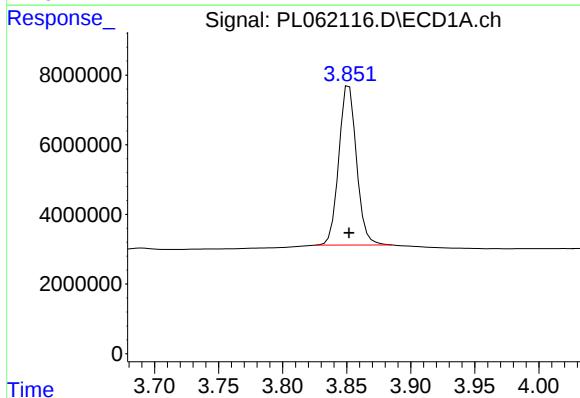


#2 alpha-BHC

R.T.: 3.852 min
Delta R.T.: 0.000 min
Response: 44068720
Conc: 20.00 ng/ml

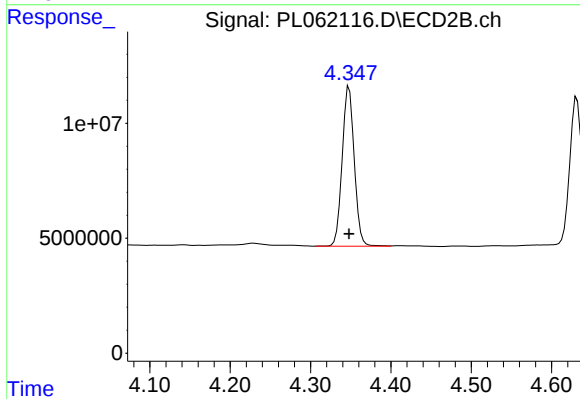

#2 alpha-BHC


R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 72729946
Conc: 20.00 ng/ml

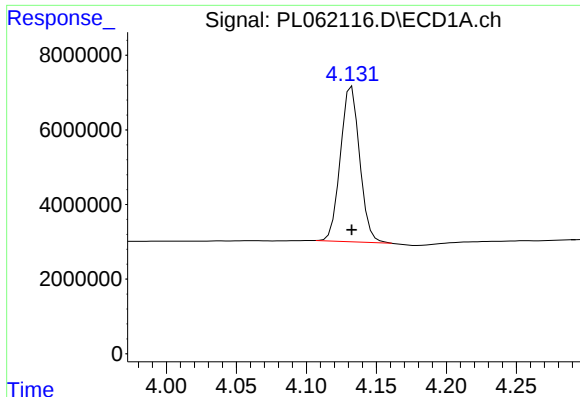

#3 gamma-BHC (Lindane)


R.T.: 4.132 min
Delta R.T.: 0.000 min
Response: 39786179
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

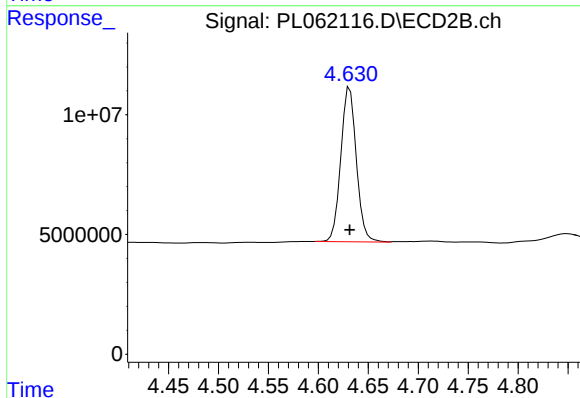


#3 gamma-BHC (Lindane)

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 69929835
Conc: 20.00 ng/ml

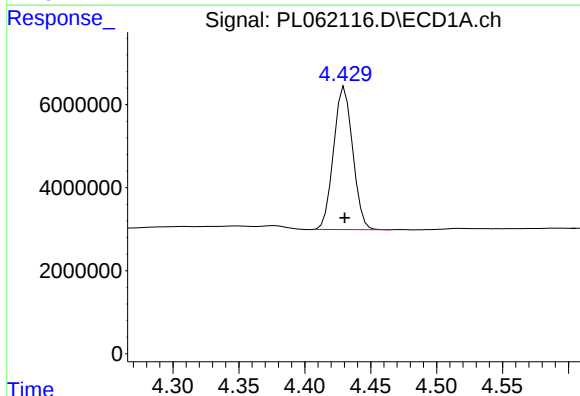


#4 Heptachlor

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 34656666
Conc: 20.00 ng/ml

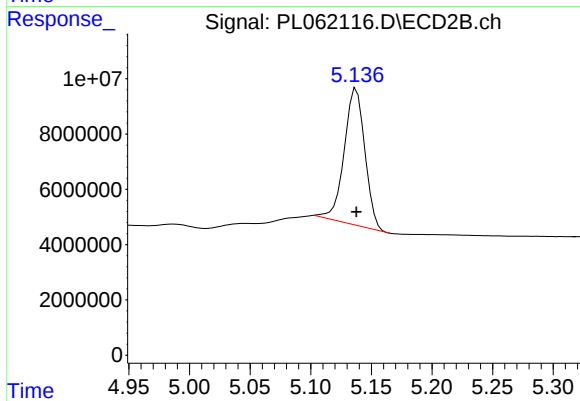

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.000 min
Response: 57881784
Conc: 20.00 ng/ml

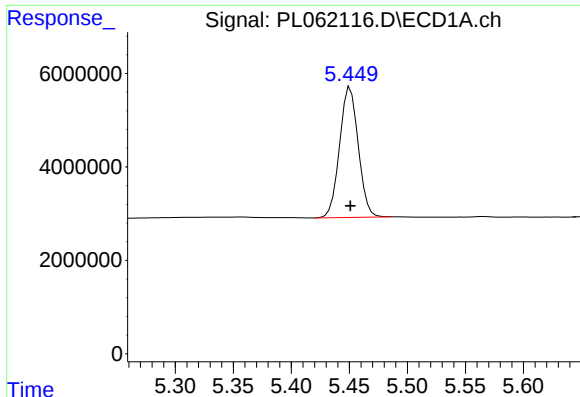

#9 Endosulfan I


R.T.: 5.451 min
Delta R.T.: 0.000 min
Response: 31238038
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

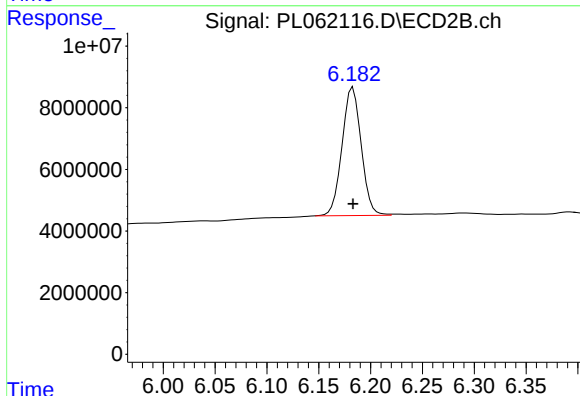


#9 Endosulfan I

R.T.: 6.183 min
Delta R.T.: 0.000 min
Response: 53548243
Conc: 20.00 ng/ml

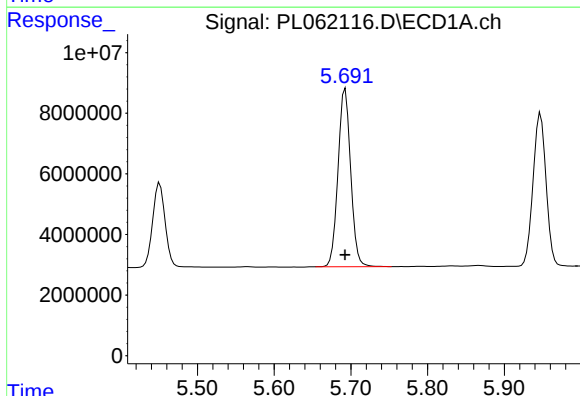


#13 Dieldrin

R.T.: 5.693 min
Delta R.T.: 0.000 min
Response: 67264949
Conc: 40.00 ng/ml

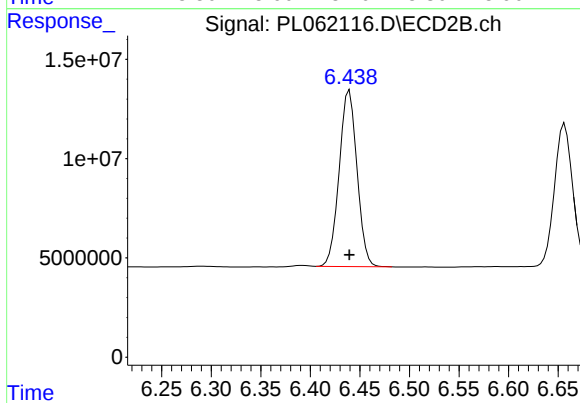

#13 Dieldrin


R.T.: 6.439 min
Delta R.T.: 0.000 min
Response: 111057358
Conc: 40.00 ng/ml

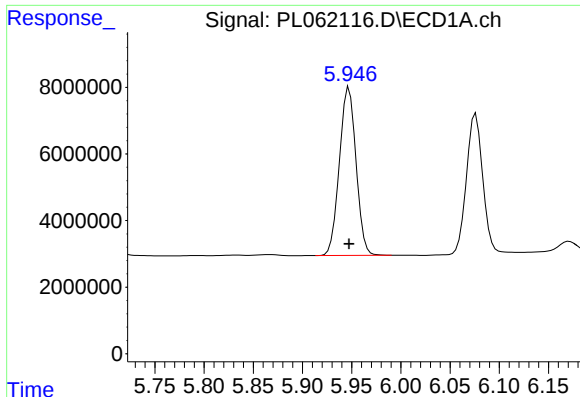

#14 Endrin


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 59440484
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

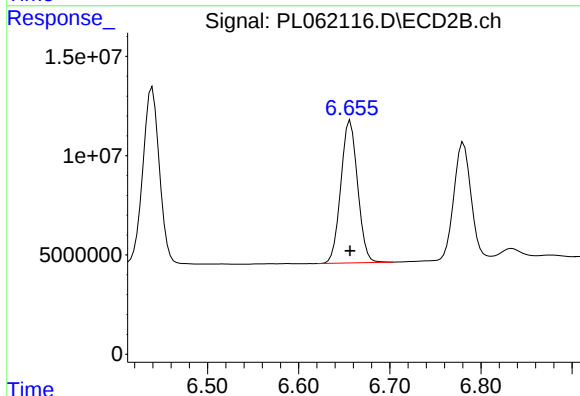


#14 Endrin

R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 91743990
Conc: 40.00 ng/ml

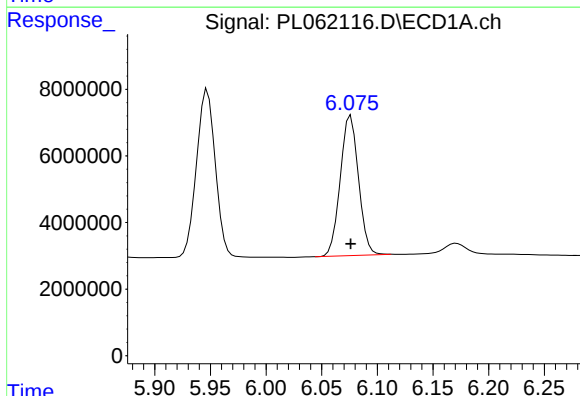


#16 4,4'-DDD

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 48126777
Conc: 40.00 ng/ml

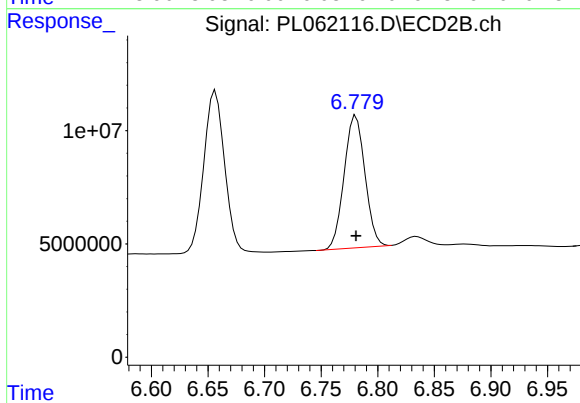

#16 4,4'-DDD


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 74745954
Conc: 40.00 ng/ml

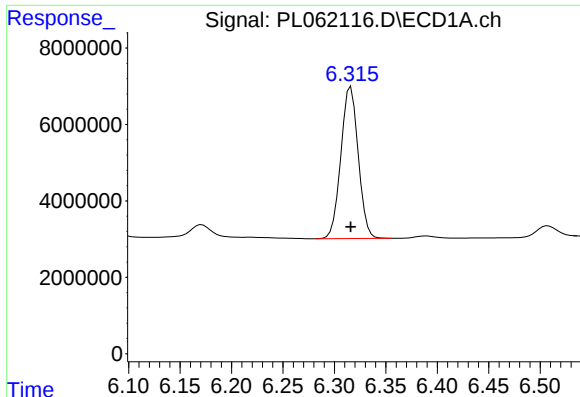

#17 4,4'-DDT


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 46586589
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

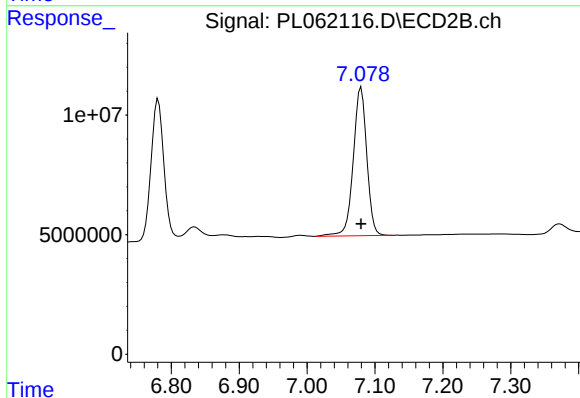


#17 4,4'-DDT

R.T.: 7.080 min
Delta R.T.: 0.000 min
Response: 86120612
Conc: 40.00 ng/ml

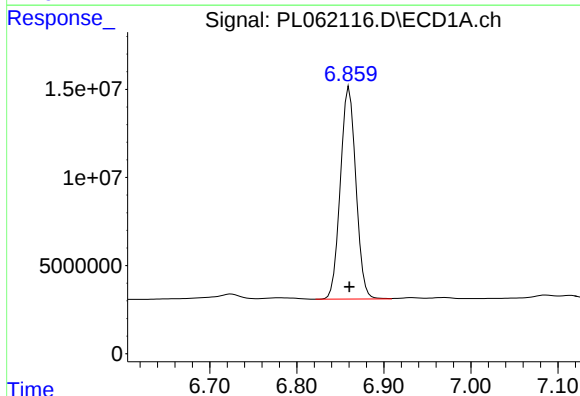


#20 Methoxychlor

R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 149237471
Conc: 200.00 ng/ml

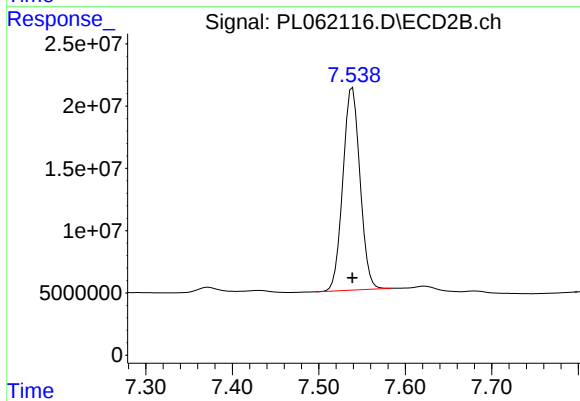

#20 Methoxychlor

R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 222334376
Conc: 200.00 ng/ml

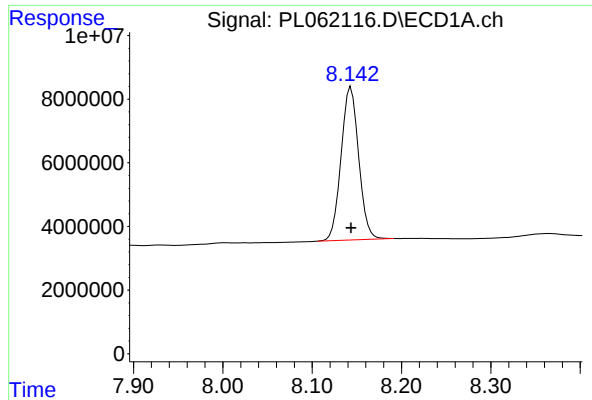

#27 Decachlorobiphenyl


R.T.: 8.143 min

Delta R.T.: 0.000 min

Response: 65819949

Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

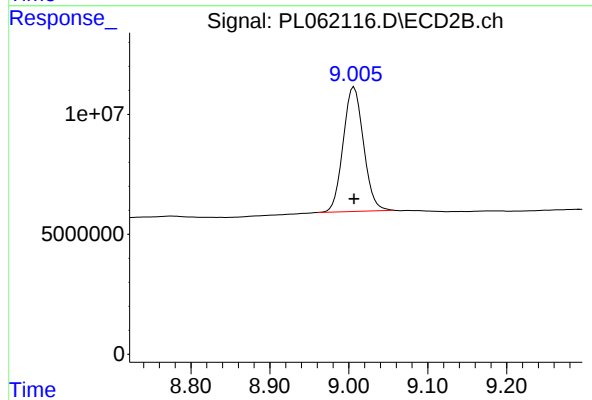

#27 Decachlorobiphenyl

R.T.: 9.007 min

Delta R.T.: 0.000 min

Response: 92966552

Conc: 40.00 ng/ml