

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100820\
 Data File : PL062118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 13:56
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 04:49:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100820CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 09 04:48:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	3.960	64960590	101.7E6	39.178	38.418
27)	SA Decachlor...	8.143	9.006	129.1E6	182.8E6	78.484	78.659
Target Compounds							
2)	A alpha-BHC	3.852	4.348	89596708	143.9E6	40.662	39.559
3)	MA gamma-BHC...	4.132	4.632	80584641	136.9E6	40.509	39.150
4)	MA Heptachlor	4.430	5.138	70985008	119.2E6	40.965	41.175
9)	A Endosulfan I	5.451	6.183	62291289	107.3E6	39.882	40.066
13)	MA Dieldrin	5.693	6.440	139.8E6	232.2E6	83.120	83.622
14)	MA Endrin	5.947	6.656	122.7E6	189.7E6	82.563	82.692
16)	A 4,4'-DDD	6.076	6.781	101.9E6	159.6E6	84.656	85.434
17)	MA 4,4'-DDT	6.316	7.079	103.0E6	175.0E6	88.417	81.286
20)	A Methoxychlor	6.860	7.539	303.4E6	455.9E6	406.594	410.115


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100820\
Data File : PL062118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 13:56
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 04:49:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100820CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 09 04:48:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

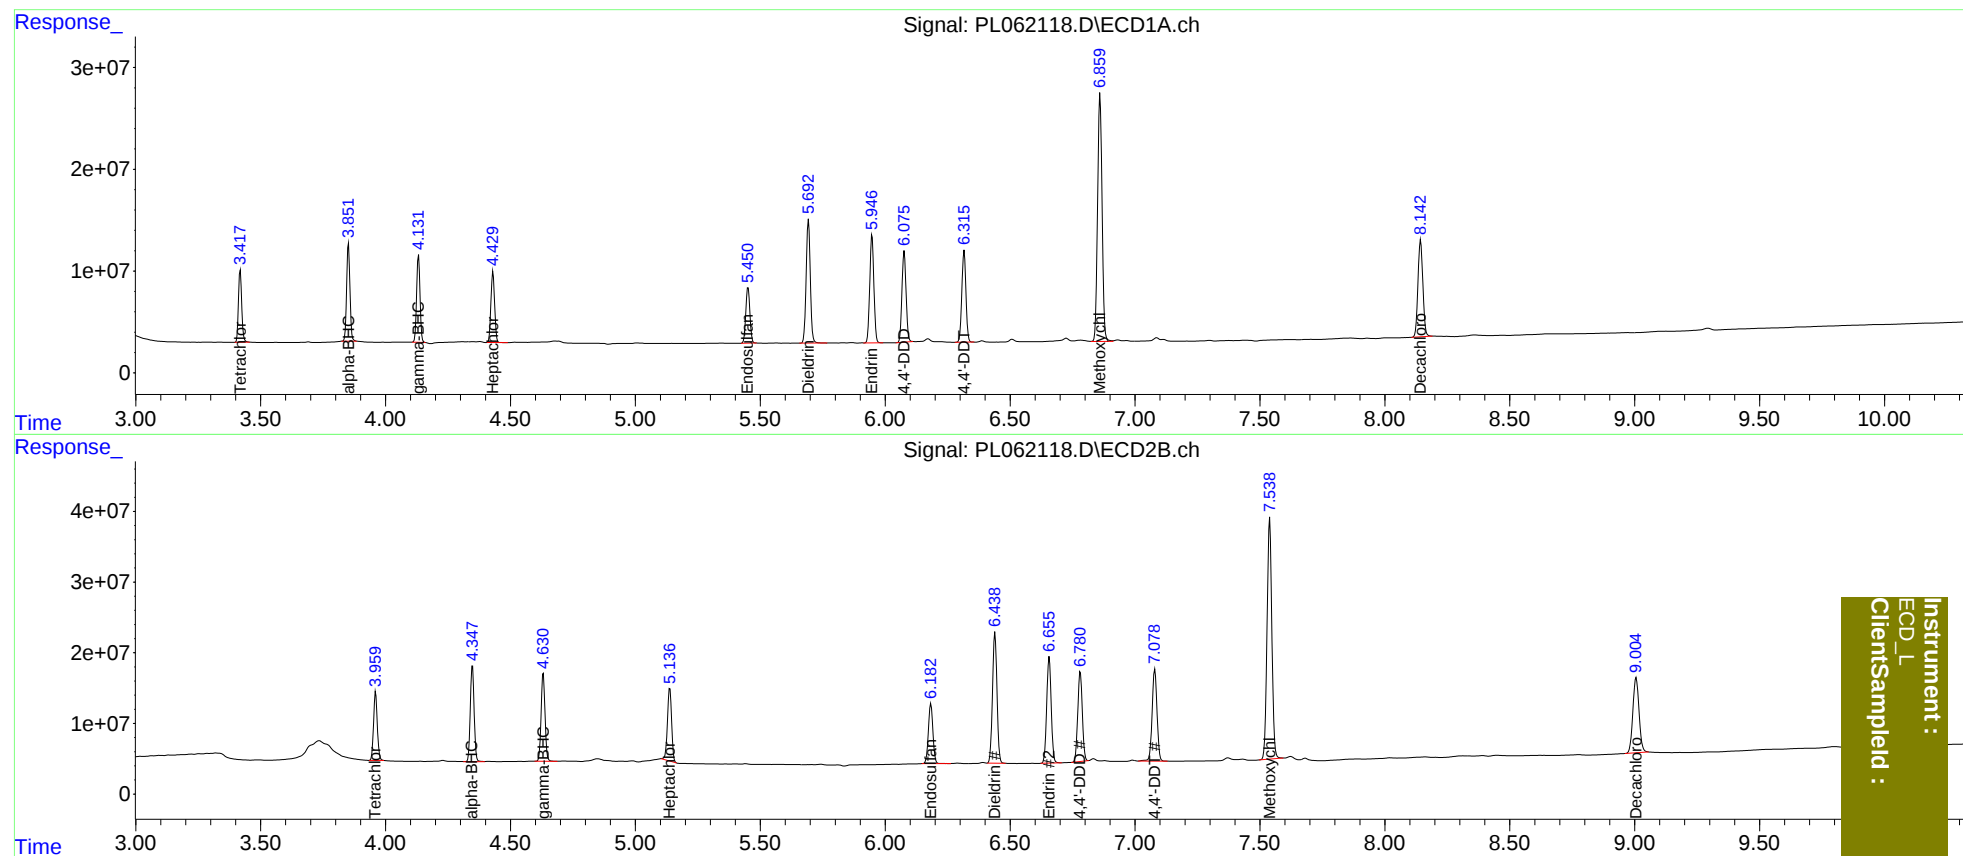


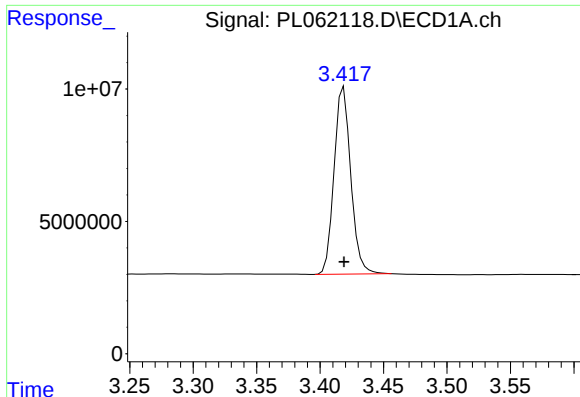

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 64960590
Conc: 39.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

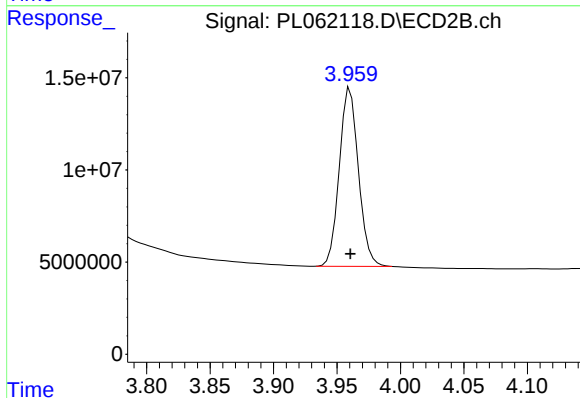


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 101681000
Conc: 38.42 ng/ml

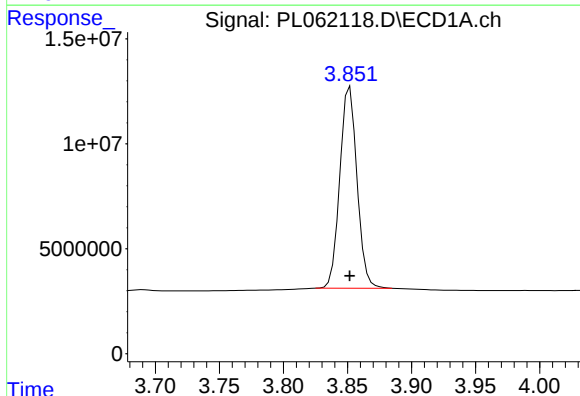


#2 alpha-BHC

R.T.: 3.852 min
Delta R.T.: 0.000 min
Response: 89596708
Conc: 40.66 ng/ml

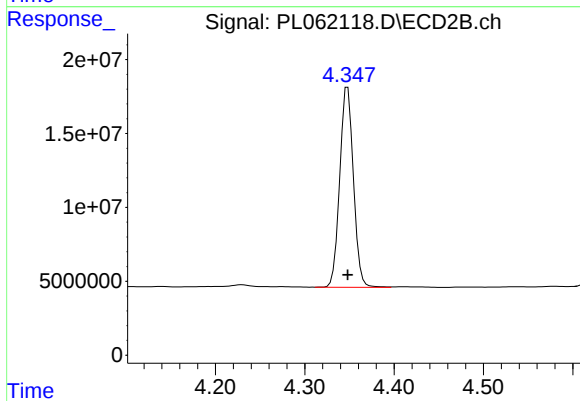

#2 alpha-BHC


R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 143855438
Conc: 39.56 ng/ml

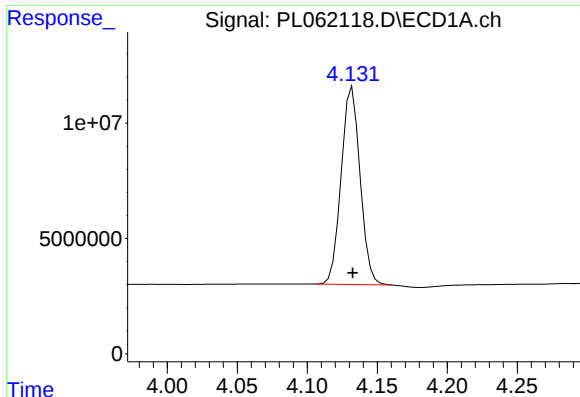

#3 gamma-BHC (Lindane)


R.T.: 4.132 min
Delta R.T.: 0.000 min
Response: 80584641
Conc: 40.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

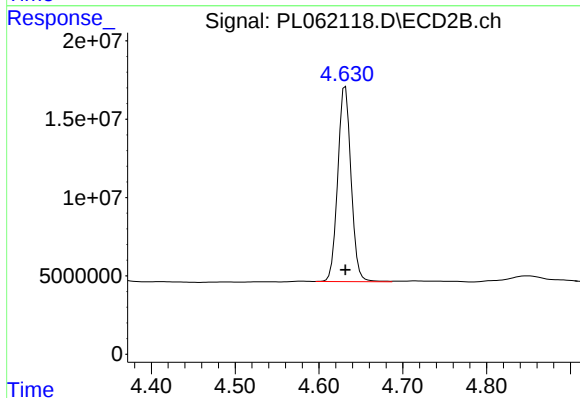


#3 gamma-BHC (Lindane)

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 136888785
Conc: 39.15 ng/ml

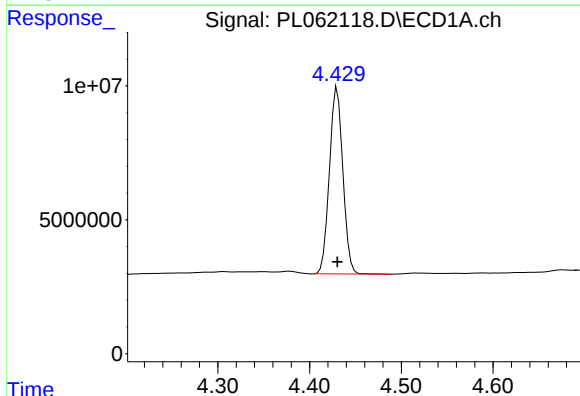


#4 Heptachlor

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 70985008
Conc: 40.96 ng/ml

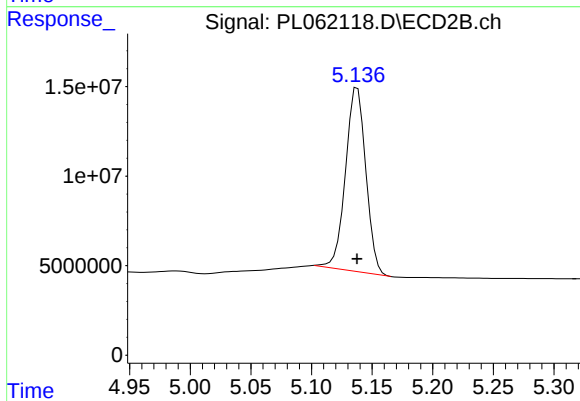

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.000 min
Response: 119164120
Conc: 41.17 ng/ml

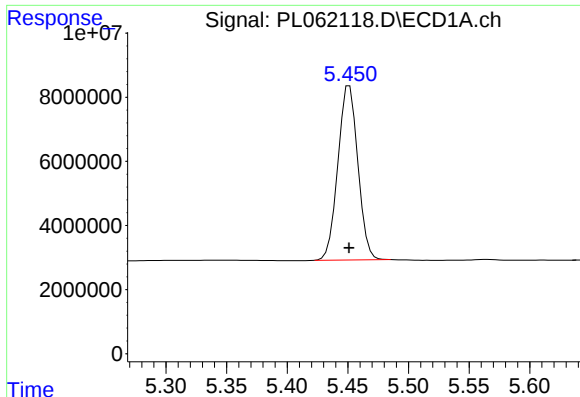

#9 Endosulfan I


R.T.: 5.451 min
Delta R.T.: 0.000 min
Response: 62291289
Conc: 39.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

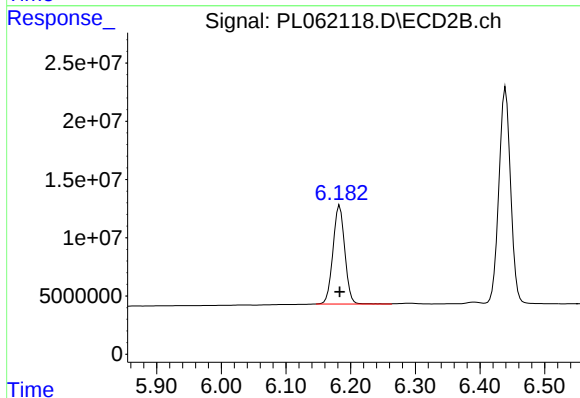


#9 Endosulfan I

R.T.: 6.183 min
Delta R.T.: 0.000 min
Response: 107273412
Conc: 40.07 ng/ml

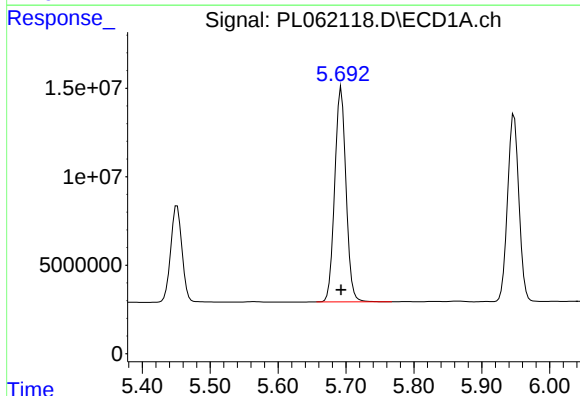


#13 Dieldrin

R.T.: 5.693 min
Delta R.T.: 0.000 min
Response: 139777245
Conc: 83.12 ng/ml

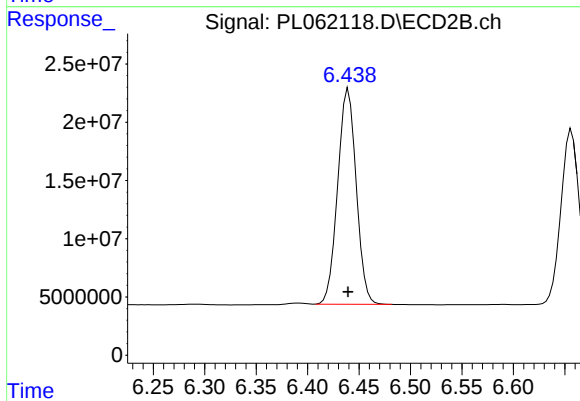

#13 Dieldrin


R.T.: 6.440 min
Delta R.T.: 0.000 min
Response: 232169832
Conc: 83.62 ng/ml

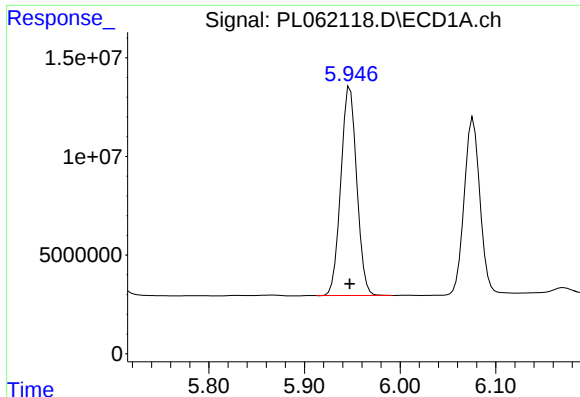

#14 Endrin


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 122689046
Conc: 82.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

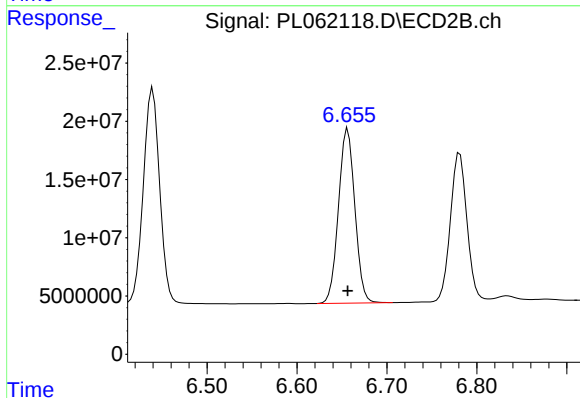


#14 Endrin

R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 189662342
Conc: 82.69 ng/ml

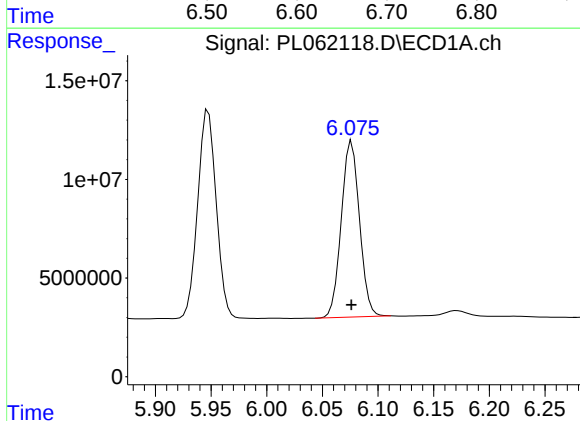


#16 4,4'-DDD

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 101855882
Conc: 84.66 ng/ml

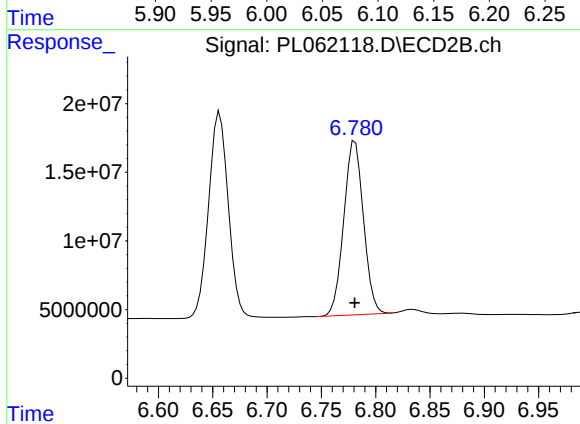

#16 4,4'-DDD


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 159646165
Conc: 85.43 ng/ml

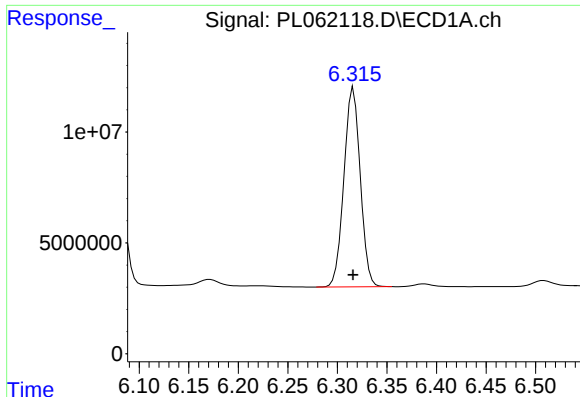

#17 4,4'-DDT


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 102976381
Conc: 88.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

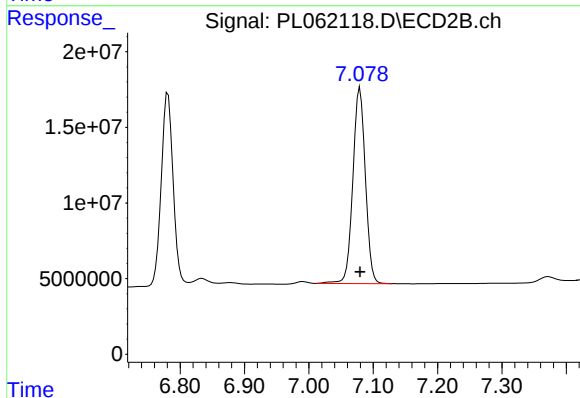


#17 4,4'-DDT

R.T.: 7.079 min
Delta R.T.: 0.000 min
Response: 175009803
Conc: 81.29 ng/ml

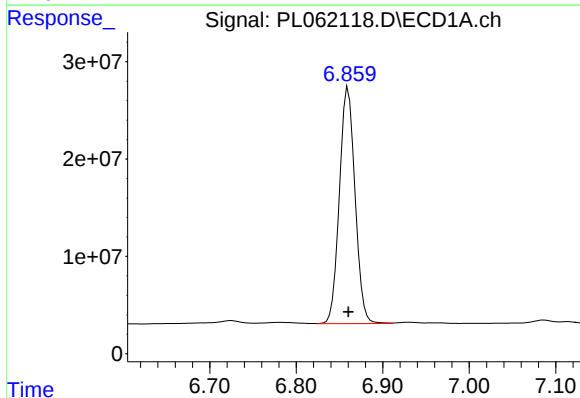


#20 Methoxychlor

R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 303395177
Conc: 406.59 ng/ml

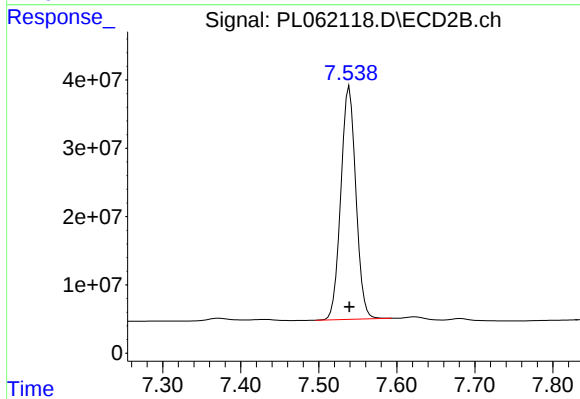

#20 Methoxychlor


R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 455913816
Conc: 410.12 ng/ml

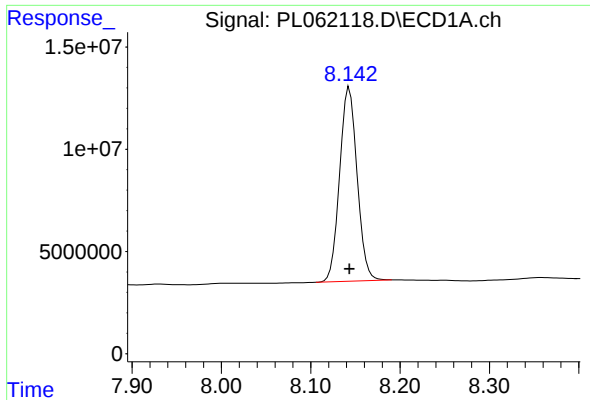

#27 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 129144611
Conc: 78.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

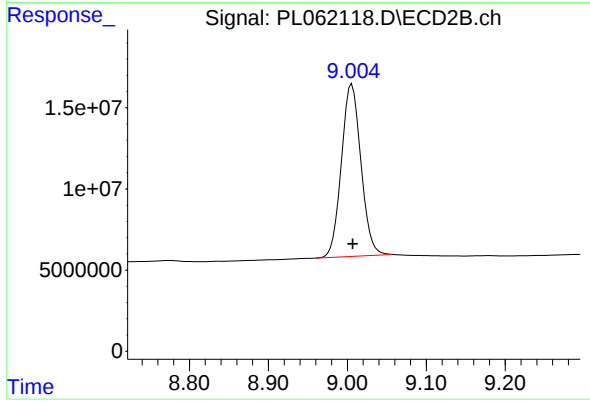

#27 Decachlorobiphenyl

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 182815521
Conc: 78.66 ng/ml