

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100820\
 Data File : PL062120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 14:24
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 04:50:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100820CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 09 04:48:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	3.961	126.5E6	203.5E6	76.266	76.878
27)	SA Decachlor...	8.143	9.005	243.4E6	344.7E6	147.922	148.323
Target Compounds							
2)	A alpha-BHC	3.852	4.348	183.0E6	304.8E6	83.070	83.811
3)	MA gamma-BHC...	4.132	4.631	163.4E6	280.8E6	82.138	80.308
4)	MA Heptachlor	4.431	5.138	140.7E6	242.7E6	81.195	83.845
9)	A Endosulfan I	5.451	6.182	121.8E6	211.7E6	77.956	79.065
13)	MA Dieldrin	5.693	6.439	281.1E6	469.6E6	167.154	169.123
14)	MA Endrin	5.947	6.656	245.3E6	382.9E6	165.098	166.935
16)	A 4,4'-DDD	6.076	6.781	204.7E6	323.9E6	170.130	173.337
17)	MA 4,4'-DDT	6.316	7.079	212.5E6	344.5E6	182.480	160.001
20)	A Methoxychlor	6.860	7.538	571.0E6	879.6E6	765.252	791.281

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100820\
Data File : PL062120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 14:24
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 04:50:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100820CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 09 04:48:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

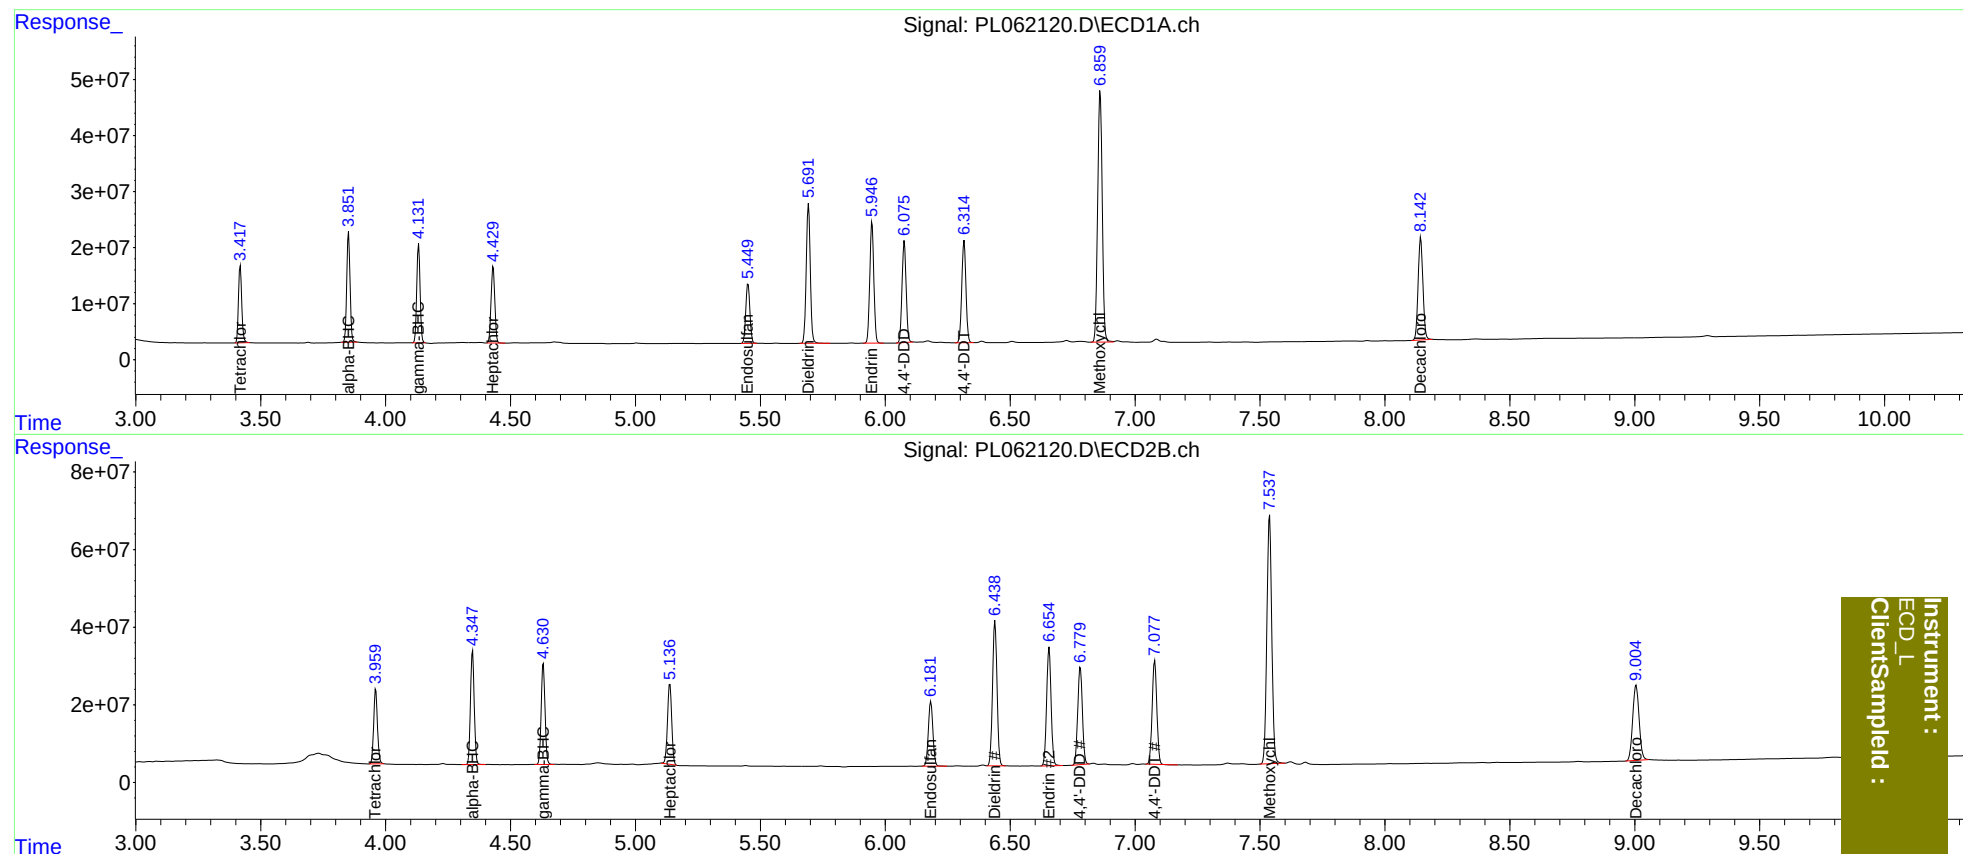


Instrument :
ECD_L
ClientSampled :

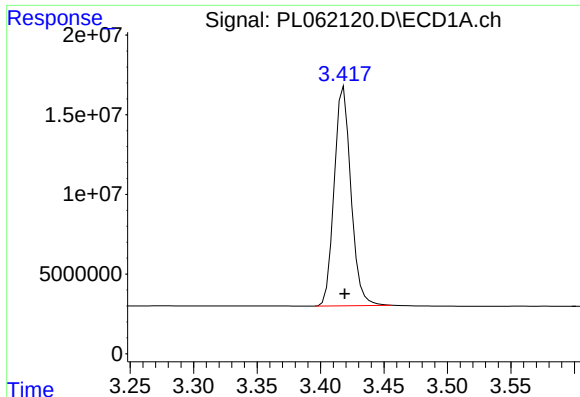

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.000 min
Response: 126455456
Conc: 76.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

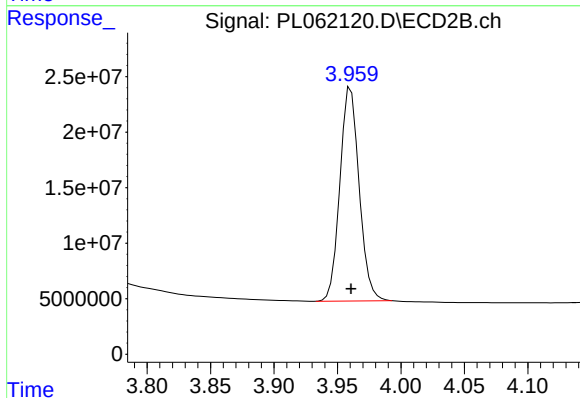


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 203474755
Conc: 76.88 ng/ml

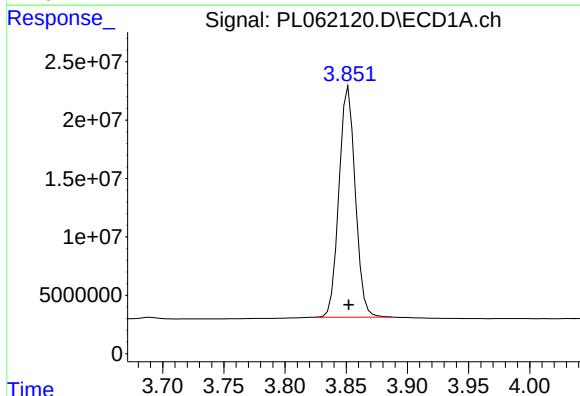


#2 alpha-BHC

R.T.: 3.852 min
Delta R.T.: 0.000 min
Response: 183039792
Conc: 83.07 ng/ml

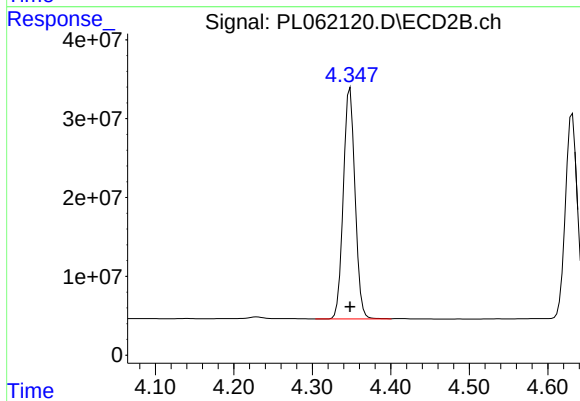

#2 alpha-BHC


R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 304776659
Conc: 83.81 ng/ml

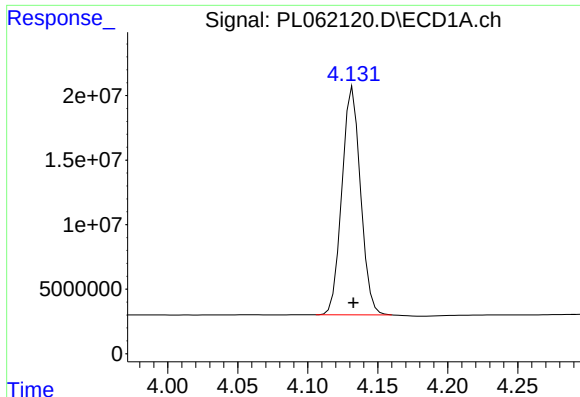

#3 gamma-BHC (Lindane)


R.T.: 4.132 min
Delta R.T.: 0.000 min
Response: 163397771
Conc: 82.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

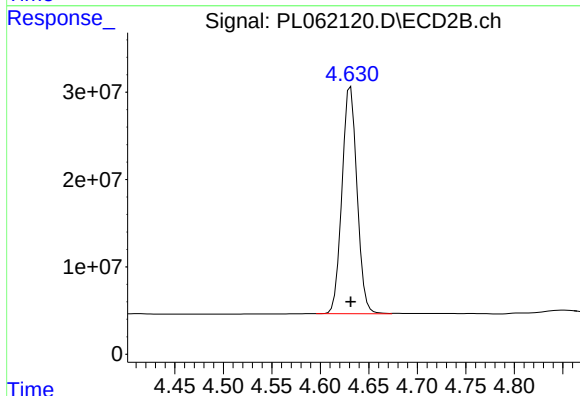


#3 gamma-BHC (Lindane)

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 280795681
Conc: 80.31 ng/ml

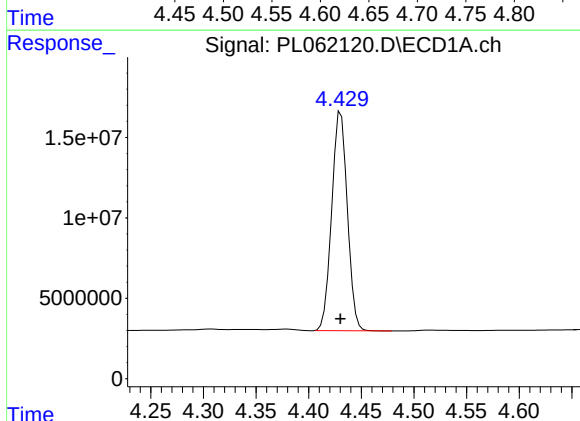


#4 Heptachlor

R.T.: 4.431 min
Delta R.T.: 0.000 min
Response: 140698122
Conc: 81.20 ng/ml

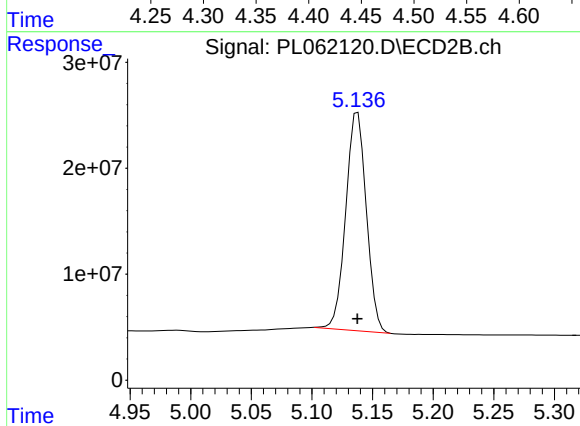

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.000 min
Response: 242653735
Conc: 83.84 ng/ml

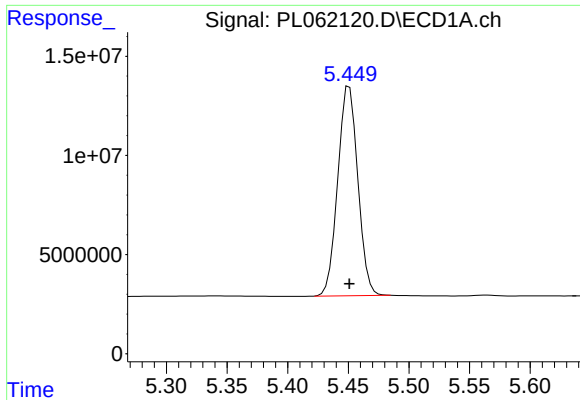

#9 Endosulfan I


R.T.: 5.451 min
Delta R.T.: 0.000 min
Response: 121759949
Conc: 77.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

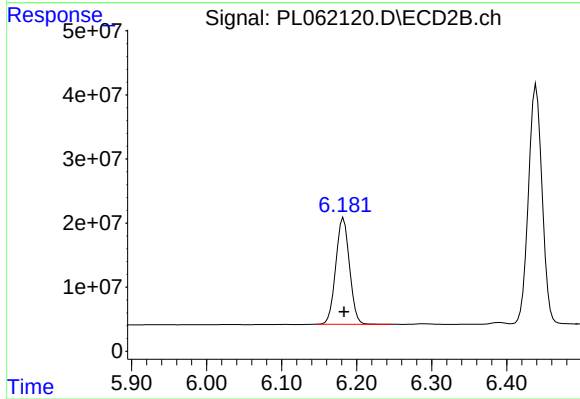


#9 Endosulfan I

R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 211690525
Conc: 79.07 ng/ml

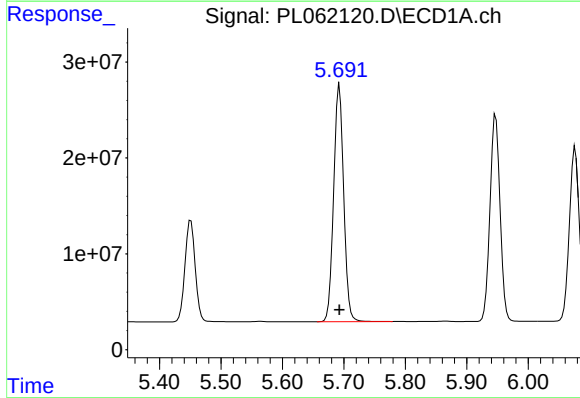


#13 Dieldrin

R.T.: 5.693 min
Delta R.T.: 0.000 min
Response: 281090709
Conc: 167.15 ng/ml

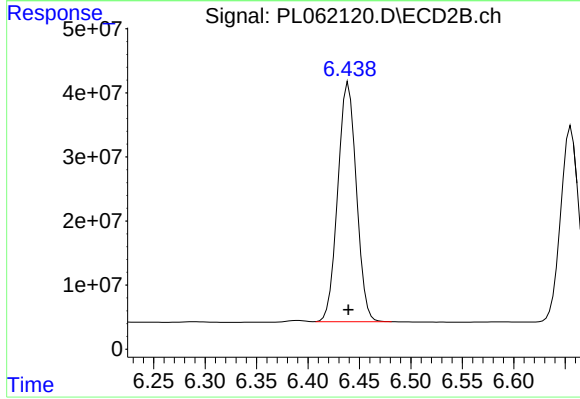

#13 Dieldrin


R.T.: 6.439 min
Delta R.T.: 0.000 min
Response: 469557850
Conc: 169.12 ng/ml

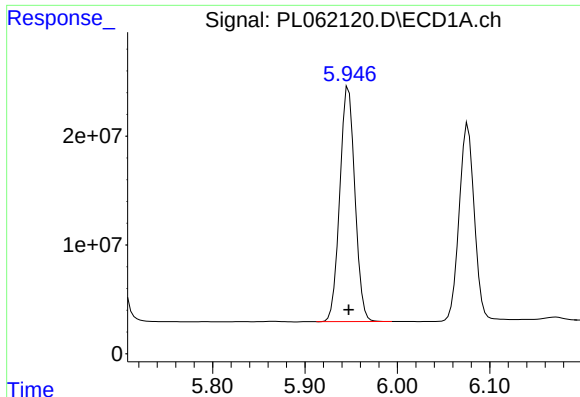

#14 Endrin


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 245337513
Conc: 165.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

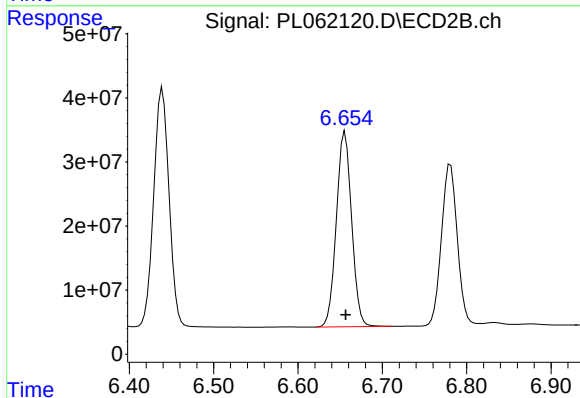


#14 Endrin

R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 382883052
Conc: 166.94 ng/ml

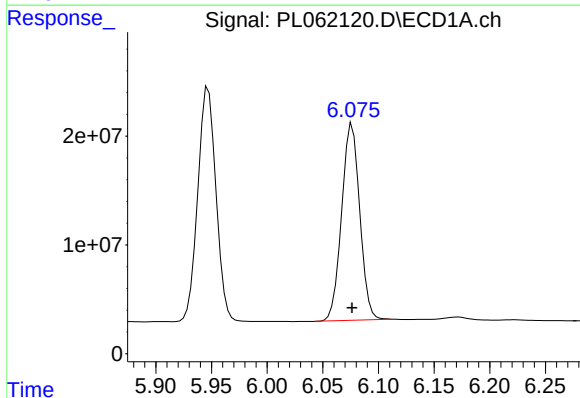


#16 4,4'-DDD

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 204695740
Conc: 170.13 ng/ml

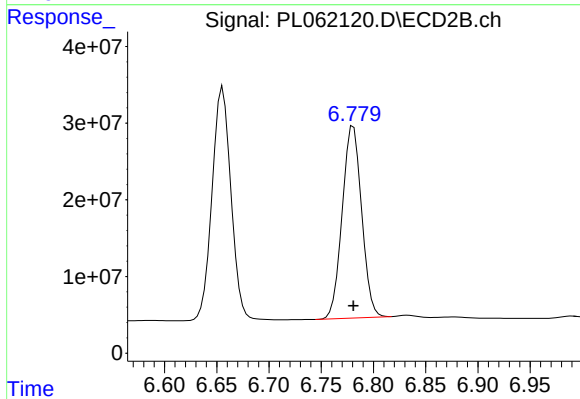

#16 4,4'-DDD


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 323906701
Conc: 173.34 ng/ml

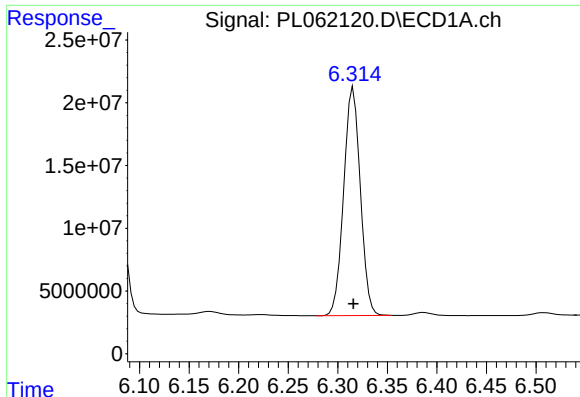

#17 4,4'-DDT


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 212527521
Conc: 182.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

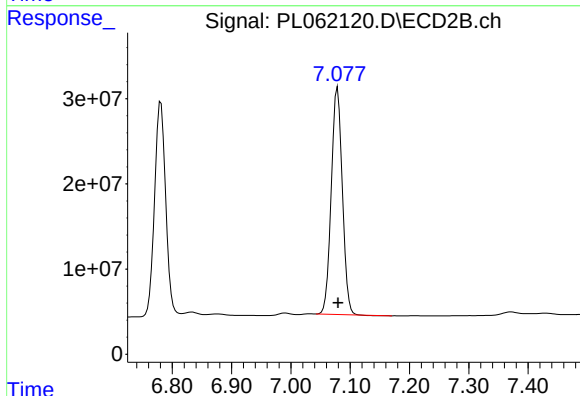


#17 4,4'-DDT

R.T.: 7.079 min
Delta R.T.: 0.000 min
Response: 344484631
Conc: 160.00 ng/ml

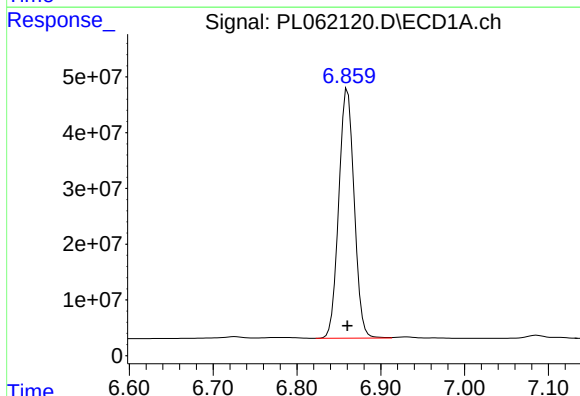


#20 Methoxychlor

R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 571021058
Conc: 765.25 ng/ml

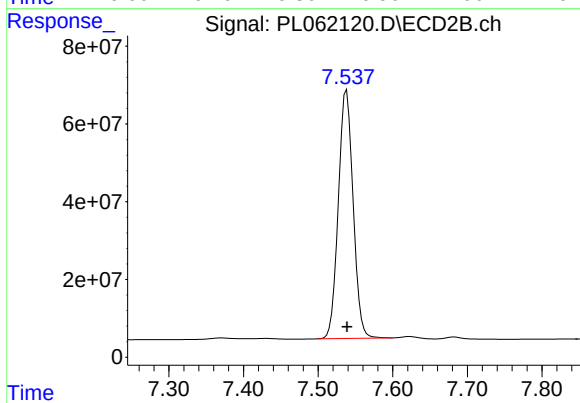

#20 Methoxychlor


R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 879644604
Conc: 791.28 ng/ml

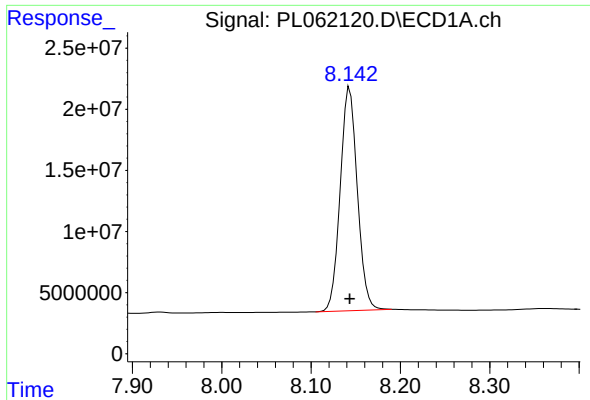

#27 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 243405153
Conc: 147.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

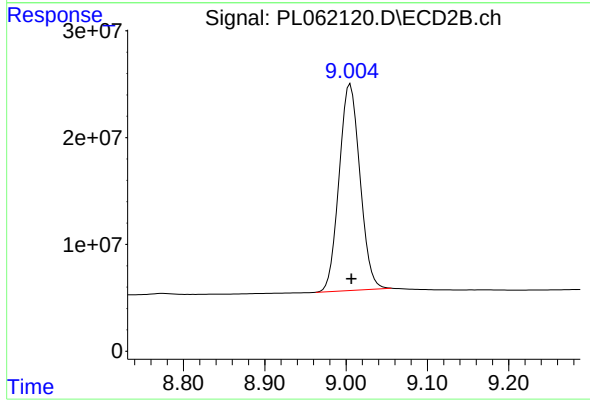

#27 Decachlorobiphenyl

R.T.: 9.005 min
Delta R.T.: -0.001 min
Response: 344726758
Conc: 148.32 ng/ml