

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100821\
 Data File : PL070201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2021 15:42
 Operator : AR\AJ
 Sample : M4113-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

mohammad
 10/12/2021 8:49:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 00:09:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.627	5.565	6437609	18707478	12.865	14.144
28)	SA Decachlor...	10.395	11.488	8012158	14105206	11.579	11.656
Target Compounds							
12)	B 4,4'-DDE	7.627	8.562	583783	1331933	0.917m	0.860
17)	MA 4,4'-DDT	8.473	9.424	424999	492801	0.695	0.377m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100821\
Data File : PL070201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2021 15:42
Operator : AR\AJ
Sample : M4113-05
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-3


Manual Integrations
APPROVED

mohammad
10/12/2021 8:49:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 00:09:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

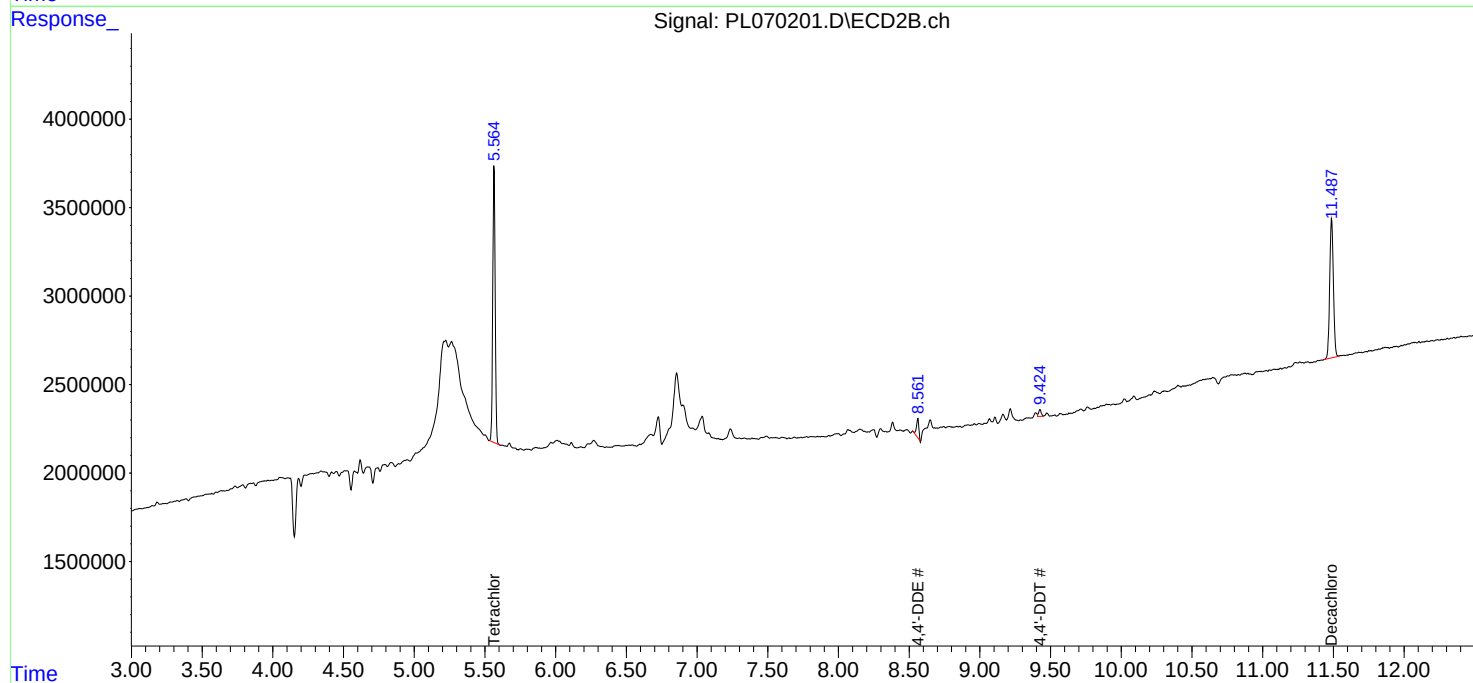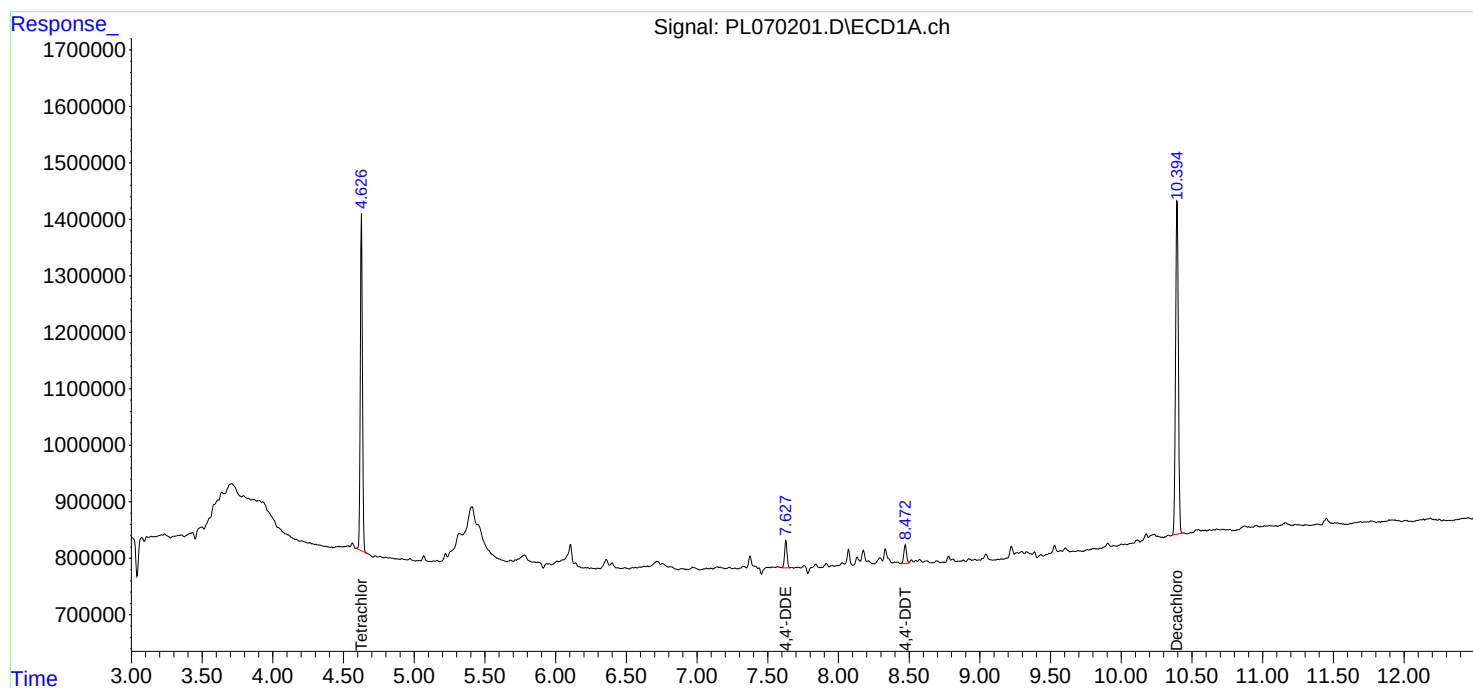

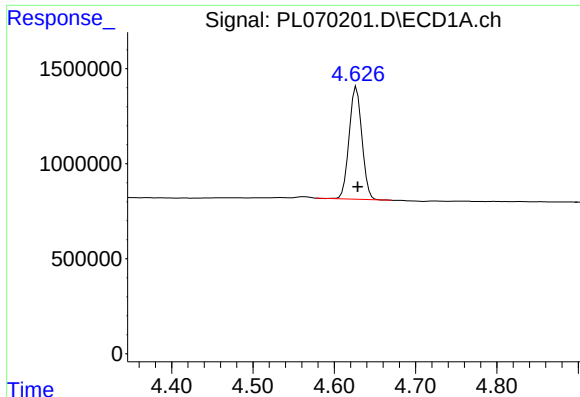


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: -0.002 min
Response: 6437609
Conc: 12.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

mohammad
10/12/2021 8:49:44 AM

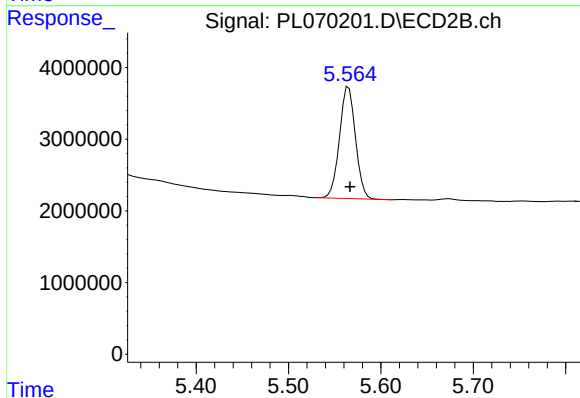


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: -0.002 min
Response: 18707478
Conc: 14.14 ng/ml

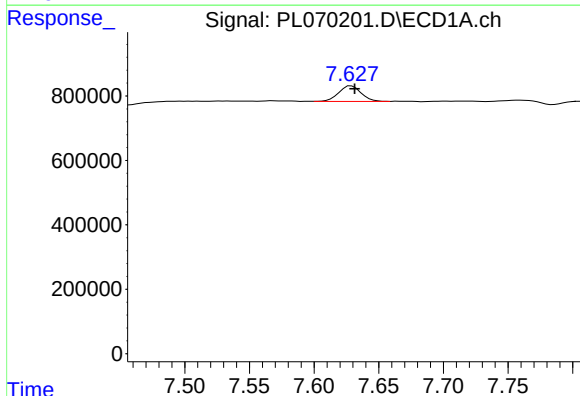


#12 4,4'-DDE

R.T.: 7.627 min
Delta R.T.: -0.004 min
Response: 583783
Conc: 0.92 ng/ml m

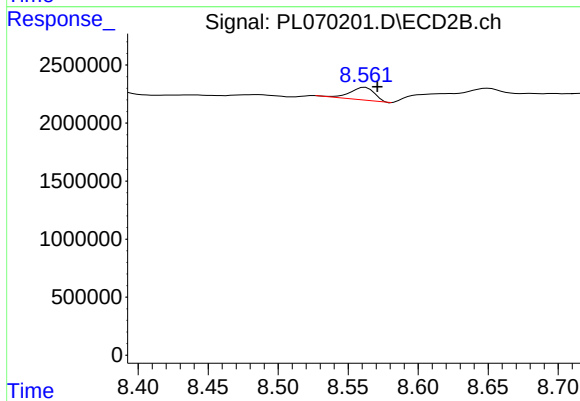

#12 4,4'-DDE

R.T.: 8.562 min
Delta R.T.: -0.009 min
Response: 1331933
Conc: 0.86 ng/ml

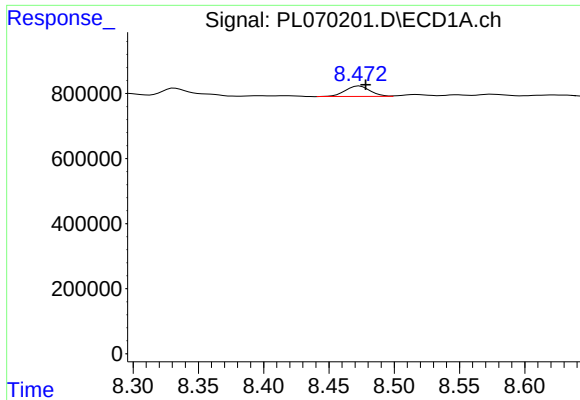


#17 4,4'-DDT

R.T.: 8.473 min
Delta R.T.: -0.005 min
Response: 424999
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

mohammad
10/12/2021 8:49:44 AM

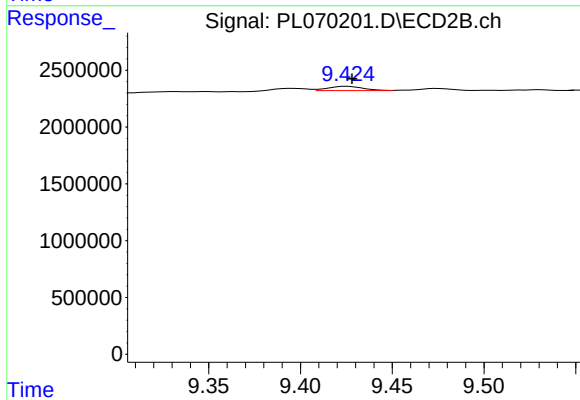


#17 4,4'-DDT

R.T.: 9.424 min
Delta R.T.: -0.004 min
Response: 492801
Conc: 0.38 ng/ml m

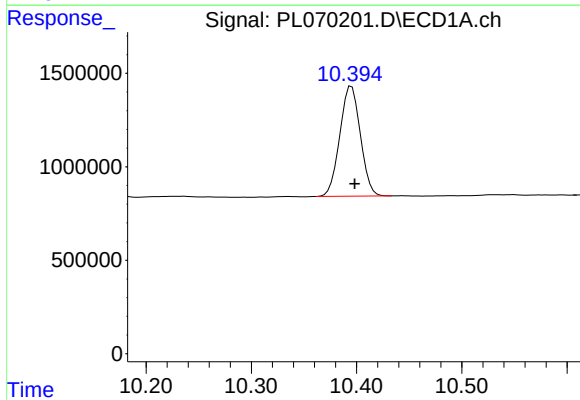

#28 Decachlorobiphenyl

R.T.: 10.395 min
Delta R.T.: -0.003 min
Response: 8012158
Conc: 11.58 ng/ml

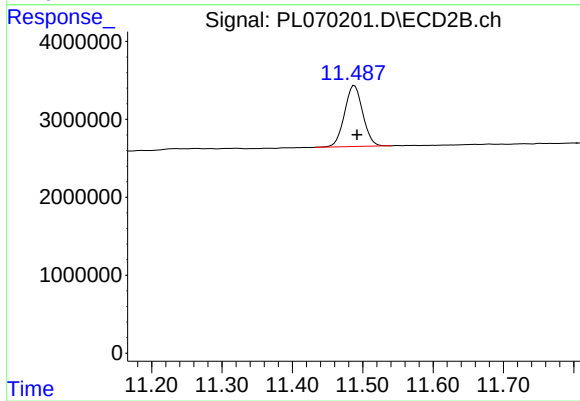

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.003 min
Response: 14105206
Conc: 11.66 ng/ml