

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100824\
 Data File : PL092269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2024 14:56
 Operator : AR\AJ
 Sample : P4321-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 IB-6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/09/2024
 Supervised By : Ankita Jodhani 10/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 02:11:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.780	3237100	3936212	1.455m	1.569
28) SA Decachlor...	9.059	7.919	1284005	1621660	0.784m	0.648m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100824\
Data File : PL092269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2024 14:56
Operator : AR\AJ
Sample : P4321-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
IB-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/09/2024
Supervised By : Ankita Jodhani 10/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 02:11:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

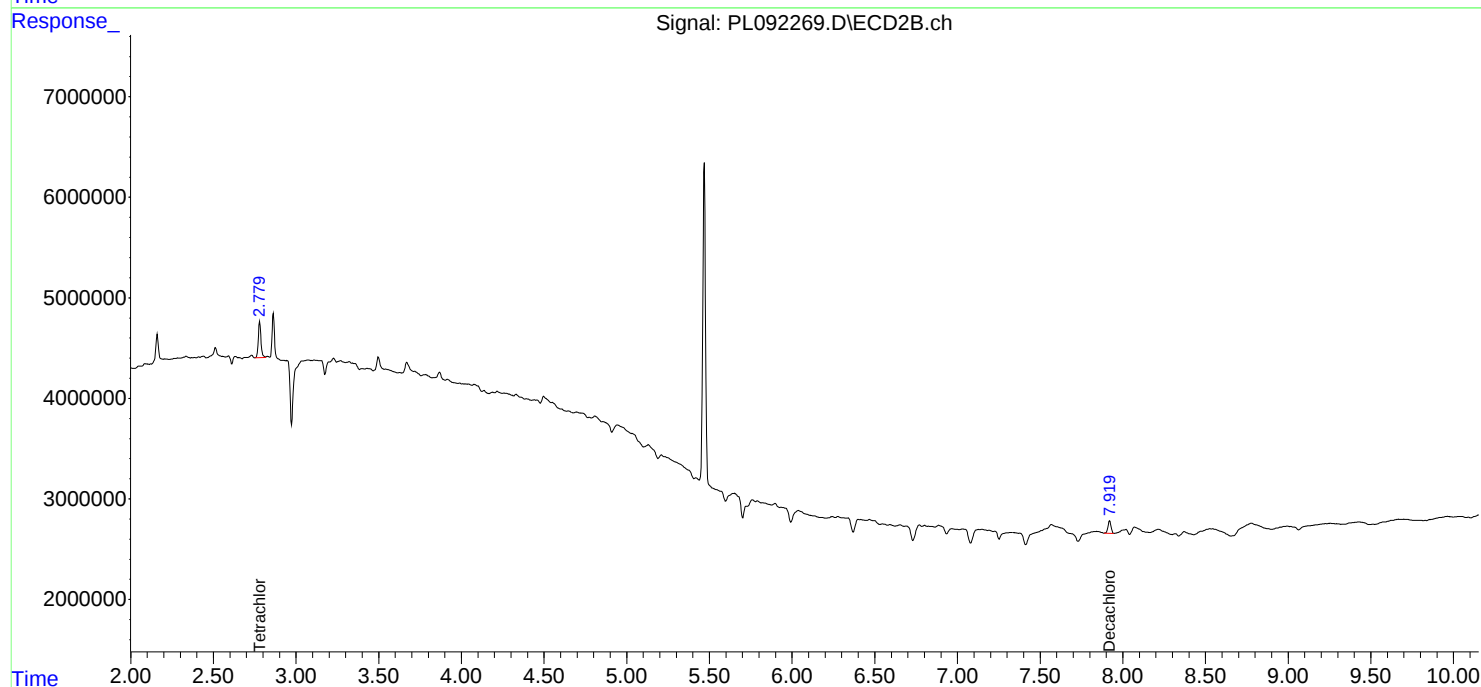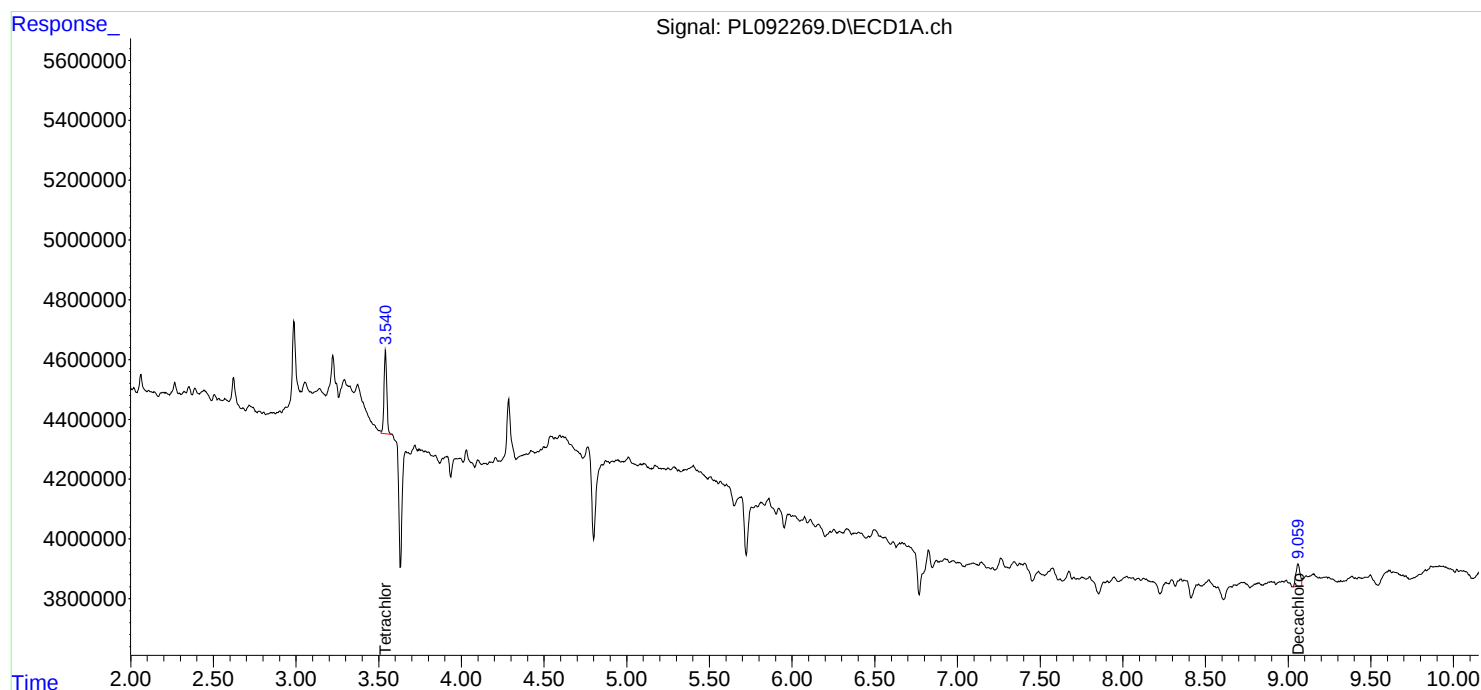

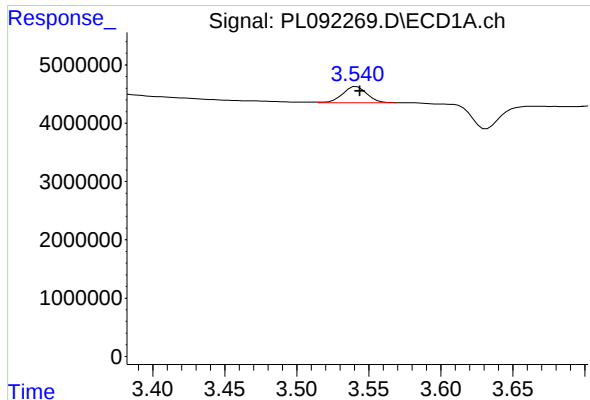


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 3237100
Conc: 1.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
IB-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/09/2024
Supervised By :Ankita Jodhani 10/09/2024

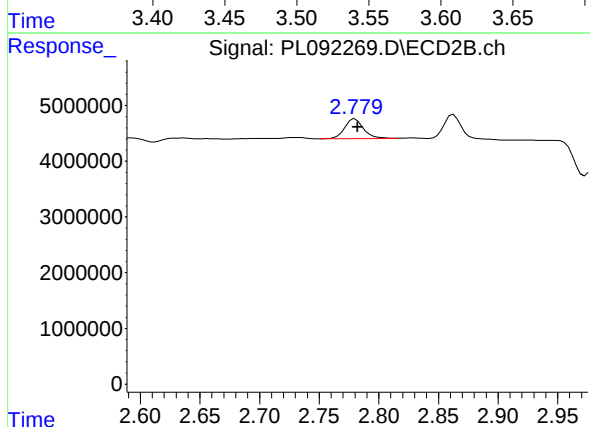


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: -0.002 min
Response: 3936212
Conc: 1.57 ng/ml

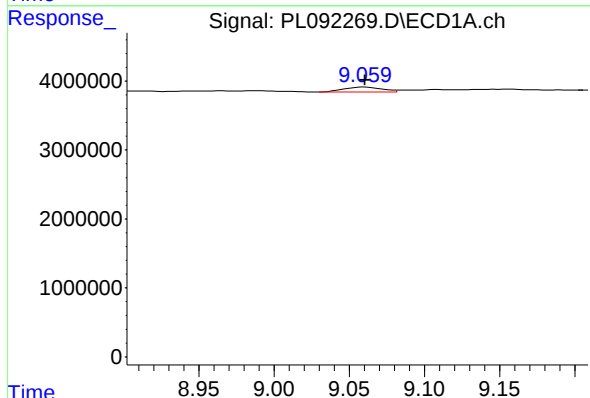

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: -0.002 min
Response: 1284005
Conc: 0.78 ng/ml m

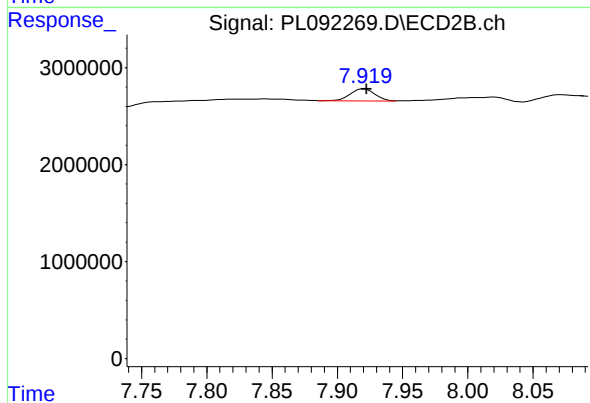

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: -0.003 min
Response: 1621660
Conc: 0.65 ng/ml m