

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
 Data File : PL040825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 19:04
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:16:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 10 01:15:52 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.483	4.101	213.6E6	129.3E6	45.119	48.345
28)	SA Decachlor...	8.240	9.224	219.3E6	112.9E6	46.323	46.926
Target Compounds							
23)	Chlordane-1	4.356	5.110	94914478	55952349	452.626	490.236
24)	Chlordane-2	4.858	5.581	100.8E6	59545050	446.953	484.426
25)	Chlordane-3	5.427	6.230	288.8E6	186.0E6	457.841	481.051
26)	Chlordane-4	5.485	6.306	254.7E6	217.7E6	458.431	480.395
27)	Chlordane-5	6.322	7.115	69547767	38573945	426.762	464.021



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
Data File : PL040825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 19:04
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:16:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
Quant Title : GC Extractables
QLast Update : Wed Oct 10 01:15:52 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

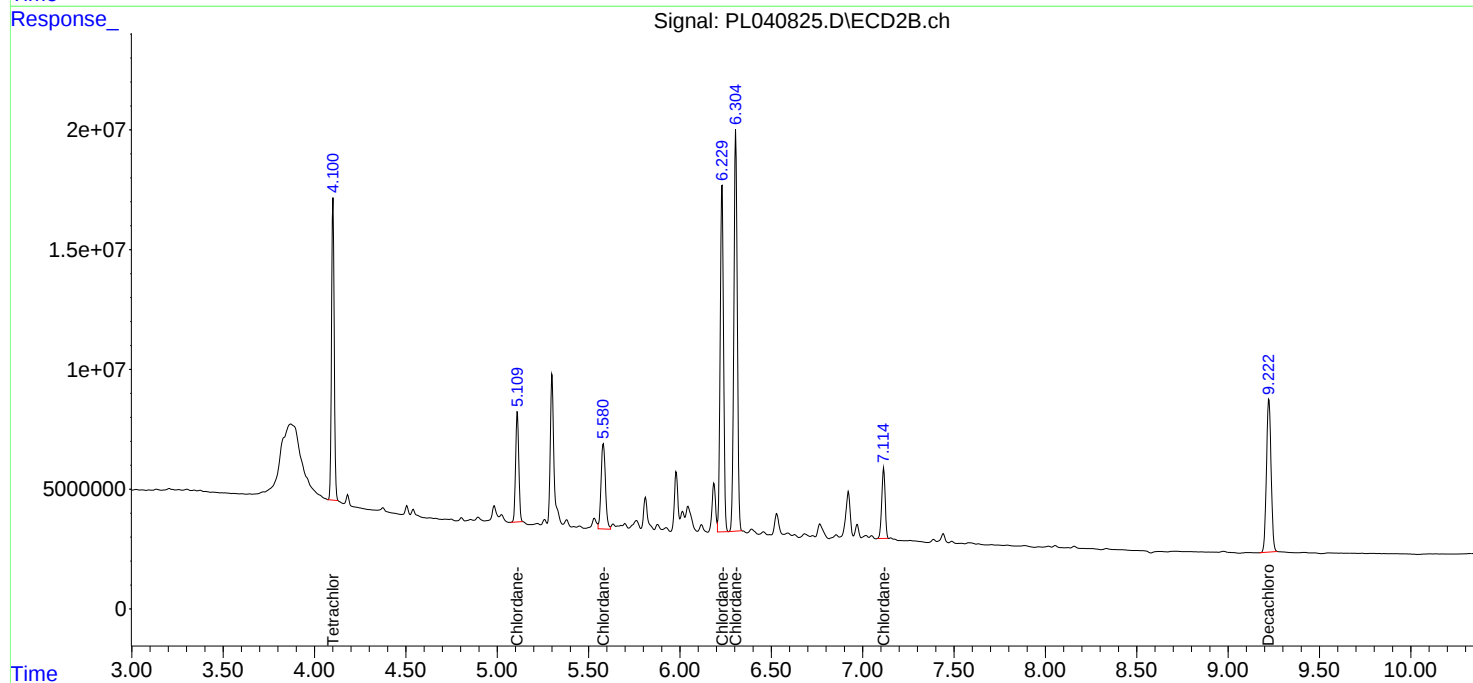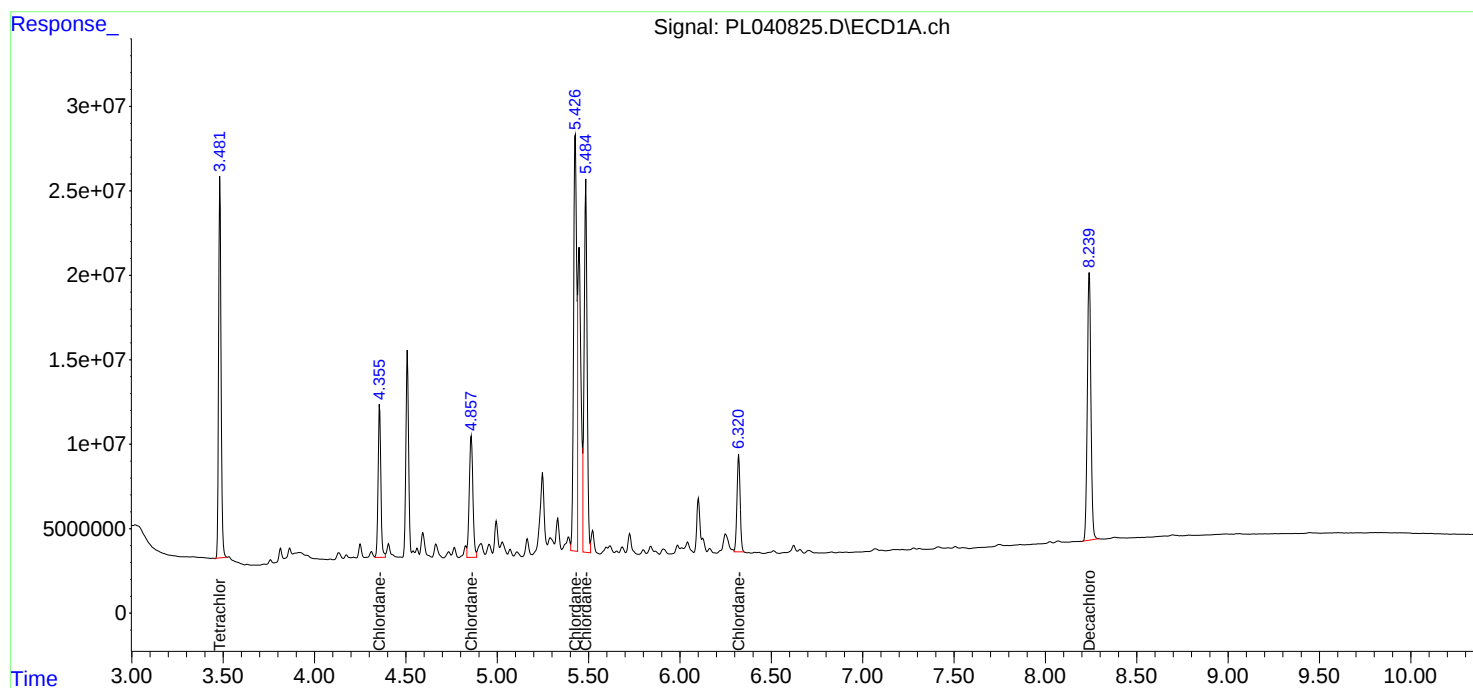


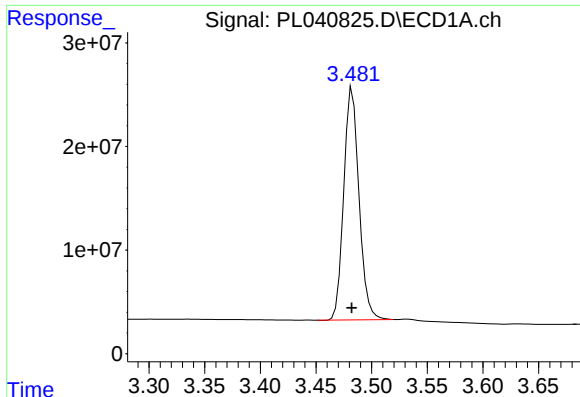

#1 Tetrachloro-m-xylene


R.T.: 3.483 min
Delta R.T.: 0.000 min
Response: 213628039
Conc: 45.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

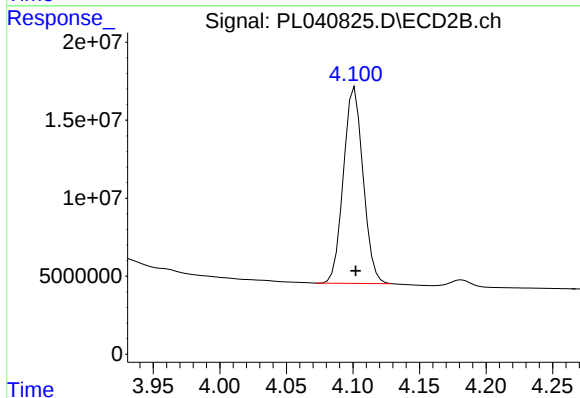


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 129336242
Conc: 48.35 ng/ml

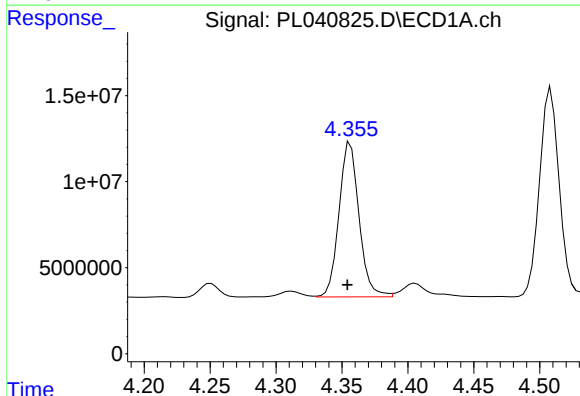


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.002 min
Response: 94914478
Conc: 452.63 ng/ml

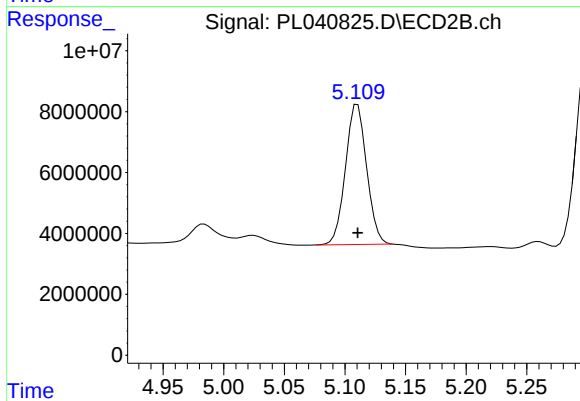

#23 Chlordane-1


R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 55952349
Conc: 490.24 ng/ml

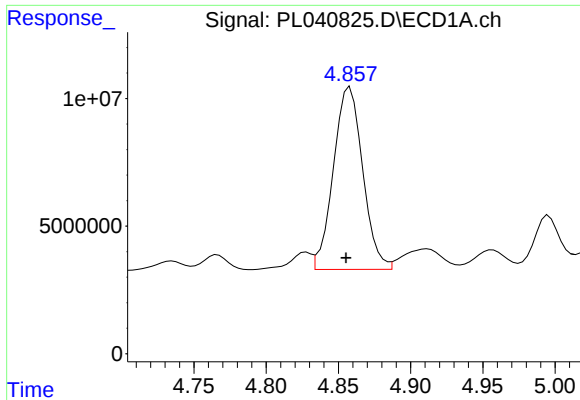

#24 Chlordane-2


R.T.: 4.858 min
Delta R.T.: 0.003 min
Response: 100843010
Conc: 446.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

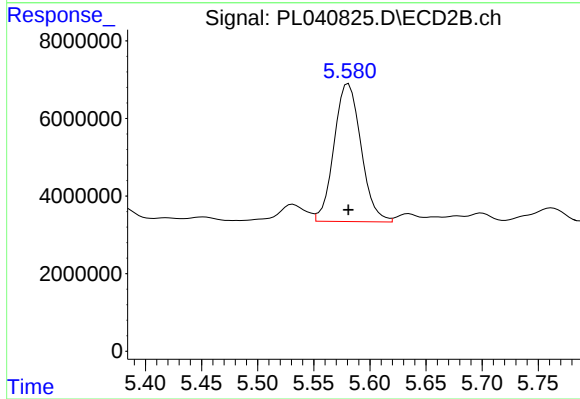


#24 Chlordane-2

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 59545050
Conc: 484.43 ng/ml

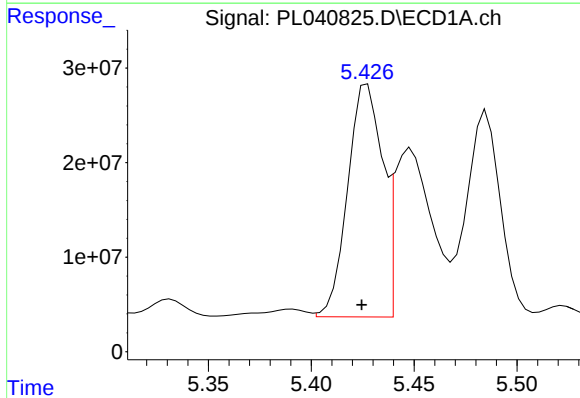


#25 Chlordane-3

R.T.: 5.427 min
Delta R.T.: 0.003 min
Response: 288806866
Conc: 457.84 ng/ml

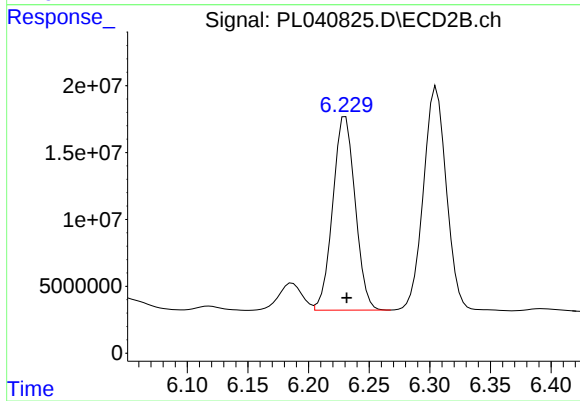

#25 Chlordane-3


R.T.: 6.230 min
Delta R.T.: -0.001 min
Response: 185956915
Conc: 481.05 ng/ml

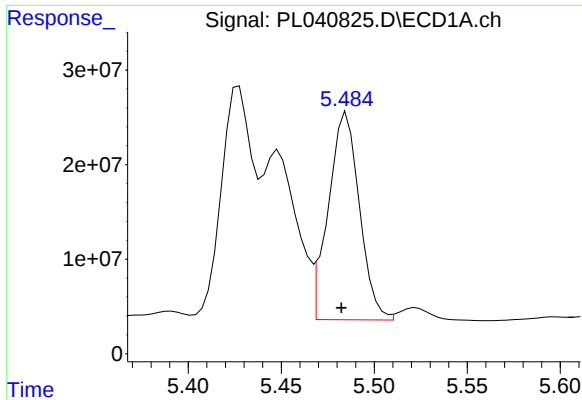

#26 Chlordane-4


R.T.: 5.485 min
Delta R.T.: 0.003 min
Response: 254682000
Conc: 458.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

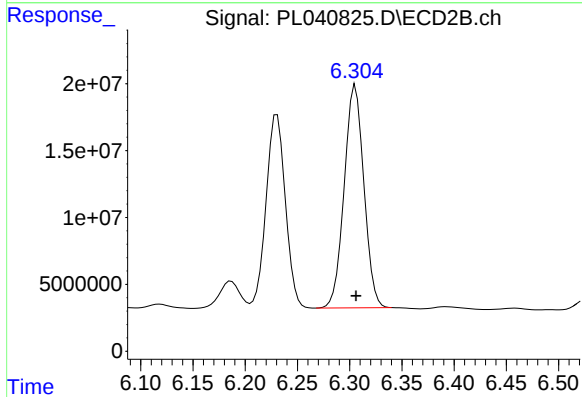


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: 0.000 min
Response: 217678716
Conc: 480.40 ng/ml

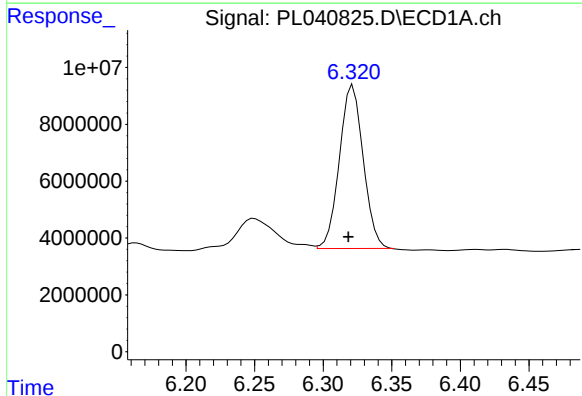


#27 Chlordane-5

R.T.: 6.322 min
Delta R.T.: 0.003 min
Response: 69547767
Conc: 426.76 ng/ml

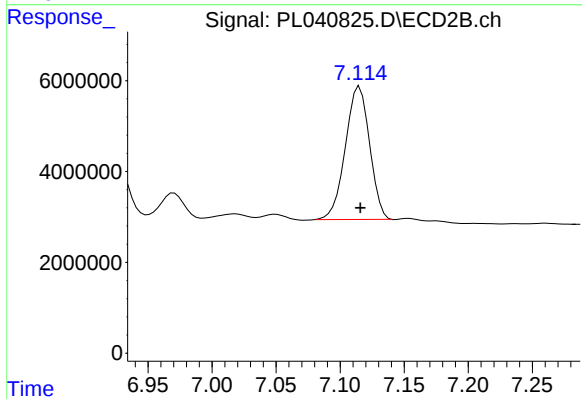

#27 Chlordane-5


R.T.: 7.115 min
Delta R.T.: 0.000 min
Response: 38573945
Conc: 464.02 ng/ml

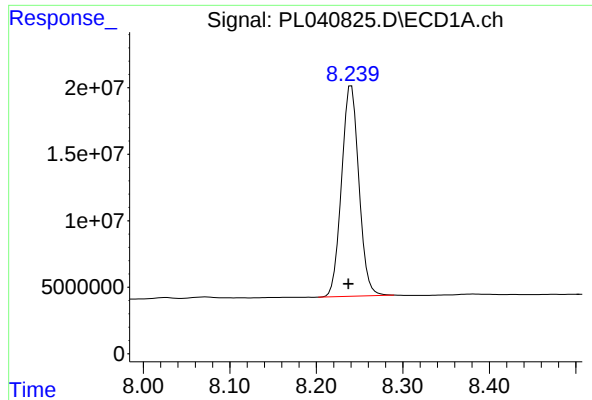

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.003 min
Response: 219279028
Conc: 46.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

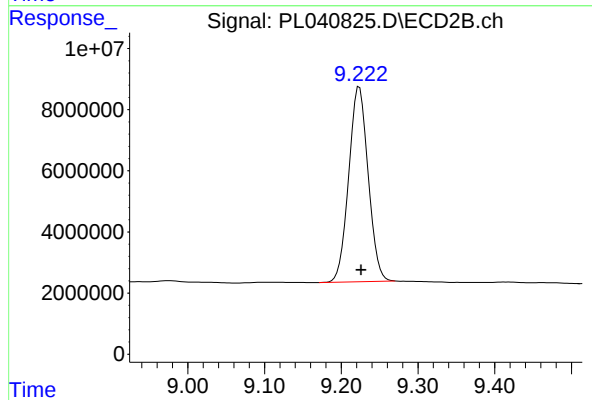

#28 Decachlorobiphenyl

R.T.: 9.224 min
Delta R.T.: -0.002 min
Response: 112867539
Conc: 46.93 ng/ml