

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
 Data File : PL040834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 03:56
 Operator : AJ\SJ
 Sample : J5200-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 06:52:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 10 02:11:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.481	4.102	98895898	53827089	21.497	20.385
28)	SA Decachlor...	8.236	9.227	93105610	47582945	20.145	20.035
Target Compounds							
3)	MA gamma-BHC...	4.215	0.000	2722382	0	0.458	N.D. #
5)	MB Aldrin	4.761	0.000	1041597	0	0.185	N.D. #
6)	B beta-BHC	4.424f	4.992f	7030175	8228803	2.702	5.195 #
8)	B Heptachlo...	5.261f	0.000	4033429	0	0.742	N.D. #
9)	A Endosulfan I	5.562	0.000	2676930	0	0.543	N.D. #
15)	B Endosulfa...	6.243f	0.000	15241549	0	3.272	N.D. #
16)	A 4,4'-DDD	0.000	6.911f	0	11071599	N.D.	5.359 #
23)	Chlordane-1	4.395	0.000	1877251	0	8.952	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
Data File : PL040834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 03:56
Operator : AJ\SJ
Sample : J5200-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 06:52:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
Quant Title : GC Extractables
QLast Update : Wed Oct 10 02:11:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

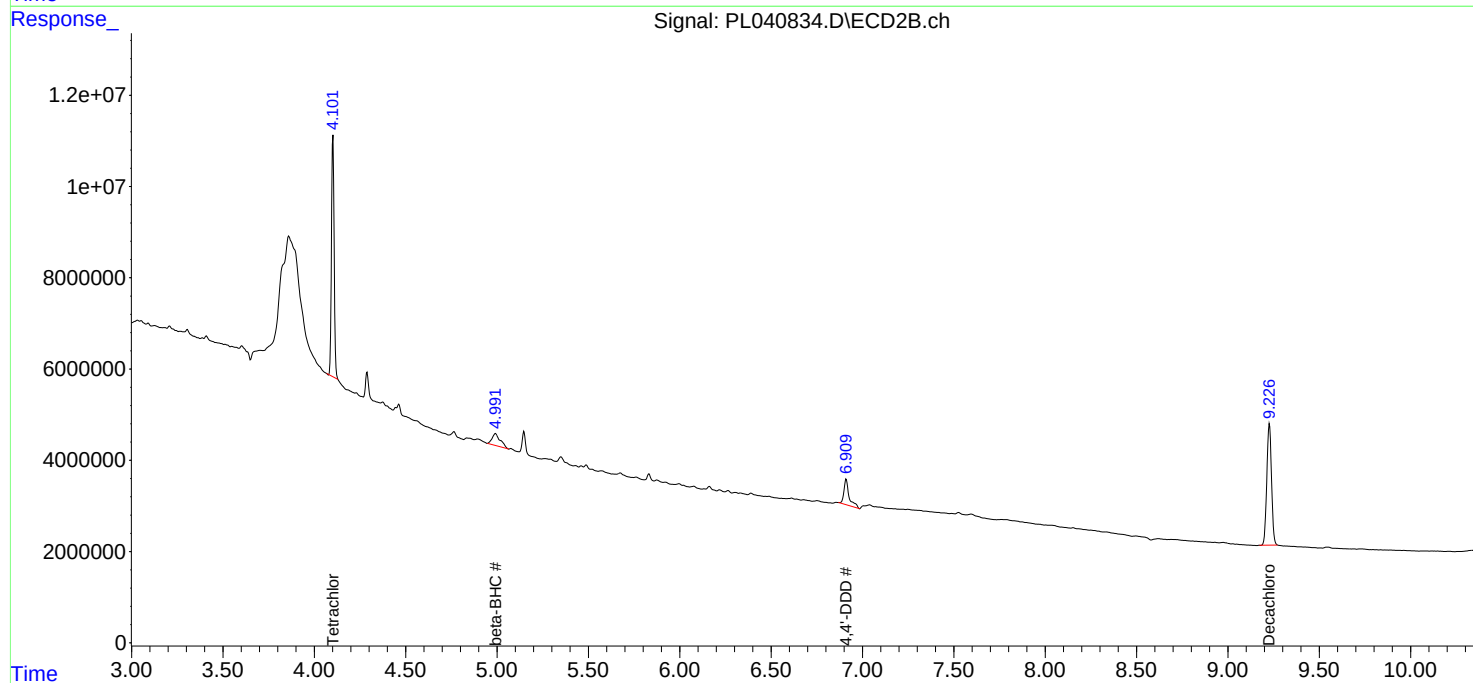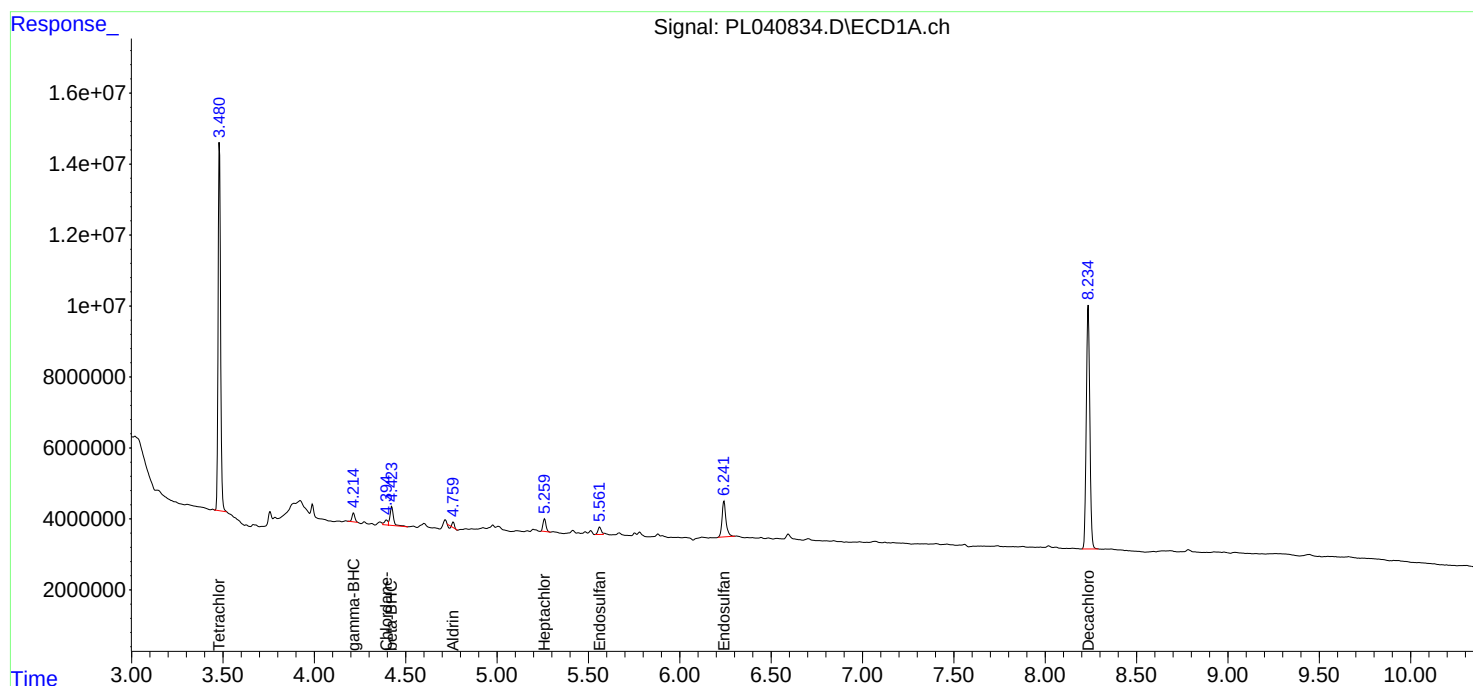


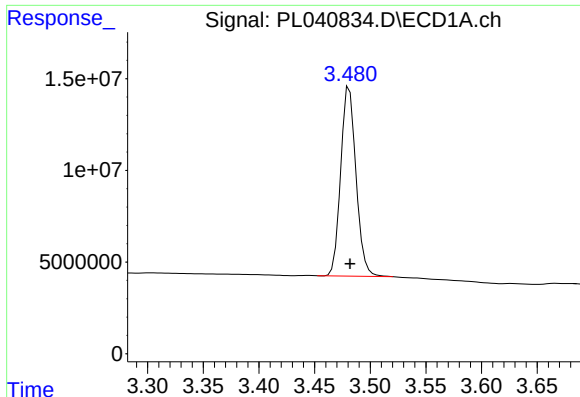

#1 Tetrachloro-m-xylene


R.T.: 3.481 min
Delta R.T.: 0.000 min
Response: 98895898
Conc: 21.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

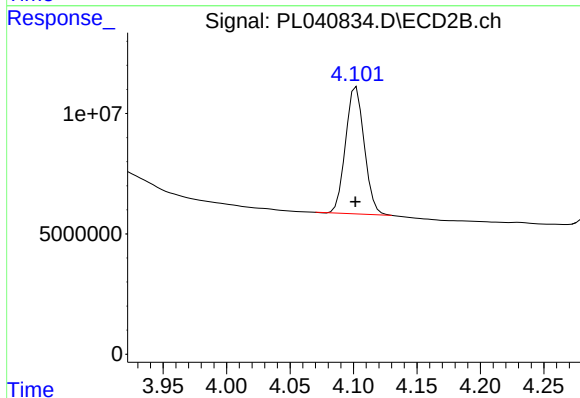


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 53827089
Conc: 20.39 ng/ml

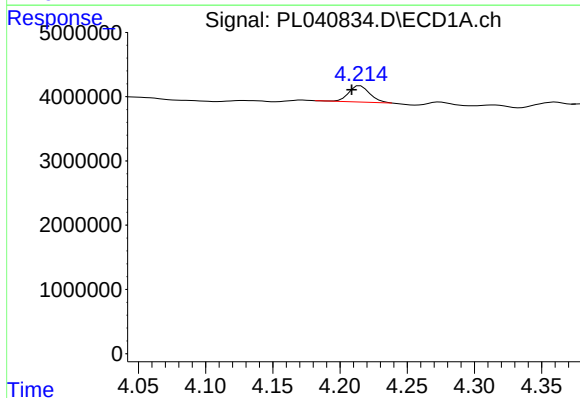


#3 gamma-BHC (Lindane)

R.T.: 4.215 min
Delta R.T.: 0.006 min
Response: 2722382
Conc: 0.46 ng/ml

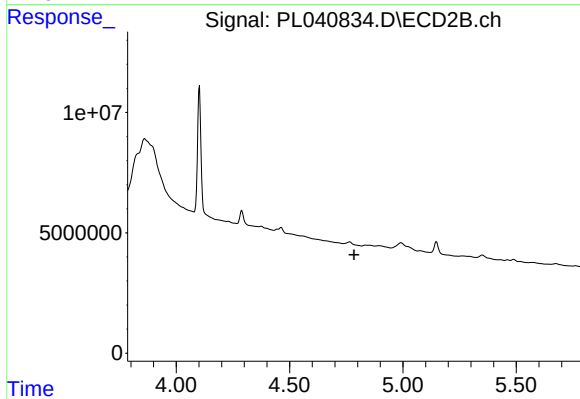

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

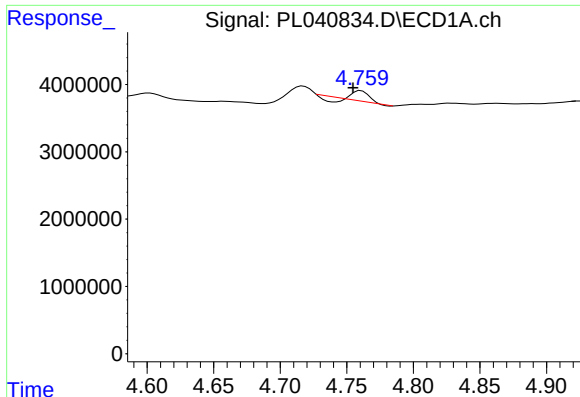

#5 Aldrin


R.T.: 4.761 min
Delta R.T.: 0.006 min
Response: 1041597
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

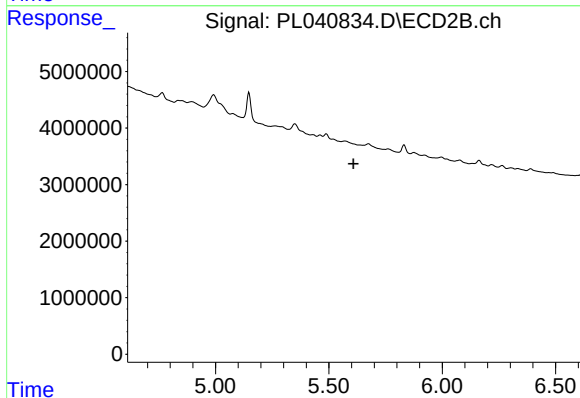


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.609 min
Response: 0
Conc: N.D.

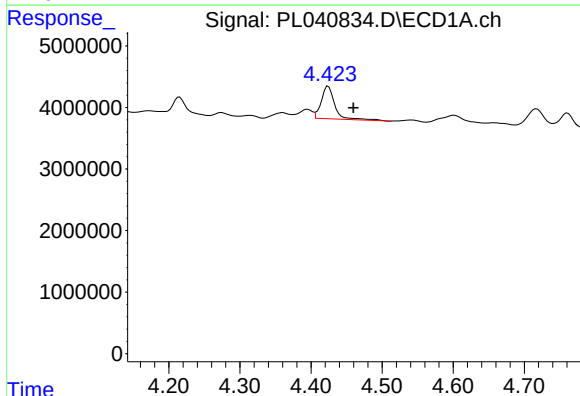


#6 beta-BHC

R.T.: 4.424 min
Delta R.T.: -0.035 min
Response: 7030175
Conc: 2.70 ng/ml

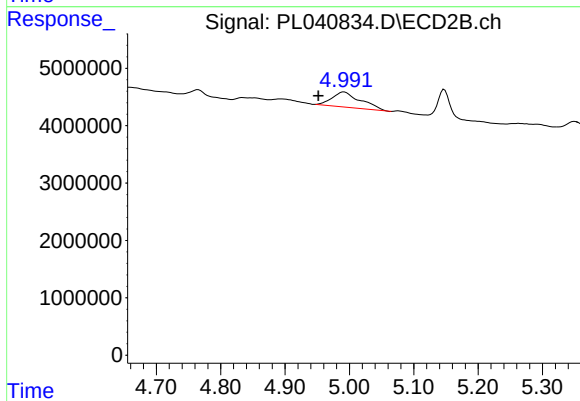

#6 beta-BHC


R.T.: 4.992 min
Delta R.T.: 0.040 min
Response: 8228803
Conc: 5.20 ng/ml

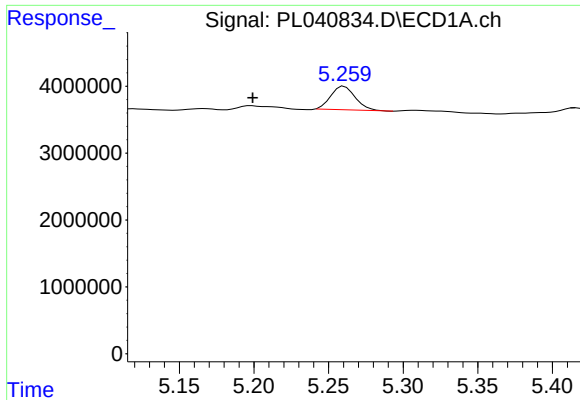

#8 Heptachlor epoxide


R.T.: 5.261 min
Delta R.T.: 0.061 min
Response: 4033429
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

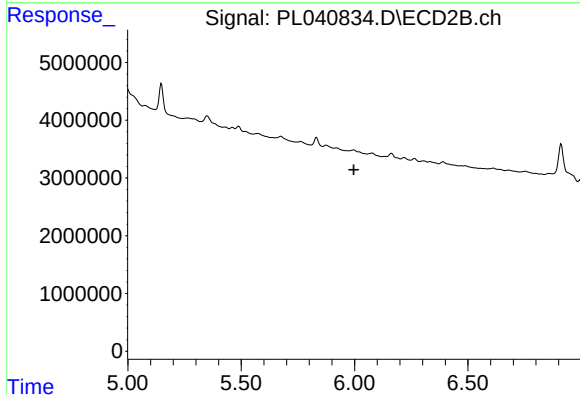


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.997 min
Response: 0
Conc: N.D.

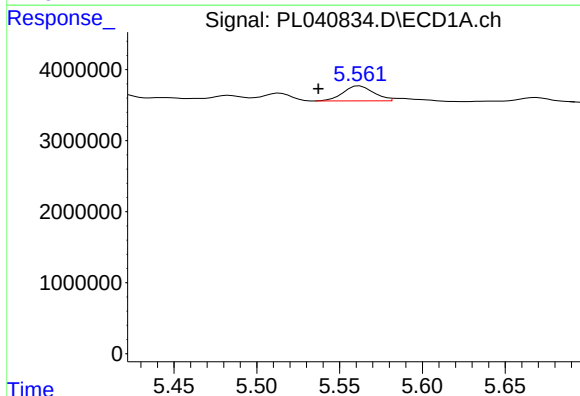


#9 Endosulfan I

R.T.: 5.562 min
Delta R.T.: 0.025 min
Response: 2676930
Conc: 0.54 ng/ml

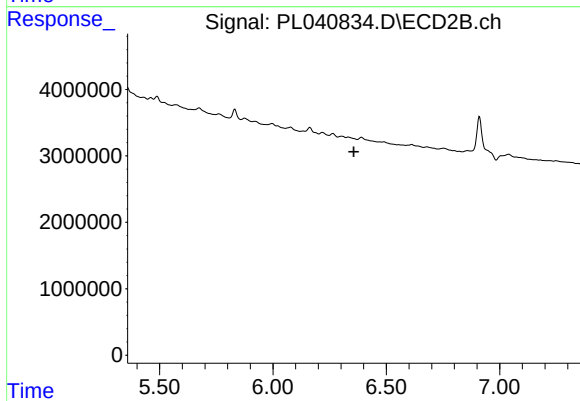

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.356 min
Response: 0
Conc: N.D.

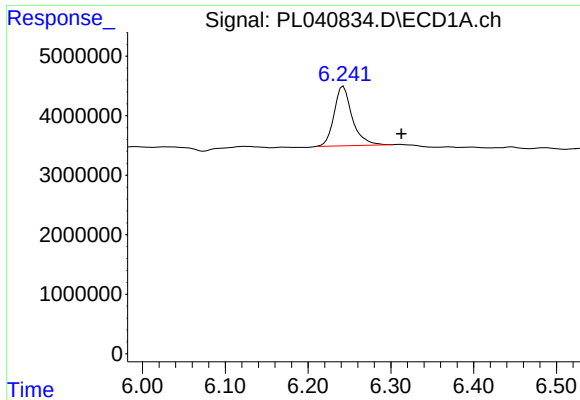

#15 Endosulfan II


R.T.: 6.243 min
Delta R.T.: -0.070 min
Response: 15241549
Conc: 3.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

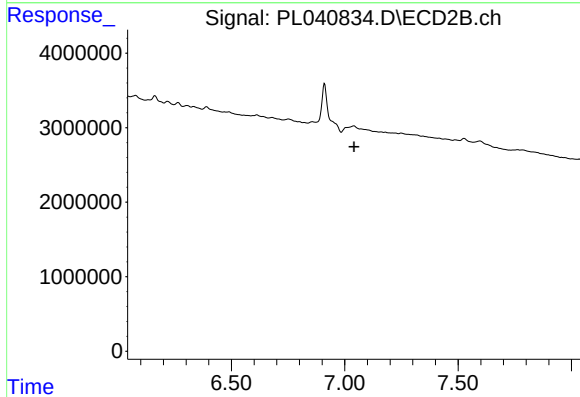


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

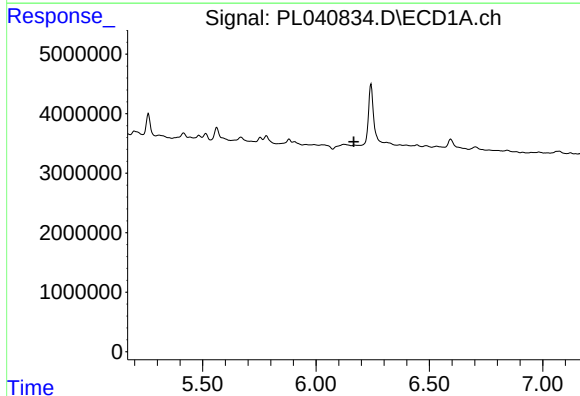


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.166 min
Response: 0
Conc: N.D.

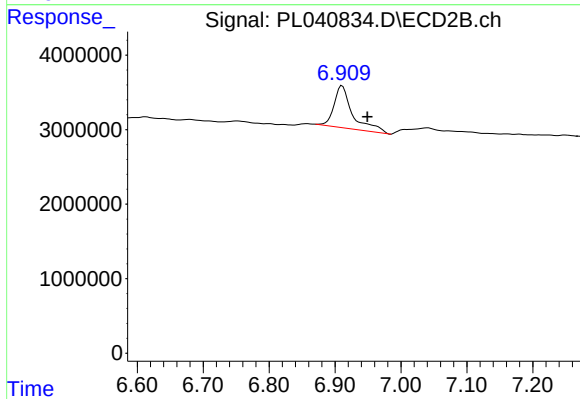

#16 4,4'-DDD


R.T.: 6.911 min
Delta R.T.: -0.038 min
Response: 11071599
Conc: 5.36 ng/ml

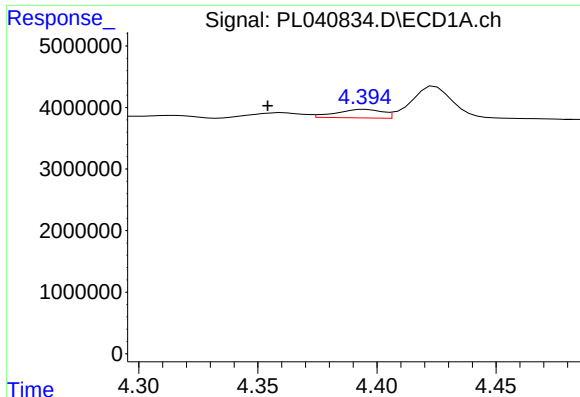

#23 Chlordane-1


R.T.: 4.395 min
Delta R.T.: 0.041 min
Response: 1877251
Conc: 8.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

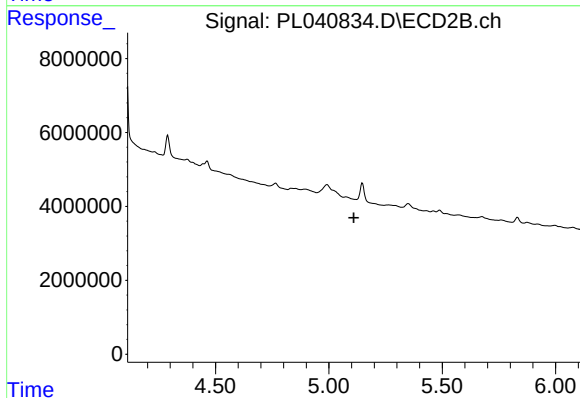


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

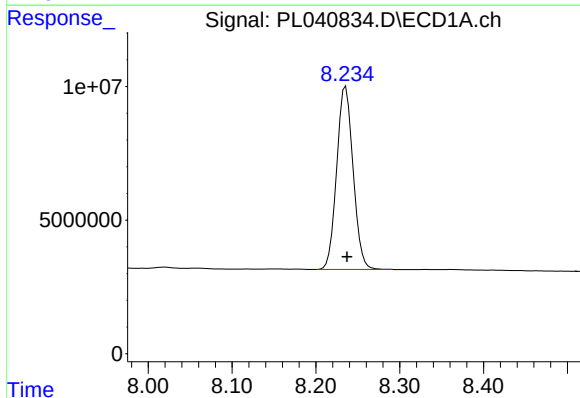

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: -0.002 min
Response: 93105610
Conc: 20.15 ng/ml

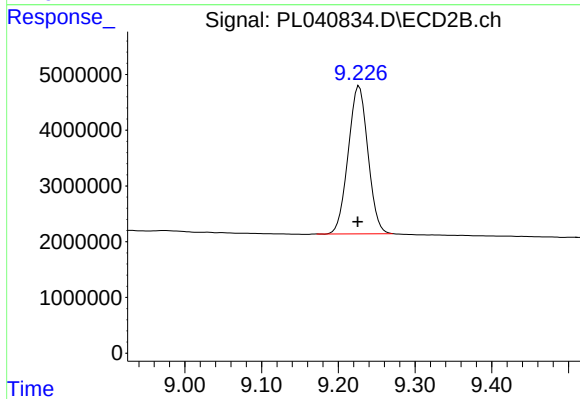

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.002 min
Response: 47582945
Conc: 20.04 ng/ml