

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
 Data File : PL040814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 22:52
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:09:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 10 01:06:41 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.482	4.102	471.1E6	262.7E6	99.448	98.913
28)	SA Decachlor...	8.238	9.225	440.9E6	222.8E6	97.284	97.257
Target Compounds							
23)	Chlordane-1	4.355	5.111	207.9E6	114.9E6	992.820	995.652
24)	Chlordane-2	4.856	5.581	210.6E6	118.2E6	973.733	975.619
25)	Chlordane-3	5.425	6.231	652.6E6	385.6E6	1012.219	1001.180
26)	Chlordane-4	5.483	6.306	565.8E6	447.0E6	1001.969	999.136
27)	Chlordane-5	6.318	7.116	162.1E6	80583190	1003.435	990.662



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
Data File : PL040814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 22:52
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:09:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
Quant Title : GC Extractables
QLast Update : Wed Oct 10 01:06:41 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

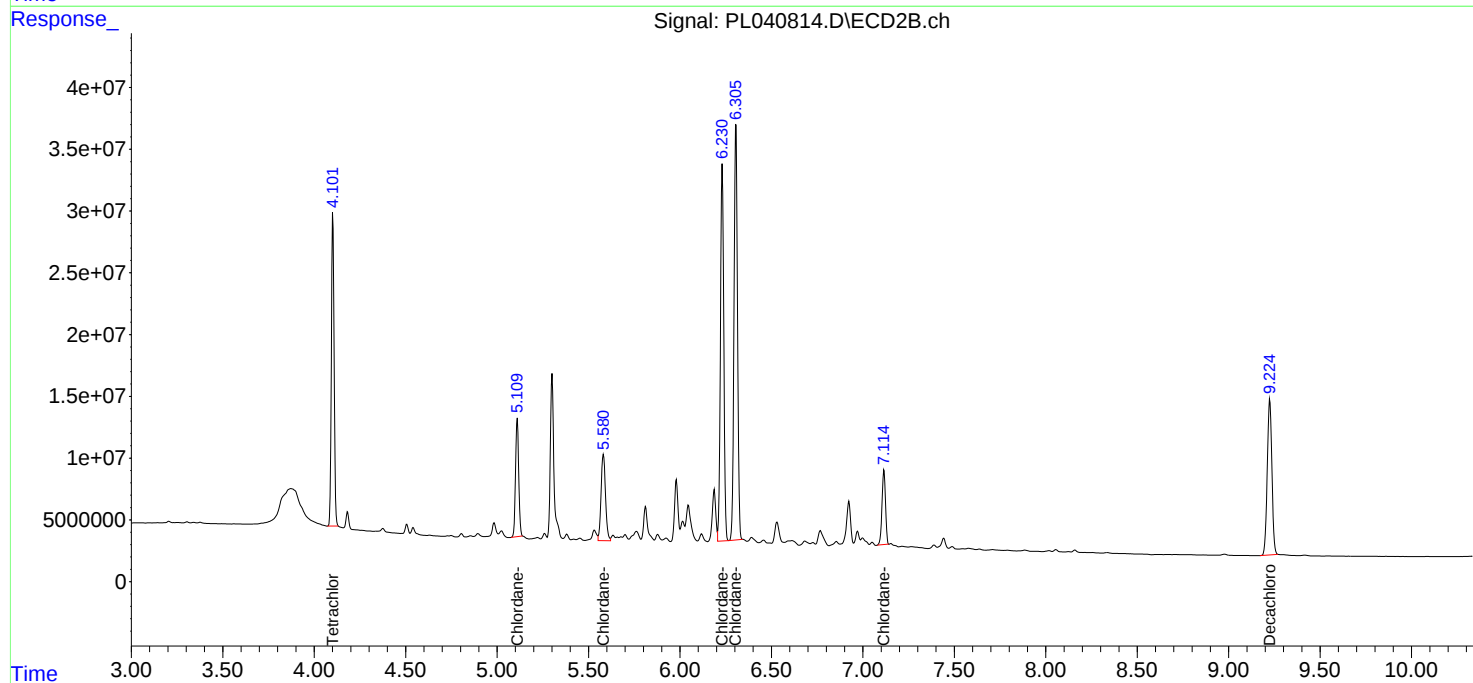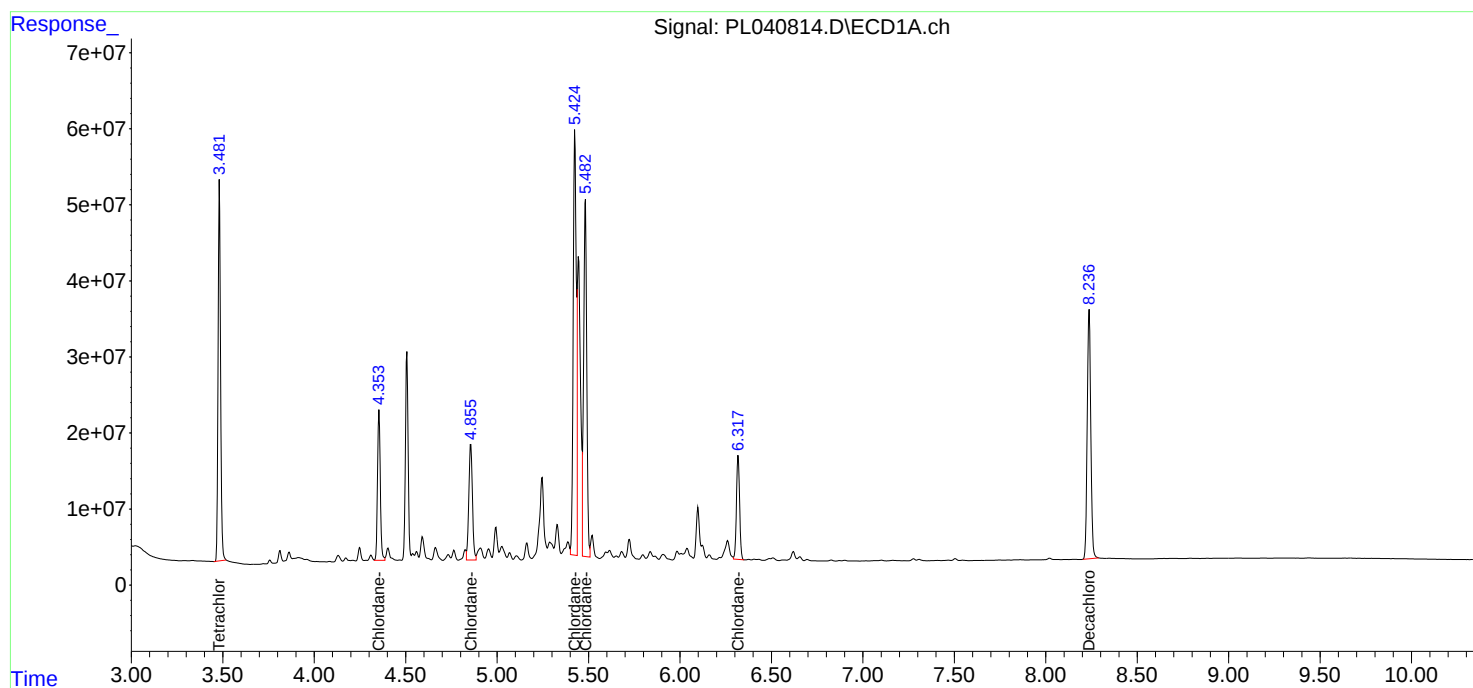


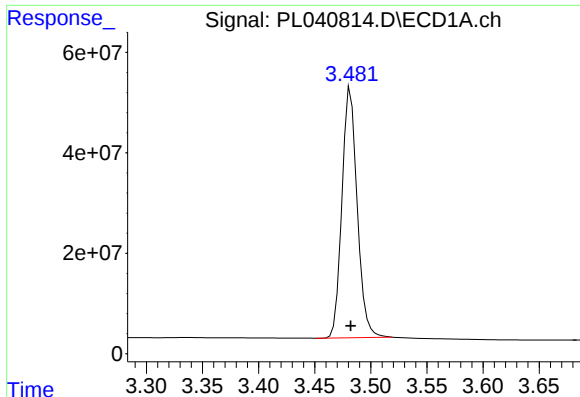

#1 Tetrachloro-m-xylene


R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 471088426
Conc: 99.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

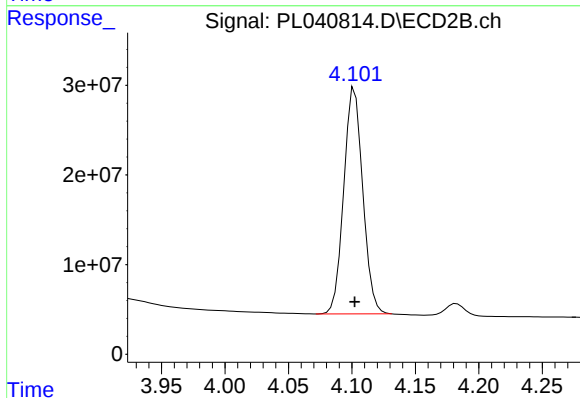


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 262697457
Conc: 98.91 ng/ml

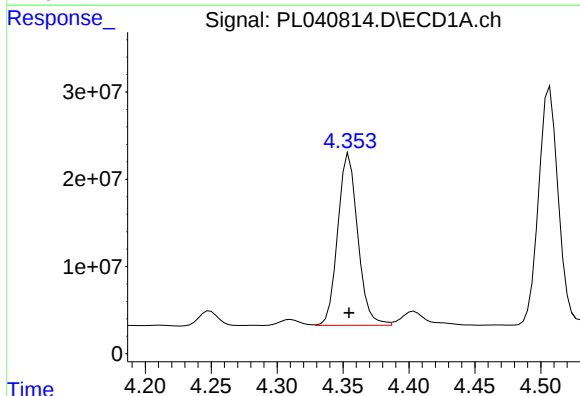


#23 Chlordane-1

R.T.: 4.355 min
Delta R.T.: 0.000 min
Response: 207896497
Conc: 992.82 ng/ml

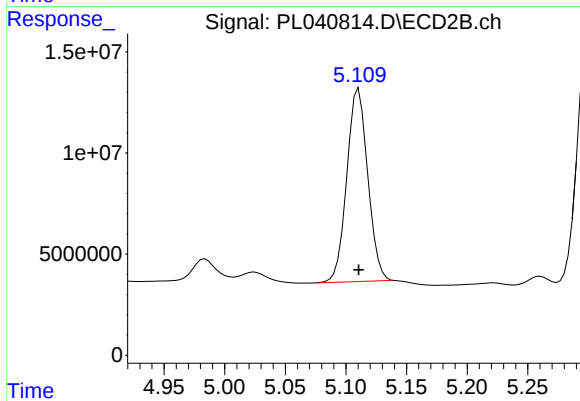

#23 Chlordane-1


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 114945309
Conc: 995.65 ng/ml

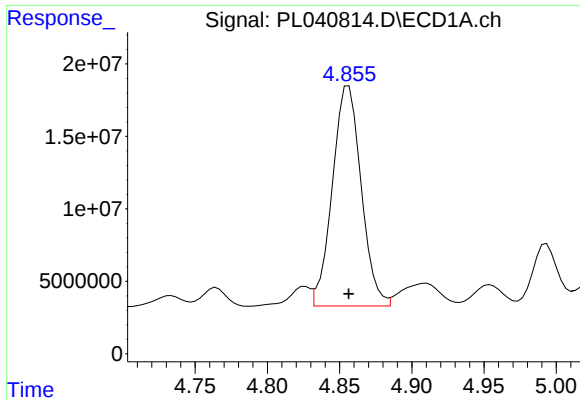

#24 Chlordane-2


R.T.: 4.856 min
Delta R.T.: 0.000 min
Response: 210560925
Conc: 973.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

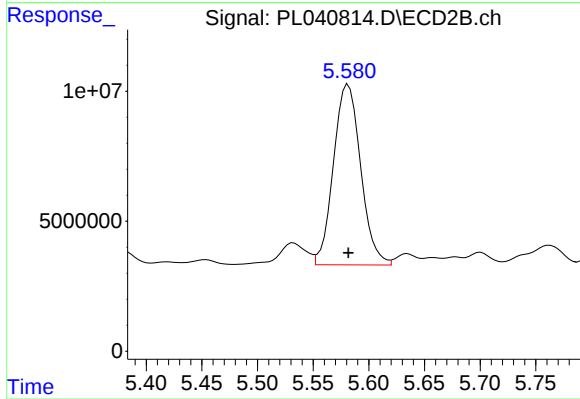


#24 Chlordane-2

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 118177706
Conc: 975.62 ng/ml

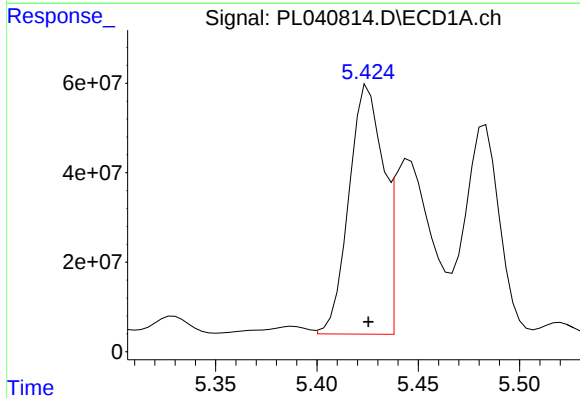


#25 Chlordane-3

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 652584768
Conc: 1012.22 ng/ml

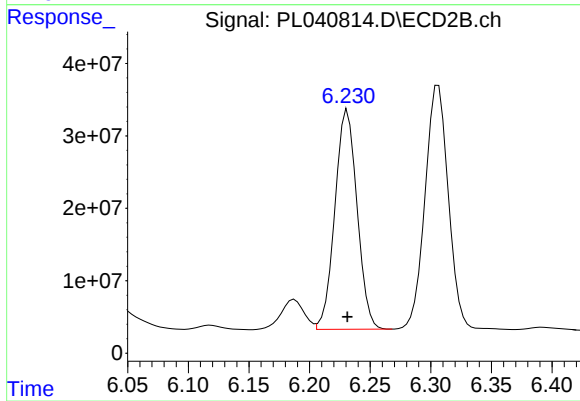

#25 Chlordane-3


R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 385619947
Conc: 1001.18 ng/ml

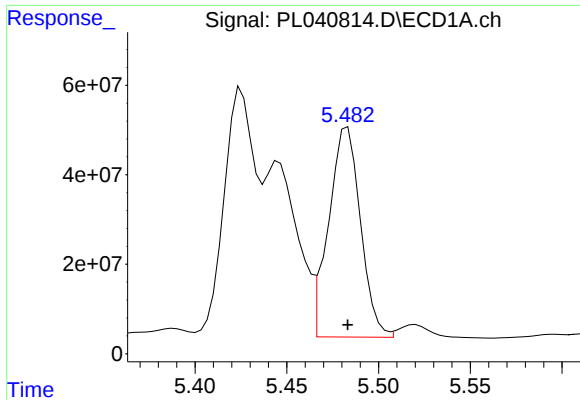

#26 Chlordane-4


R.T.: 5.483 min
Delta R.T.: 0.000 min
Response: 565778465
Conc: 1001.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

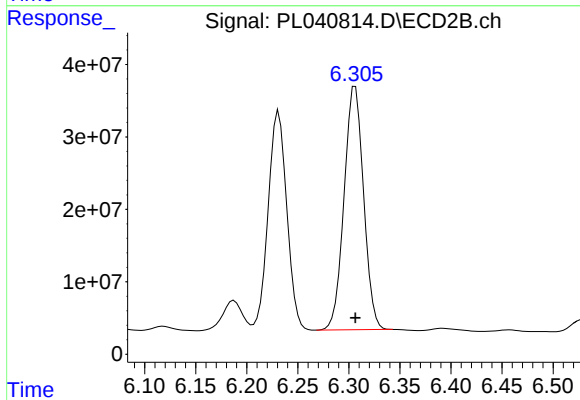


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: 0.000 min
Response: 447045540
Conc: 999.14 ng/ml

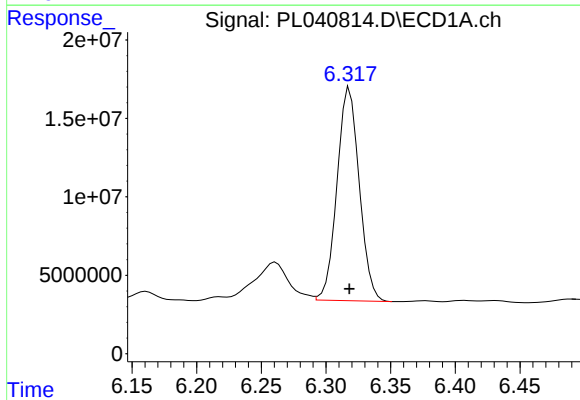


#27 Chlordane-5

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 162077118
Conc: 1003.44 ng/ml

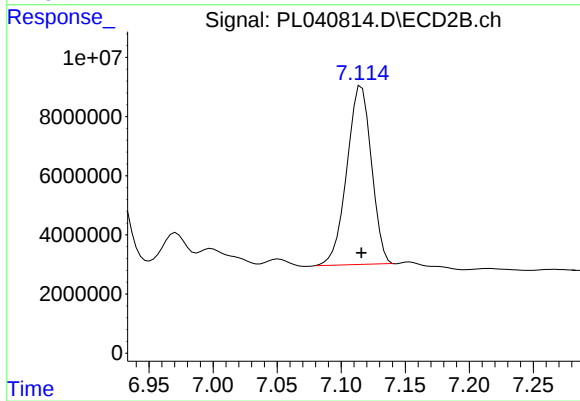

#27 Chlordane-5


R.T.: 7.116 min
Delta R.T.: 0.000 min
Response: 80583190
Conc: 990.66 ng/ml

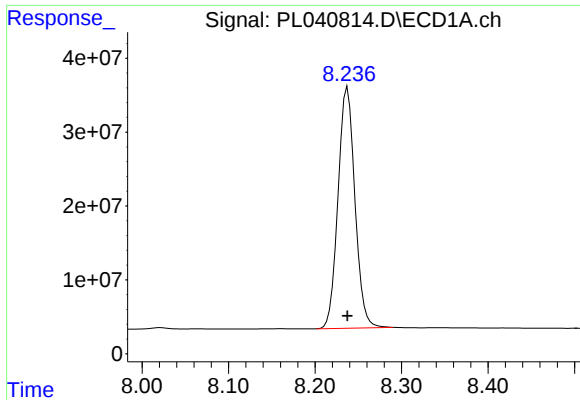

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 440917003
Conc: 97.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

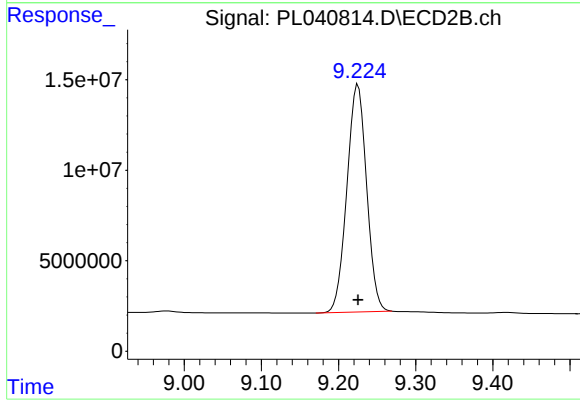

#28 Decachlorobiphenyl

R.T.: 9.225 min
Delta R.T.: 0.000 min
Response: 222820296
Conc: 97.26 ng/ml