

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
 Data File : PL040815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 23:06
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:10:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 10 01:06:41 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.482	4.102	356.7E6	198.8E6	75.204	74.891
28)	SA Decachlor...	8.236	9.225	342.2E6	175.8E6	75.334	76.155
Target Compounds							
23)	Chlordane-1	4.355	5.111	158.2E6	87686507	753.661	756.331
24)	Chlordane-2	4.856	5.581	163.1E6	91367344	752.813	752.852
25)	Chlordane-3	5.425	6.231	487.3E6	294.4E6	753.902	759.552
26)	Chlordane-4	5.483	6.306	430.2E6	342.5E6	757.911	760.181
27)	Chlordane-5	6.319	7.116	123.3E6	62439193	758.922	761.646



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
Data File : PL040815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 23:06
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:10:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
Quant Title : GC Extractables
QLast Update : Wed Oct 10 01:06:41 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

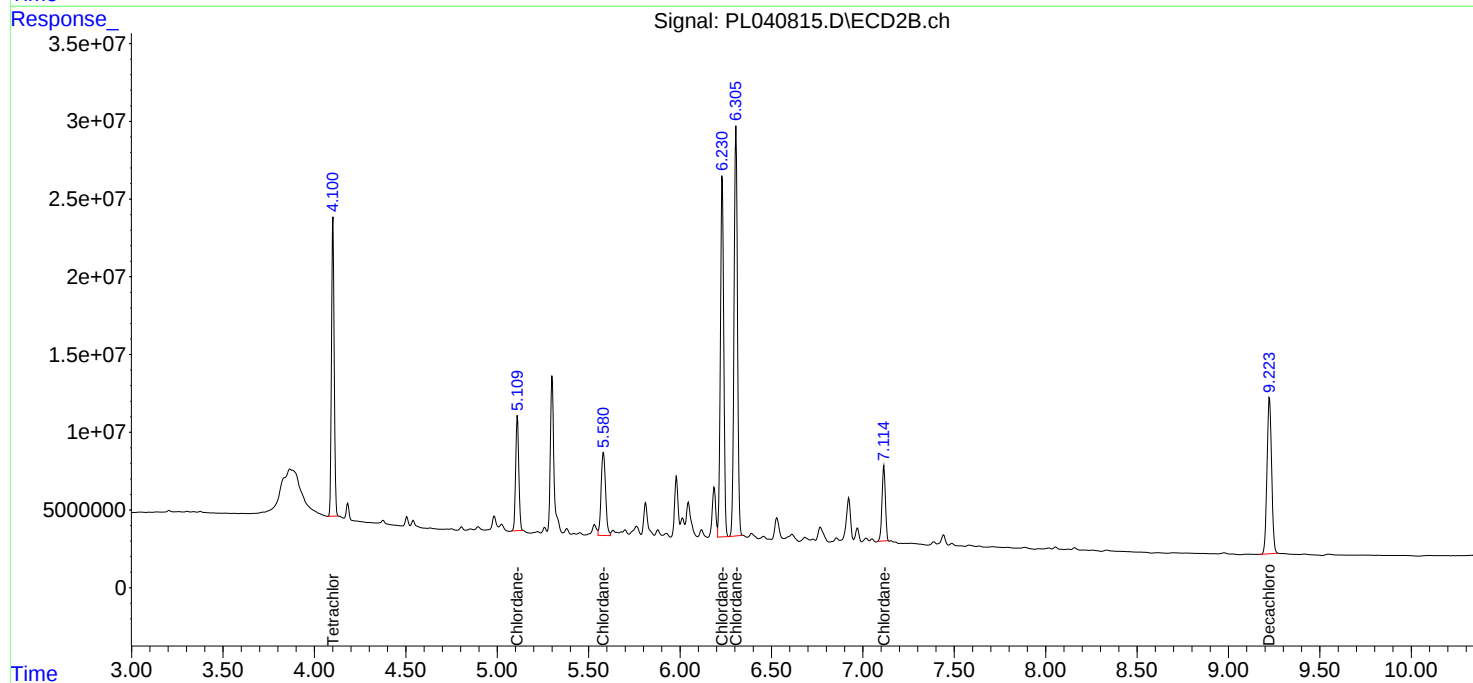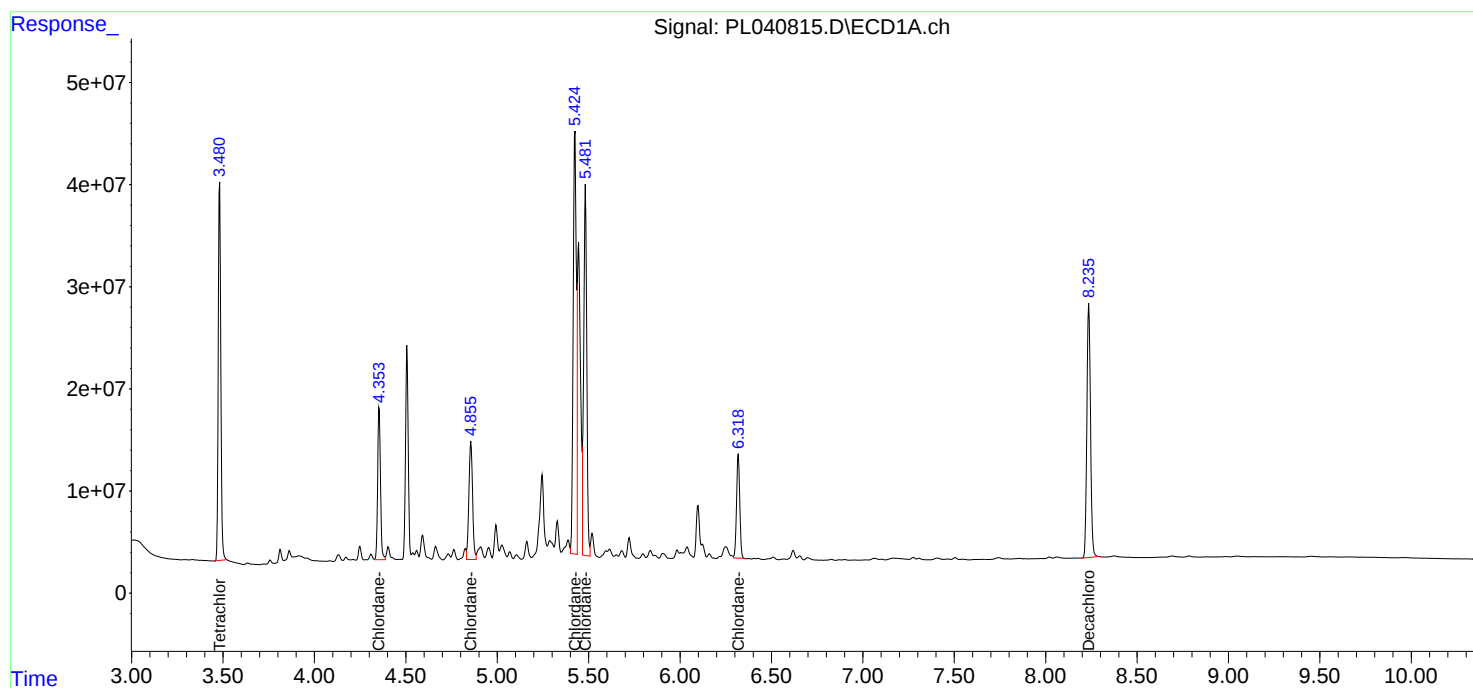


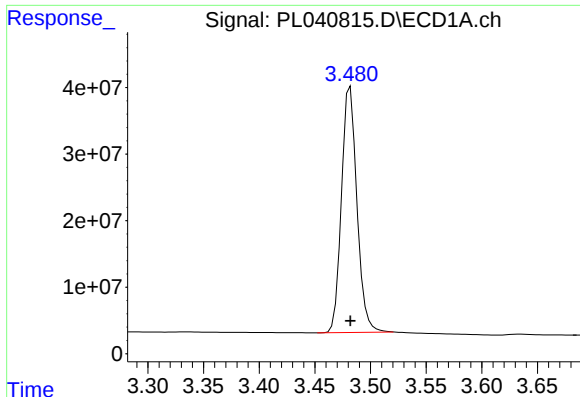

#1 Tetrachloro-m-xylene


R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 356731812
Conc: 75.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

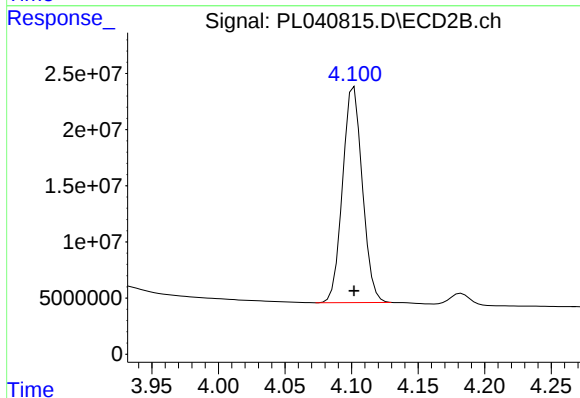


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 198754823
Conc: 74.89 ng/ml

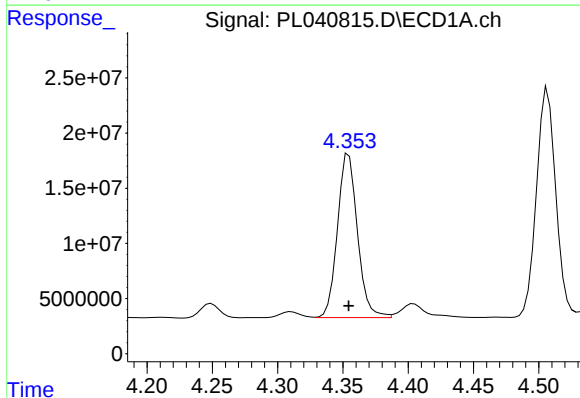


#23 Chlordane-1

R.T.: 4.355 min
Delta R.T.: 0.000 min
Response: 158202642
Conc: 753.66 ng/ml

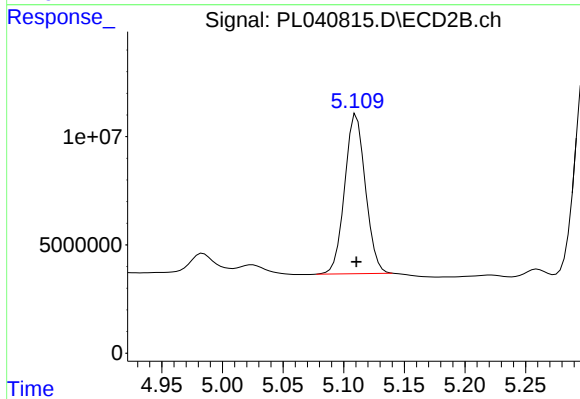

#23 Chlordane-1


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 87686507
Conc: 756.33 ng/ml

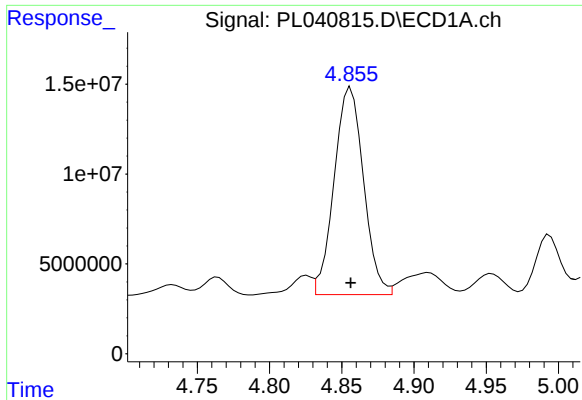

#24 Chlordane-2


R.T.: 4.856 min
Delta R.T.: 0.000 min
Response: 163094798
Conc: 752.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

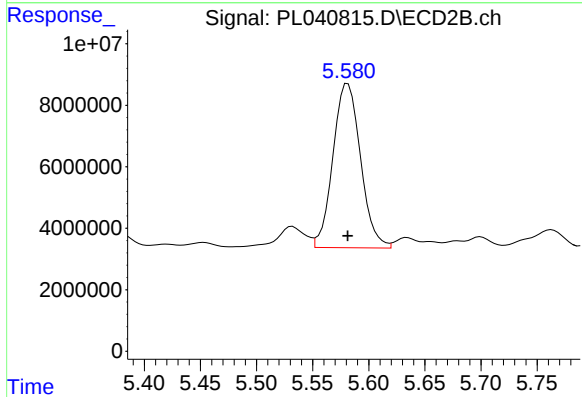


#24 Chlordane-2

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 91367344
Conc: 752.85 ng/ml

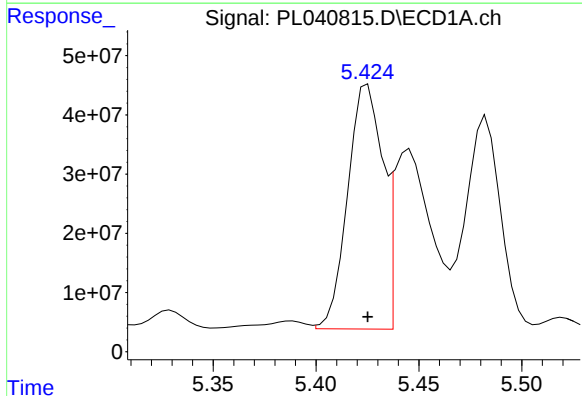


#25 Chlordane-3

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 487313661
Conc: 753.90 ng/ml

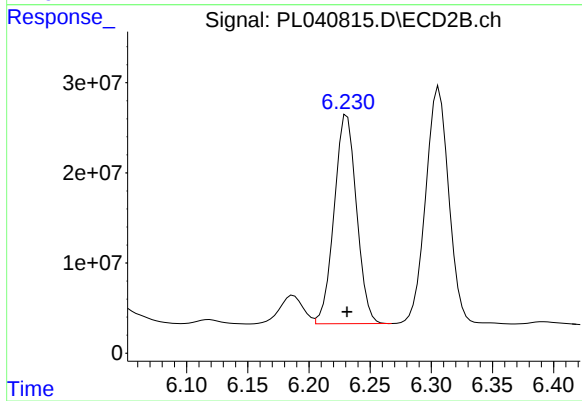

#25 Chlordane-3


R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 294428501
Conc: 759.55 ng/ml

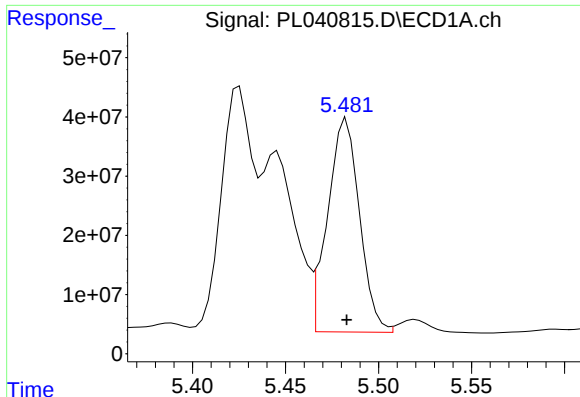

#26 Chlordane-4


R.T.: 5.483 min
Delta R.T.: 0.000 min
Response: 430236561
Conc: 757.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

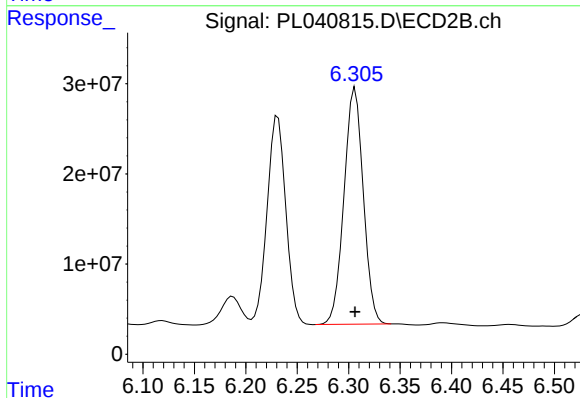


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: 0.000 min
Response: 342453480
Conc: 760.18 ng/ml

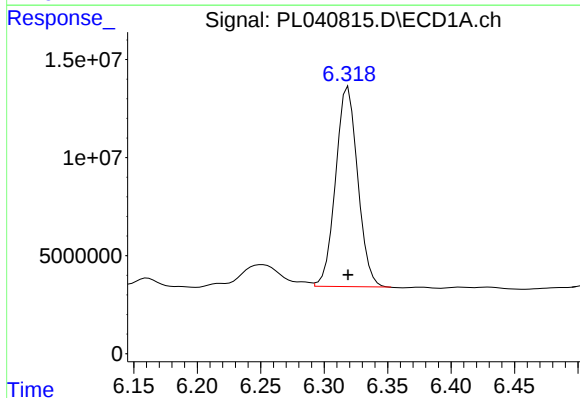


#27 Chlordane-5

R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 123316325
Conc: 758.92 ng/ml

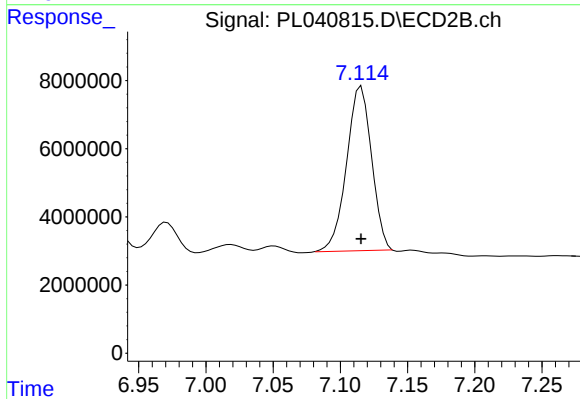

#27 Chlordane-5


R.T.: 7.116 min
Delta R.T.: 0.000 min
Response: 62439193
Conc: 761.65 ng/ml

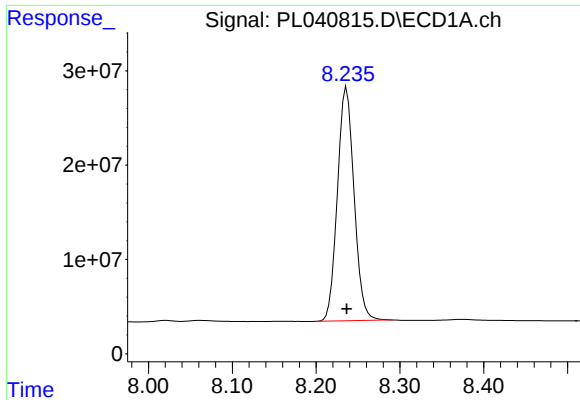

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 342197767
Conc: 75.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

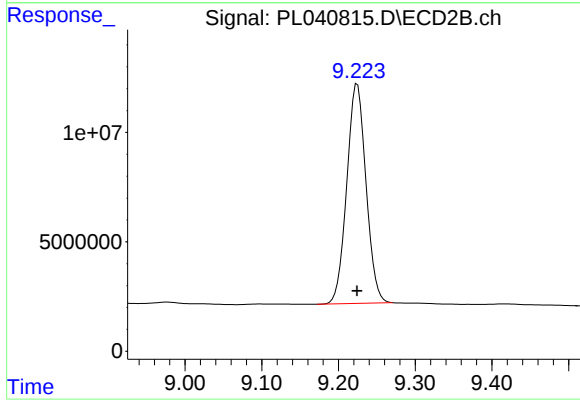

#28 Decachlorobiphenyl

R.T.: 9.225 min
Delta R.T.: 0.000 min
Response: 175827802
Conc: 76.15 ng/ml