

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
 Data File : PL040816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 23:20
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:07:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 10 01:06:41 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.482	4.102	238.2E6	134.2E6	50.000	50.000
28)	SA Decachlor...	8.238	9.225	232.8E6	117.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.355	5.111	105.5E6	57974592	522.673	489.862
24)	Chlordane-2	4.857	5.582	111.0E6	62042135	541.647	510.219
25)	Chlordane-3	5.426	6.231	318.4E6	192.4E6	457.829	496.239
26)	Chlordane-4	5.484	6.306	281.8E6	223.9E6	494.899	489.452
27)	Chlordane-5	6.319	7.116	80483724	41051135	485.551	480.720



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
Data File : PL040816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 23:20
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:07:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
Quant Title : GC Extractables
QLast Update : Wed Oct 10 01:06:41 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

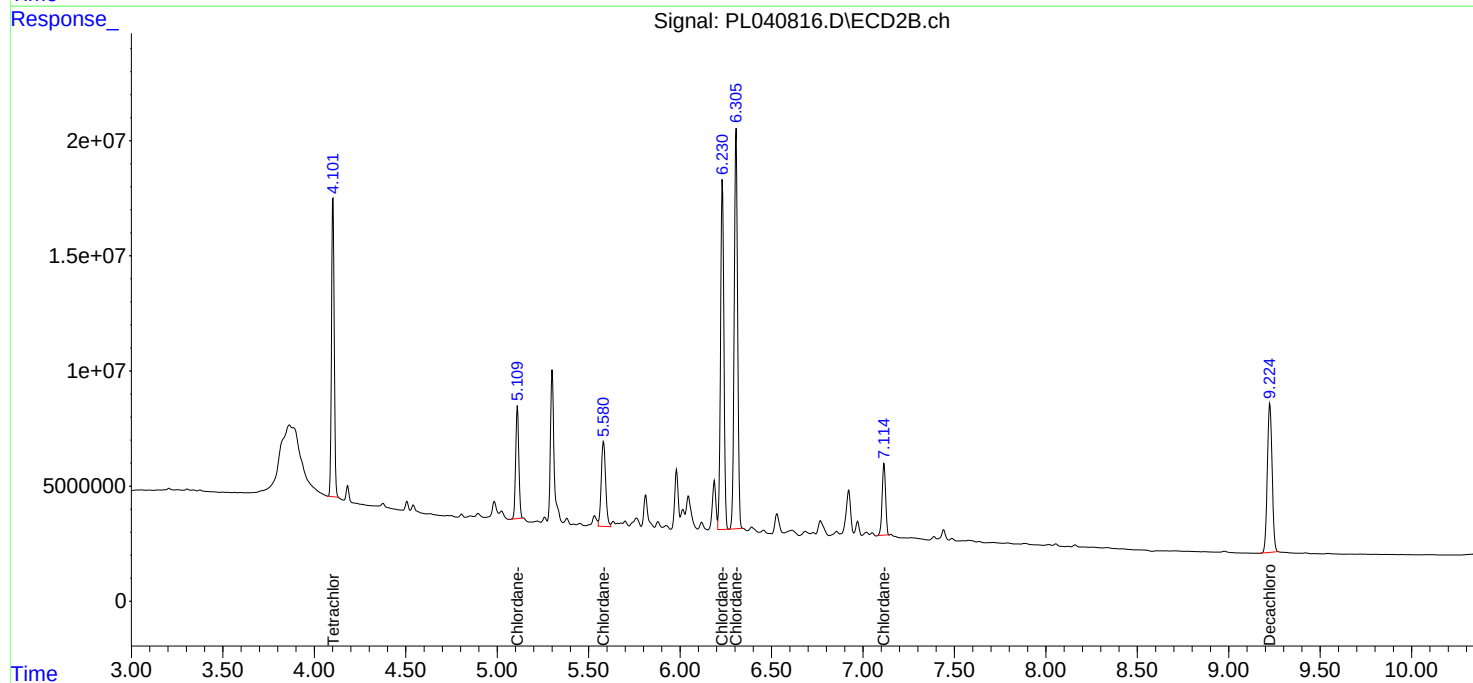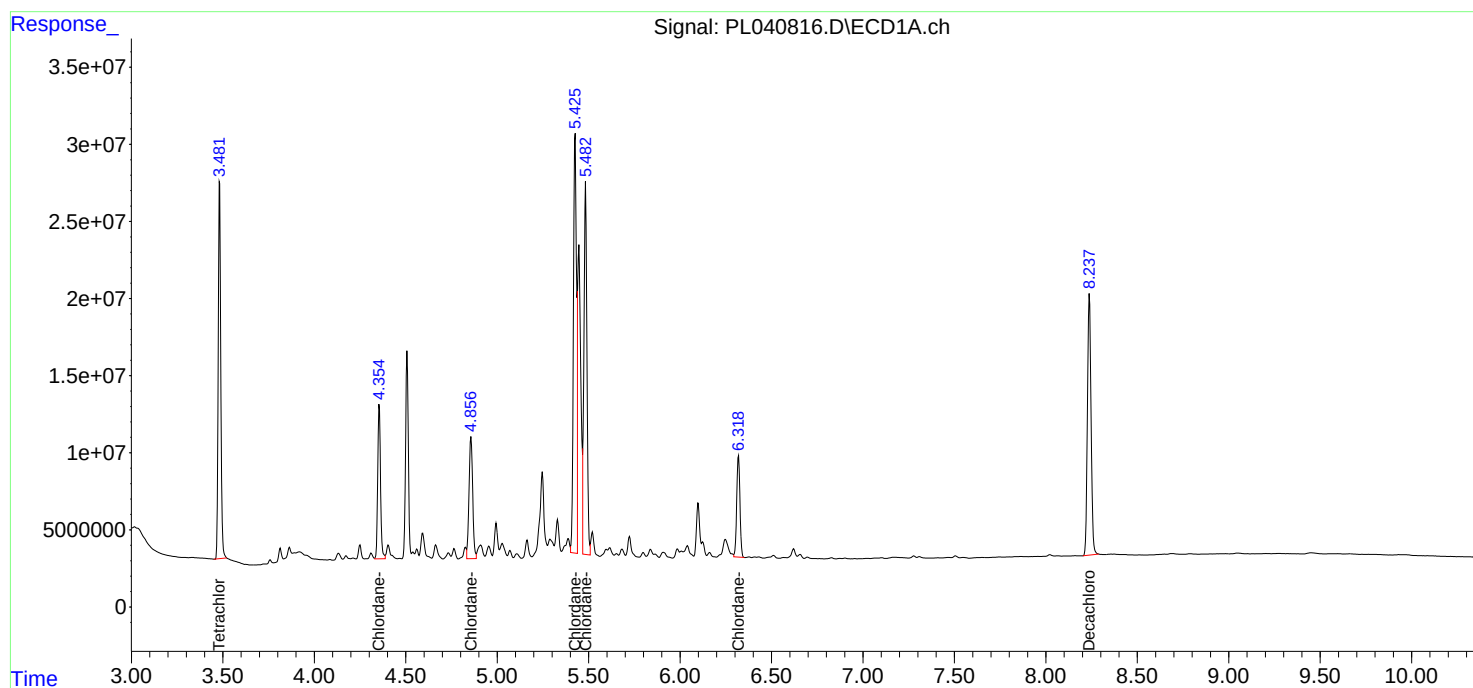


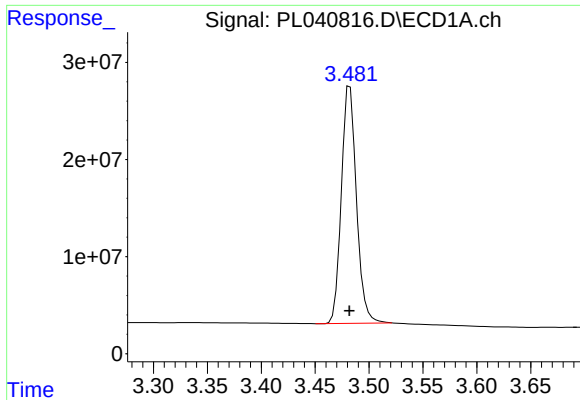

#1 Tetrachloro-m-xylene


R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 238158481
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

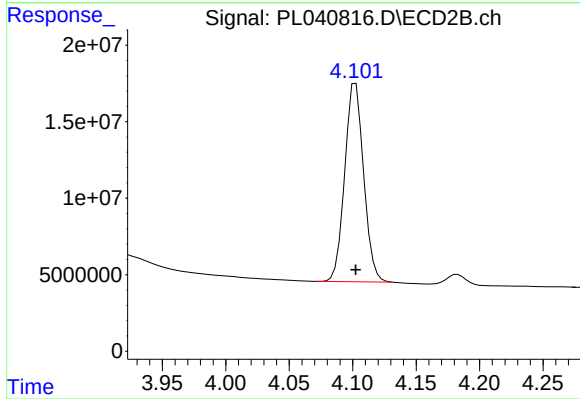


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 134234809
Conc: 50.00 ng/ml

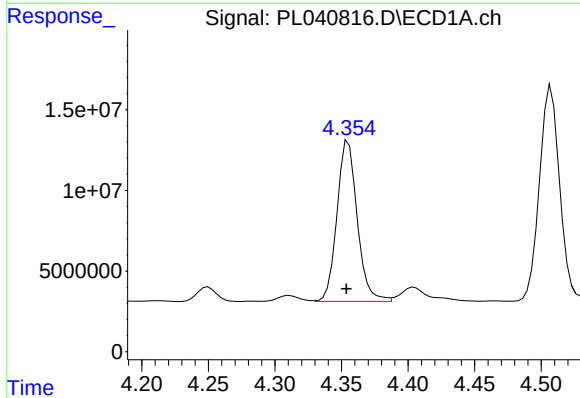


#23 Chlordane-1

R.T.: 4.355 min
Delta R.T.: 0.001 min
Response: 105451698
Conc: 522.67 ng/ml

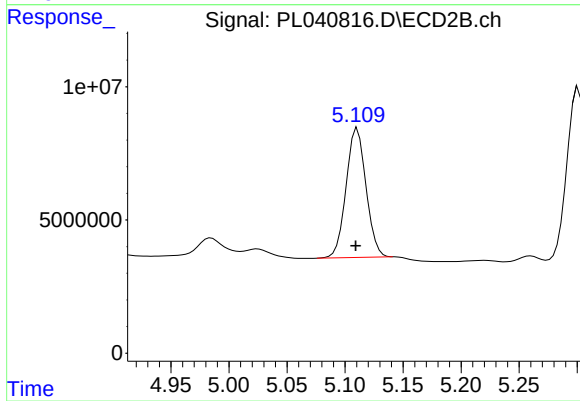

#23 Chlordane-1


R.T.: 5.111 min
Delta R.T.: 0.001 min
Response: 57974592
Conc: 489.86 ng/ml

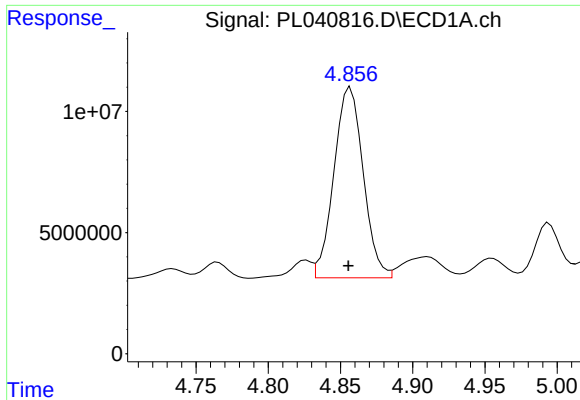

#24 Chlordane-2


R.T.: 4.857 min
Delta R.T.: 0.001 min
Response: 110960574
Conc: 541.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

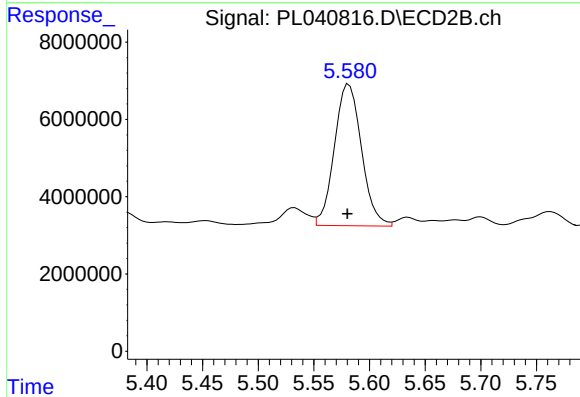


#24 Chlordane-2

R.T.: 5.582 min
Delta R.T.: 0.001 min
Response: 62042135
Conc: 510.22 ng/ml

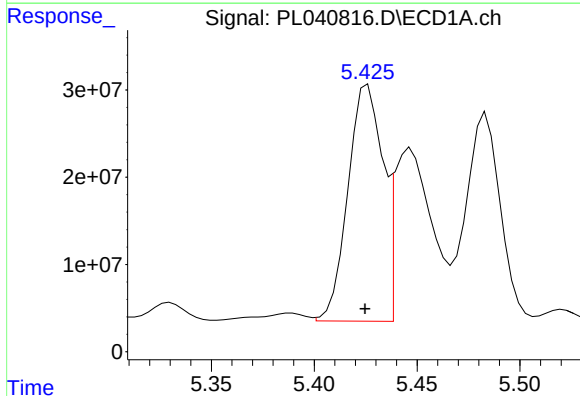


#25 Chlordane-3

R.T.: 5.426 min
Delta R.T.: 0.001 min
Response: 318414647
Conc: 457.83 ng/ml

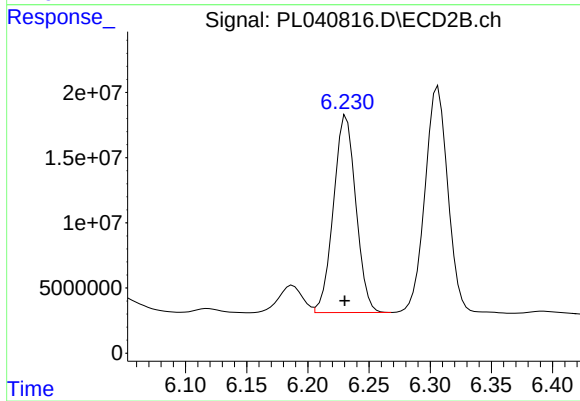

#25 Chlordane-3


R.T.: 6.231 min
Delta R.T.: 0.001 min
Response: 192355619
Conc: 496.24 ng/ml

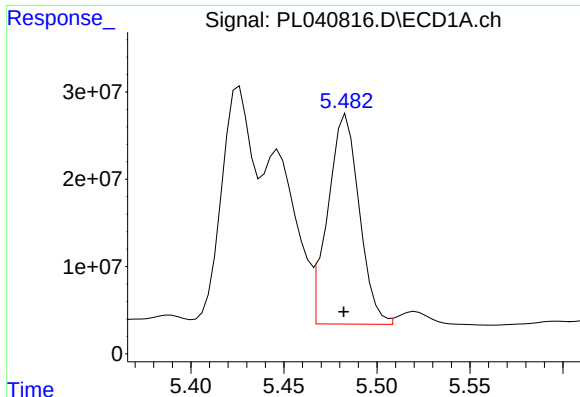

#26 Chlordane-4


R.T.: 5.484 min
Delta R.T.: 0.001 min
Response: 281777509
Conc: 494.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

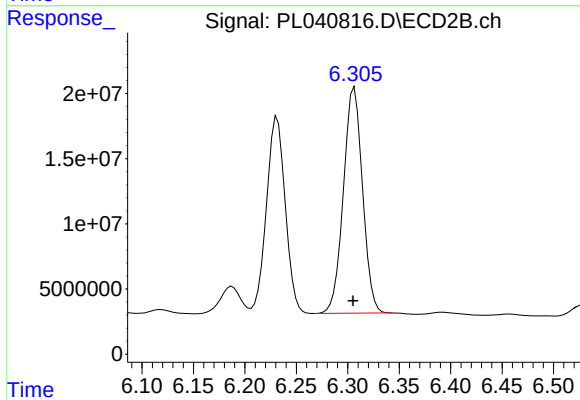


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: 0.001 min
Response: 223909263
Conc: 489.45 ng/ml

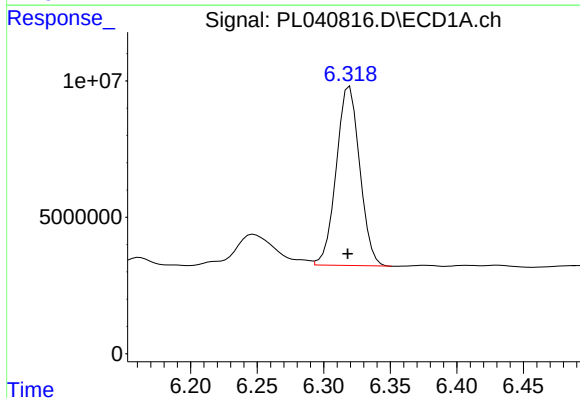


#27 Chlordane-5

R.T.: 6.319 min
Delta R.T.: 0.001 min
Response: 80483724
Conc: 485.55 ng/ml

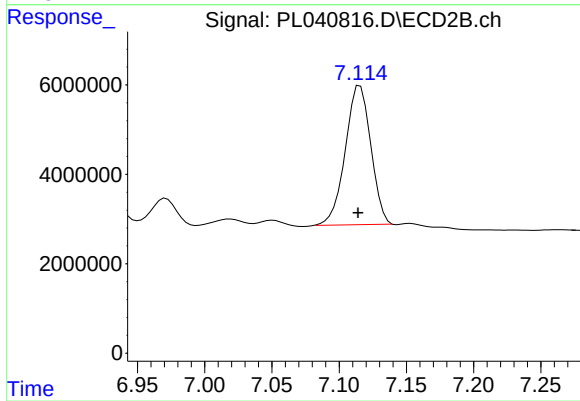

#27 Chlordane-5

R.T.: 7.116 min
Delta R.T.: 0.001 min
Response: 41051135
Conc: 480.72 ng/ml

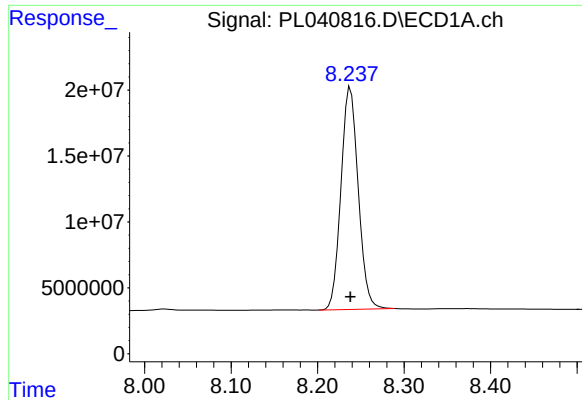

#28 Decachlorobiphenyl


R.T.: 8.238 min

Delta R.T.: 0.000 min

Response: 232768958

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

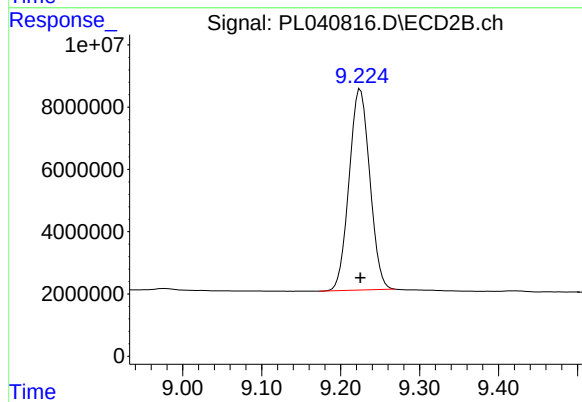

#28 Decachlorobiphenyl

R.T.: 9.225 min

Delta R.T.: 0.000 min

Response: 117695053

Conc: 50.00 ng/ml