

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
 Data File : PL040818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 23:48
 Operator : AJ\SJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Manual Integrations
 APPROVED

Sohil
 10/10/2018 3:47:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:15:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 10 01:12:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.482	4.102	24142982	13829664	5.099	5.169
28)	SA Decachlor...	8.237	9.226	26503694	13372935	5.599	5.560
Target Compounds							
23)	Chlordane-1	4.354	5.111	10557802	5540352	50.348	48.543
24)	Chlordane-2	4.855	5.581	12346197	6480996	54.587m	52.726
25)	Chlordane-3	5.425	6.231	30040708	19650199	47.623	50.833
26)	Chlordane-4	5.482	6.306	26750021	23402429	48.150	51.647
27)	Chlordane-5	6.318	7.116	8619549	4367609	52.892	52.540

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100918\
Data File : PL040818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 23:48
Operator : AJ\SJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
10/10/2018 3:47:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:15:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
Quant Title : GC Extractables
QLast Update : Wed Oct 10 01:12:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

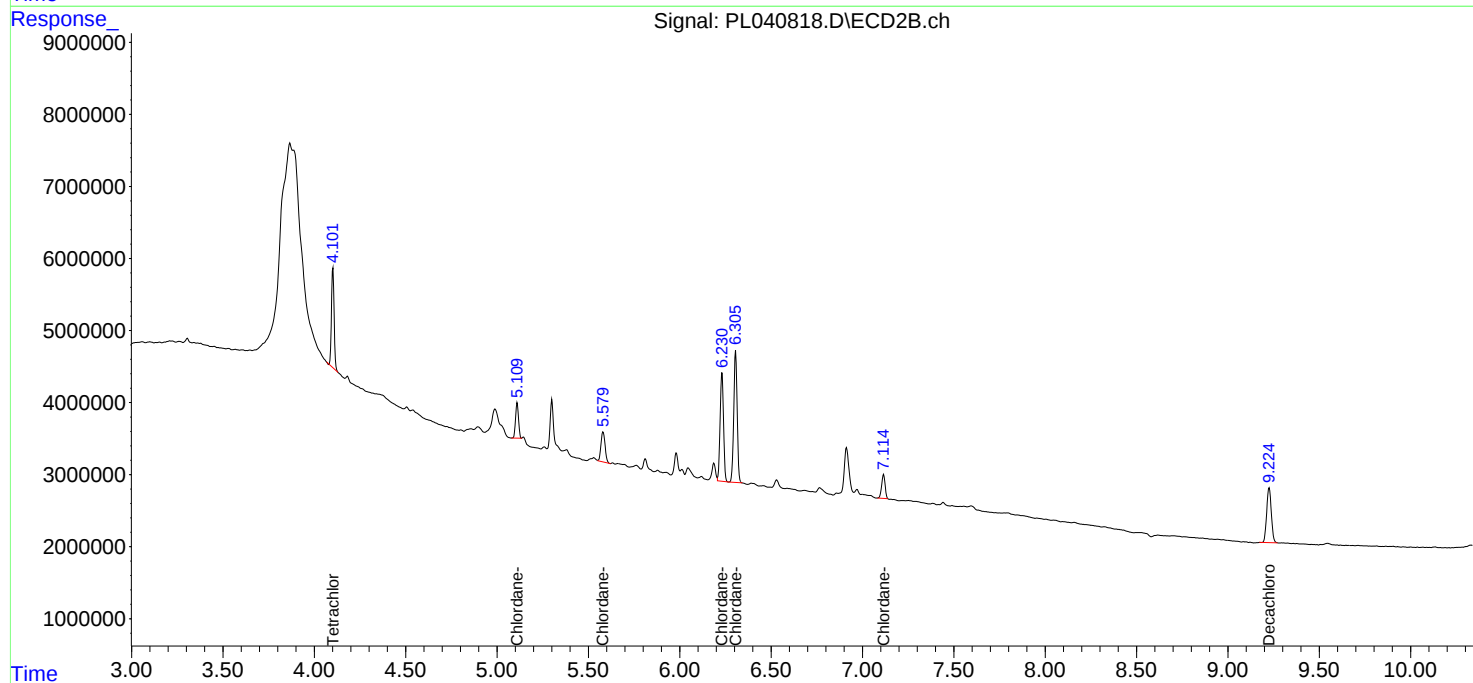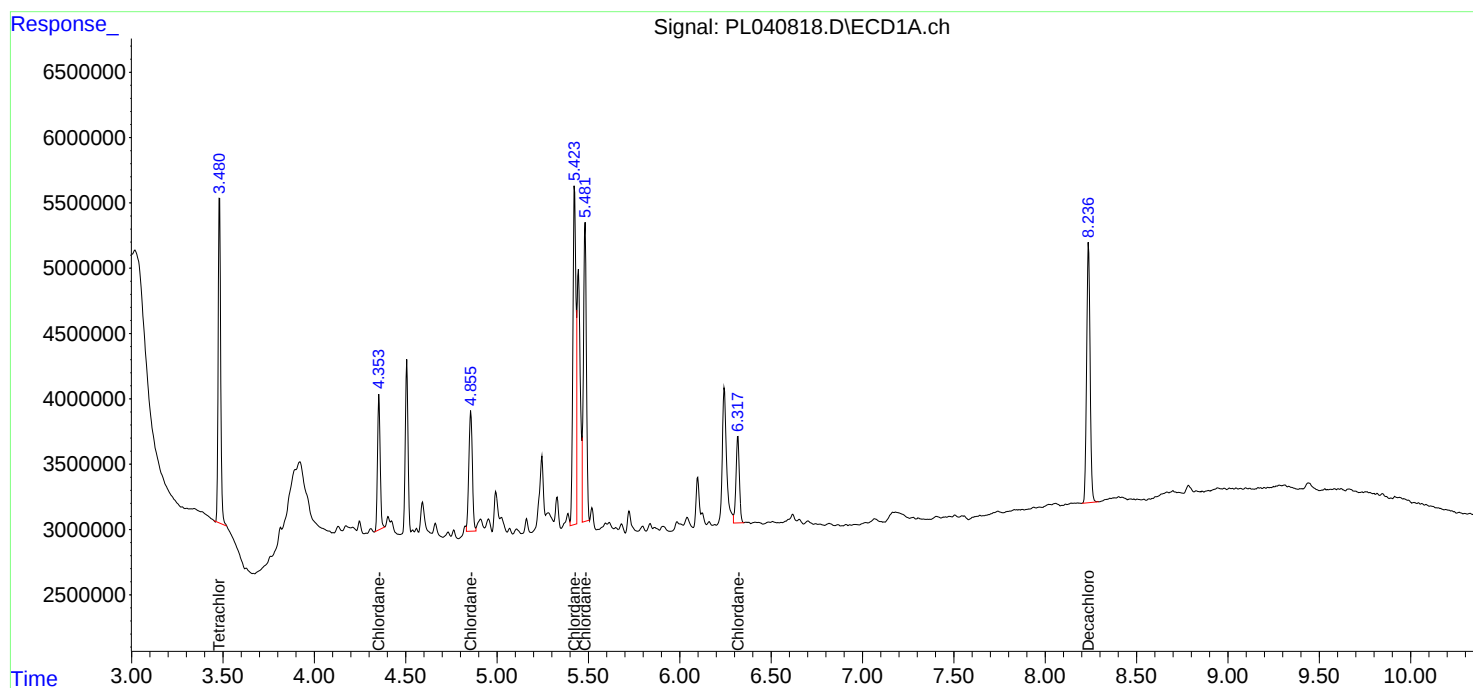

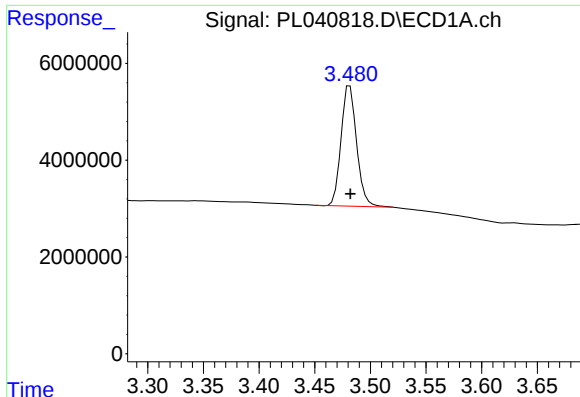


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 24142982
Conc: 5.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
10/10/2018 3:47:41 PM

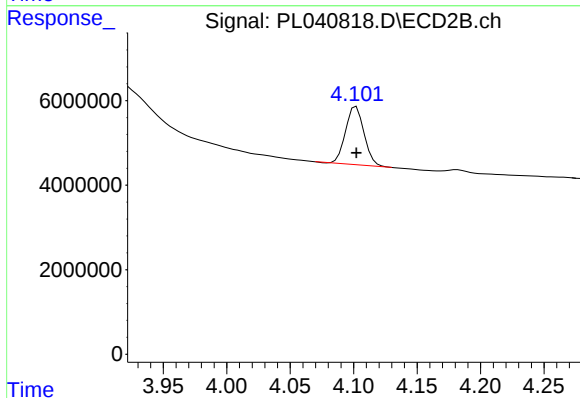


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 13829664
Conc: 5.17 ng/ml

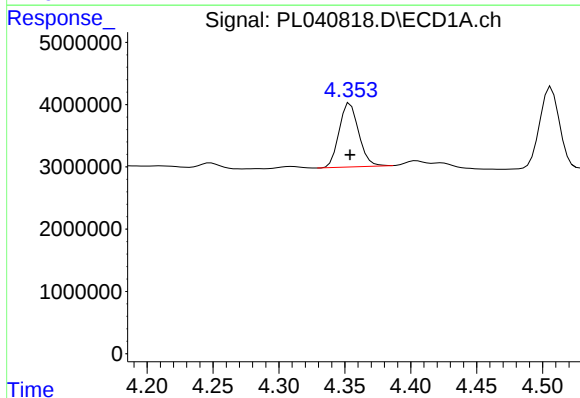


#23 Chlordane-1

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 10557802
Conc: 50.35 ng/ml

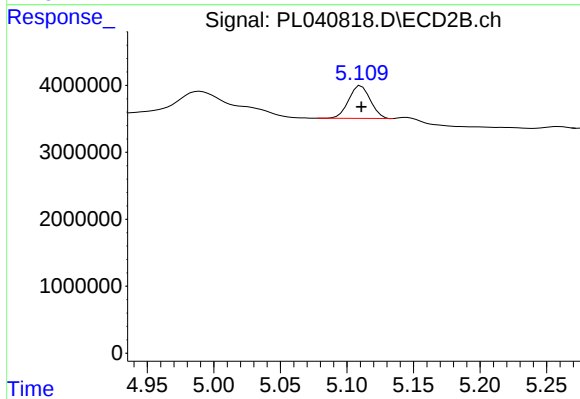

#23 Chlordane-1

R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 5540352
Conc: 48.54 ng/ml

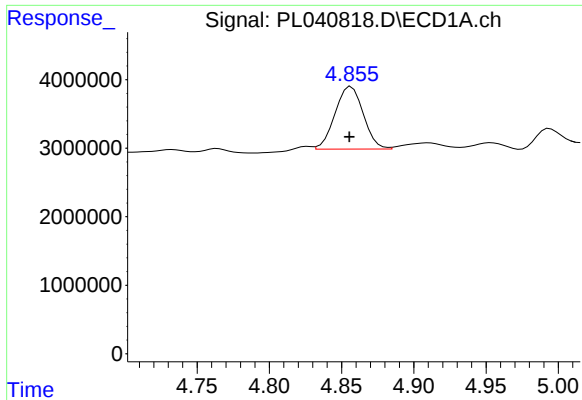


#24 Chlordane-2

R.T.: 4.855 min
Delta R.T.: 0.000 min
Response: 12346197
Conc: 54.59 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
10/10/2018 3:47:41 PM

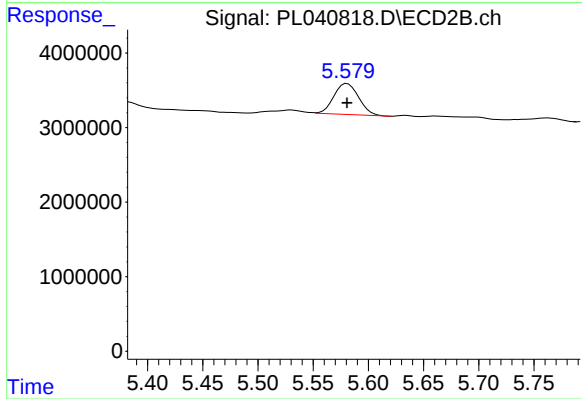


#24 Chlordane-2

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 6480996
Conc: 52.73 ng/ml

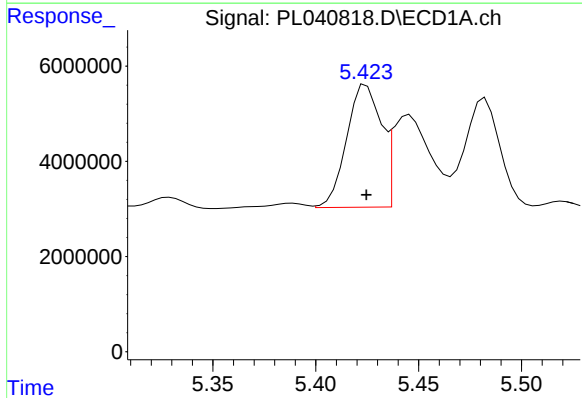


#25 Chlordane-3

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 30040708
Conc: 47.62 ng/ml

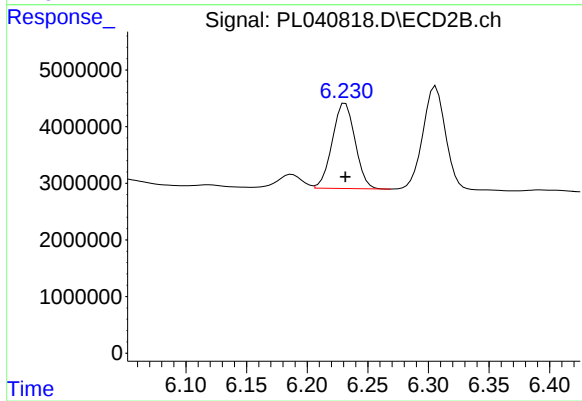

#25 Chlordane-3

R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 19650199
Conc: 50.83 ng/ml

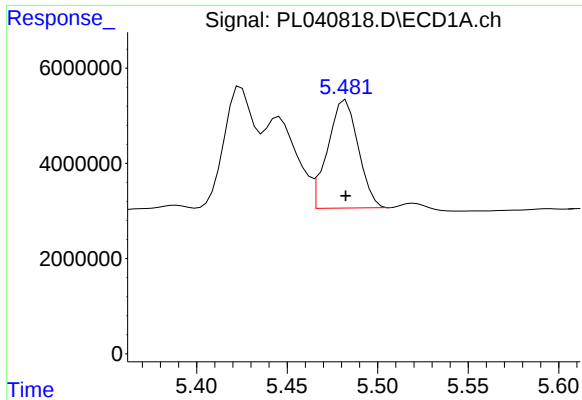


#26 Chlordane-4

R.T.: 5.482 min
Delta R.T.: 0.000 min
Response: 26750021
Conc: 48.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
10/10/2018 3:47:41 PM

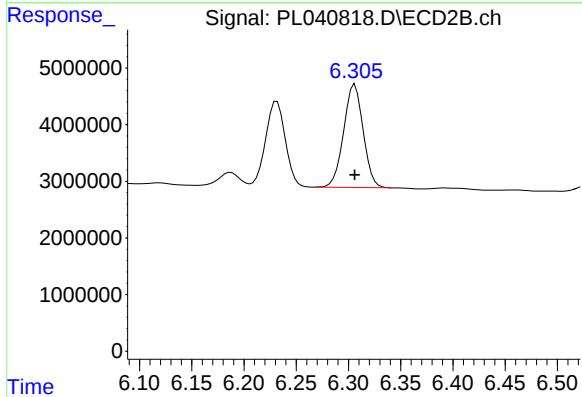


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: 0.000 min
Response: 23402429
Conc: 51.65 ng/ml

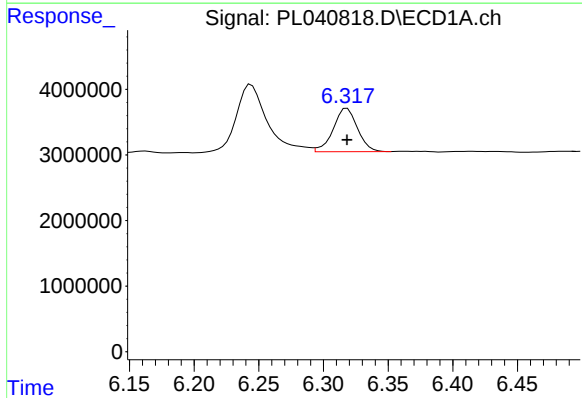


#27 Chlordane-5

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 8619549
Conc: 52.89 ng/ml

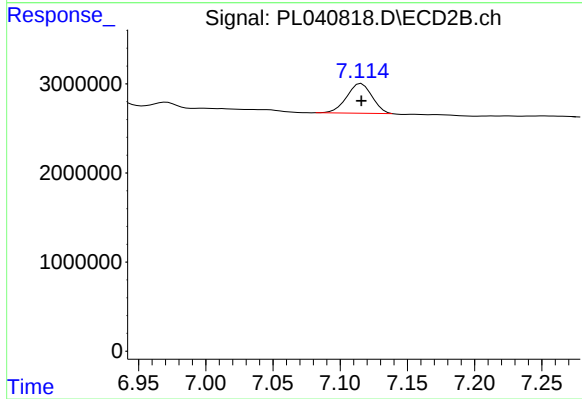

#27 Chlordane-5

R.T.: 7.116 min
Delta R.T.: 0.000 min
Response: 4367609
Conc: 52.54 ng/ml

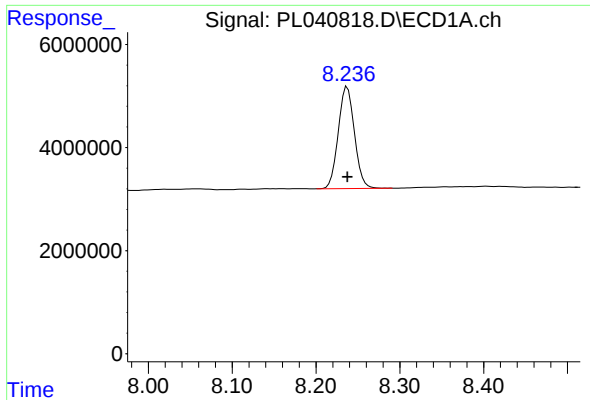


#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 26503694
Conc: 5.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Manual Integrations
APPROVED

Sohil
10/10/2018 3:47:41 PM

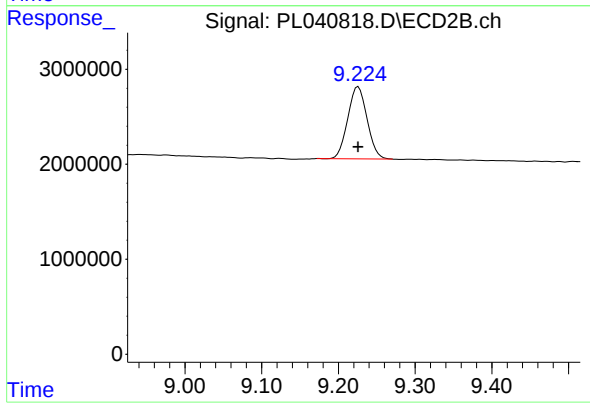

#28 Decachlorobiphenyl

R.T.: 9.226 min
Delta R.T.: 0.000 min
Response: 13372935
Conc: 5.56 ng/ml