

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100919\
 Data File : PL053180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2019 14:41
 Operator : SG\AJ
 Sample : K5281-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-062

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:08:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 00:43:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	4.048	115.7E6	28716403	11.634	10.694
28)	SA Decachlor...	8.343	9.129	92404677	25019478	9.226	8.528
Target Compounds							
10)	B gamma-Chl...	5.524	6.160	5554775	2859752	0.413m	0.845m#
11)	B alpha-Chl...	5.578	6.236	13088574	7676683	0.992	2.281 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100919\
Data File : PL053180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2019 14:41
Operator : SG\AJ
Sample : K5281-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-PS-01-062


Manual Integrations
APPROVED

Ankita
10/11/2019 2:08:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 00:43:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

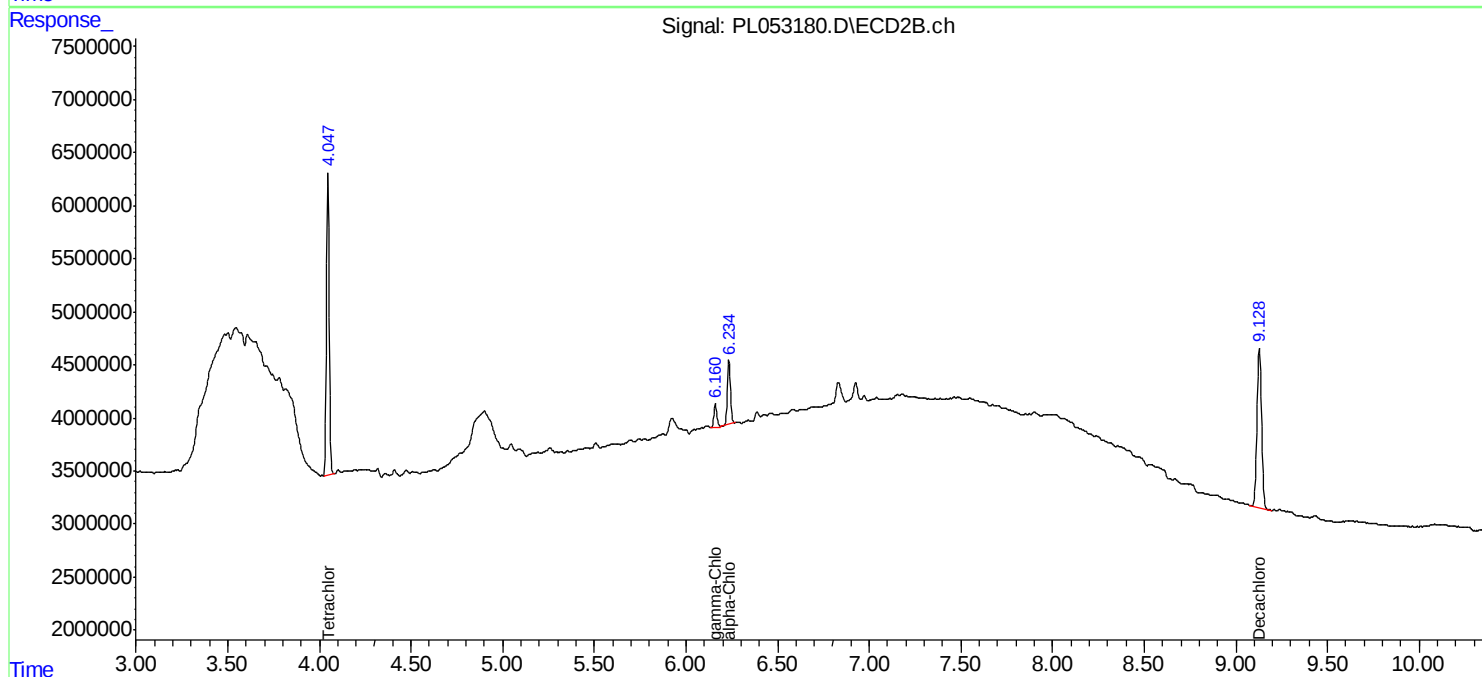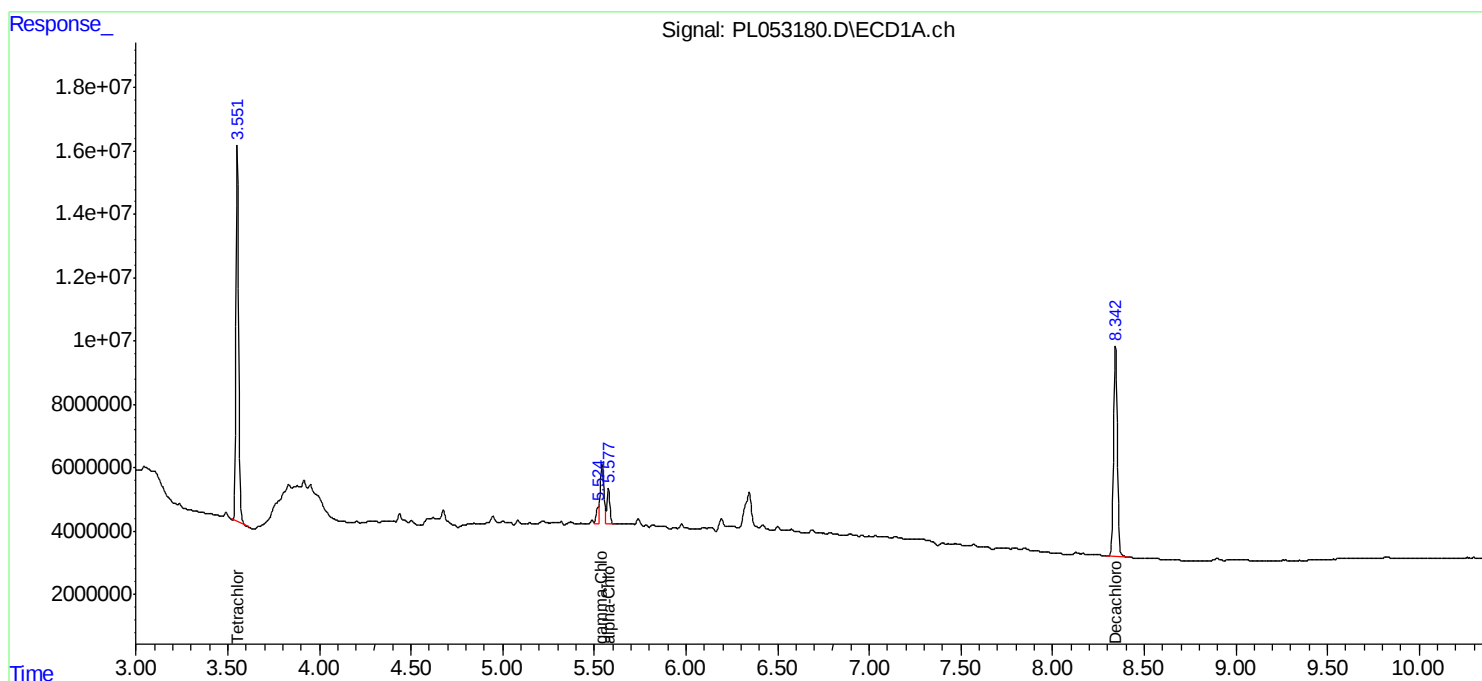

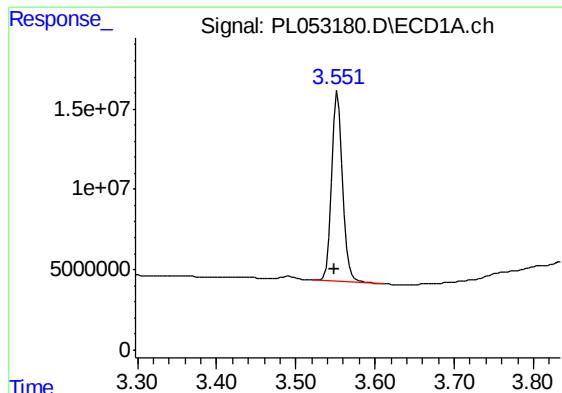


#1 Tetrachloro-m-xylene

R.T.: 3.553 min
Delta R.T.: 0.004 min
Response: 115724176
Conc: 11.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-062


Manual Integrations
APPROVED

Ankita
10/11/2019 2:08:23 PM

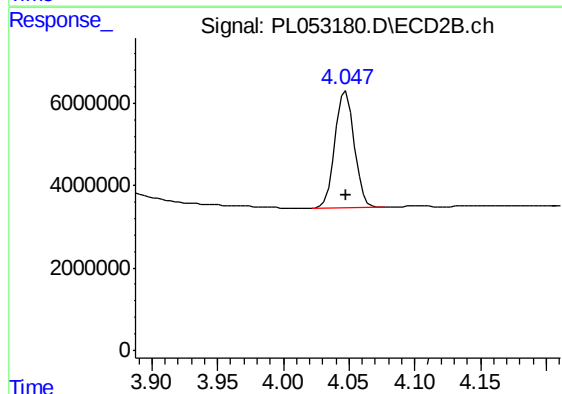


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 28716403
Conc: 10.69 ng/ml

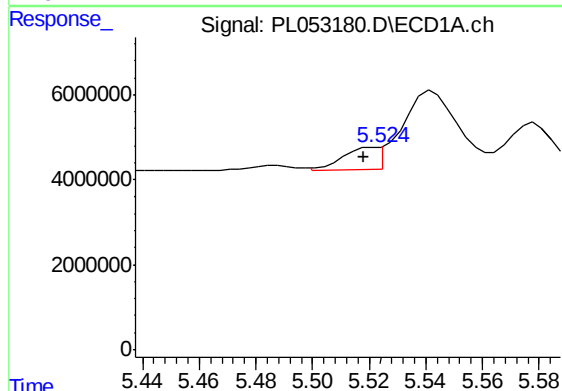


#10 gamma-Chlordane

R.T.: 5.524 min
Delta R.T.: 0.006 min
Response: 5554775
Conc: 0.41 ng/ml m

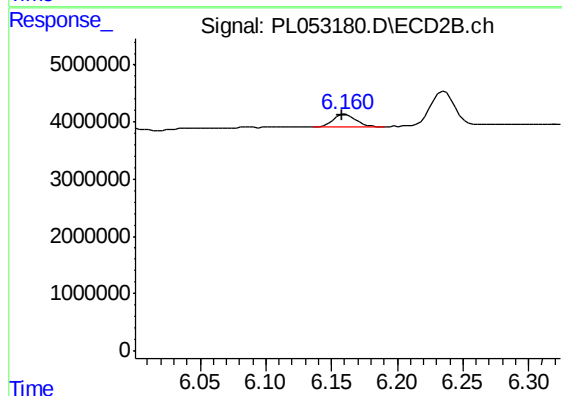

#10 gamma-Chlordane

R.T.: 6.160 min
Delta R.T.: 0.001 min
Response: 2859752
Conc: 0.85 ng/ml m

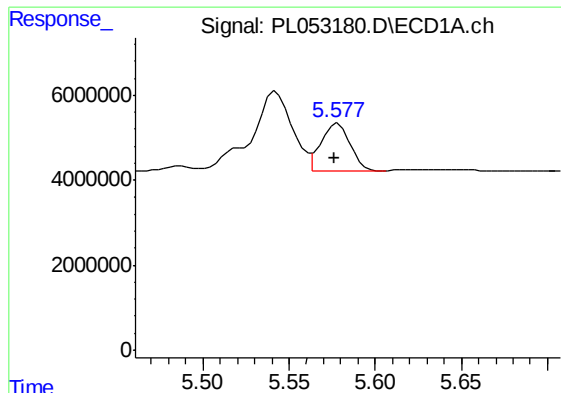


#11 alpha-Chlordane

R.T.: 5.578 min
Delta R.T.: 0.002 min
Response: 13088574
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-062


Manual Integrations
APPROVED

Ankita
10/11/2019 2:08:23 PM

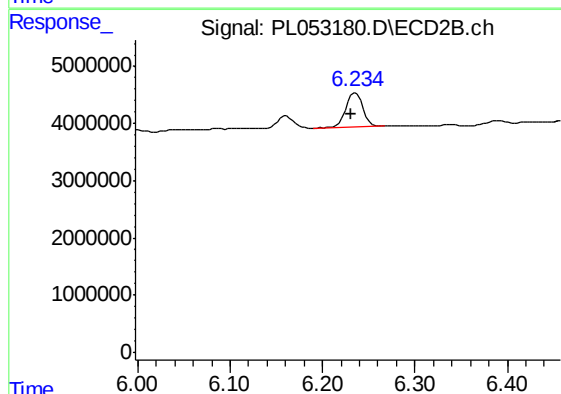


#11 alpha-Chlordane

R.T.: 6.236 min
Delta R.T.: 0.005 min
Response: 7676683
Conc: 2.28 ng/ml

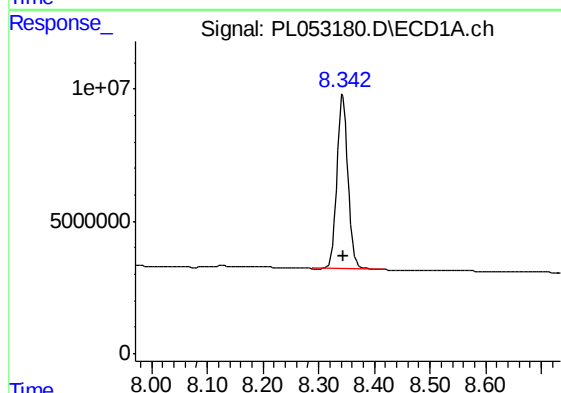

#28 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.002 min
Response: 92404677
Conc: 9.23 ng/ml

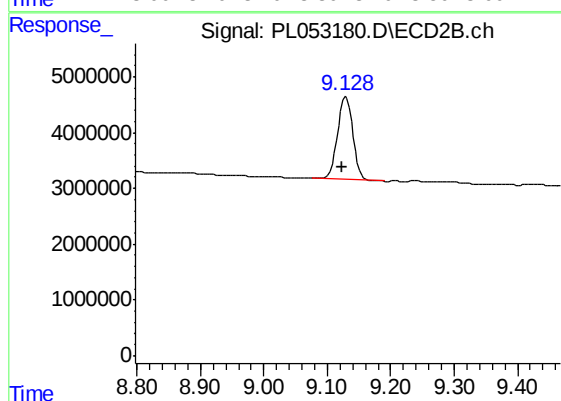

#28 Decachlorobiphenyl

R.T.: 9.129 min
Delta R.T.: 0.005 min
Response: 25019478
Conc: 8.53 ng/ml