

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100920\
 Data File : PL062140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2020 22:44
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 05:12:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 10 05:11:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.952	138.0E6	226.2E6	77.844	79.528
27)	SA Decachlor...	8.126	8.990	283.2E6	406.5E6	149.056	145.094
Target Compounds							
2)	A alpha-BHC	3.845	4.338	200.2E6	341.4E6	83.676	85.352
3)	MA gamma-BHC...	4.124	4.622	179.6E6	311.0E6	81.970	83.995
4)	MA Heptachlor	4.421	5.127	161.3E6	293.5E6	81.029	80.592
9)	A Endosulfan I	5.439	6.171	127.7E6	230.1E6	79.110	80.273
13)	MA Dieldrin	5.680	6.427	293.5E6	509.7E6	165.756	167.312
14)	MA Endrin	5.934	6.644	259.5E6	414.6E6	164.298	170.109
16)	A 4,4'-DDD	6.063	6.769	233.1E6	390.9E6	168.699	168.091
17)	MA 4,4'-DDT	6.302	7.068	236.7E6	393.6E6	177.807	172.005
20)	A Methoxychlor	6.845	7.527	629.0E6	1031.4E6	753.119	767.866


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100920\
Data File : PL062140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2020 22:44
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 05:12:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 10 05:11:25 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

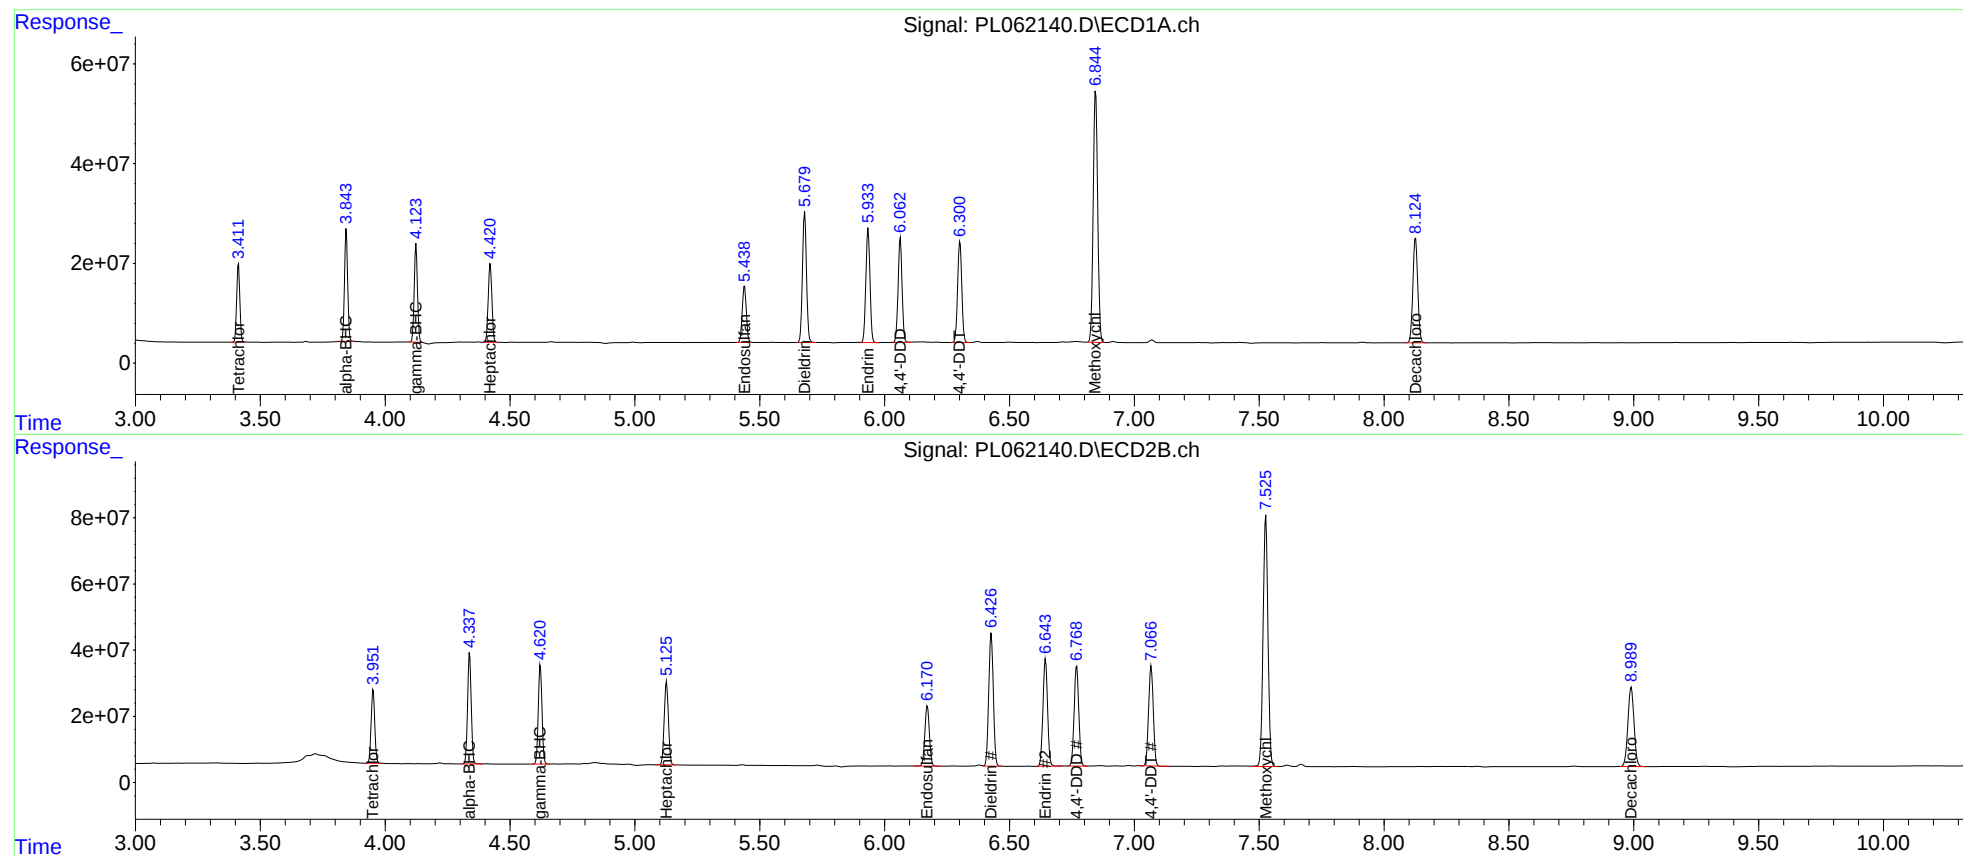

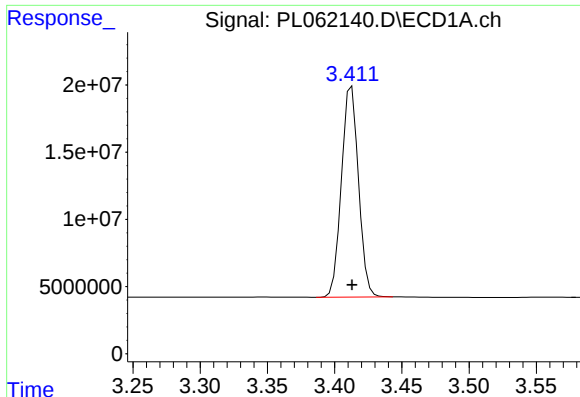


#1 Tetrachloro-m-xylene

R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 138047219
Conc: 77.84 ng/ml

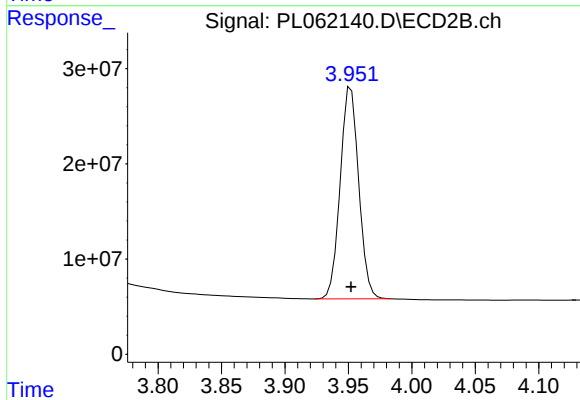


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 226204424
Conc: 79.53 ng/ml

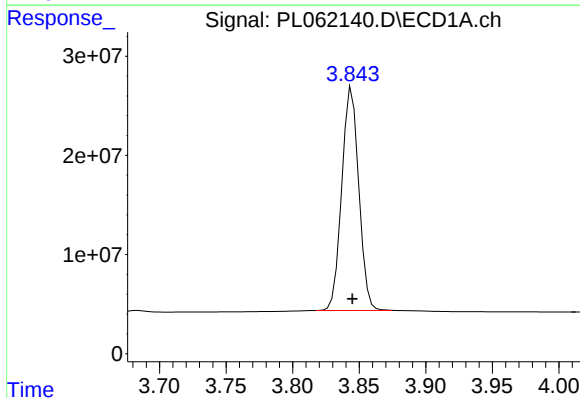


#2 alpha-BHC

R.T.: 3.845 min
Delta R.T.: 0.000 min
Response: 200243619
Conc: 83.68 ng/ml

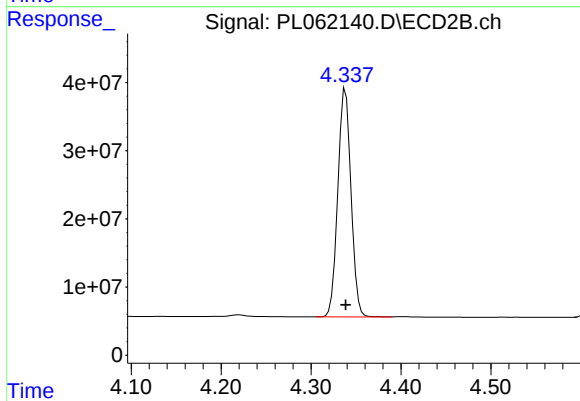


#2 alpha-BHC

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 341427477
Conc: 85.35 ng/ml

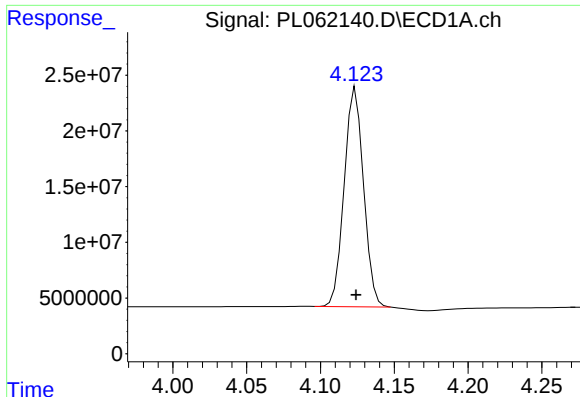


#3 gamma-BHC (Lindane)

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 179568335
Conc: 81.97 ng/ml

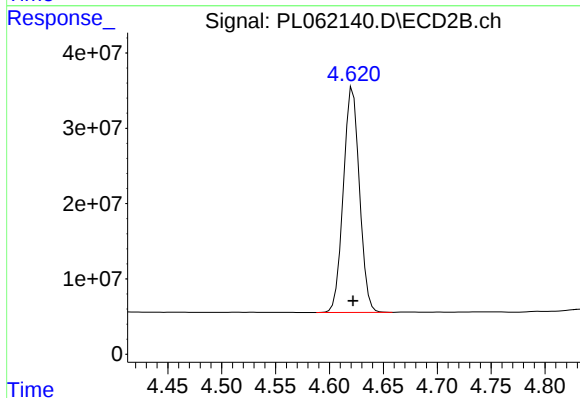


#3 gamma-BHC (Lindane)

R.T.: 4.622 min
Delta R.T.: 0.000 min
Response: 311006346
Conc: 84.00 ng/ml

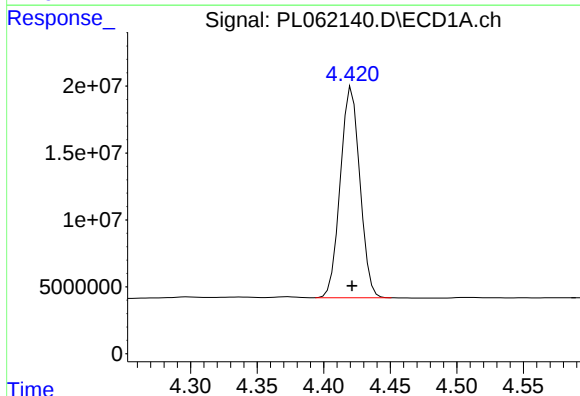


#4 Heptachlor

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 161312487
Conc: 81.03 ng/ml

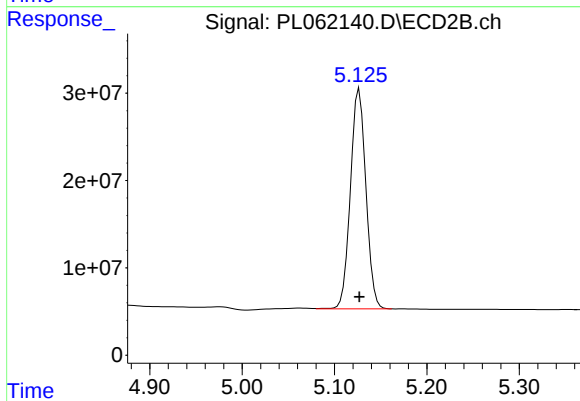


#4 Heptachlor

R.T.: 5.127 min
Delta R.T.: 0.000 min
Response: 293538466
Conc: 80.59 ng/ml

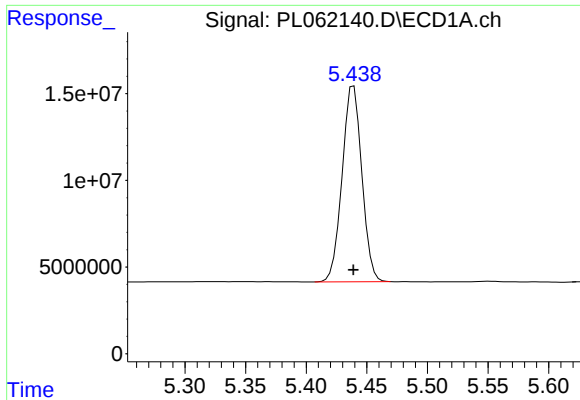


#9 Endosulfan I

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 127716303
Conc: 79.11 ng/ml

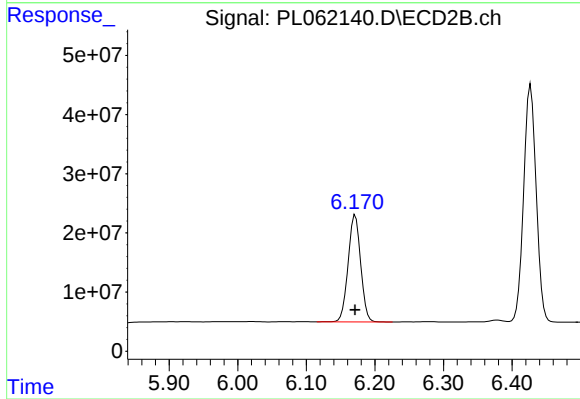


#9 Endosulfan I

R.T.: 6.171 min
Delta R.T.: 0.000 min
Response: 230108996
Conc: 80.27 ng/ml

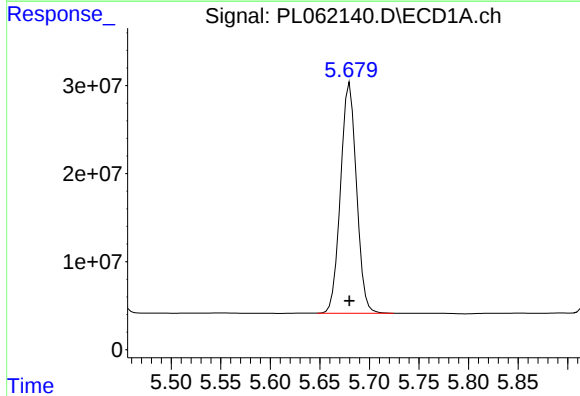


#13 Dieldrin

R.T.: 5.680 min
Delta R.T.: 0.000 min
Response: 293540223
Conc: 165.76 ng/ml

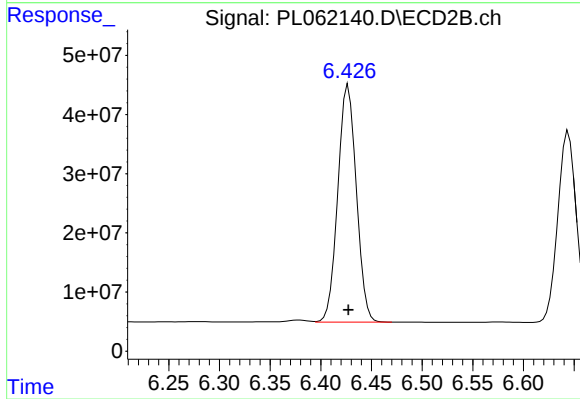


#13 Dieldrin

R.T.: 6.427 min
Delta R.T.: 0.000 min
Response: 509723324
Conc: 167.31 ng/ml

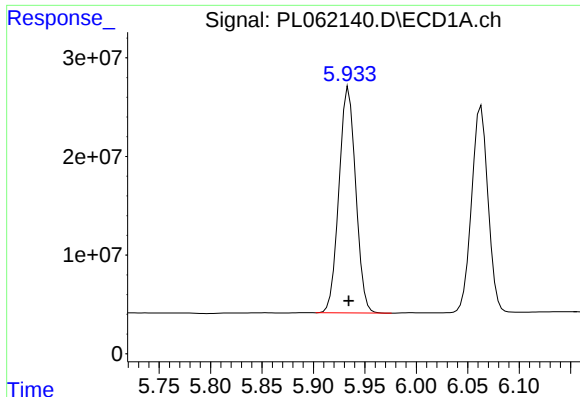


#14 Endrin

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 259478645
Conc: 164.30 ng/ml

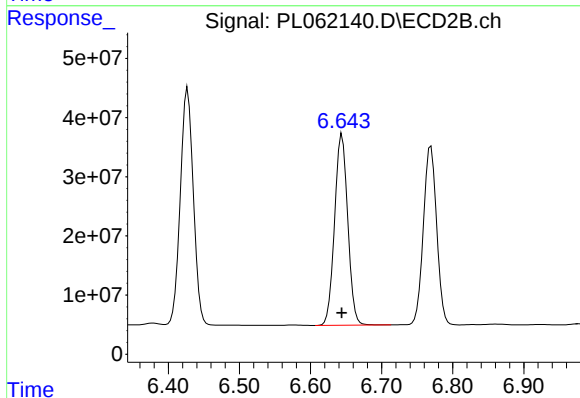


#14 Endrin

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 414605617
Conc: 170.11 ng/ml

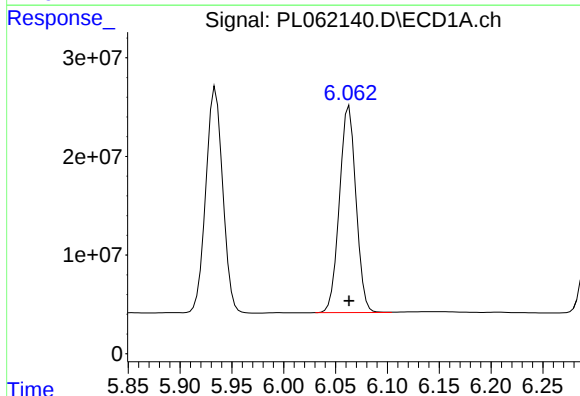


#16 4,4'-DDD

R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 233115798
Conc: 168.70 ng/ml

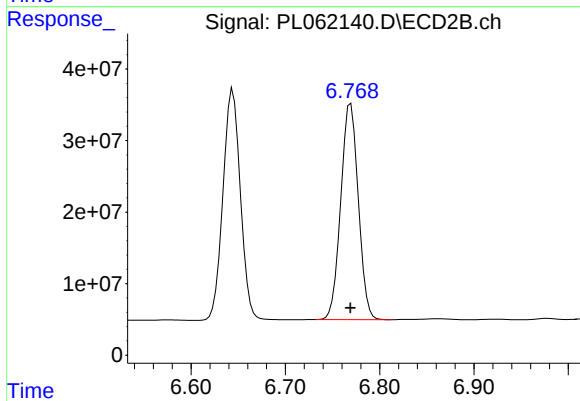


#16 4,4'-DDD

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 390926744
Conc: 168.09 ng/ml

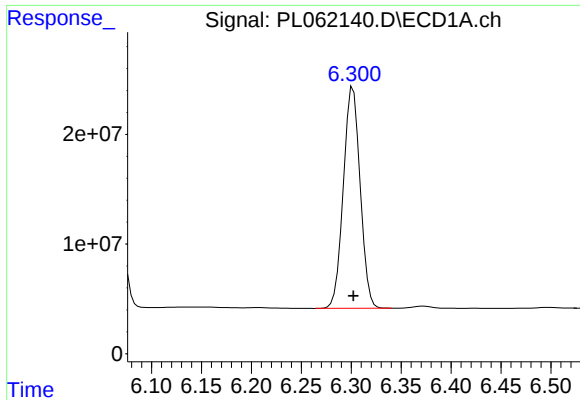


#17 4,4'-DDT

R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 236740465
Conc: 177.81 ng/ml

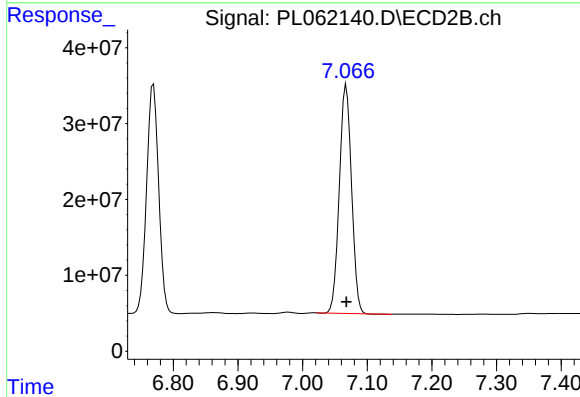


#17 4,4'-DDT

R.T.: 7.068 min
Delta R.T.: 0.000 min
Response: 393581717
Conc: 172.00 ng/ml

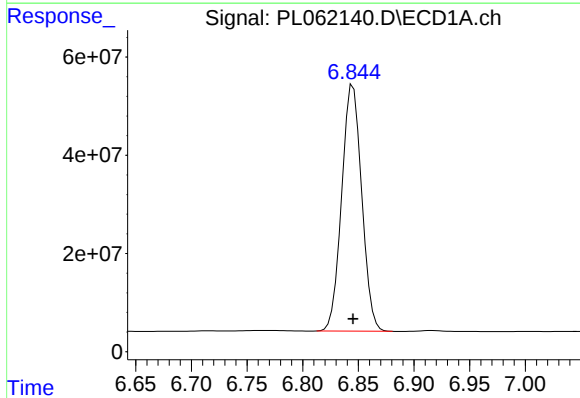


#20 Methoxychlor

R.T.: 6.845 min
Delta R.T.: 0.000 min
Response: 628953386
Conc: 753.12 ng/ml

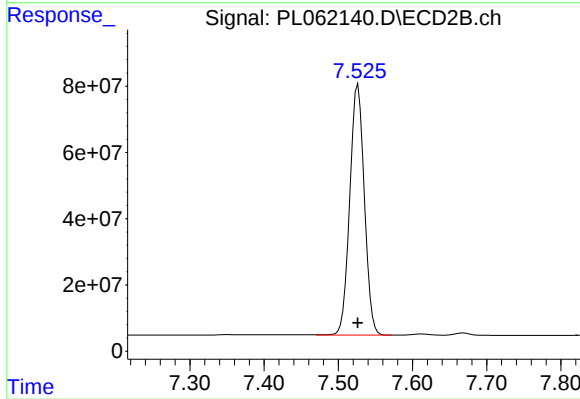


#20 Methoxychlor

R.T.: 7.527 min
Delta R.T.: 0.000 min
Response: 1031409422
Conc: 767.87 ng/ml

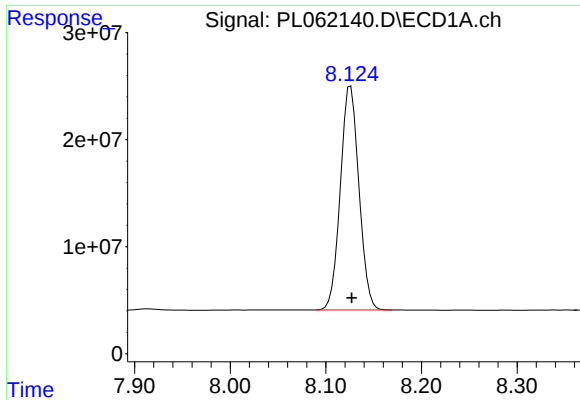

#27 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: -0.001 min
Response: 283244417
Conc: 149.06 ng/ml

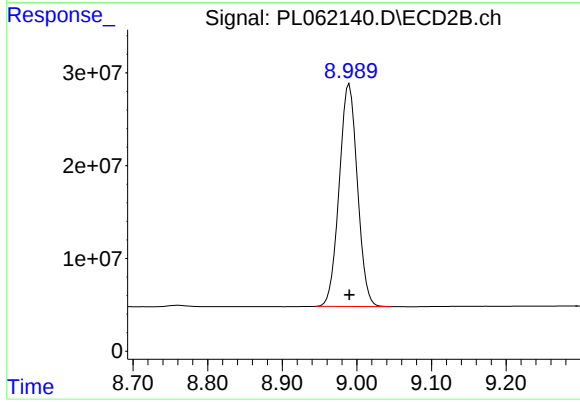

#27 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 406530978
Conc: 145.09 ng/ml