

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100923\
Data File : PL085773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 14:15
Operator : AR\AJ
Sample : 04804-01 (Sig #1); 04801-04 (Sig #2)
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-02-100623

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 03:15:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	2.622	26831736	8928501	9.022	9.558
28)	SA Decachlor...	8.862	7.777	25142032	9214626	11.543	9.984

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100923\
Data File : PL085773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 14:15
Operator : AR\AJ
Sample : 04804-01 (Sig #1); 04801-04 (Sig #2)
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-02-100623

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 03:15:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

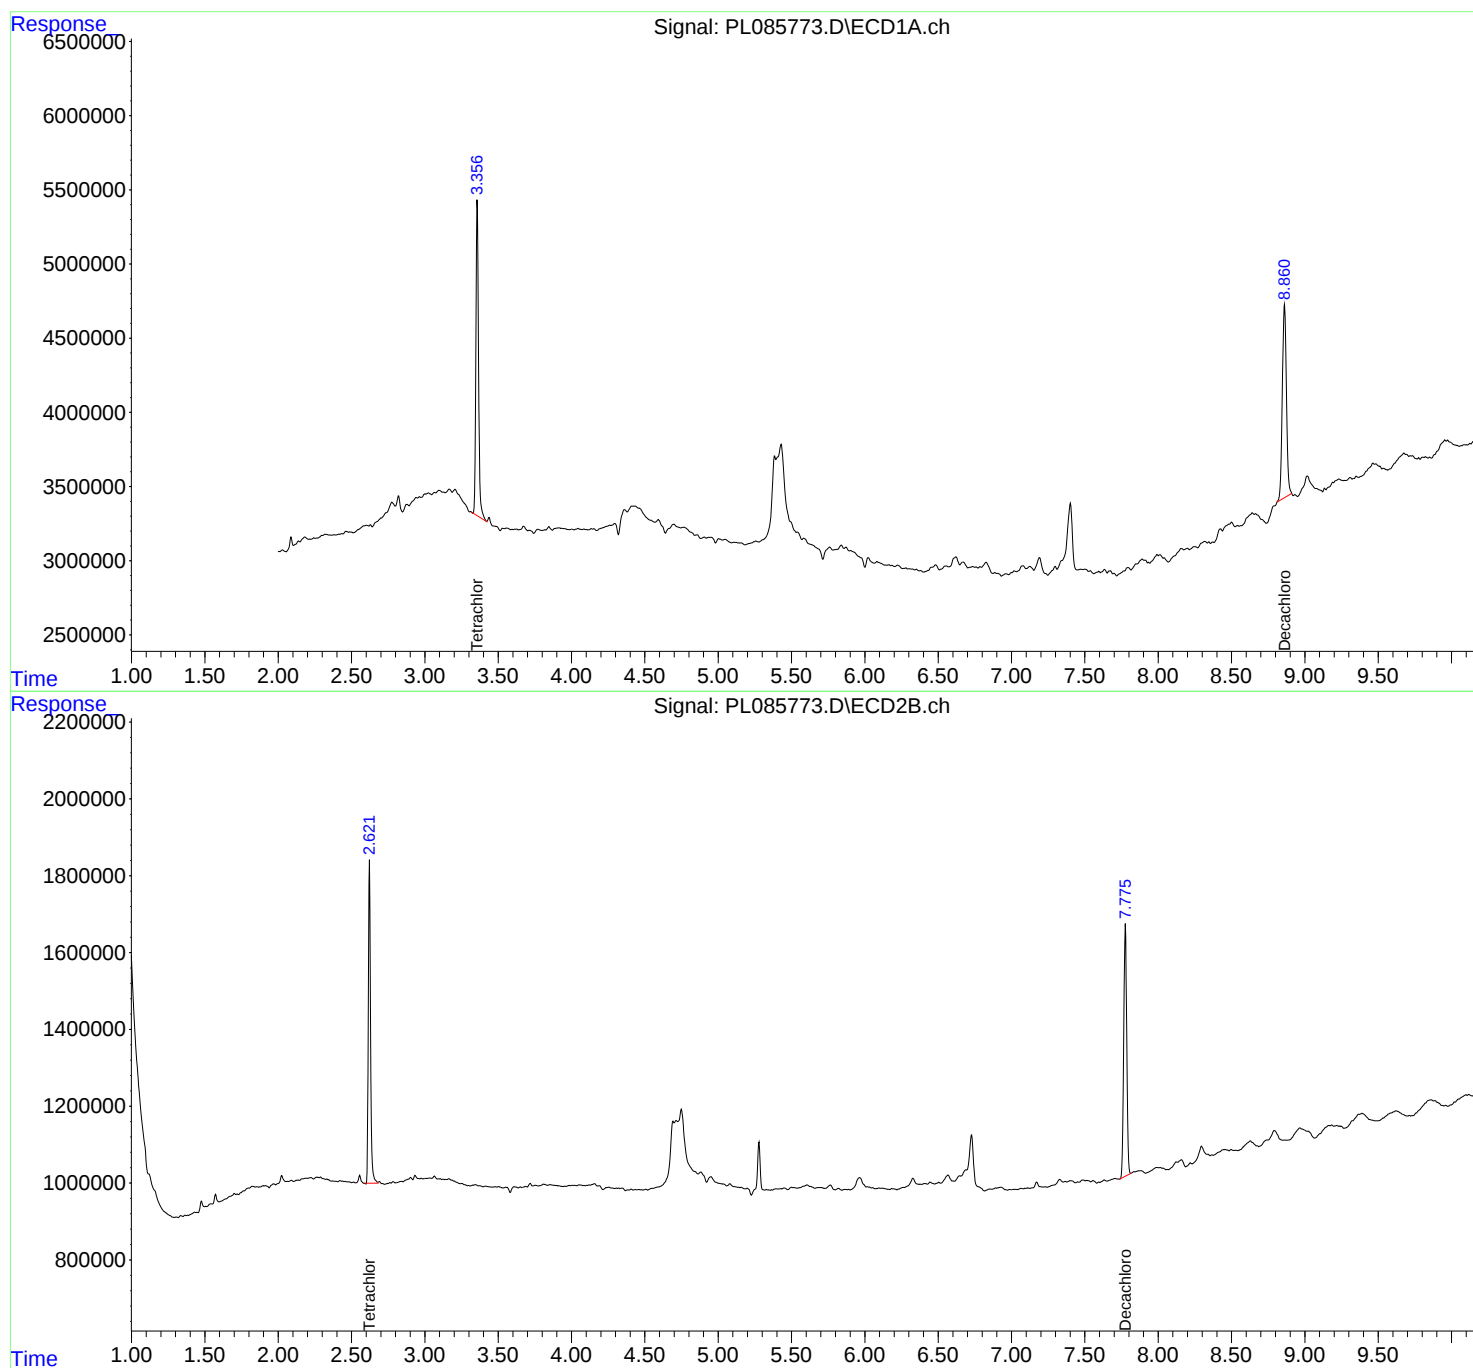


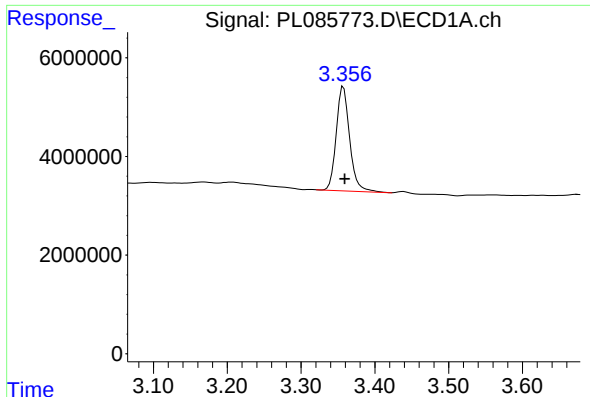

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.002 min
Response: 26831736
Conc: 9.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-100623

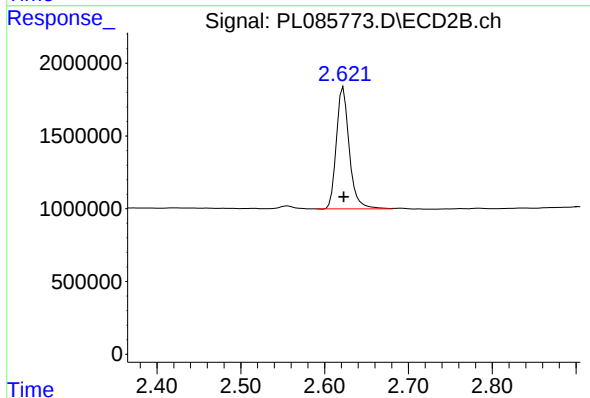


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 8928501
Conc: 9.56 ng/ml

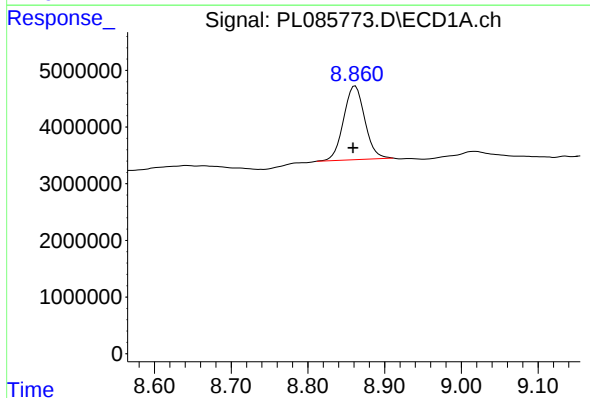

#28 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.003 min
Response: 25142032
Conc: 11.54 ng/ml

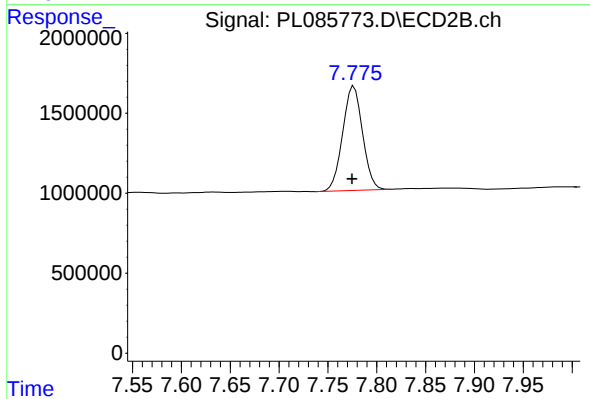

#28 Decachlorobiphenyl

R.T.: 7.777 min
Delta R.T.: 0.002 min
Response: 9214626
Conc: 9.98 ng/ml