

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101018\
 Data File : PL040865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 12:39
 Operator : AJ\SJ
 Sample : J5287-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:46:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 10 02:11:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.480	4.103	51475787	27647218	11.189	10.471
28)	SA Decachlor...	8.234	9.229	61931668	31294670	13.400	13.177
Target Compounds							
6)	B beta-BHC	4.422f	4.994f	3116138	5996466	1.198	3.786 #
10)	B gamma-Chl...	5.442	0.000	975694	0	0.180	N.D. #
11)	B alpha-Chl...	5.442f	0.000	975694	0	0.183	N.D. #
12)	B 4,4'-DDE	5.646	6.460	2832560	1393946	0.605	0.549
16)	A 4,4'-DDD	0.000	6.912f	0	6517728	N.D.	3.155 #
17)	MA 4,4'-DDT	6.397	0.000	2664532	0	0.934	N.D. #
23)	Chlordane-1	4.422	0.000	3116138	0	14.860	N.D. #
24)	Chlordane-2	4.856	0.000	1518726	0	6.731	N.D. #
25)	Chlordane-3	5.442	0.000	975694	0	1.547	N.D. #
26)	Chlordane-4	5.442	0.000	975694	0	1.756	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101018\
Data File : PL040865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 12:39
Operator : AJ\SJ
Sample : J5287-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:46:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100918.M
Quant Title : GC Extractables
QLast Update : Wed Oct 10 02:11:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

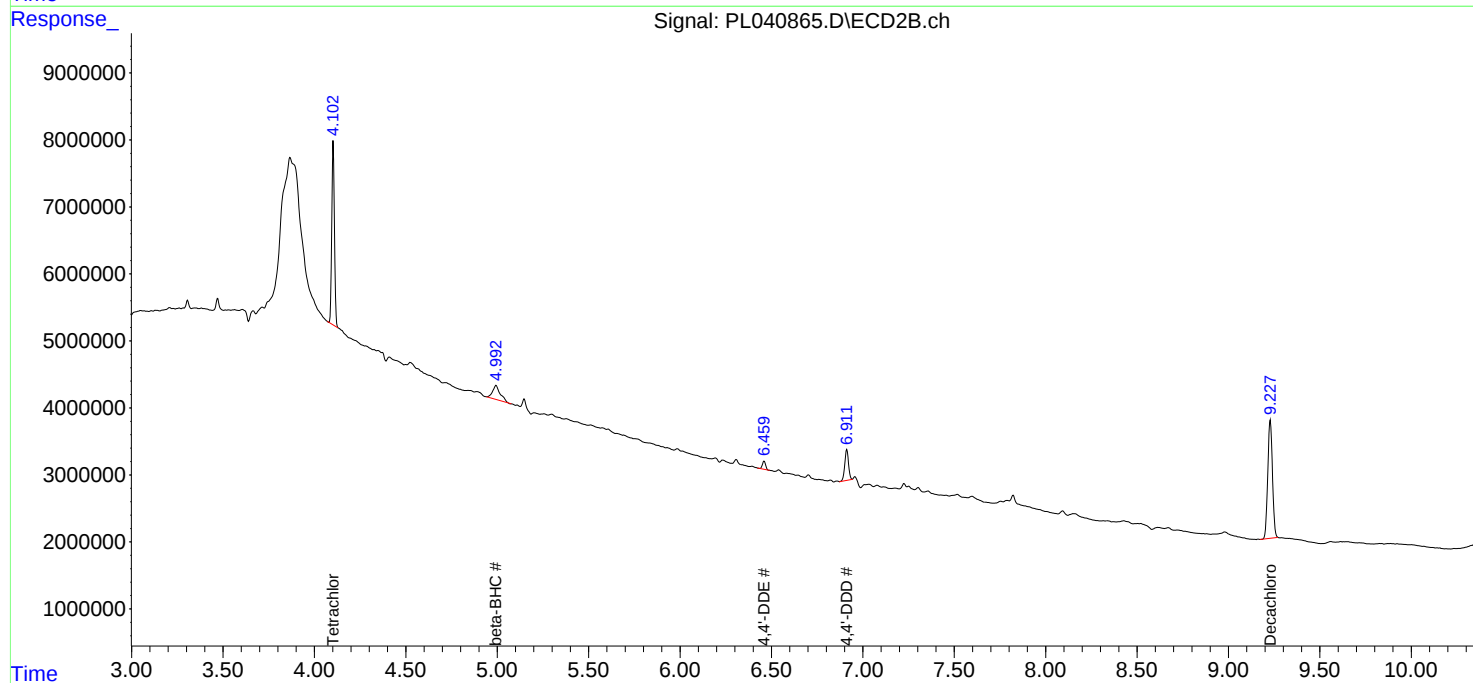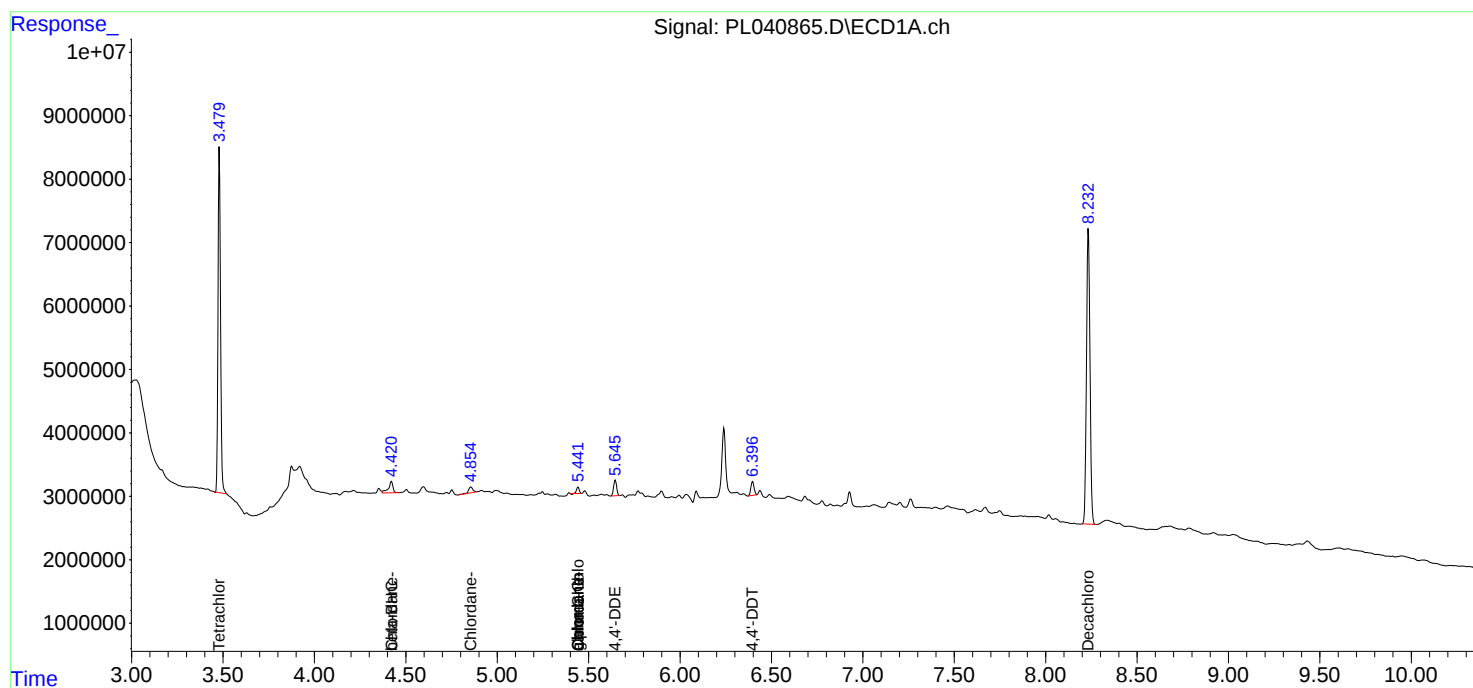


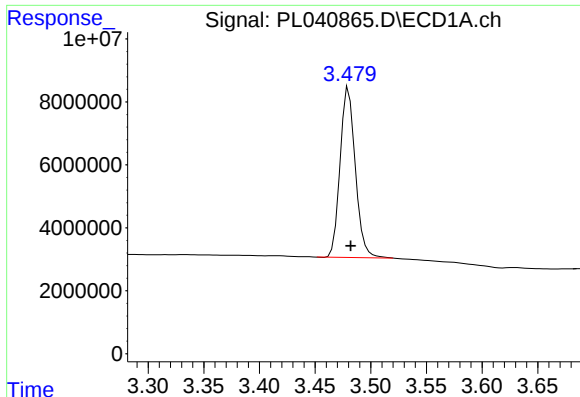

#1 Tetrachloro-m-xylene


R.T.: 3.480 min
Delta R.T.: -0.002 min
Response: 51475787
Conc: 11.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

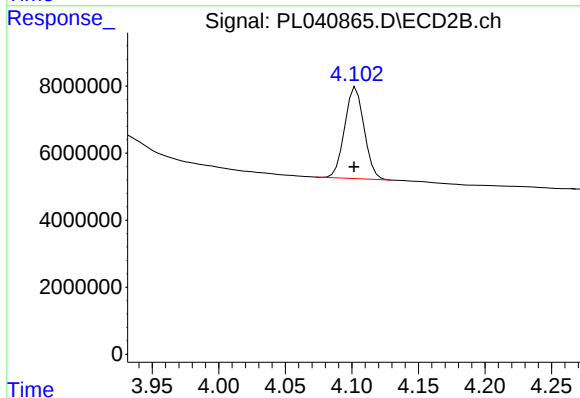


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.002 min
Response: 27647218
Conc: 10.47 ng/ml

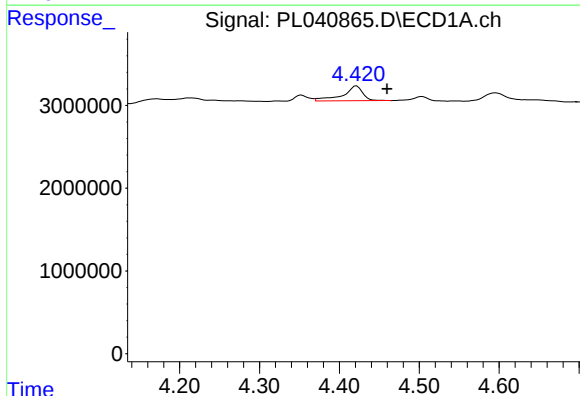


#6 beta-BHC

R.T.: 4.422 min
Delta R.T.: -0.038 min
Response: 3116138
Conc: 1.20 ng/ml

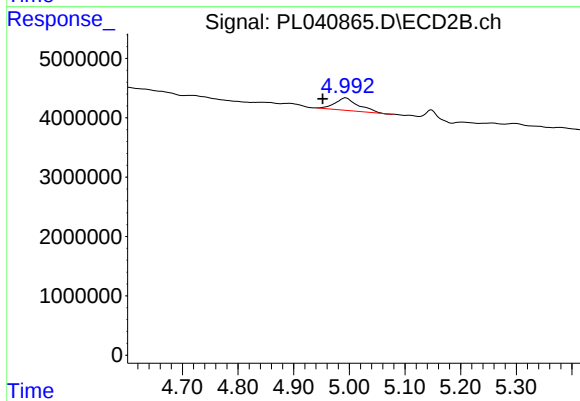

#6 beta-BHC


R.T.: 4.994 min
Delta R.T.: 0.042 min
Response: 5996466
Conc: 3.79 ng/ml

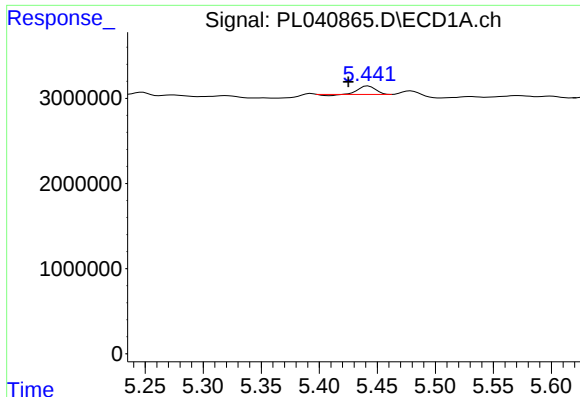

#10 gamma-Chlordane


R.T.: 5.442 min
Delta R.T.: 0.017 min
Response: 975694
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

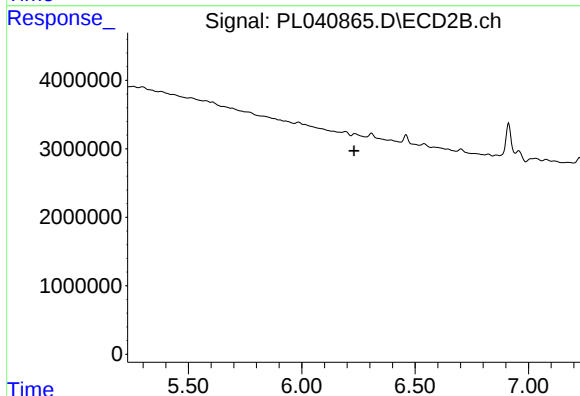


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

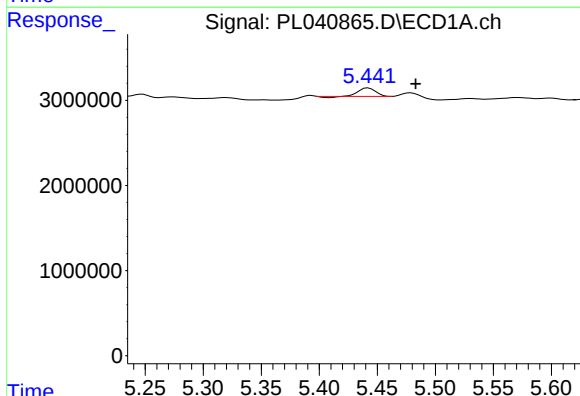


#11 alpha-Chlordane

R.T.: 5.442 min
Delta R.T.: -0.041 min
Response: 975694
Conc: 0.18 ng/ml

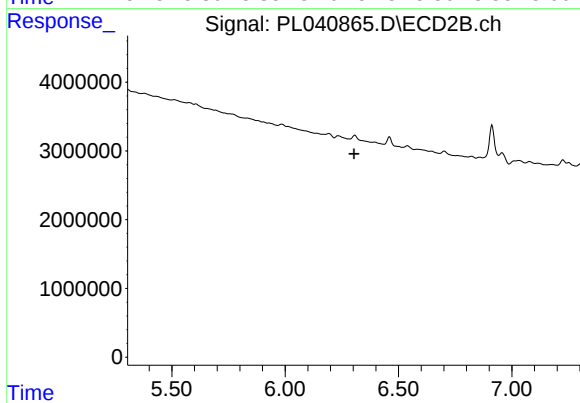

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.305 min
Response: 0
Conc: N.D.

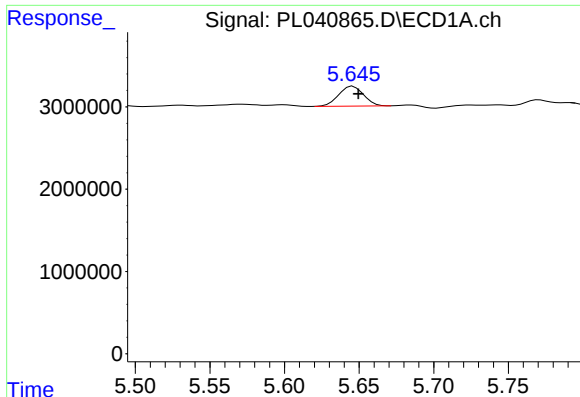

#12 4,4'-DDE


R.T.: 5.646 min
Delta R.T.: -0.004 min
Response: 2832560
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

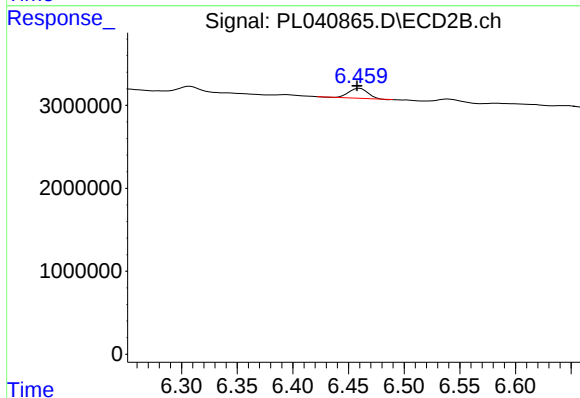


#12 4,4'-DDE

R.T.: 6.460 min
Delta R.T.: 0.002 min
Response: 1393946
Conc: 0.55 ng/ml

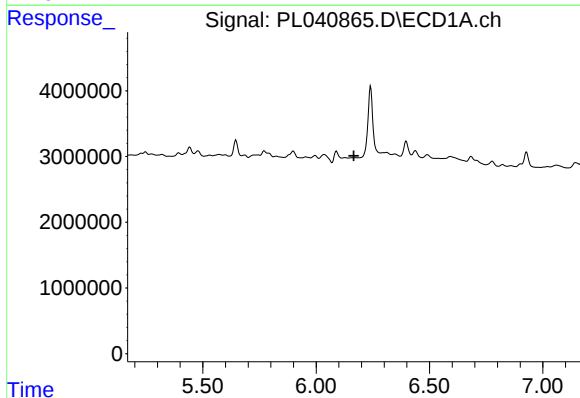


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.166 min
Response: 0
Conc: N.D.

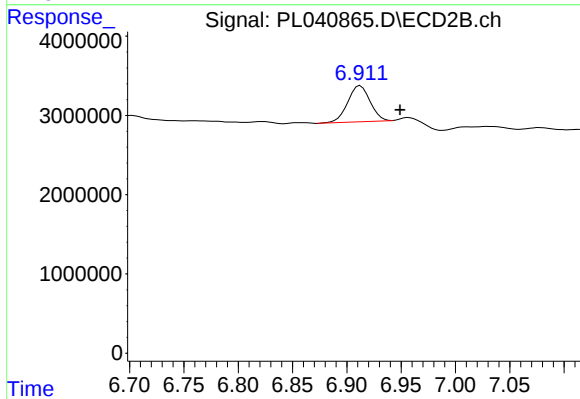

#16 4,4'-DDD


R.T.: 6.912 min
Delta R.T.: -0.037 min
Response: 6517728
Conc: 3.16 ng/ml

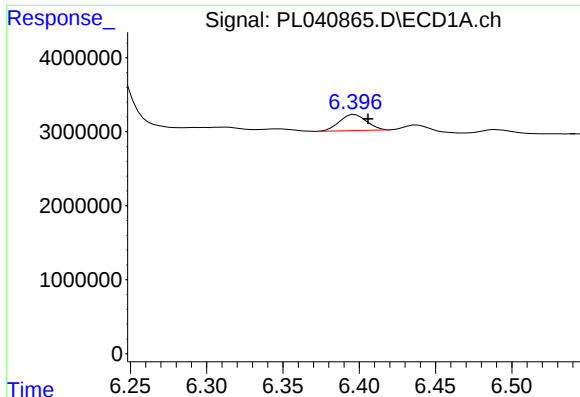

#17 4,4'-DDT


R.T.: 6.397 min
Delta R.T.: -0.009 min
Response: 2664532
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

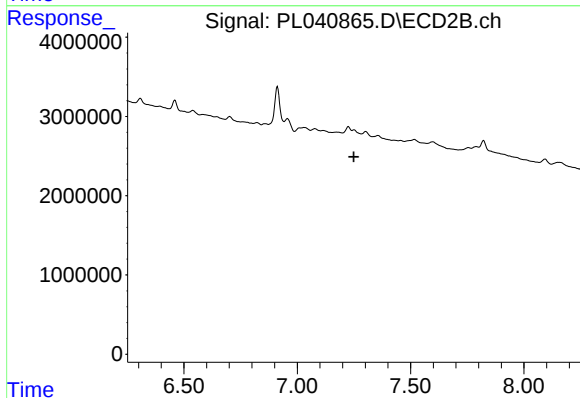


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

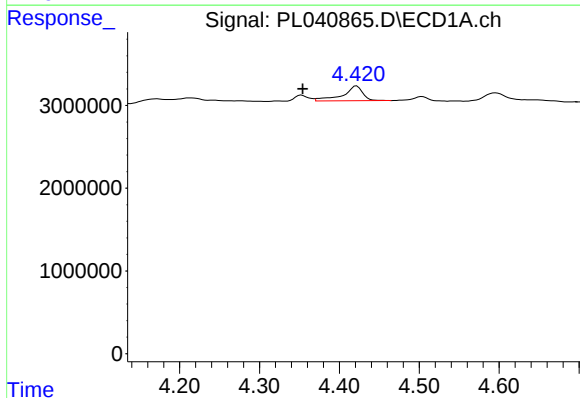


#23 Chlordane-1

R.T.: 4.422 min
Delta R.T.: 0.068 min
Response: 3116138
Conc: 14.86 ng/ml

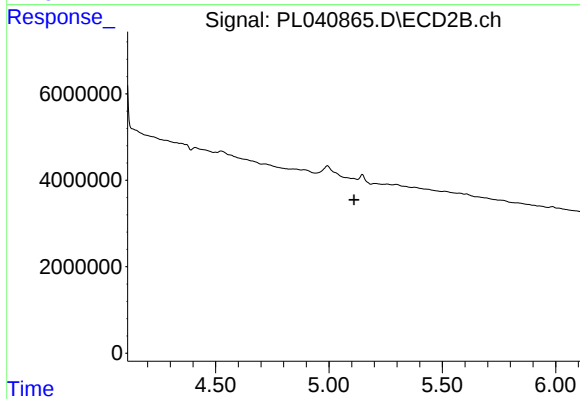

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

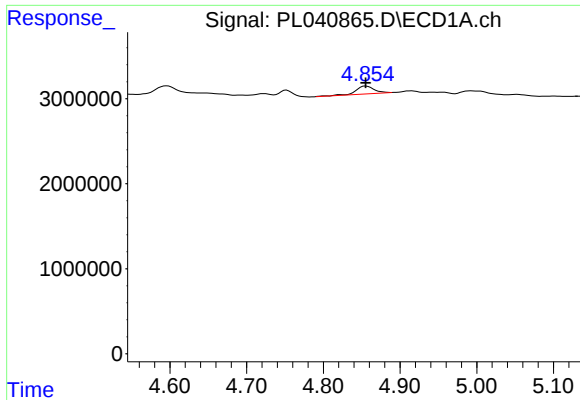

#24 Chlordane-2


R.T.: 4.856 min
Delta R.T.: 0.000 min
Response: 1518726
Conc: 6.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

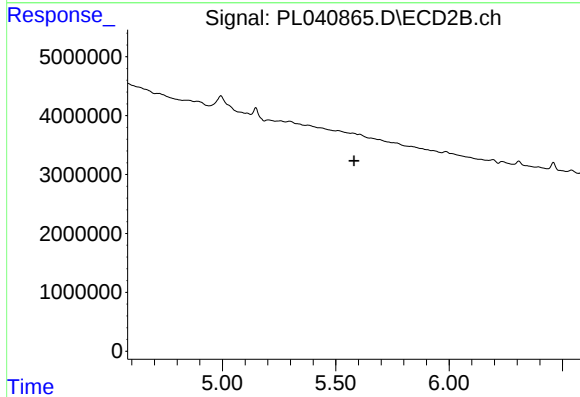


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.581 min
Response: 0
Conc: N.D.

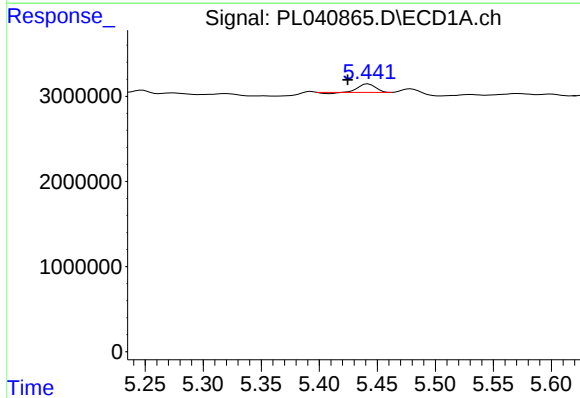


#25 Chlordane-3

R.T.: 5.442 min
Delta R.T.: 0.018 min
Response: 975694
Conc: 1.55 ng/ml

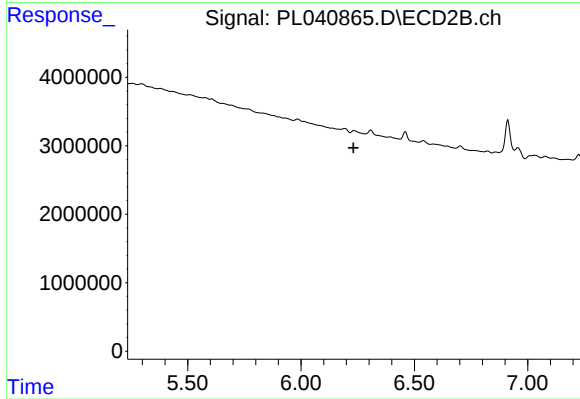

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

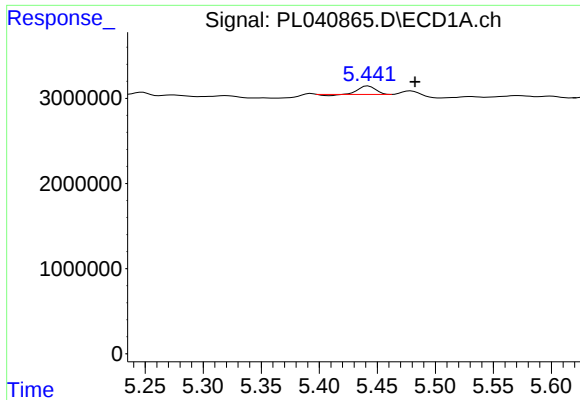

#26 Chlordane-4


R.T.: 5.442 min
Delta R.T.: -0.040 min
Response: 975694
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

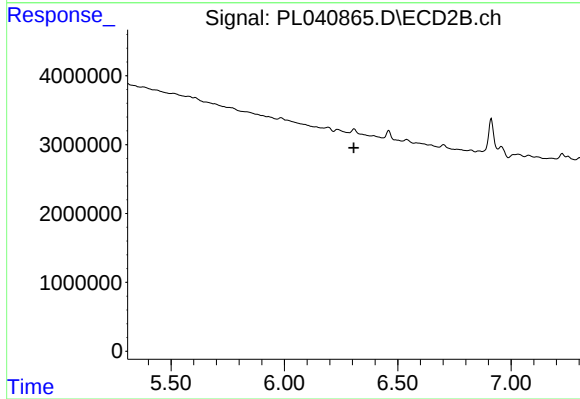


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

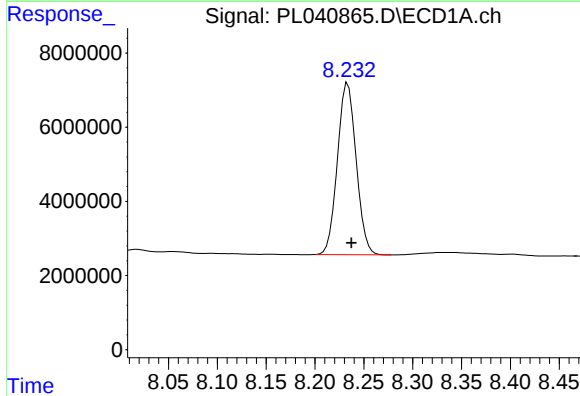

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: -0.004 min
Response: 61931668
Conc: 13.40 ng/ml

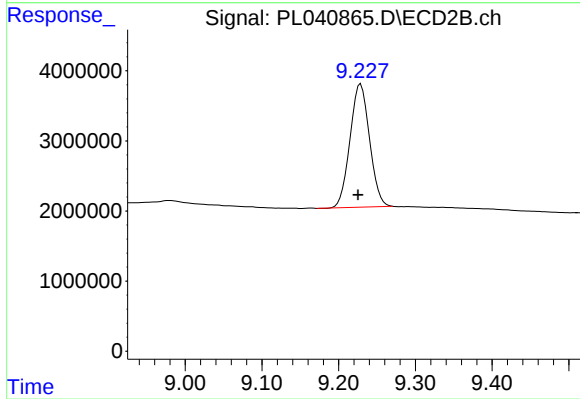

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.003 min
Response: 31294670
Conc: 13.18 ng/ml