

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
 Data File : PL053194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 10:52
 Operator : SG\AJ
 Sample : MDL-S-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-S-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 11:37:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 05:45:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	4.047	182.0E6	45585293	19.557	18.152
27)	SA Decachlor...	8.338	9.125	314.3E6	91179378	34.665	34.136
Target Compounds							
2)	A alpha-BHC	3.990	0.000	12974872	0	0.920	N.D. #
3)	MA gamma-BHC...	4.278	0.000	11194046	0	0.866	N.D. #
4)	MA Heptachlor	4.586	0.000	12160329	0	0.891	N.D. #
5)	MB Aldrin	4.837	0.000	10222769	0	0.826	N.D. #
8)	B Heptachlo...	5.284	0.000	10953384	0	0.921	N.D. #
9)	A Endosulfan I	5.626	0.000	9690251	0	0.878	N.D. #
10)	B trans-Chl...	5.513	0.000	11018918	0	0.911	N.D. #
11)	B cis-Chlor...	5.572	0.000	10812193	0	0.921	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
Data File : PL053194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 10:52
Operator : SG\AJ
Sample : MDL-S-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 11:37:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 05:45:16 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

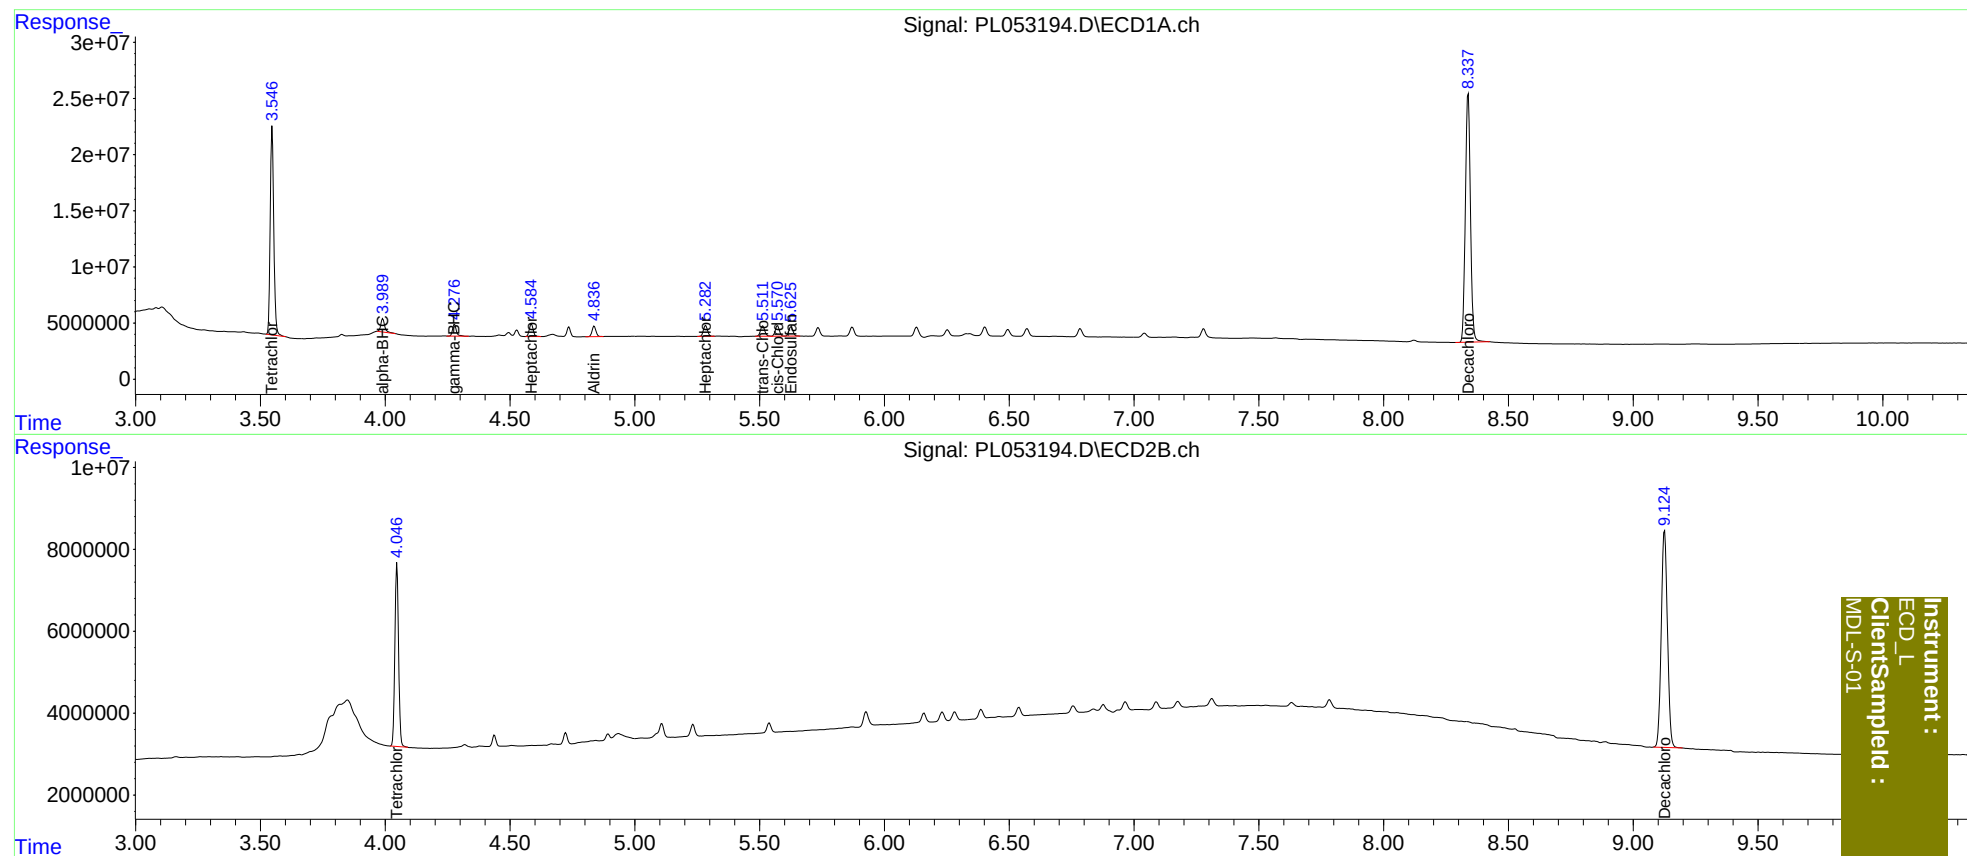


Instrument :
ECD_L
ClientSampleId :
MDL-S-01

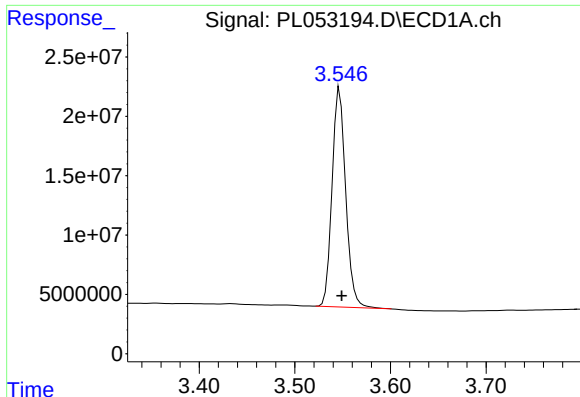

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: -0.002 min
Response: 182006684
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-01

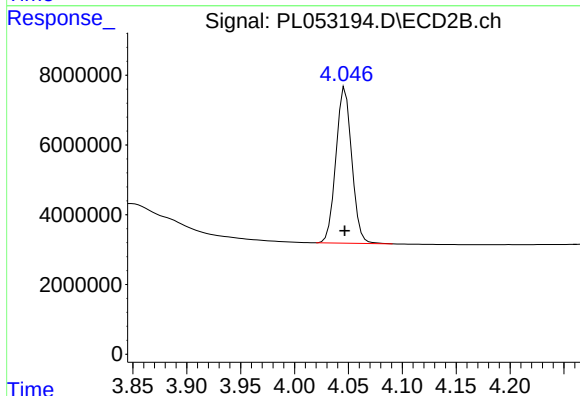


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 45585293
Conc: 18.15 ng/ml

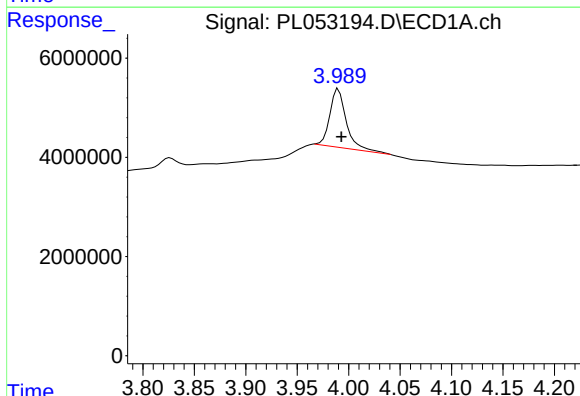


#2 alpha-BHC

R.T.: 3.990 min
Delta R.T.: -0.003 min
Response: 12974872
Conc: 0.92 ng/ml

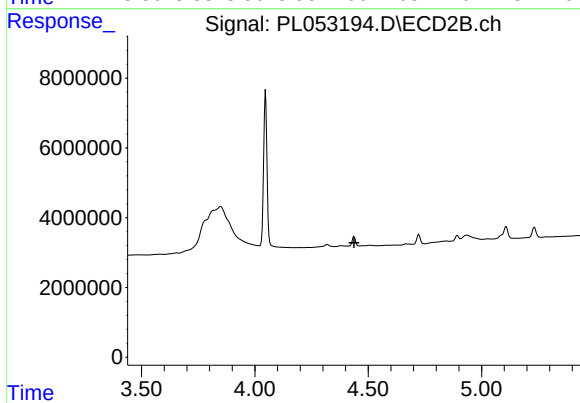

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.437 min
Response: 0
Conc: N.D.

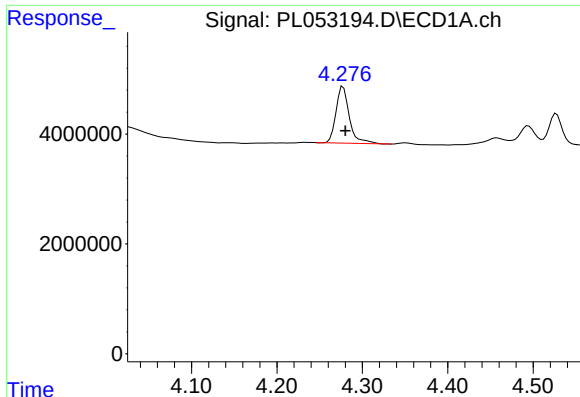

#3 gamma-BHC (Lindane)


R.T.: 4.278 min
Delta R.T.: -0.003 min
Response: 11194046
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-01

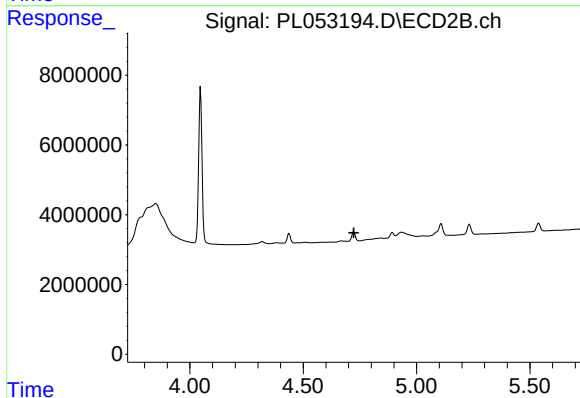


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

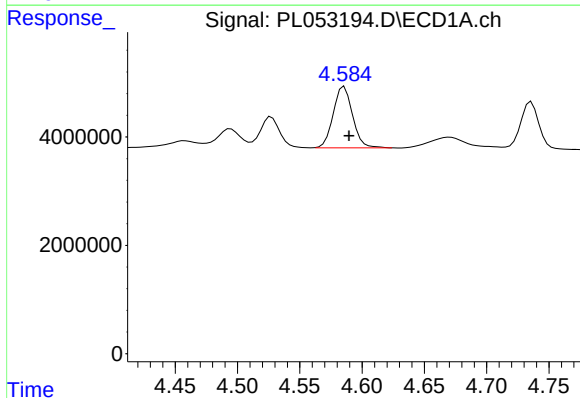


#4 Heptachlor

R.T.: 4.586 min
Delta R.T.: -0.004 min
Response: 12160329
Conc: 0.89 ng/ml

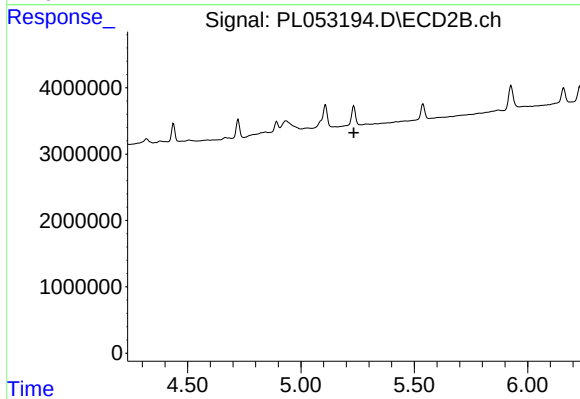

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

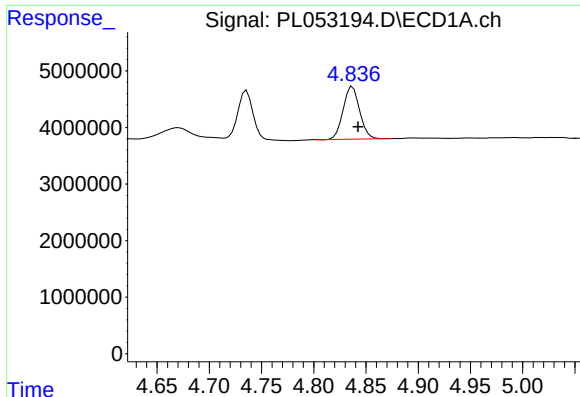

#5 Aldrin


R.T.: 4.837 min
Delta R.T.: -0.005 min
Response: 10222769
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-01

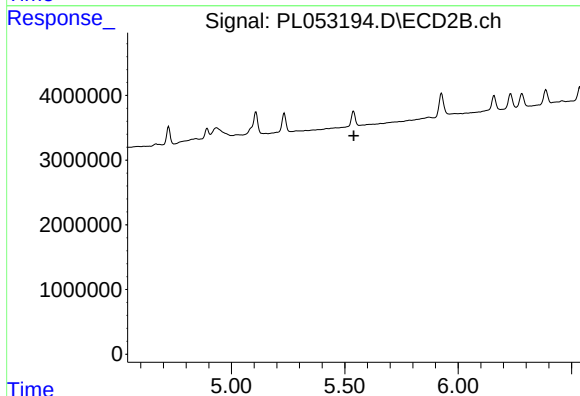


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.539 min
Response: 0
Conc: N.D.

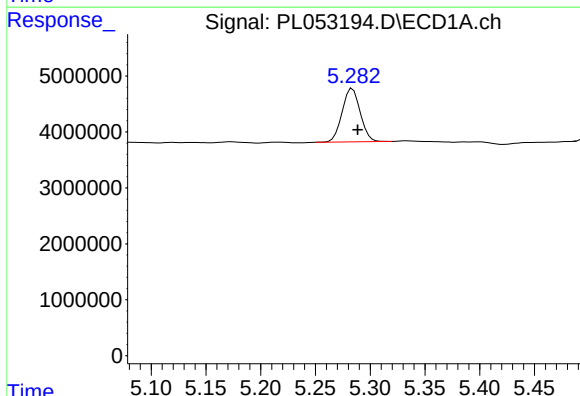


#8 Heptachlor epoxide

R.T.: 5.284 min
Delta R.T.: -0.005 min
Response: 10953384
Conc: 0.92 ng/ml

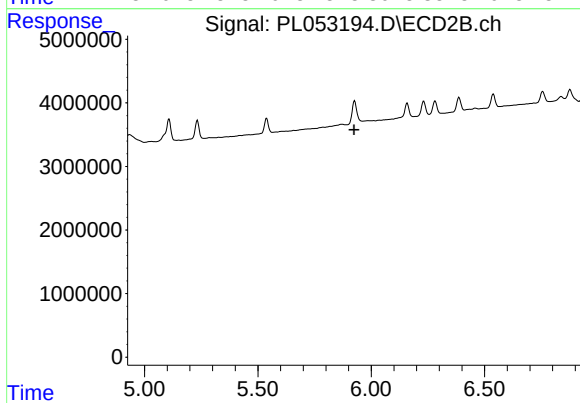

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

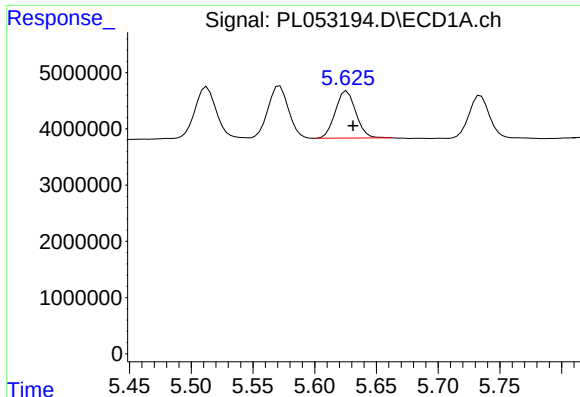

#9 Endosulfan I


R.T.: 5.626 min
Delta R.T.: -0.005 min
Response: 9690251
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-01

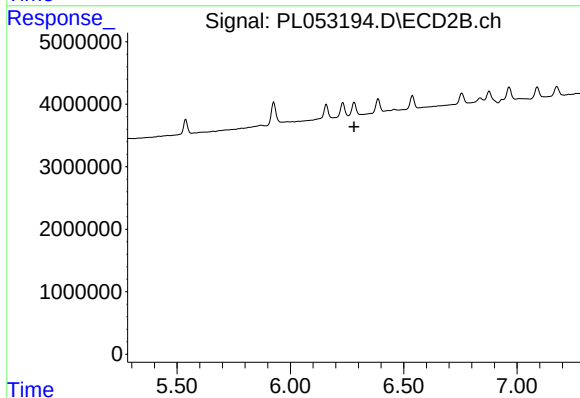


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

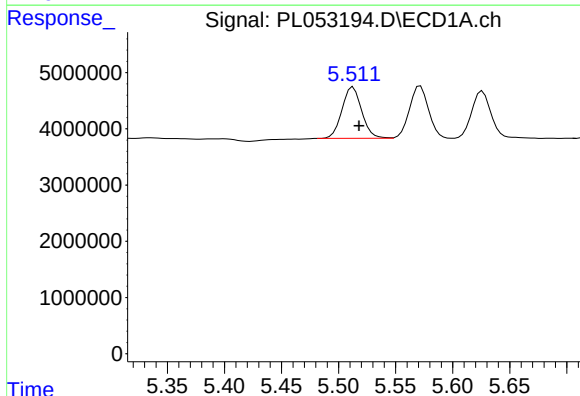


#10 trans-Chlordane

R.T.: 5.513 min
Delta R.T.: -0.005 min
Response: 11018918
Conc: 0.91 ng/ml

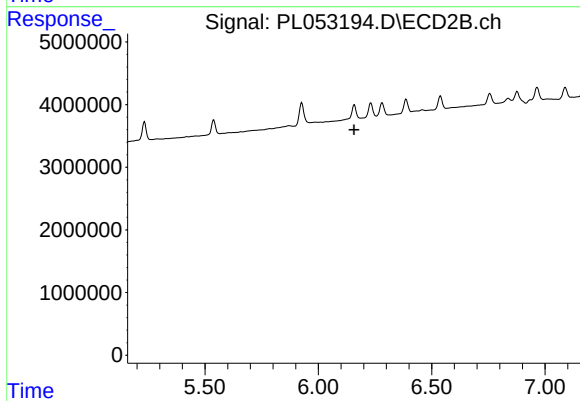

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

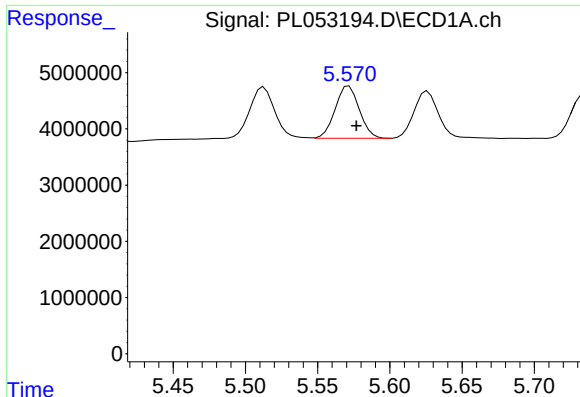

#11 cis-Chlordane


R.T.: 5.572 min
Delta R.T.: -0.005 min
Response: 10812193
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-01

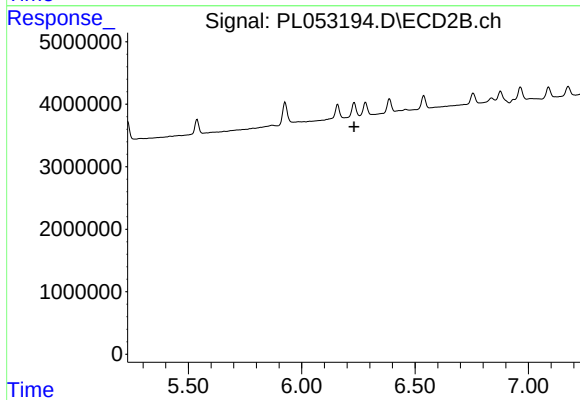


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

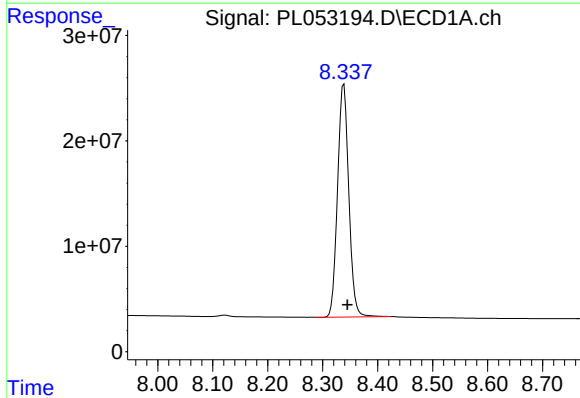

#27 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.006 min
Response: 314254354
Conc: 34.66 ng/ml

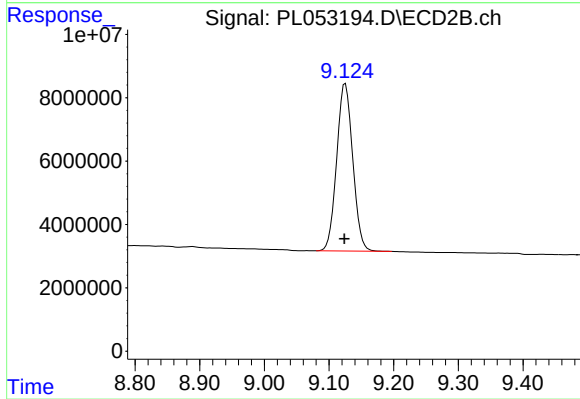

#27 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.002 min
Response: 91179378
Conc: 34.14 ng/ml