

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
 Data File : PL053195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 11:06
 Operator : SG\AJ
 Sample : MDL-S-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-S-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 11:38:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 05:45:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.047	168.7E6	41550694	18.124	16.546
27)	SA Decachlor...	8.336	9.124	292.3E6	86900421	32.240	32.534
Target Compounds							
2)	A alpha-BHC	3.989	0.000	14188622	0	1.006	N.D. #
3)	MA gamma-BHC...	4.276	0.000	11775089	0	0.911	N.D. #
4)	MA Heptachlor	4.584	0.000	11232572	0	0.823	N.D. #
5)	MB Aldrin	4.836	0.000	9689287	0	0.783	N.D. #
6)	B beta-BHC	4.494f	0.000	8238175	0	1.403	N.D. #
8)	B Heptachlo...	5.283	5.927	10356115	5507129	0.870	1.779 #
9)	A Endosulfan I	5.570f	0.000	10242934	0	0.928	N.D. #
10)	B trans-Chl...	5.511	0.000	10254663	0	0.847	N.D. #
11)	B cis-Chlor...	5.570	0.000	10242934	0	0.873	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
Data File : PL053195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 11:06
Operator : SG\AJ
Sample : MDL-S-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 11:38:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 05:45:16 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

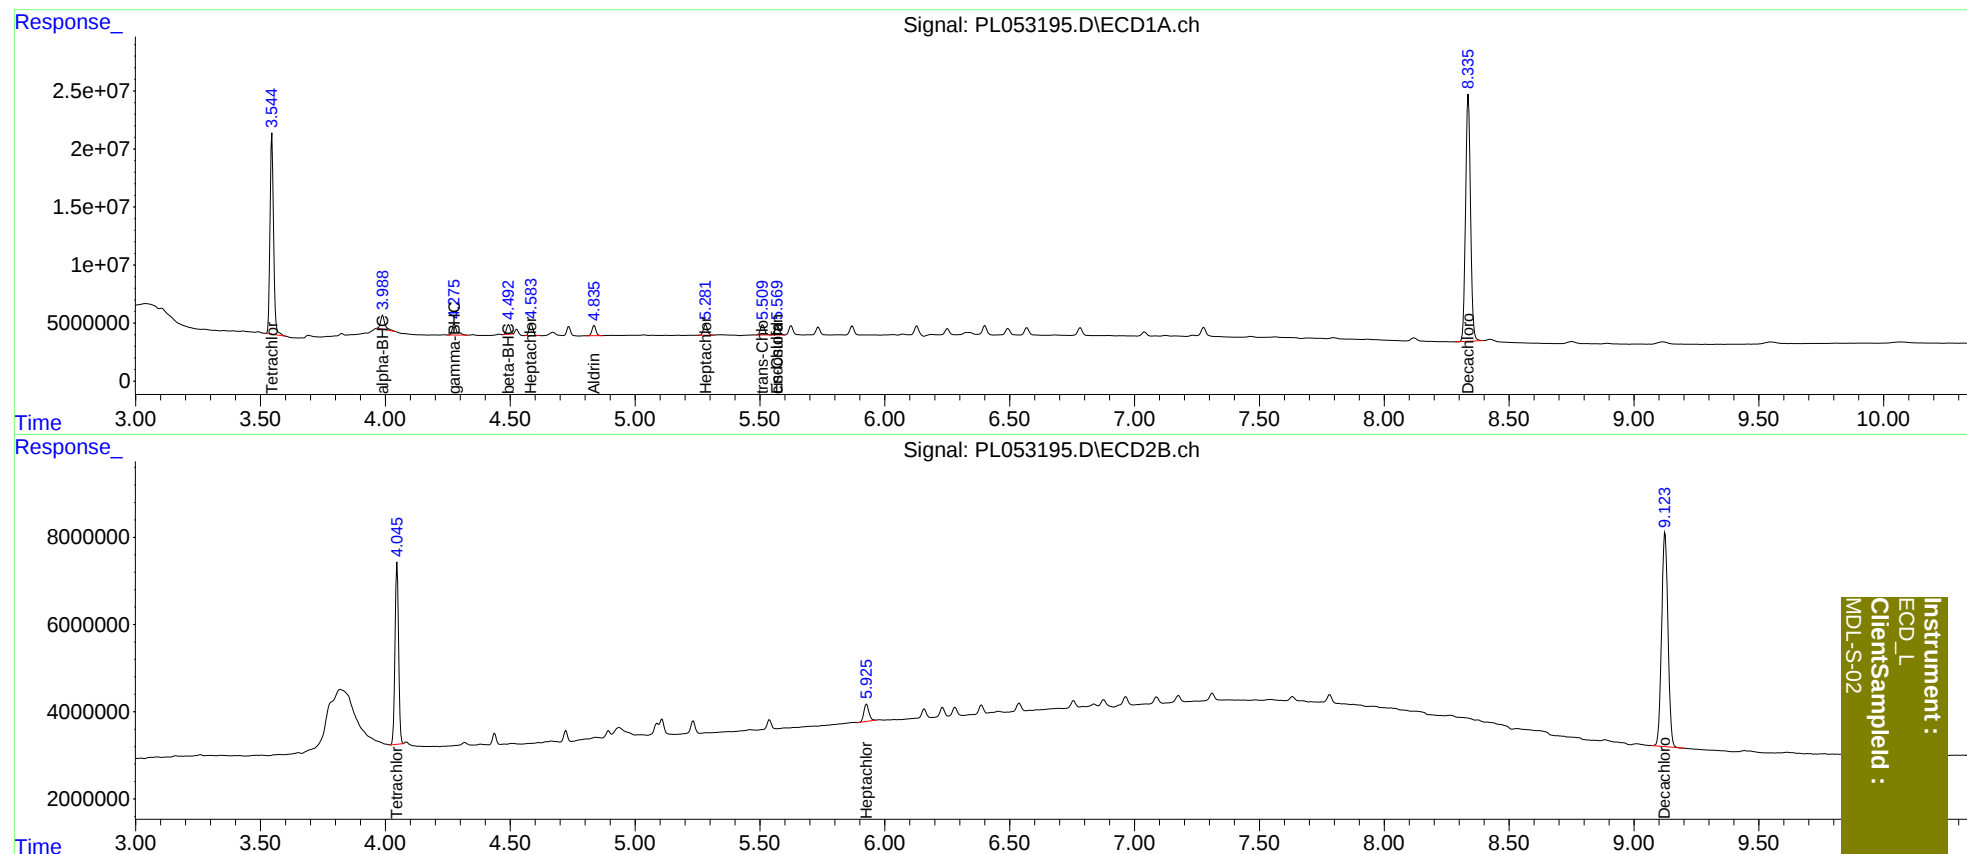


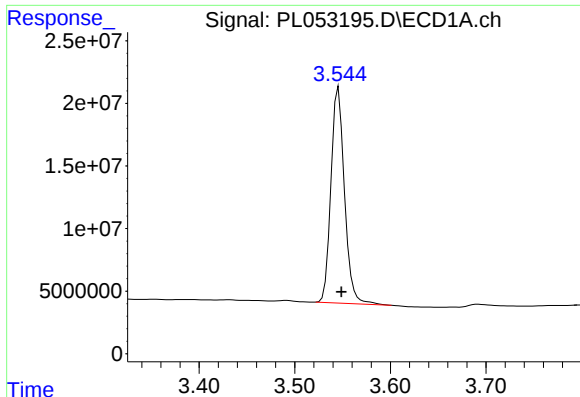

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 168677753
Conc: 18.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-02

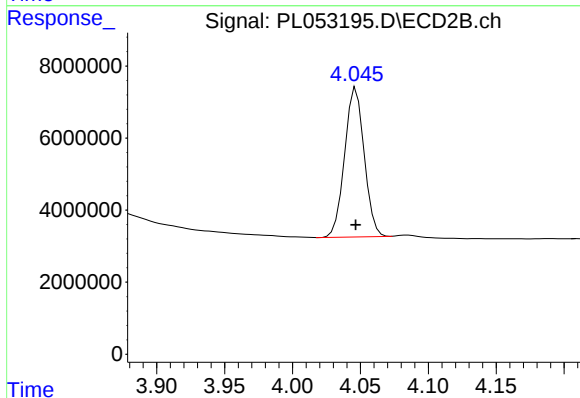


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 41550694
Conc: 16.55 ng/ml

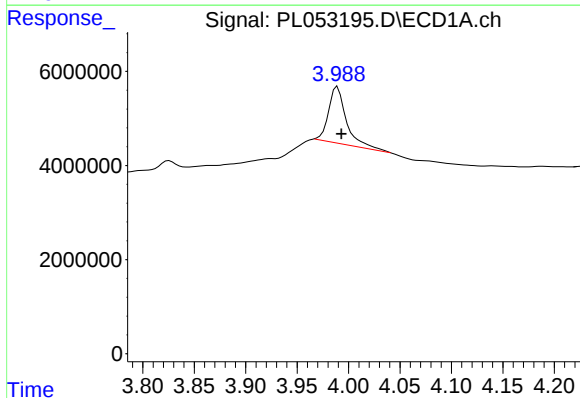


#2 alpha-BHC

R.T.: 3.989 min
Delta R.T.: -0.004 min
Response: 14188622
Conc: 1.01 ng/ml

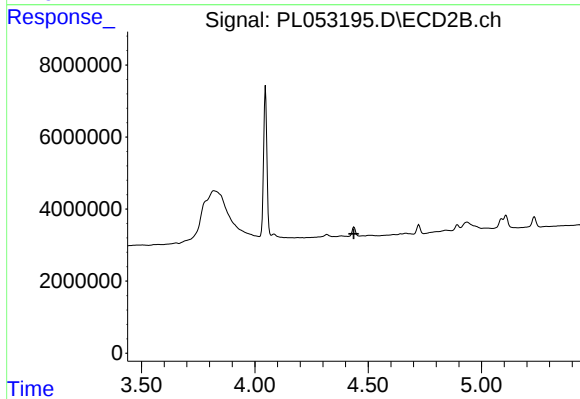

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.437 min
Response: 0
Conc: N.D.

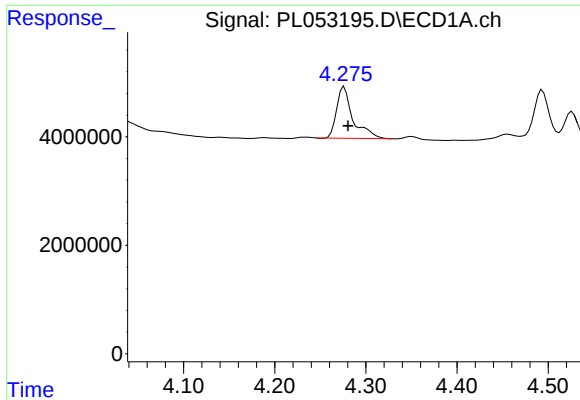

#3 gamma-BHC (Lindane)


R.T.: 4.276 min
Delta R.T.: -0.004 min
Response: 11775089
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-02

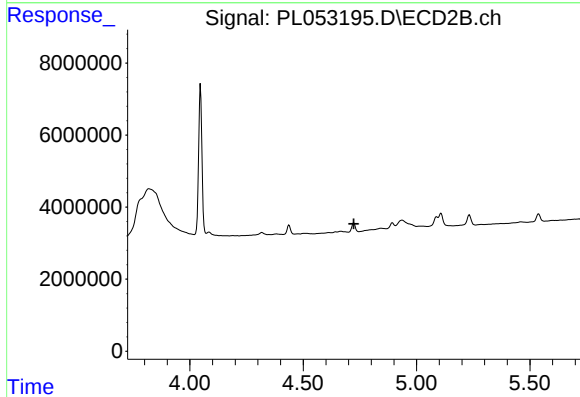


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

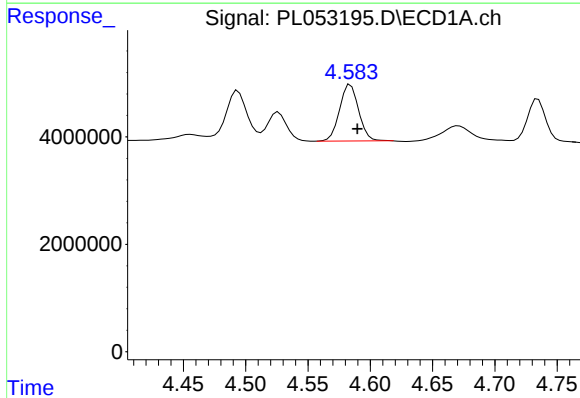


#4 Heptachlor

R.T.: 4.584 min
Delta R.T.: -0.006 min
Response: 11232572
Conc: 0.82 ng/ml

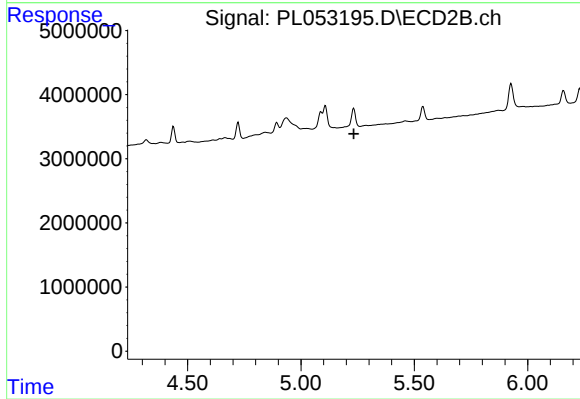

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

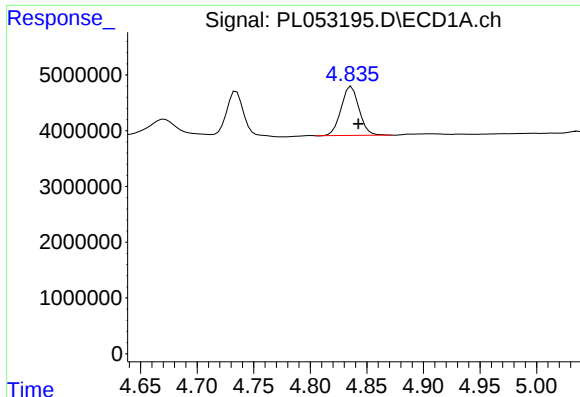

#5 Aldrin


R.T.: 4.836 min
Delta R.T.: -0.006 min
Response: 9689287
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-02

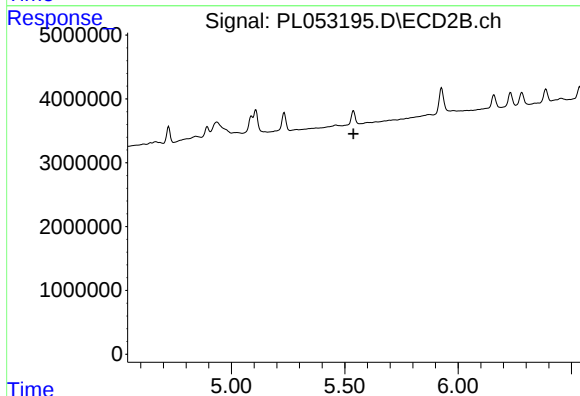


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.539 min
Response: 0
Conc: N.D.

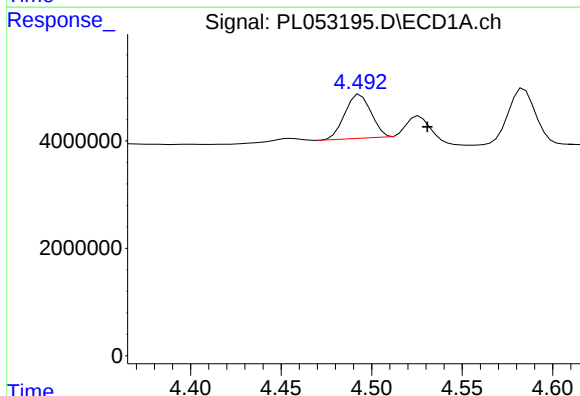


#6 beta-BHC

R.T.: 4.494 min
Delta R.T.: -0.037 min
Response: 8238175
Conc: 1.40 ng/ml

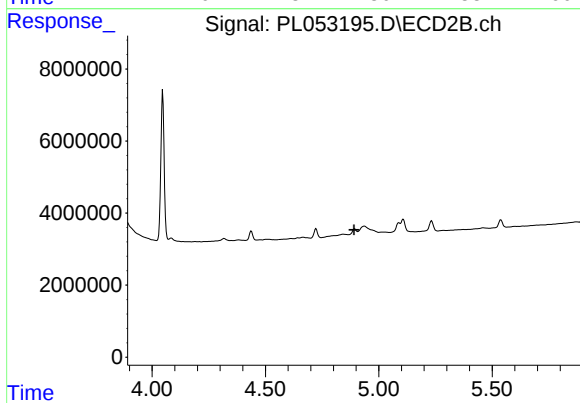

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.891 min
Response: 0
Conc: N.D.

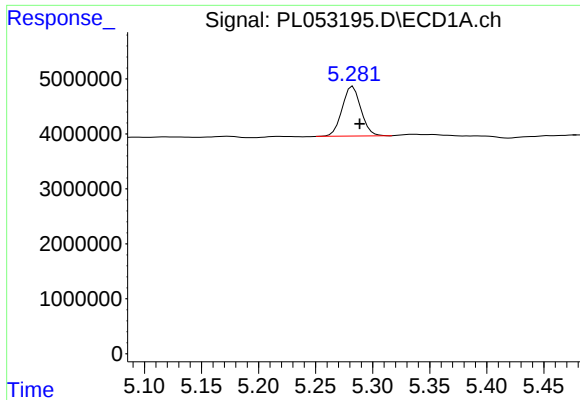

#8 Heptachlor epoxide


R.T.: 5.283 min
Delta R.T.: -0.006 min
Response: 10356115
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-02

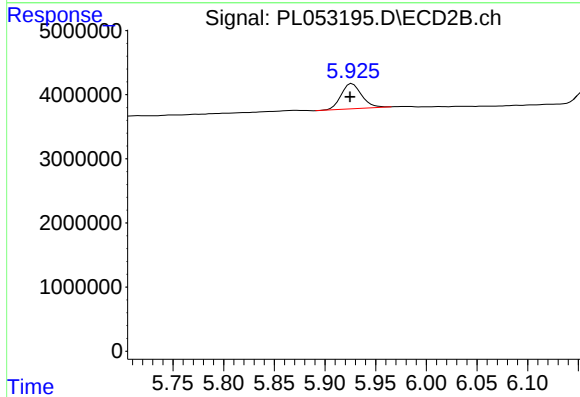


#8 Heptachlor epoxide

R.T.: 5.927 min
Delta R.T.: 0.002 min
Response: 5507129
Conc: 1.78 ng/ml

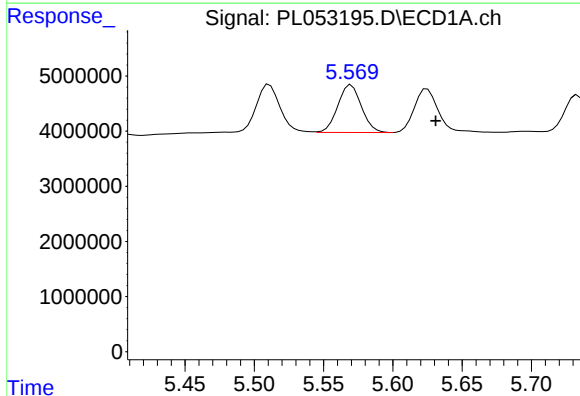


#9 Endosulfan I

R.T.: 5.570 min
Delta R.T.: -0.061 min
Response: 10242934
Conc: 0.93 ng/ml

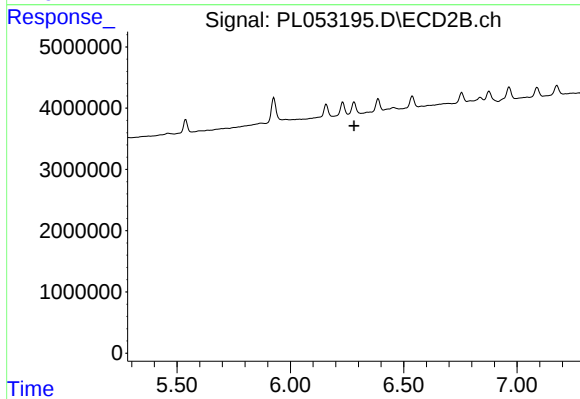

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

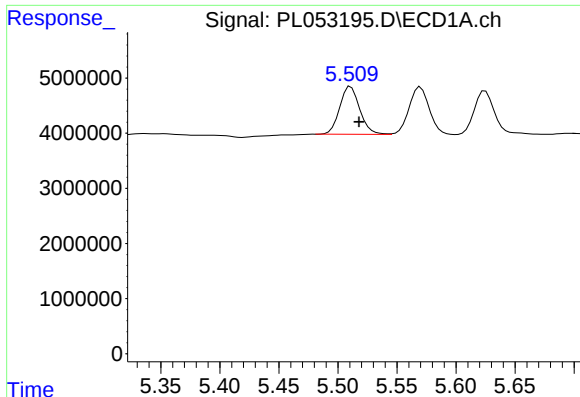

#10 trans-Chlordane


R.T.: 5.511 min
Delta R.T.: -0.007 min
Response: 10254663
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-02

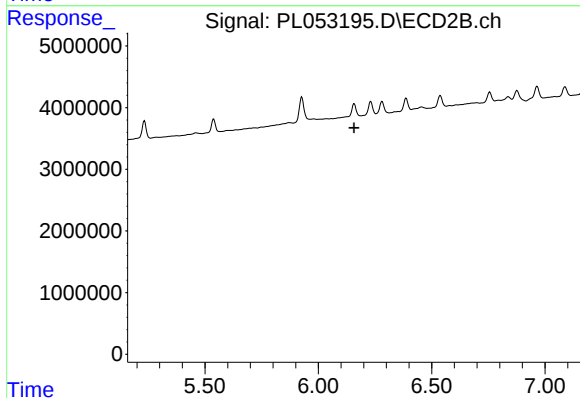


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

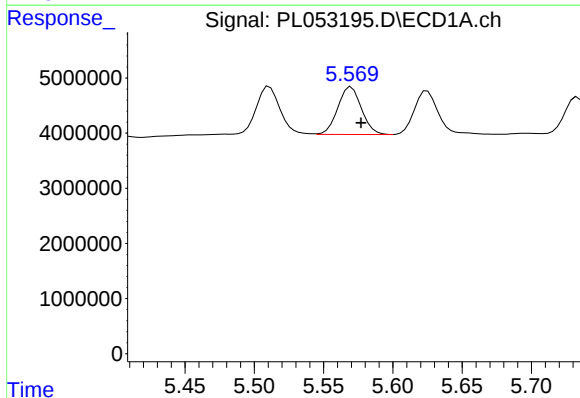


#11 cis-Chlordane

R.T.: 5.570 min
Delta R.T.: -0.007 min
Response: 10242934
Conc: 0.87 ng/ml

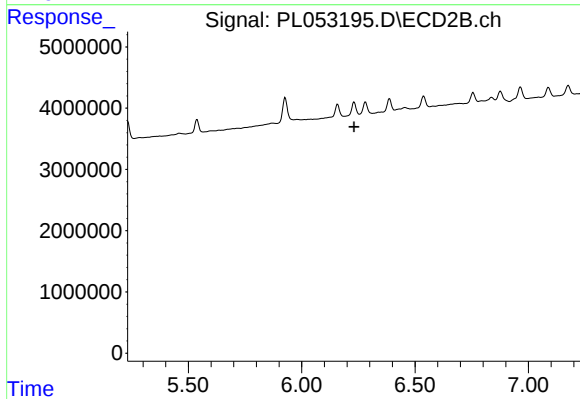

#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

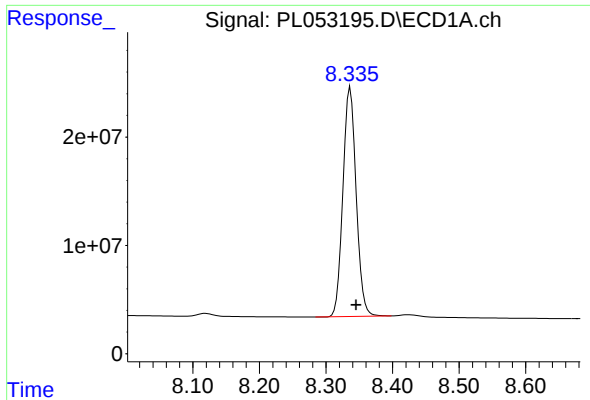

#27 Decachlorobiphenyl


R.T.: 8.336 min

Delta R.T.: -0.009 min

Response: 292270002

Conc: 32.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-02

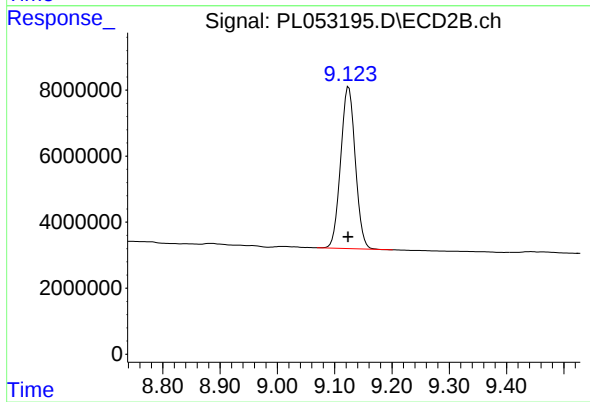

#27 Decachlorobiphenyl

R.T.: 9.124 min

Delta R.T.: 0.000 min

Response: 86900421

Conc: 32.53 ng/ml