

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
 Data File : PL053196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 11:20
 Operator : SG\AJ
 Sample : MDL-S-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-S-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 12:02:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 05:45:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.047	176.6E6	44551380	18.974	17.741
27)	SA Decachlor...	8.336	9.125	311.2E6	92419493	34.333	34.601
Target Compounds							
2)	A alpha-BHC	3.989	0.000	14808289	0	1.050	N.D. #
3)	MA gamma-BHC...	4.276	0.000	12161502	0	0.941	N.D. #
4)	MA Heptachlor	4.584	0.000	11632691	0	0.852	N.D. #
5)	MB Aldrin	4.836	0.000	10033598	0	0.811	N.D. #
8)	B Heptachlo...	5.282	0.000	10820197	0	0.909	N.D. #
9)	A Endosulfan I	5.570f	0.000	10725958	0	0.972	N.D. #
10)	B trans-Chl...	5.511	0.000	10760228	0	0.889	N.D. #
11)	B cis-Chlor...	5.570	0.000	10725958	0	0.914	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
Data File : PL053196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 11:20
Operator : SG\AJ
Sample : MDL-S-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 12:02:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 05:45:16 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

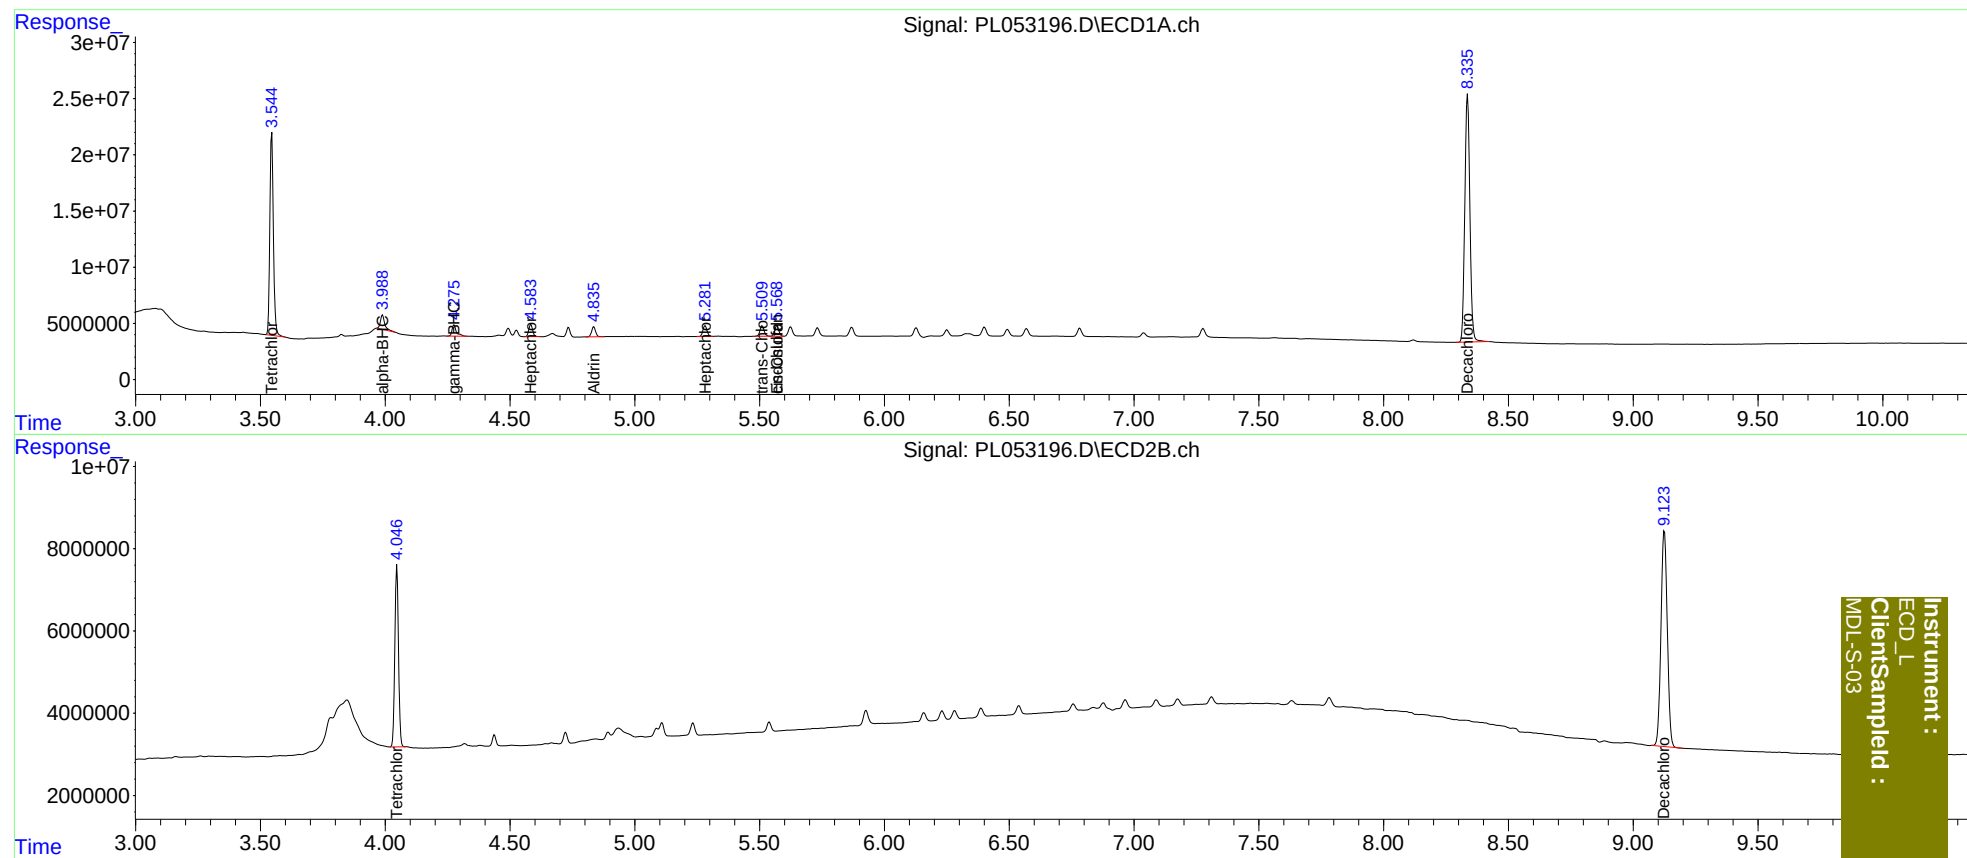


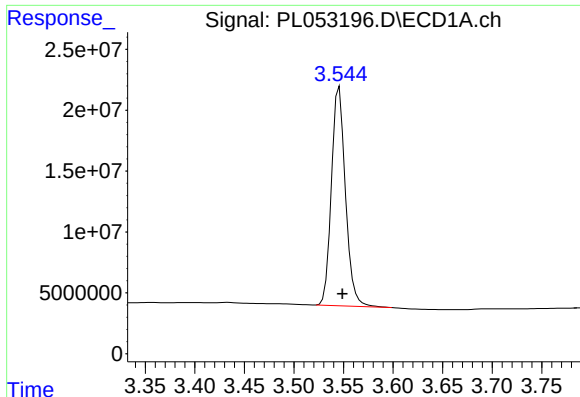

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 176582444
Conc: 18.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-03

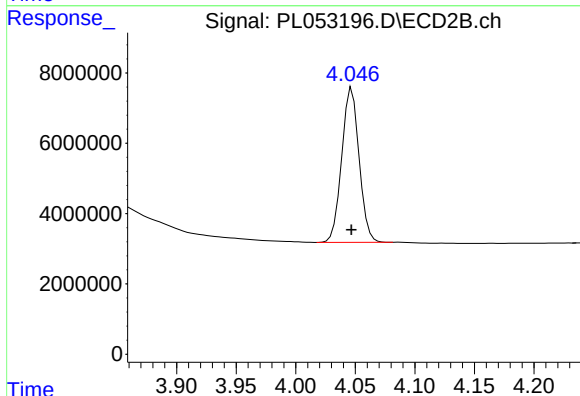


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 44551380
Conc: 17.74 ng/ml

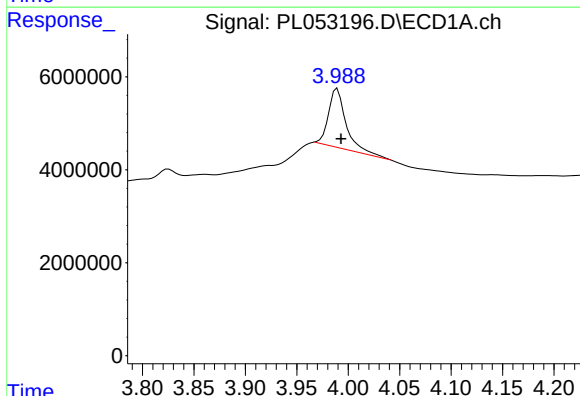


#2 alpha-BHC

R.T.: 3.989 min
Delta R.T.: -0.004 min
Response: 14808289
Conc: 1.05 ng/ml

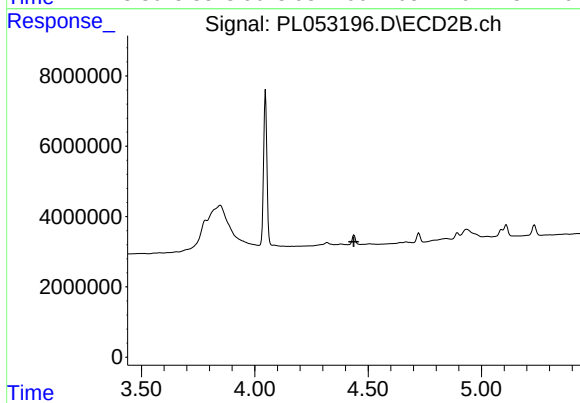

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.437 min
Response: 0
Conc: N.D.

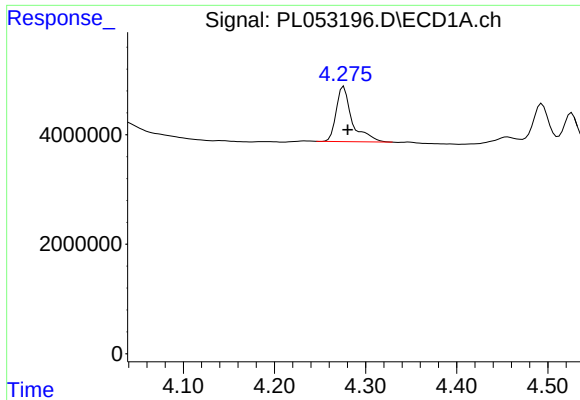

#3 gamma-BHC (Lindane)


R.T.: 4.276 min
Delta R.T.: -0.004 min
Response: 12161502
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-03

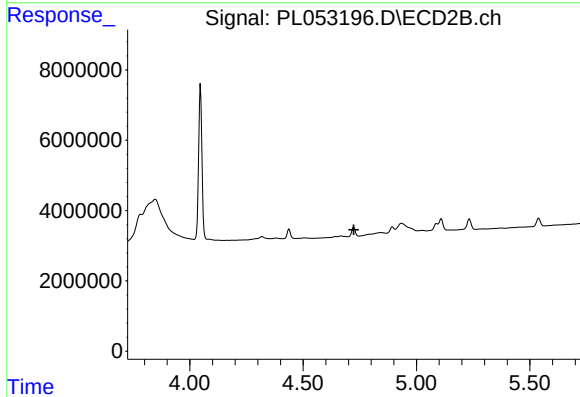


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

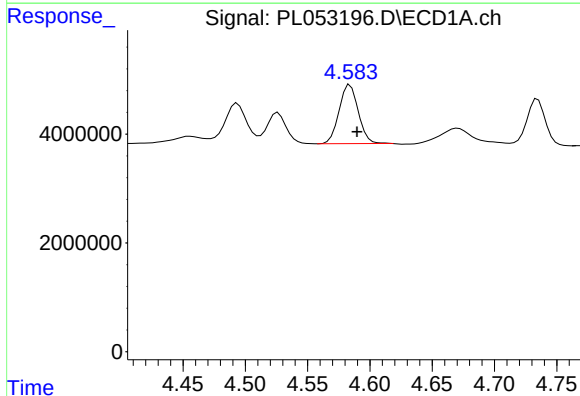


#4 Heptachlor

R.T.: 4.584 min
Delta R.T.: -0.006 min
Response: 11632691
Conc: 0.85 ng/ml

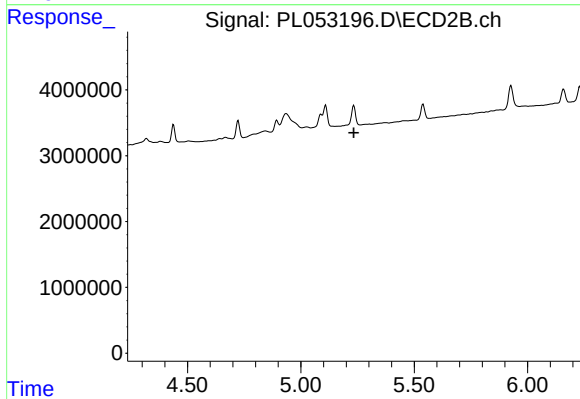

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

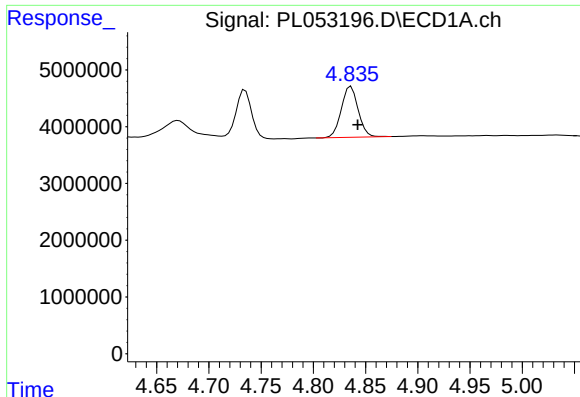

#5 Aldrin


R.T.: 4.836 min
Delta R.T.: -0.006 min
Response: 10033598
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-03

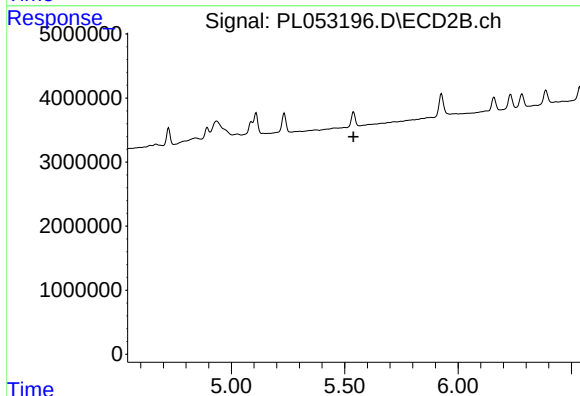


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.539 min
Response: 0
Conc: N.D.

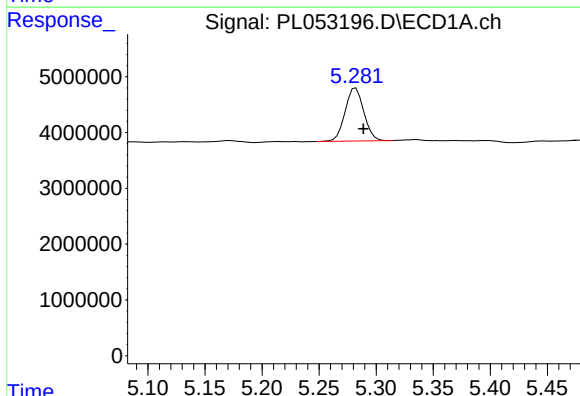


#8 Heptachlor epoxide

R.T.: 5.282 min
Delta R.T.: -0.006 min
Response: 10820197
Conc: 0.91 ng/ml

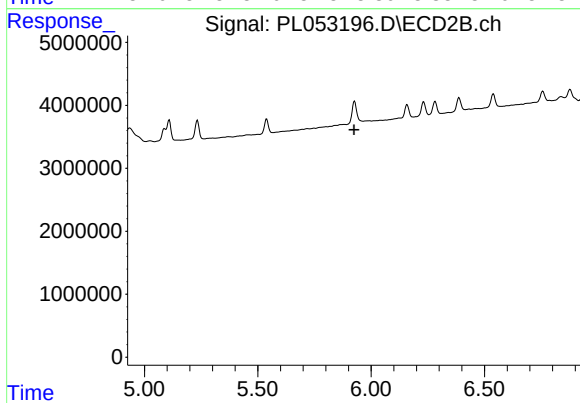

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

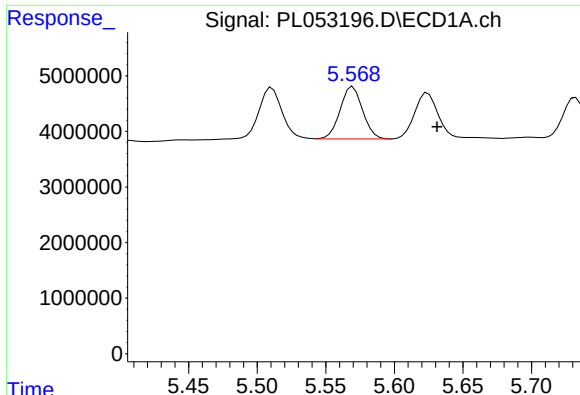

#9 Endosulfan I


R.T.: 5.570 min
Delta R.T.: -0.061 min
Response: 10725958
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-03

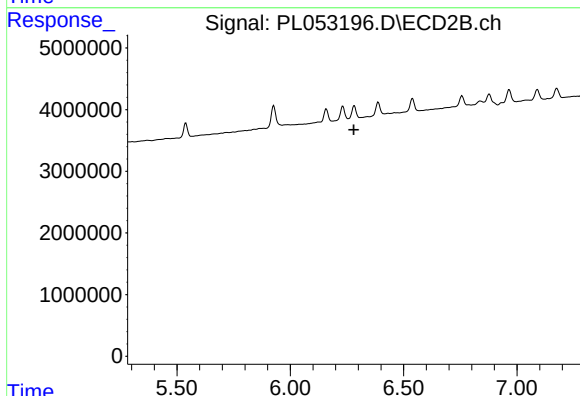


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

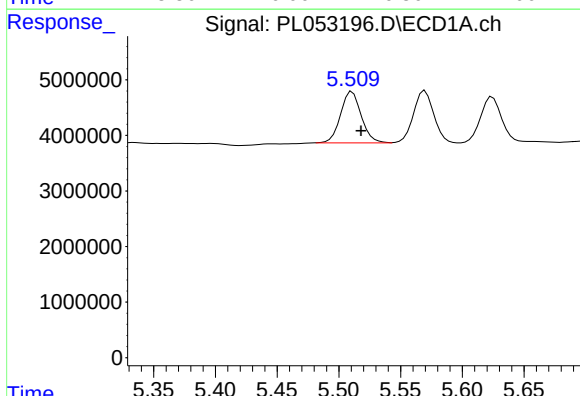


#10 trans-Chlordane

R.T.: 5.511 min
Delta R.T.: -0.007 min
Response: 10760228
Conc: 0.89 ng/ml

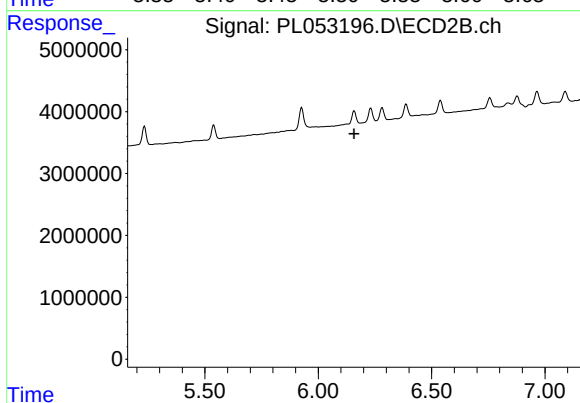

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

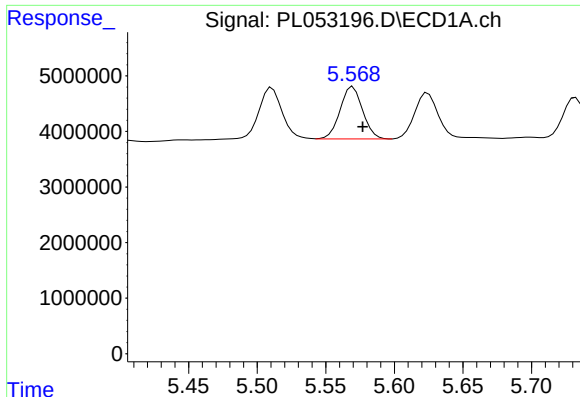

#11 cis-Chlordane


R.T.: 5.570 min
Delta R.T.: -0.007 min
Response: 10725958
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-S-03

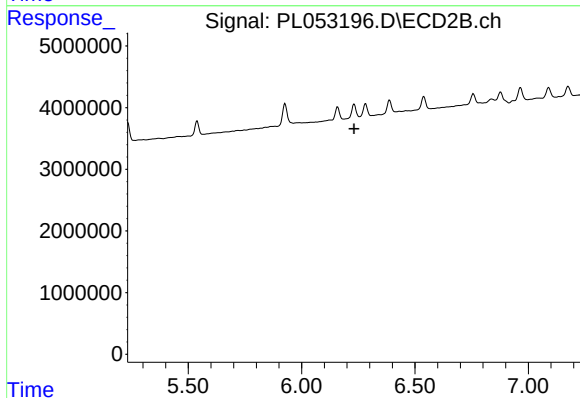


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

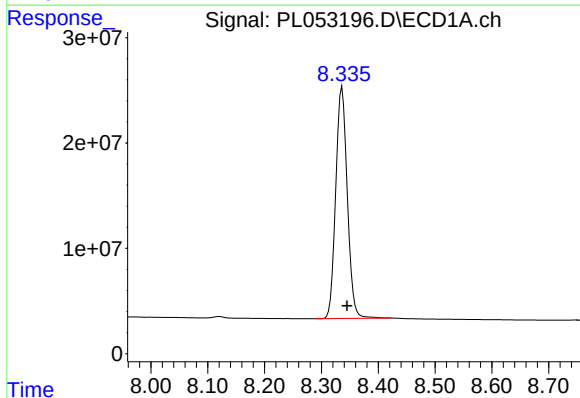

#27 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.008 min
Response: 311248312
Conc: 34.33 ng/ml

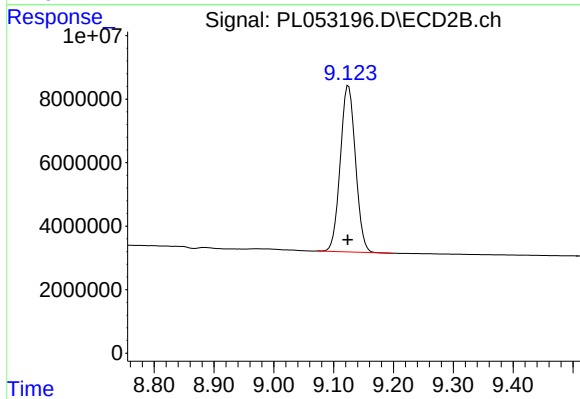

#27 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.001 min
Response: 92419493
Conc: 34.60 ng/ml