

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
 Data File : PL053203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 12:57
 Operator : SG\AJ
 Sample : MDL-W-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-W-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 13:45:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 05:45:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.546	4.047	144.6E6	36844810	15.532	14.672
2) SA Decachlor...	8.336	9.126	258.1E6	75841426	28.468	28.394
Target Compounds						
2) A alpha-BHC	3.990	0.000	13230651	0	0.938	N.D. #
4) MA Heptachlor	4.585	0.000	9378592	0	0.687	N.D. #
6) B beta-BHC	4.494f	0.000	12425135	0	2.115	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
Data File : PL053203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 12:57
Operator : SG\AJ
Sample : MDL-W-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 13:45:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 05:45:16 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

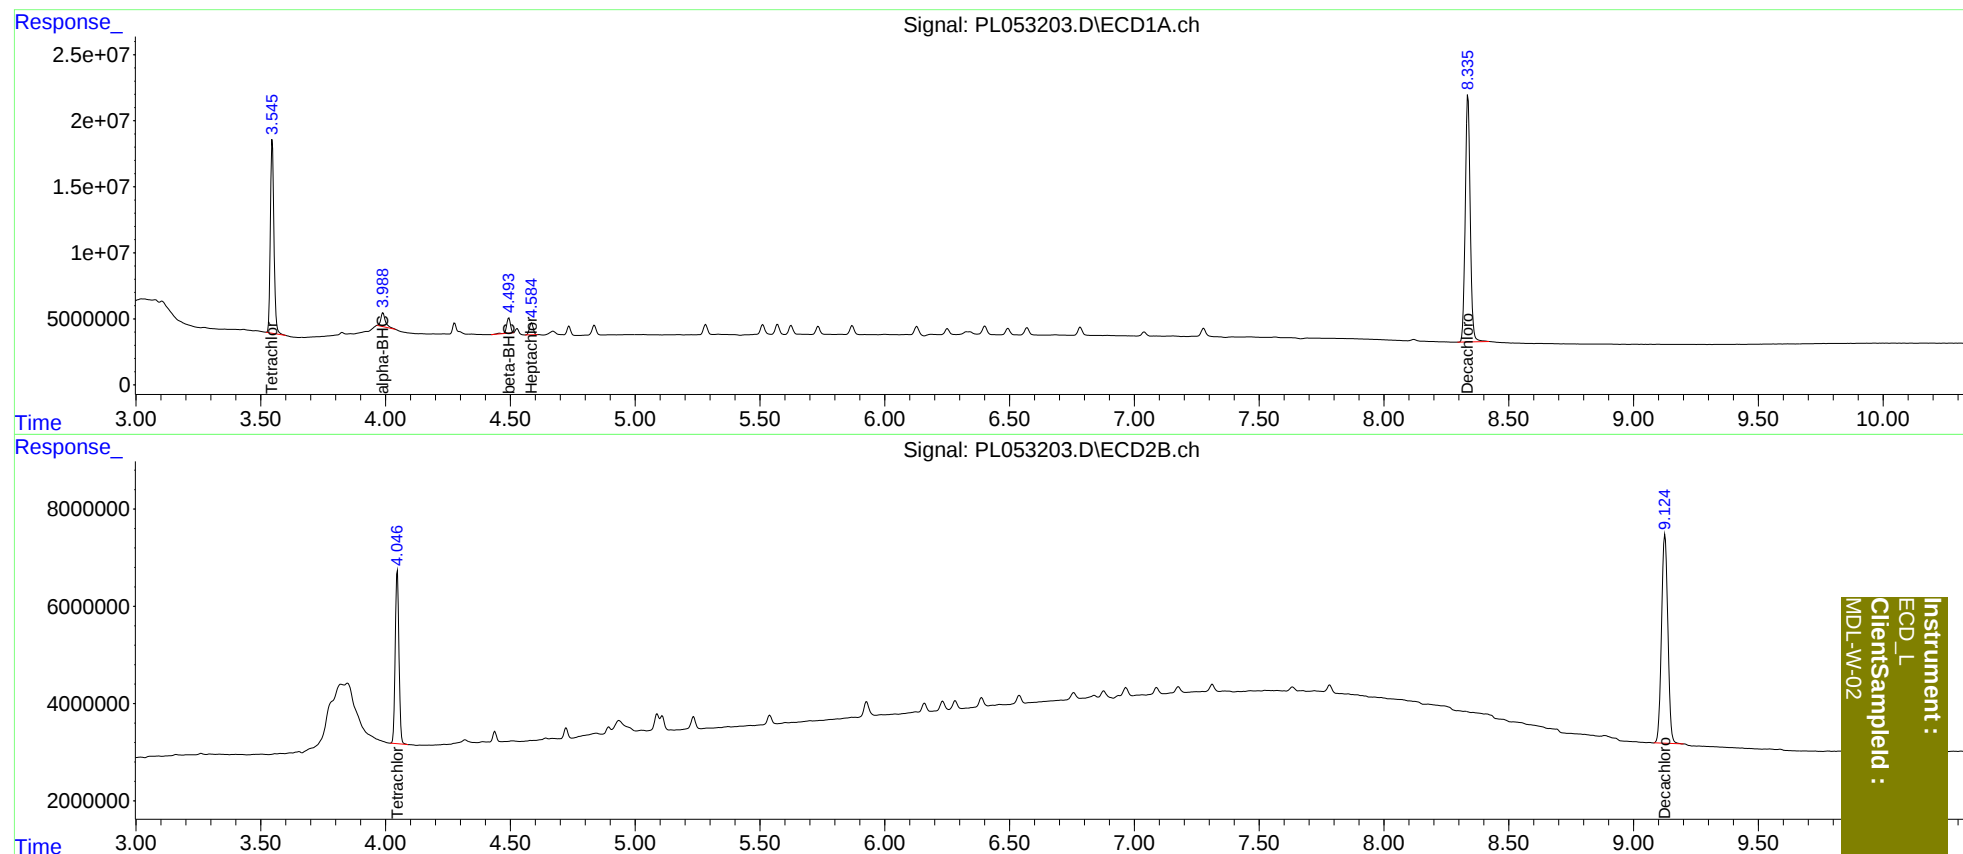


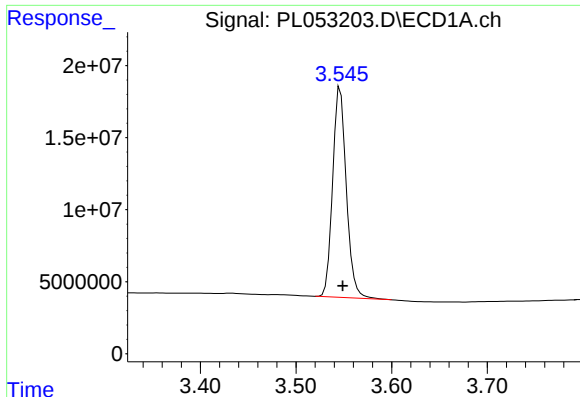

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 144555306
Conc: 15.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-02

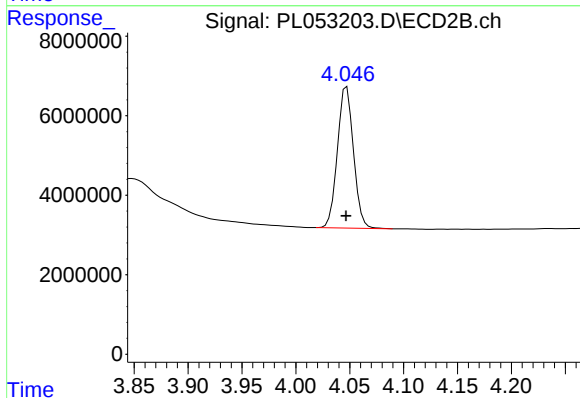


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 36844810
Conc: 14.67 ng/ml

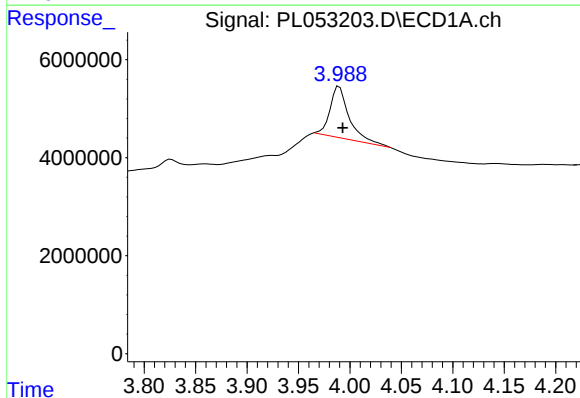


#2 alpha-BHC

R.T.: 3.990 min
Delta R.T.: -0.003 min
Response: 13230651
Conc: 0.94 ng/ml

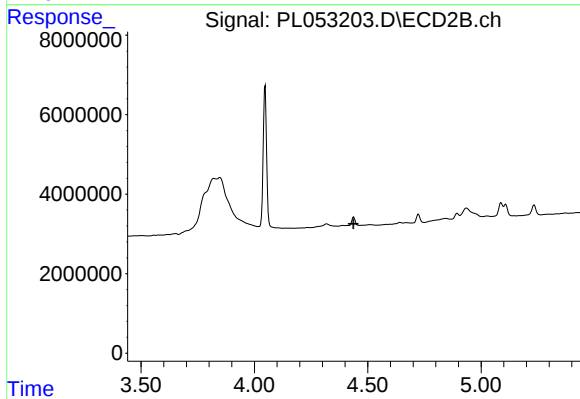

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.437 min
Response: 0
Conc: N.D.

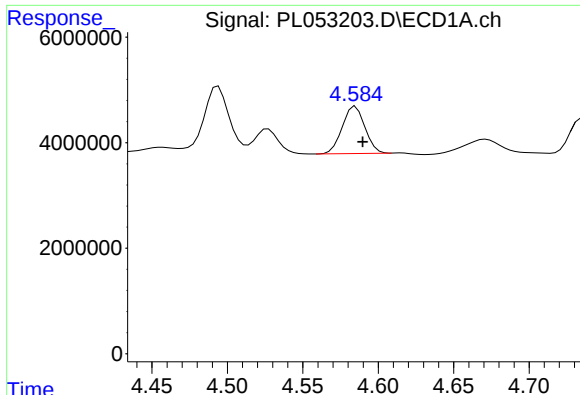

#4 Heptachlor


R.T.: 4.585 min
Delta R.T.: -0.005 min
Response: 9378592
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-02

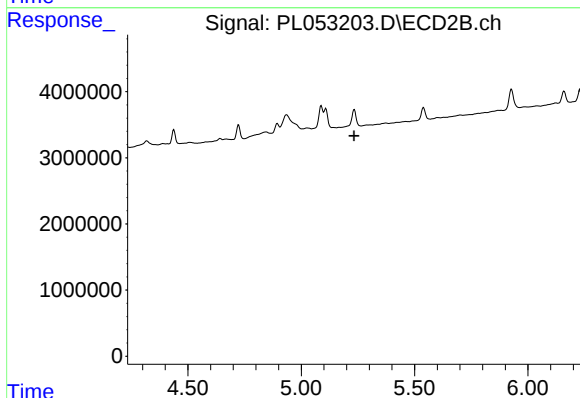


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

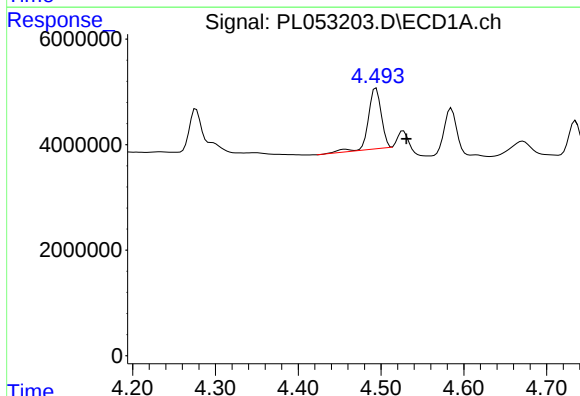


#6 beta-BHC

R.T.: 4.494 min
Delta R.T.: -0.037 min
Response: 12425135
Conc: 2.12 ng/ml

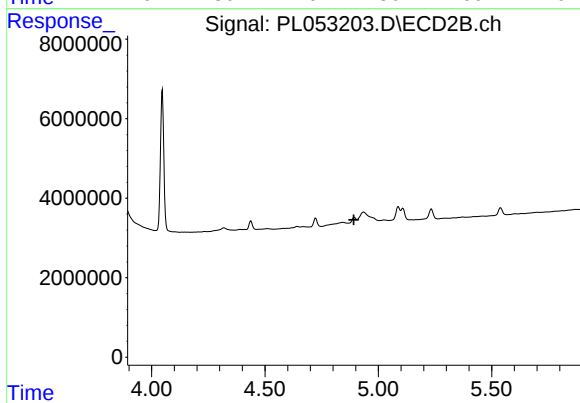

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.891 min
Response: 0
Conc: N.D.

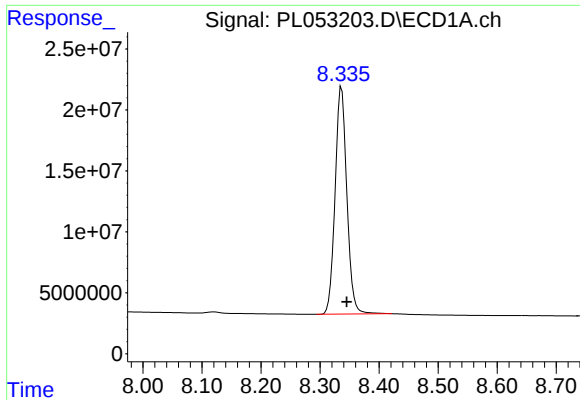

#27 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.009 min
Response: 258080799
Conc: 28.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-02

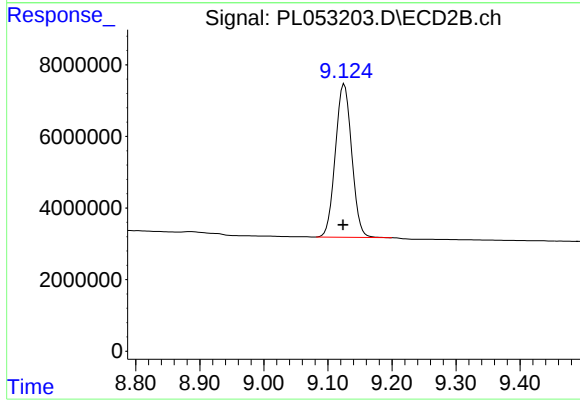

#27 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.002 min
Response: 75841426
Conc: 28.39 ng/ml