

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
 Data File : PL053204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 13:11
 Operator : SG\AJ
 Sample : MDL-W-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-W-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 13:45:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 05:45:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.047	162.9E6	41078586	17.505	16.358
27)	SA Decachlor...	8.336	9.125	293.5E6	85979944	32.379	32.190
Target Compounds							
2)	A alpha-BHC	3.989	0.000	12523768	0	0.888	N.D. #
3)	MA gamma-BHC...	4.277	0.000	11691806	0	0.905	N.D. #
4)	MA Heptachlor	4.584	0.000	10827206	0	0.793	N.D. #
5)	MB Aldrin	4.836	0.000	9313113	0	0.753	N.D. #
6)	B beta-BHC	4.494f	0.000	9346560	0	1.591	N.D. #
8)	B Heptachlo...	5.282	0.000	9850278	0	0.828	N.D. #
9)	A Endosulfan I	5.570f	0.000	9761544	0	0.885	N.D. #
10)	B trans-Chl...	5.570f	0.000	9761544	0	0.807	N.D. #
11)	B cis-Chlor...	5.570	0.000	9761544	0	0.832	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101019\
Data File : PL053204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 13:11
Operator : SG\AJ
Sample : MDL-W-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 13:45:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 05:45:16 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

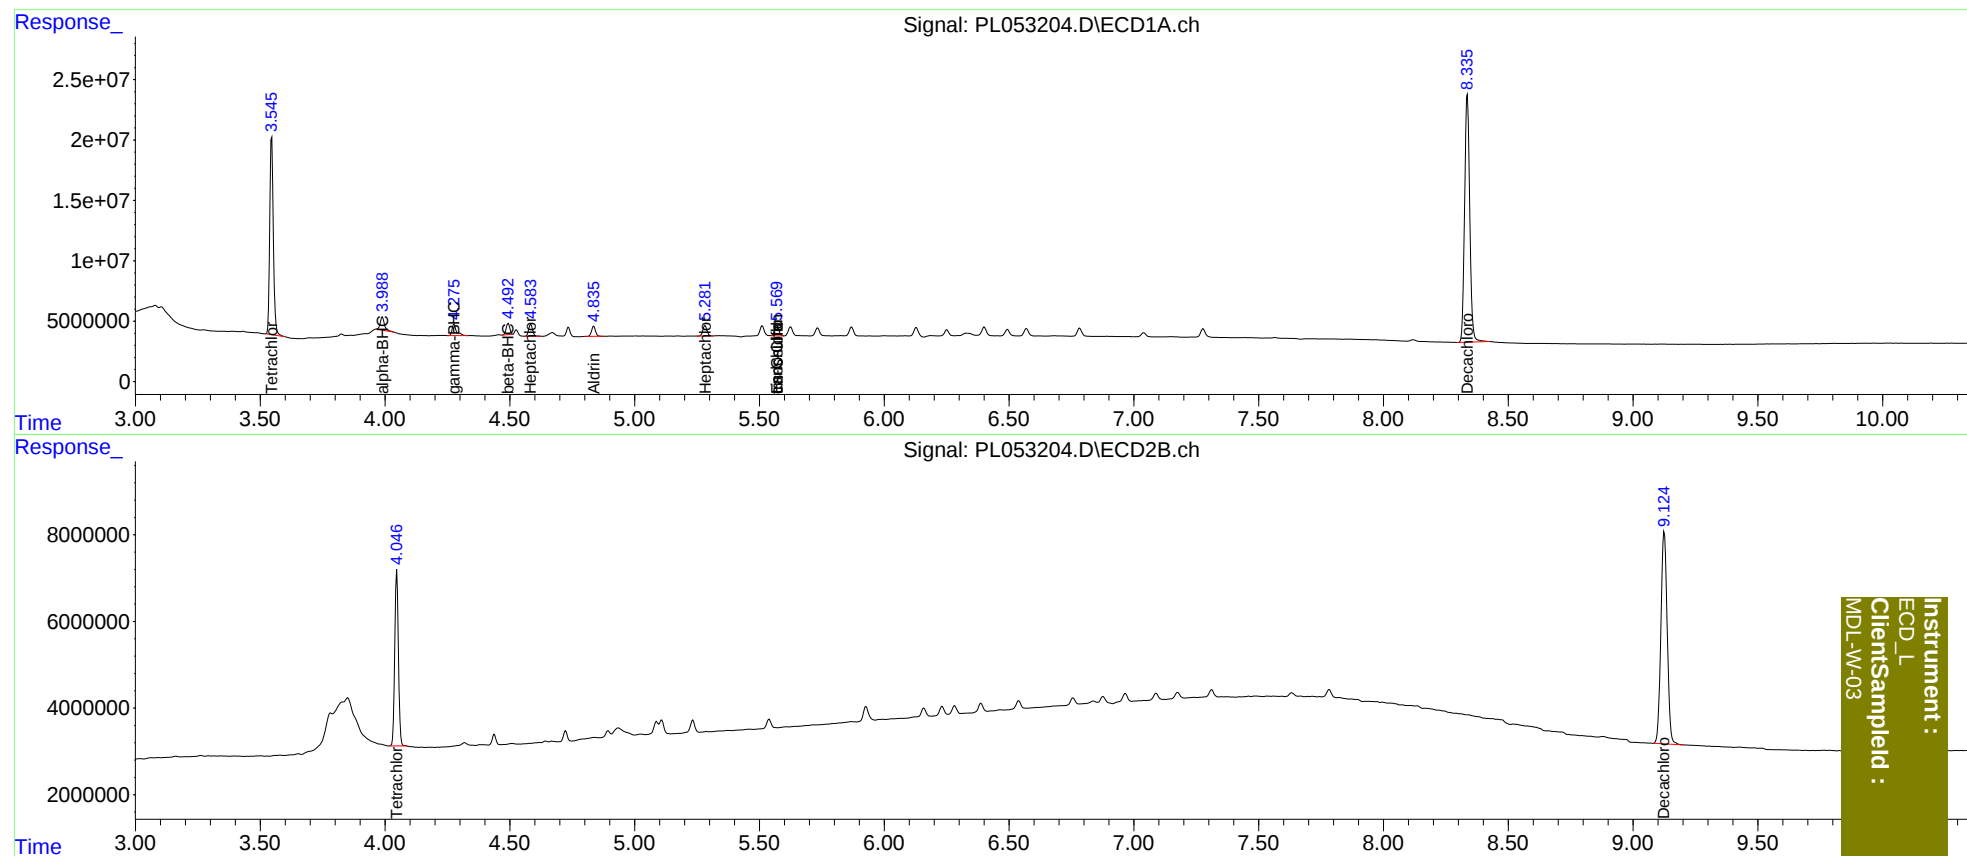


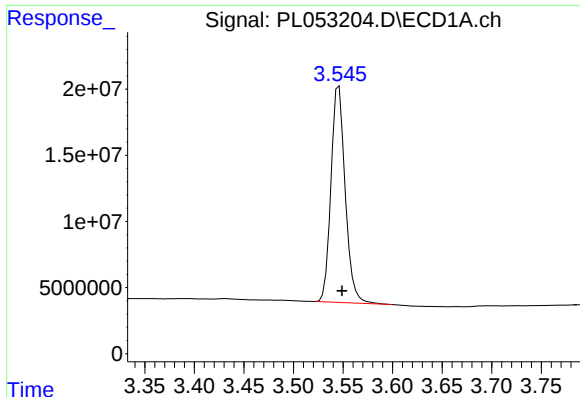

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 162910897
Conc: 17.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-03

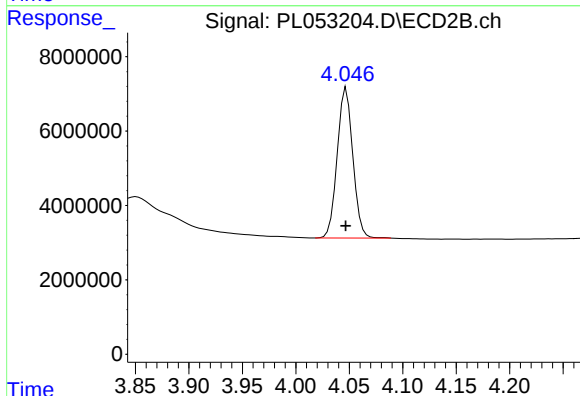


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 41078586
Conc: 16.36 ng/ml

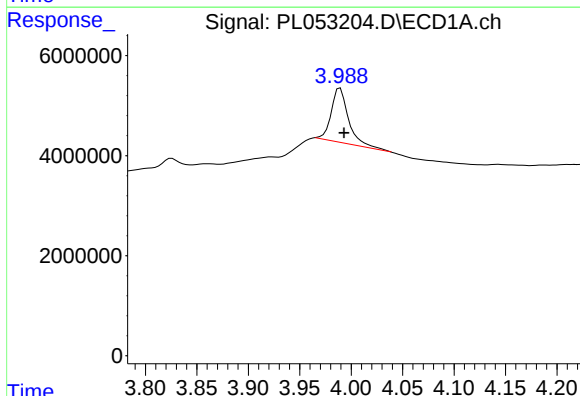


#2 alpha-BHC

R.T.: 3.989 min
Delta R.T.: -0.004 min
Response: 12523768
Conc: 0.89 ng/ml

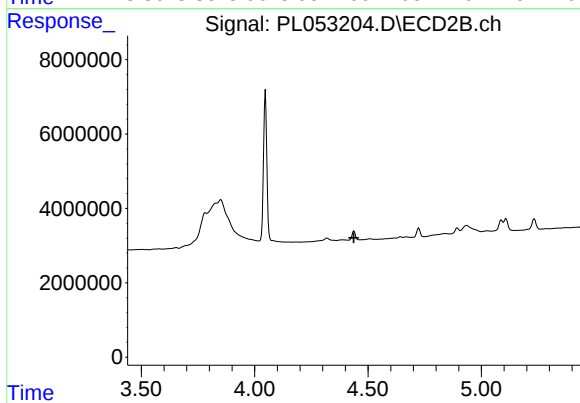

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.437 min
Response: 0
Conc: N.D.

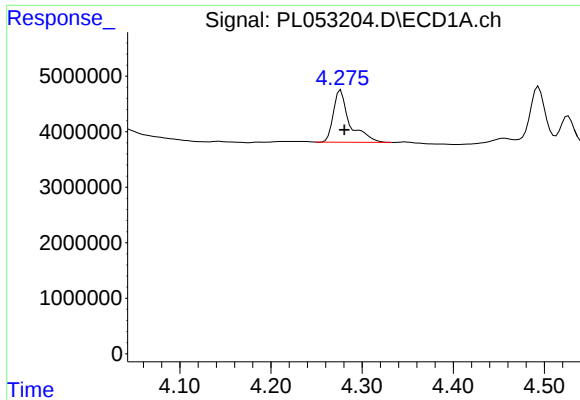

#3 gamma-BHC (Lindane)


R.T.: 4.277 min
Delta R.T.: -0.004 min
Response: 11691806
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-03

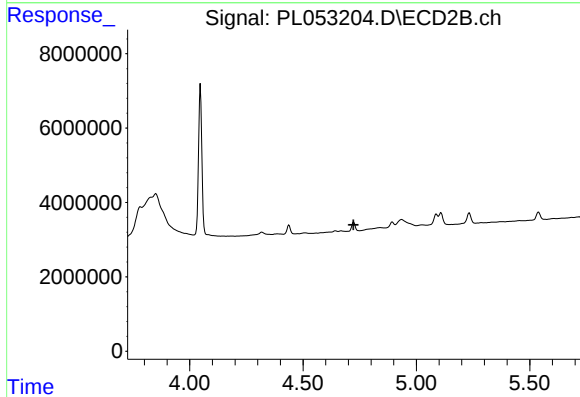


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

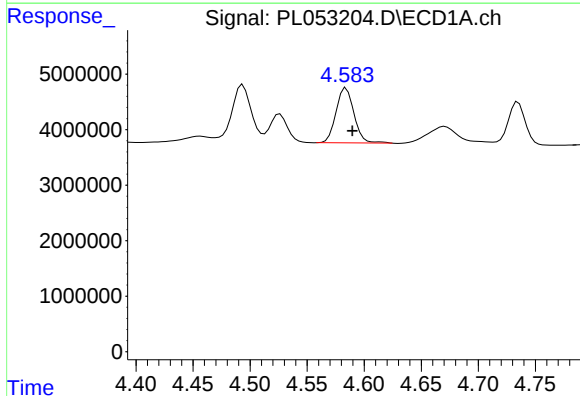


#4 Heptachlor

R.T.: 4.584 min
Delta R.T.: -0.006 min
Response: 10827206
Conc: 0.79 ng/ml

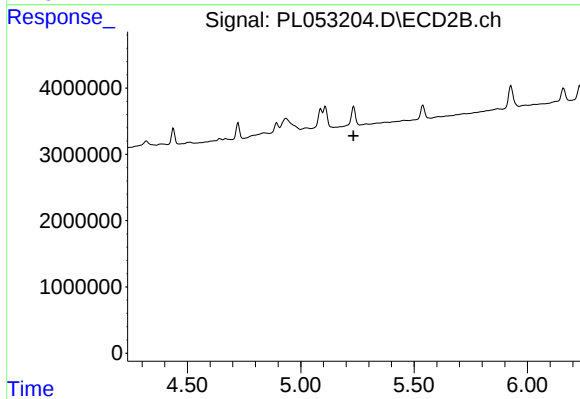

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

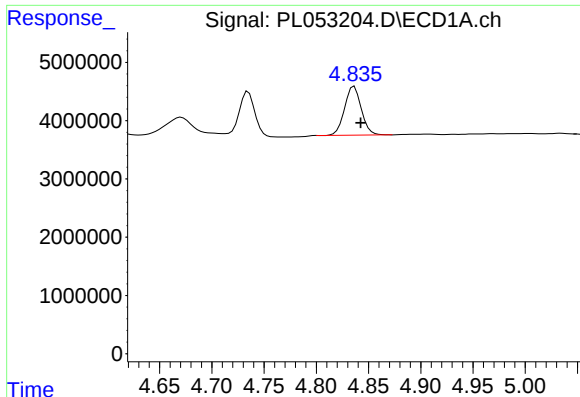

#5 Aldrin


R.T.: 4.836 min
Delta R.T.: -0.006 min
Response: 9313113
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-03

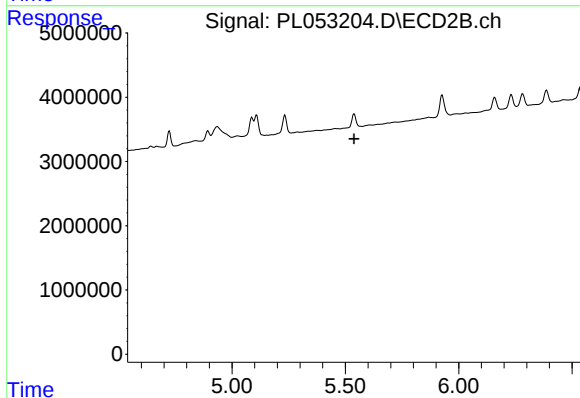


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.539 min
Response: 0
Conc: N.D.

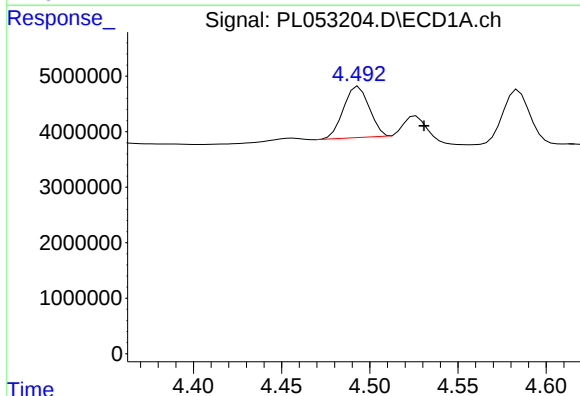


#6 beta-BHC

R.T.: 4.494 min
Delta R.T.: -0.037 min
Response: 9346560
Conc: 1.59 ng/ml

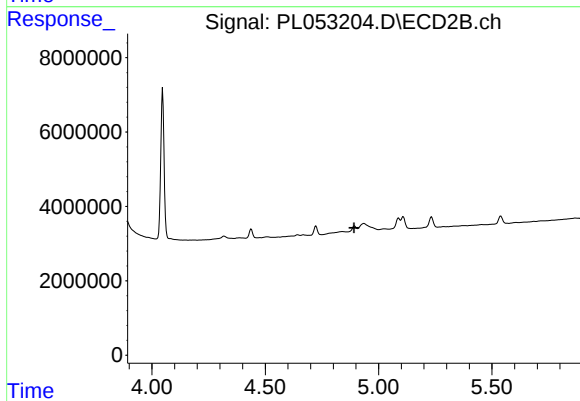

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.891 min
Response: 0
Conc: N.D.

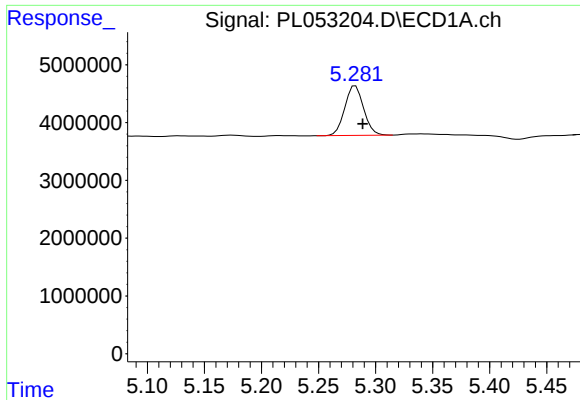

#8 Heptachlor epoxide


R.T.: 5.282 min
Delta R.T.: -0.006 min
Response: 9850278
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-03

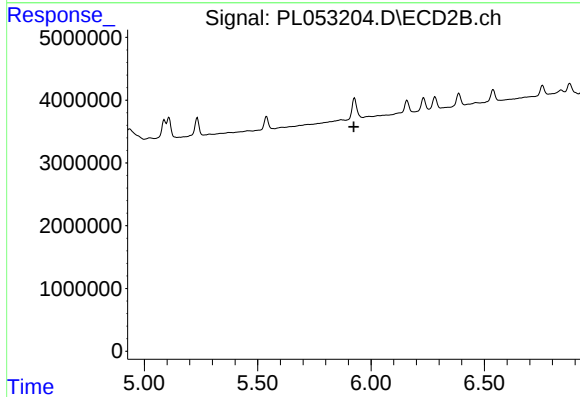


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

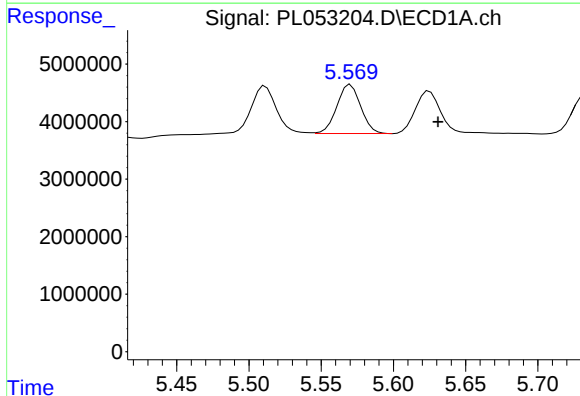


#9 Endosulfan I

R.T.: 5.570 min
Delta R.T.: -0.061 min
Response: 9761544
Conc: 0.88 ng/ml

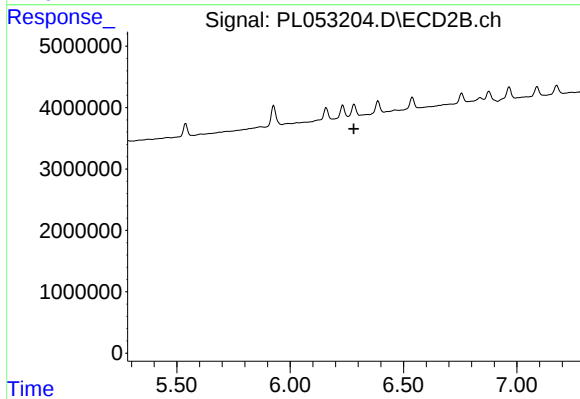

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

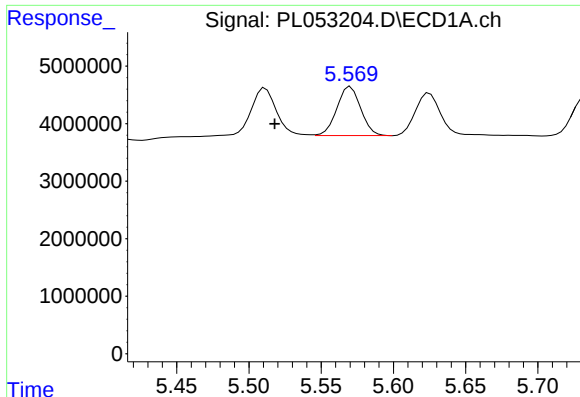

#10 trans-Chlordane


R.T.: 5.570 min
Delta R.T.: 0.052 min
Response: 9761544
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-03

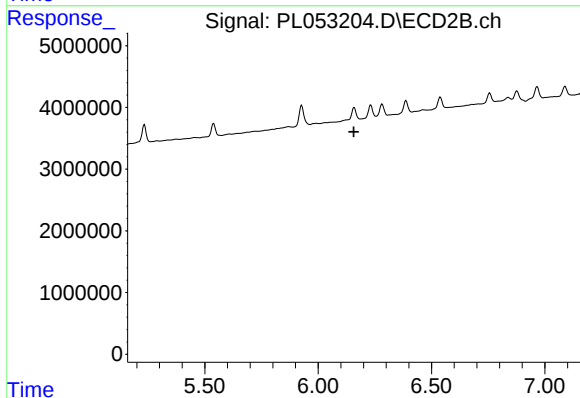


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

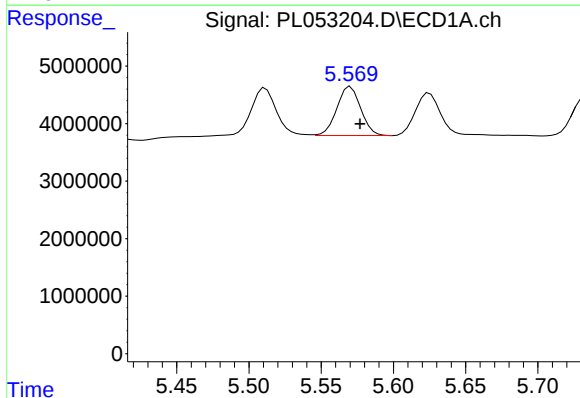


#11 cis-Chlordane

R.T.: 5.570 min
Delta R.T.: -0.006 min
Response: 9761544
Conc: 0.83 ng/ml

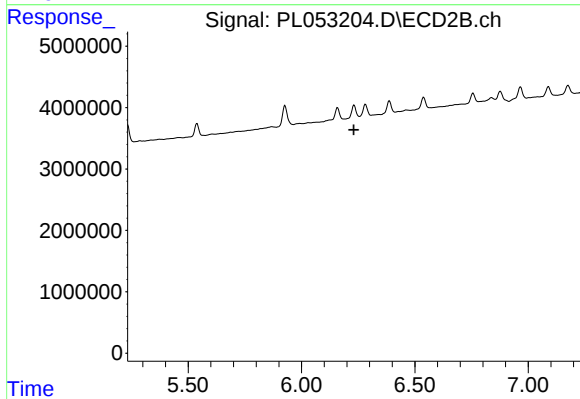

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

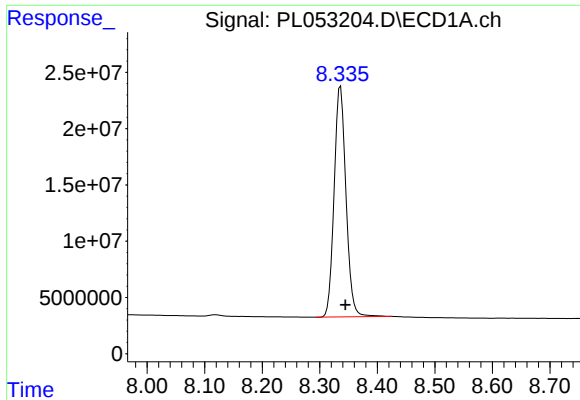

#27 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.009 min
Response: 293529884
Conc: 32.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-W-03

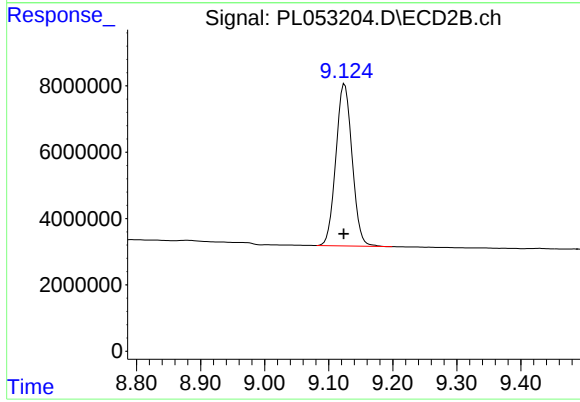

#27 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.001 min
Response: 85979944
Conc: 32.19 ng/ml