

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101020\
 Data File : PL062156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2020 10:48
 Operator : DD\AJ
 Sample : L1955-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-03

Manual Integrations
 APPROVED

Ankita
 10/13/2020 3:55:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:43:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 10 05:27:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	31512964	50555921	17.673	17.739
27)	SA Decachlor...	8.125	8.991	68564568	99153286	36.068	35.678
Target Compounds							
2)	A alpha-BHC	3.844	4.338	2904448	3335419	1.189	0.834 #
3)	MA gamma-BHC...	4.123	4.621	1730419	3250653	0.765	0.872
4)	MA Heptachlor	4.421	5.127	1883208	4941484	0.935	1.323 #
5)	MB Aldrin	4.665	5.429	1927449	2997474	1.053	0.889
6)	B beta-BHC	4.372	4.793	919010	2247269	0.964	1.251 #
7)	B delta-BHC	4.572	5.006	1814683	1785760	0.860	0.665
8)	B Heptachlo...	5.103	5.814	1656776	3352288	0.949	1.174
9)	A Endosulfan I	5.438	6.170	1528737	2913177	0.945	0.983
10)	B trans-Chl...	5.328	6.049	1707473	2555393	0.983	0.837
11)	B cis-Chlor...	5.386	6.121	1673112	2889983	0.961	0.935
12)	B 4,4'-DDE	5.551	6.279	1502128	2590913	0.916	0.872
13)	MA Dieldrin	5.678	6.427	1676165	2578735	0.940	0.841
14)	MA Endrin	5.931	6.643	1640504	1520389	1.028m	0.624 #
15)	B Endosulfa...	6.205	6.853	1571594	2641243	0.996	1.003m
16)	A 4,4'-DDD	6.062	6.767	1340965	1889910	0.960	0.806m
17)	MA 4,4'-DDT	6.301	7.068	675368	1851179	0.510	0.813 #
18)	B Endrin al...	6.372	6.976	1425987	2245611	1.050	1.005m
19)	B Endosulfa...	6.584	7.200	1652399	2649943	0.990	0.993
20)	A Methoxychlor	6.844	7.526	648173	1077301	0.792	0.810
21)	B Endrin ke...	7.070	7.669	1492652	2475373	0.880	0.951

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101020\
Data File : PL062156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2020 10:48
Operator : DD\AJ
Sample : L1955-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:43:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 10 05:27:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

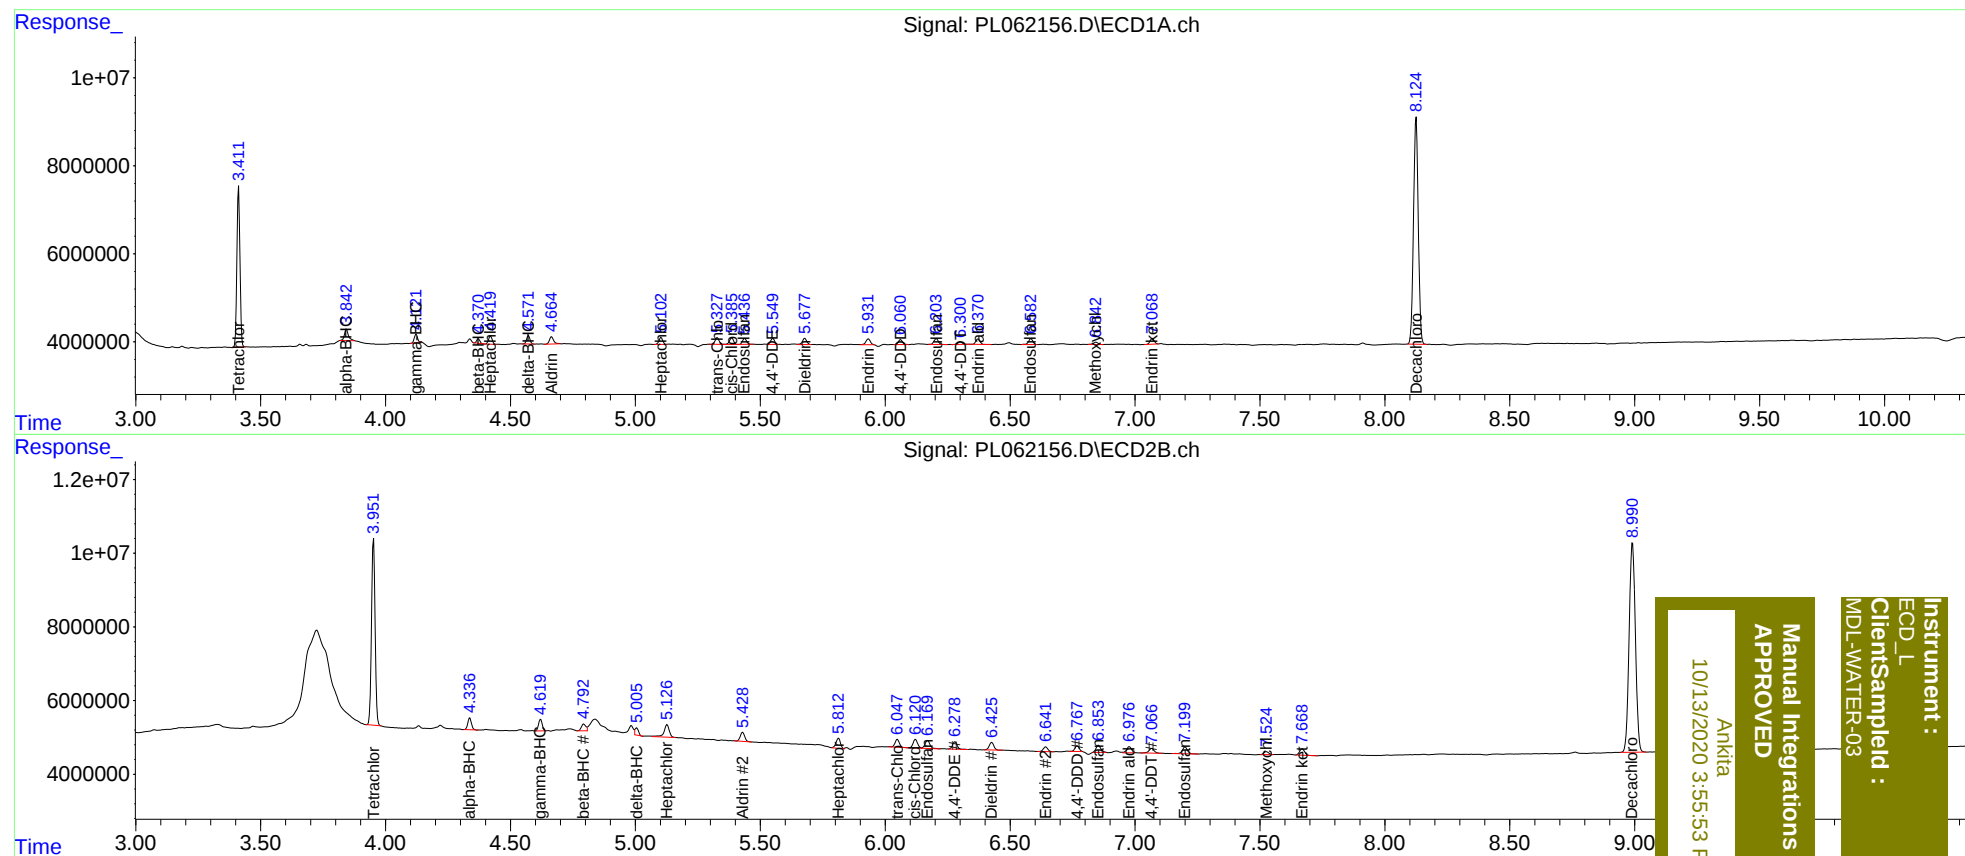

Manual Integrations
APPROVED

Ankita
10/13/2020 3:55:53 PM

Instrument :
ECD_L
Client/Sample :
MDL-WATER-03