

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101020\
 Data File : PL062165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2020 12:56
 Operator : DD\AJ
 Sample : MDL-TOX-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-TOX-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 08:32:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 10 05:27:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.952	37241482	60407480	20.886	21.196
27)	SA Decachlor...	8.127	8.992	81301517	119.2E6	42.768	42.885
Target Compounds							
22)	Toxaphene-1	5.644	6.331	1278699	1608104	120.544	117.850
23)	Toxaphene-2	5.803	6.619	820369	2231337	92.130	121.987 #
24)	Toxaphene-3	6.239	7.024	2771888	2259022	97.187	95.553
25)	Toxaphene-4	6.484	7.280	3314222	1708082	110.591	93.411
26)	Toxaphene-5	6.966	7.600	2785000	3236063	89.798	101.902

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101020\
Data File : PL062165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2020 12:56
Operator : DD\AJ
Sample : MDL-TOX-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 08:32:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 10 05:27:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

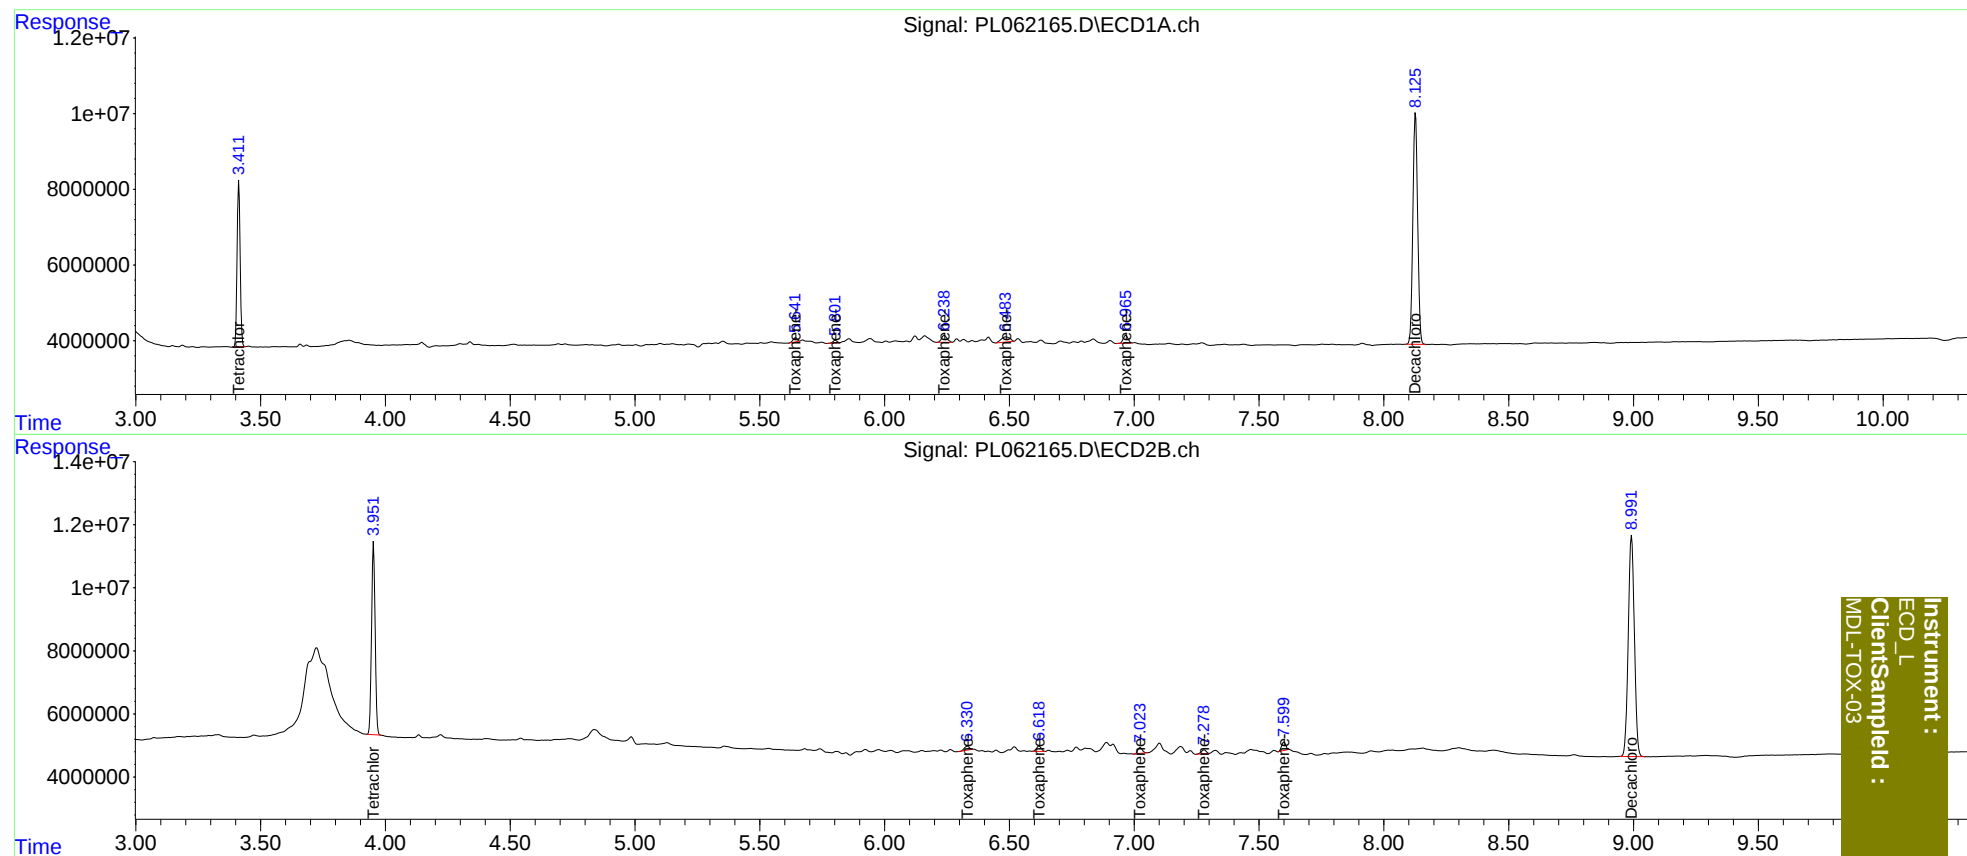

Instrument :
ECD_L
ClientSampleId :
MDL-TOX-03