

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101020\
 Data File : PL062155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2020 10:34
 Operator : DD\AJ
 Sample : L1955-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-02

Manual Integrations
 APPROVED

Ankita
 10/13/2020 3:55:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:43:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 10 05:27:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	32311066	51683711	18.121	18.135
27)	SA Decachlor...	8.126	8.990	70616345	102.4E6	37.148	36.837
Target Compounds							
2)	A alpha-BHC	3.844	4.337	2740470	3284444	1.122	0.821 #
3)	MA gamma-BHC...	4.124	4.620	1587875	3427070	0.702	0.919 #
4)	MA Heptachlor	4.421	5.127	1848255	4992287	0.918	1.337 #
5)	MB Aldrin	4.664	5.430	1754671	3116674	0.959m	0.924
6)	B beta-BHC	4.372	4.793	889745	2172562	0.934	1.209 #
7)	B delta-BHC	4.573	5.005	1818139	2170228	0.862	0.809
8)	B Heptachlo...	5.103	5.812	1800859	3303595	1.032	1.157m
9)	A Endosulfan I	5.438	6.171	1666153	2815188	1.030	0.950
10)	B trans-Chl...	5.328	6.049	1843613	2504310	1.061	0.820
11)	B cis-Chlor...	5.386	6.121	1792611	2979441	1.029	0.964
12)	B 4,4'-DDE	5.550	6.279	1544402	2790276	0.941	0.939
13)	MA Dieldrin	5.679	6.426	1796276	2838963	1.007	0.926
14)	MA Endrin	5.933	6.642	1626403	1624483	1.019m	0.667 #
15)	B Endosulfa...	6.205	6.852	1719777	2817704	1.090	1.070m
16)	A 4,4'-DDD	6.062	6.767	1411342	2291177	1.011	0.978m
17)	MA 4,4'-DDT	6.300	7.067	776312	2089094	0.587	0.918 #
18)	B Endrin al...	6.371	6.975	1474067	2213928	1.085m	0.991m
19)	B Endosulfa...	6.584	7.200	1729782	2608305	1.037	0.978
20)	A Methoxychlor	6.844	7.526	522967	1096963	0.639	0.825 #
21)	B Endrin ke...	7.070	7.668	1374073	2719552	0.811	1.045 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101020\
Data File : PL062155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2020 10:34
Operator : DD\AJ
Sample : L1955-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:43:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 10 05:27:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

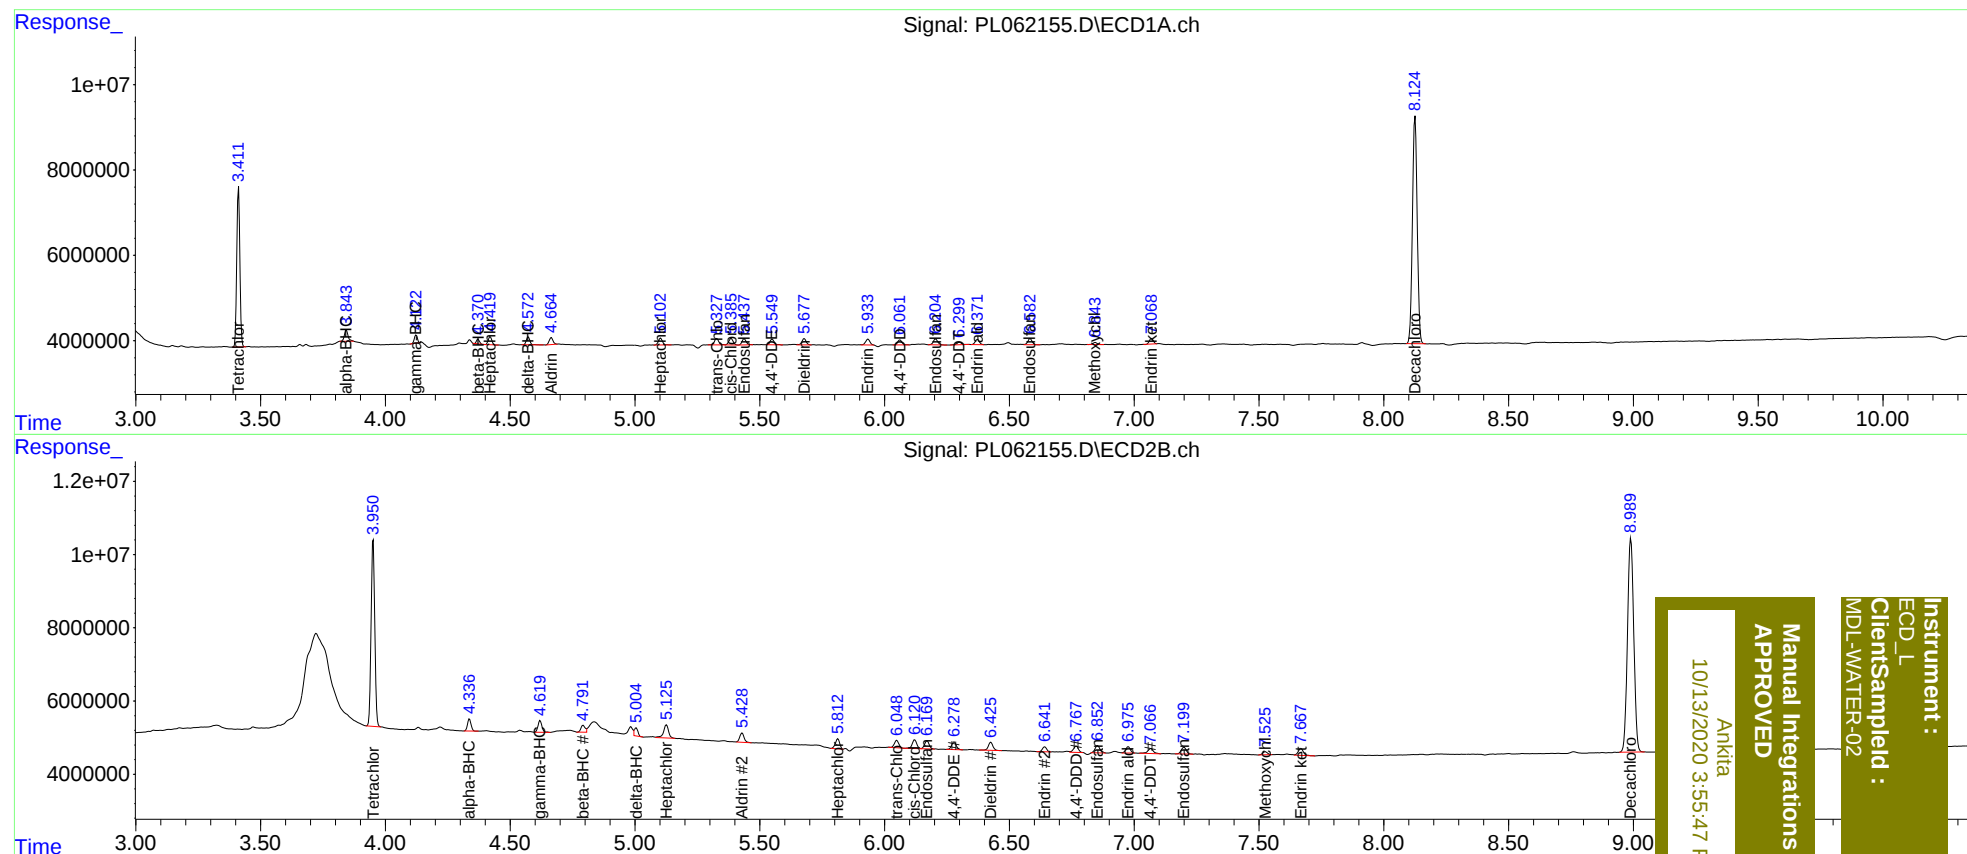

Manual Integrations
APPROVED

Ankita
10/13/2020 3:55:47 PM

Instrument :
ECD_L
Client Sample :
MDL-WATER-02