

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101023\
 Data File : PL085822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 17:53
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 20:46:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	2.621	144.4E6	54919032	48.558	58.793
28)	SA Decachlor...	8.860	7.775	116.6E6	52149715	53.523	56.501
Target Compounds							
23)	Chlordane-1	4.514	3.611	62115518	16082862	516.707	493.356
24)	Chlordane-2	5.046	4.188	66182983	21872849	508.928	562.084
25)	Chlordane-3	5.758	4.818	253.4E6	56710234	496.667	561.222
26)	Chlordane-4	5.841	4.880	312.0E6	61085538	491.718	527.581
27)	Chlordane-5	6.687	5.550	49547206	15614723	482.970	560.242


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101023\
Data File : PL085822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 17:53
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 20:46:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

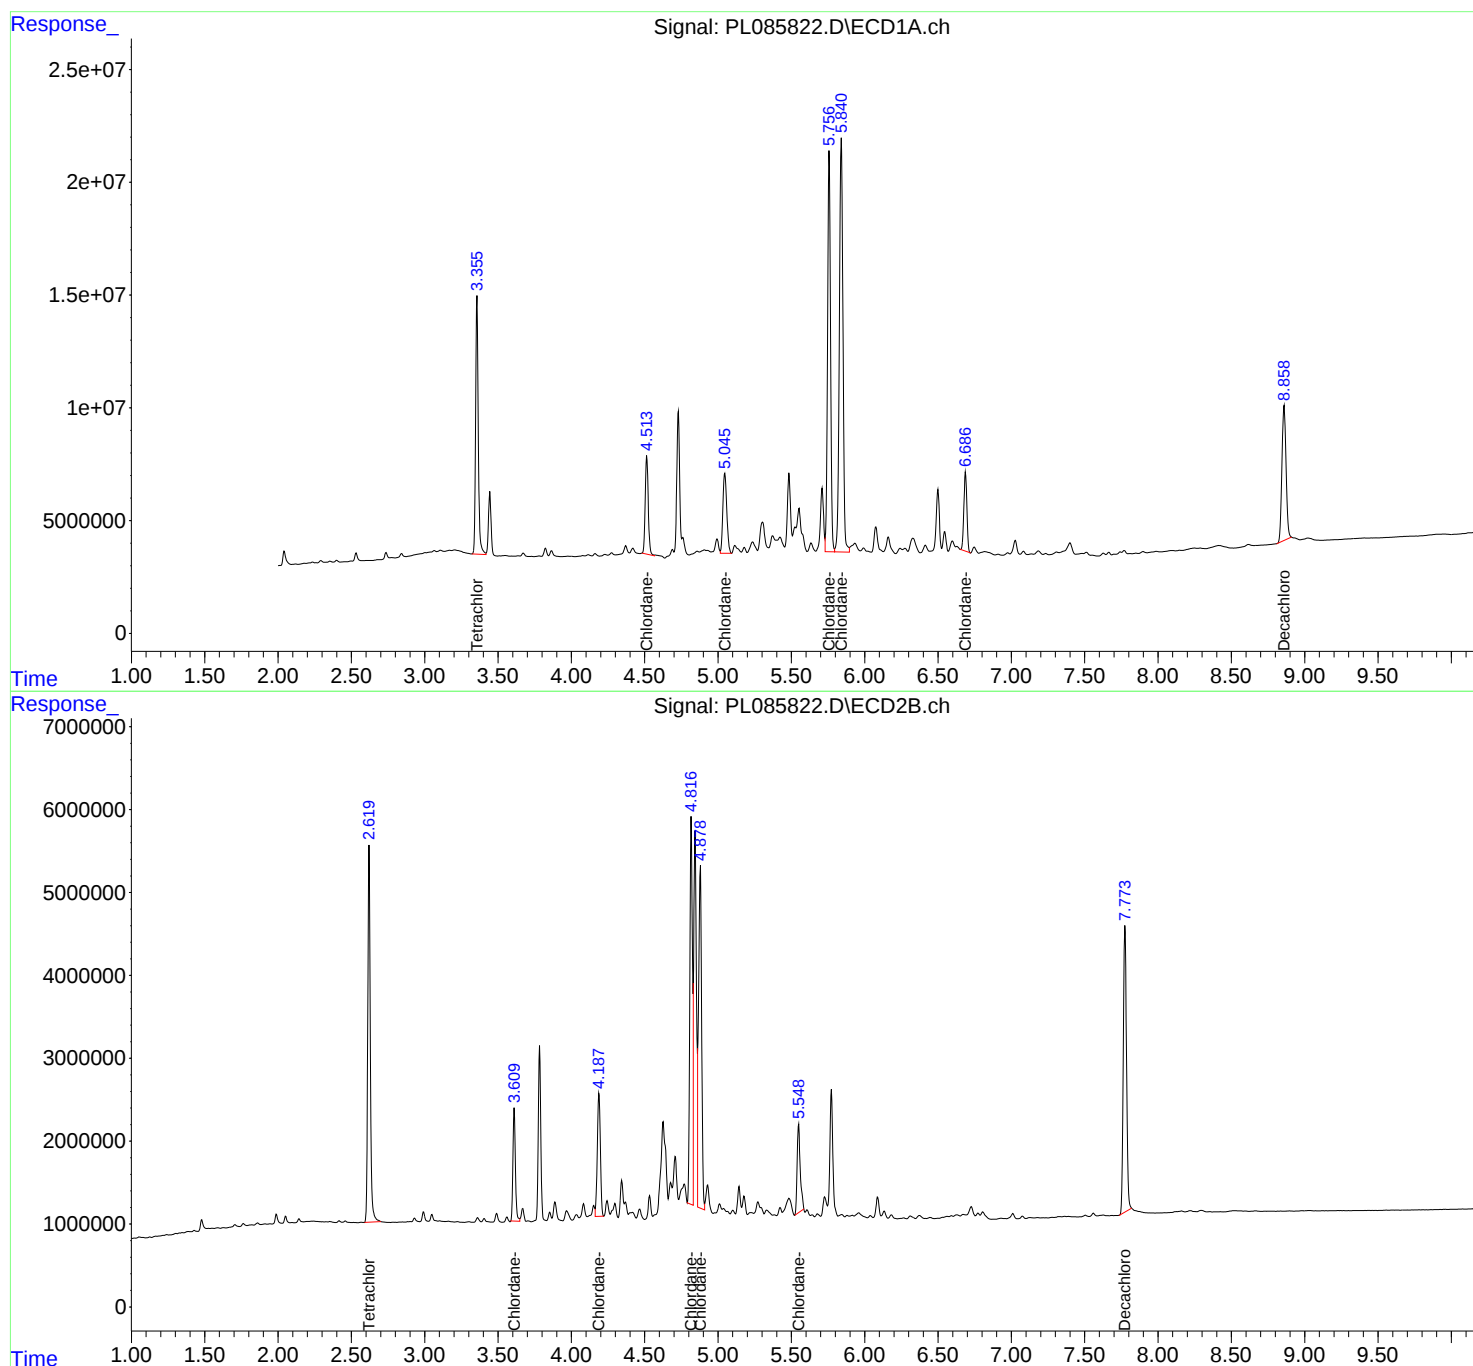


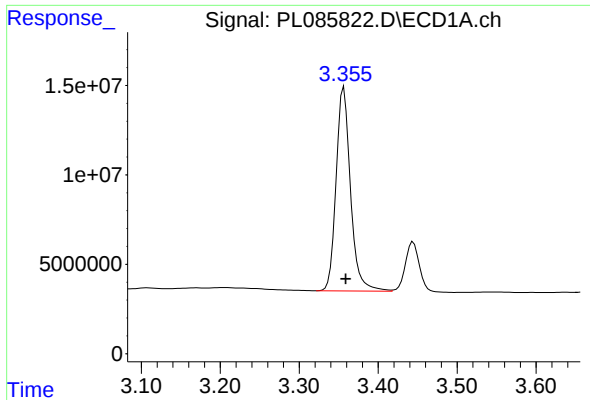

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.002 min
Response: 144419796
Conc: 48.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

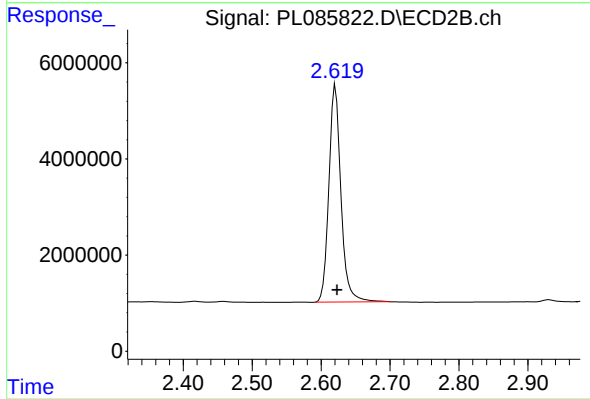


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 54919032
Conc: 58.79 ng/ml

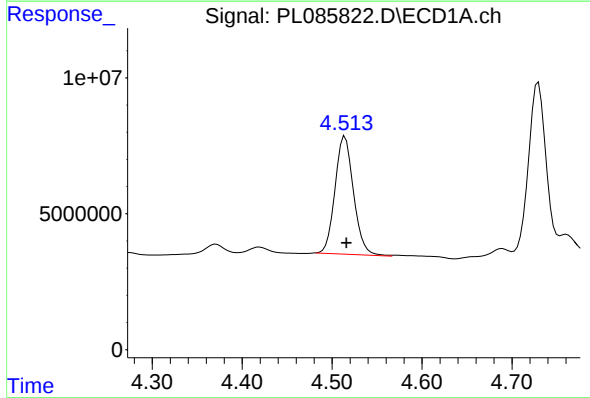


#23 Chlordane-1

R.T.: 4.514 min
Delta R.T.: -0.002 min
Response: 62115518
Conc: 516.71 ng/ml

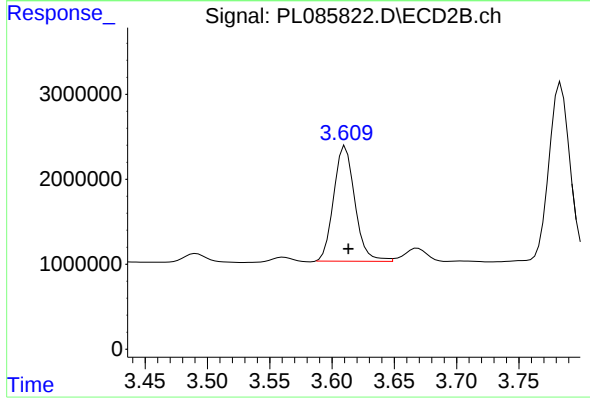

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: -0.003 min
Response: 16082862
Conc: 493.36 ng/ml

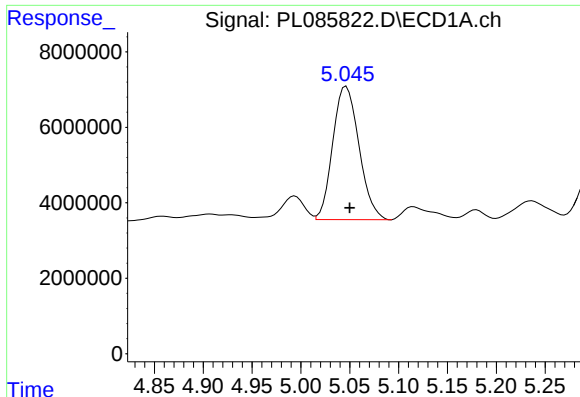

#24 Chlordane-2


R.T.: 5.046 min
Delta R.T.: -0.004 min
Response: 66182983
Conc: 508.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

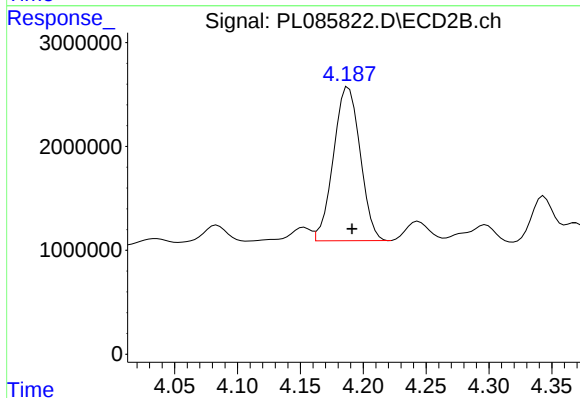


#24 Chlordane-2

R.T.: 4.188 min
Delta R.T.: -0.003 min
Response: 21872849
Conc: 562.08 ng/ml

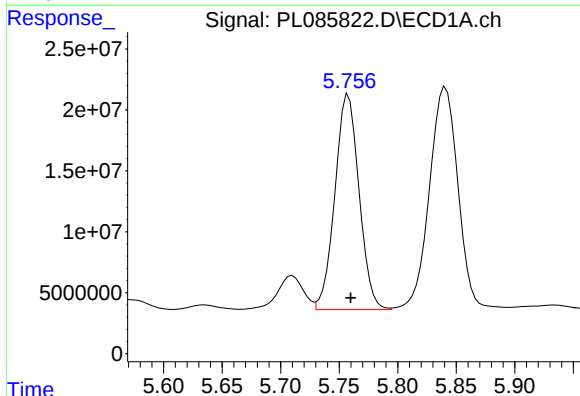


#25 Chlordane-3

R.T.: 5.758 min
Delta R.T.: -0.002 min
Response: 253399878
Conc: 496.67 ng/ml

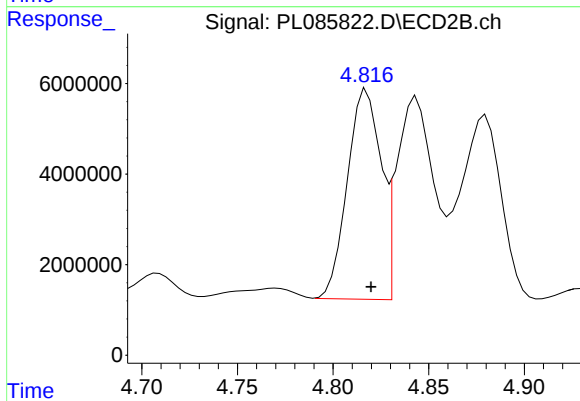

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: -0.002 min
Response: 56710234
Conc: 561.22 ng/ml

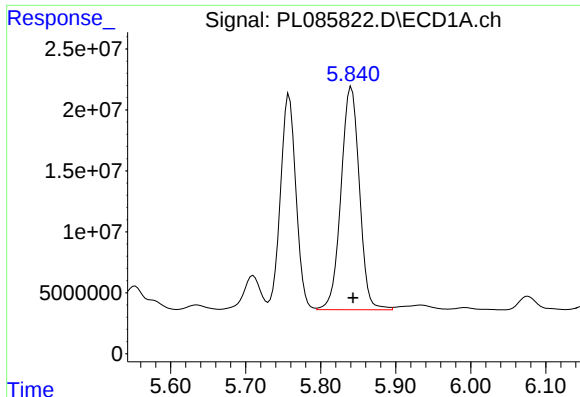

#26 Chlordane-4


R.T.: 5.841 min
Delta R.T.: -0.002 min
Response: 311966239
Conc: 491.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

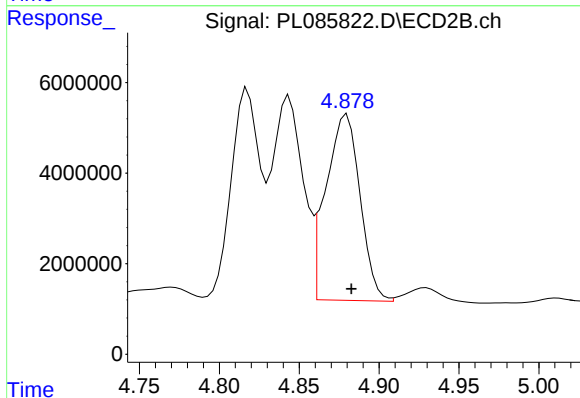


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: -0.003 min
Response: 61085538
Conc: 527.58 ng/ml

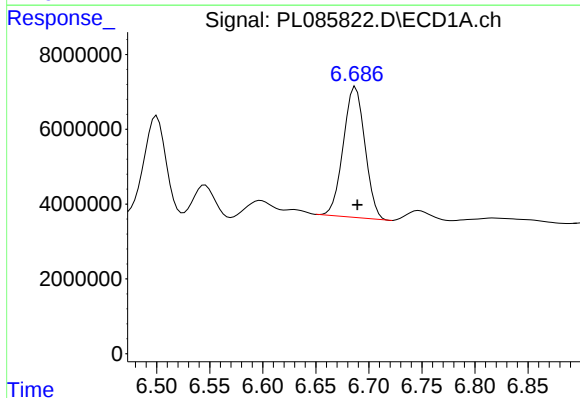


#27 Chlordane-5

R.T.: 6.687 min
Delta R.T.: -0.002 min
Response: 49547206
Conc: 482.97 ng/ml

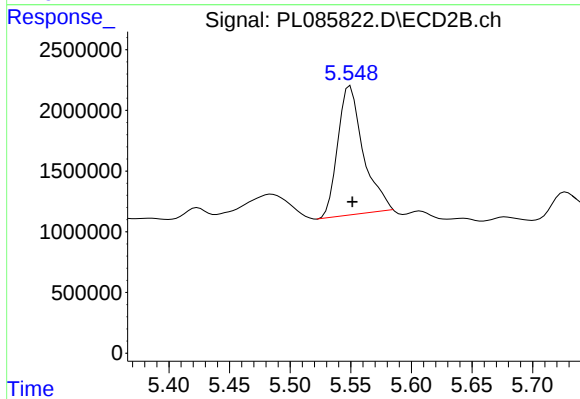

#27 Chlordane-5


R.T.: 5.550 min
Delta R.T.: -0.002 min
Response: 15614723
Conc: 560.24 ng/ml

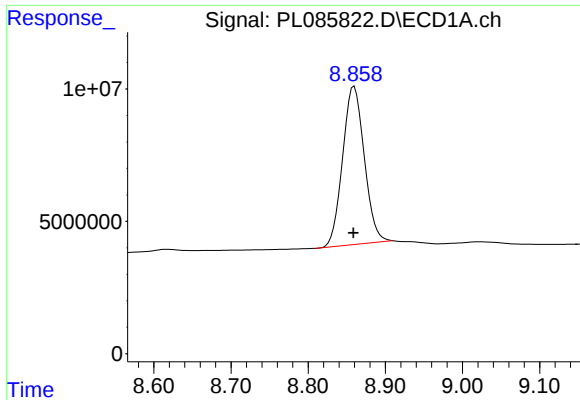

#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 116575856
Conc: 53.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

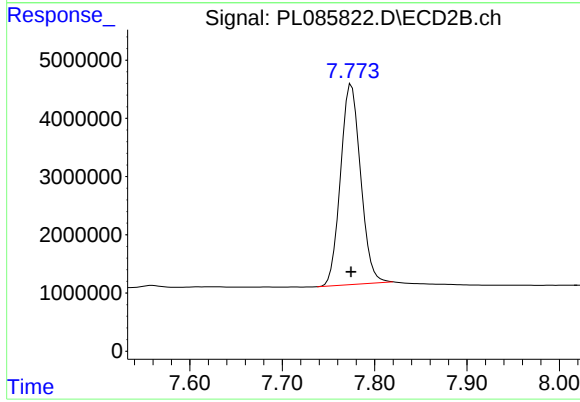

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 52149715
Conc: 56.50 ng/ml