

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101023\
 Data File : PL085829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 19:33
 Operator : AR\AJ
 Sample : 04805-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 H-1(0-5)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/11/2023
 Supervised By : Ankita Jodhani 10/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 20:52:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	2.623	25515307	10031682	8.579m	10.739 #
2)	SA Decachlor...	8.859	7.775	35711110	12798190	16.396	13.866

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101023\
Data File : PL085829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 19:33
Operator : AR\AJ
Sample : 04805-04
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
H-1(0-5)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/11/2023
Supervised By : Ankita Jodhani 10/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 20:52:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

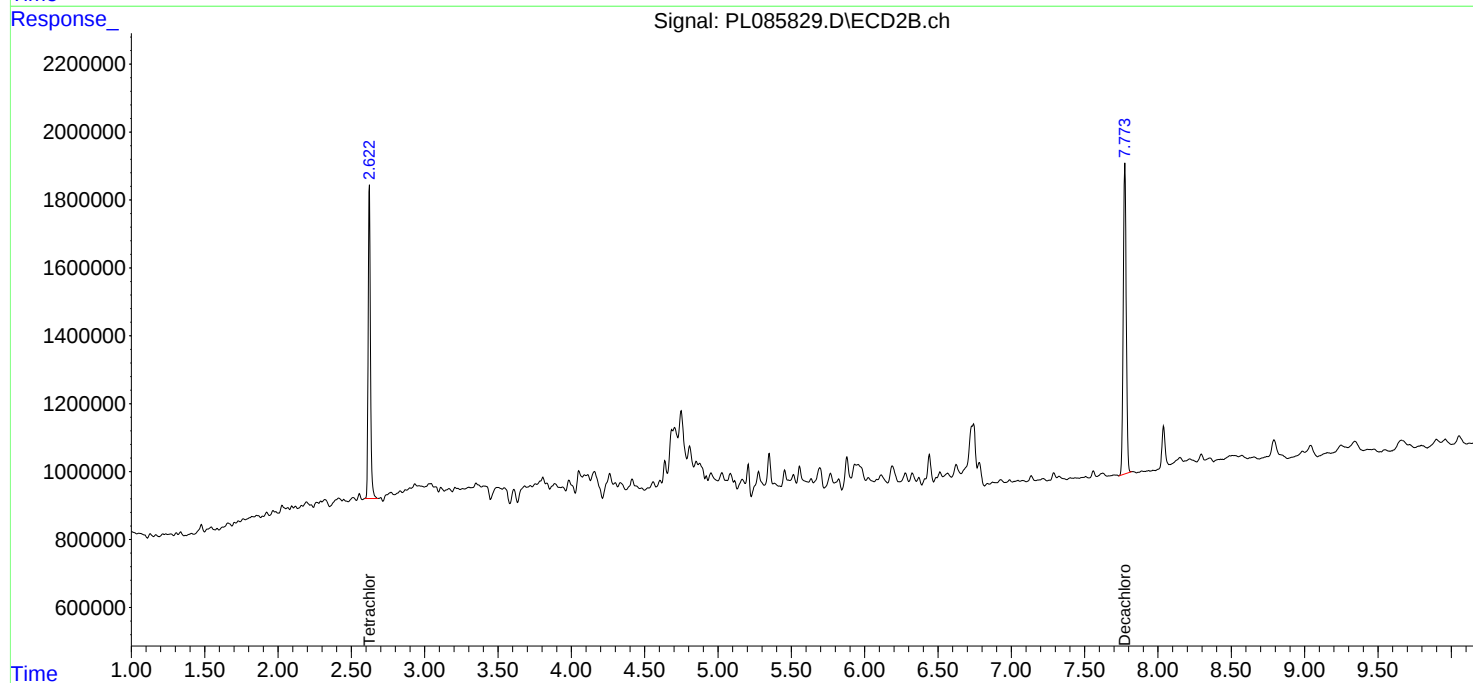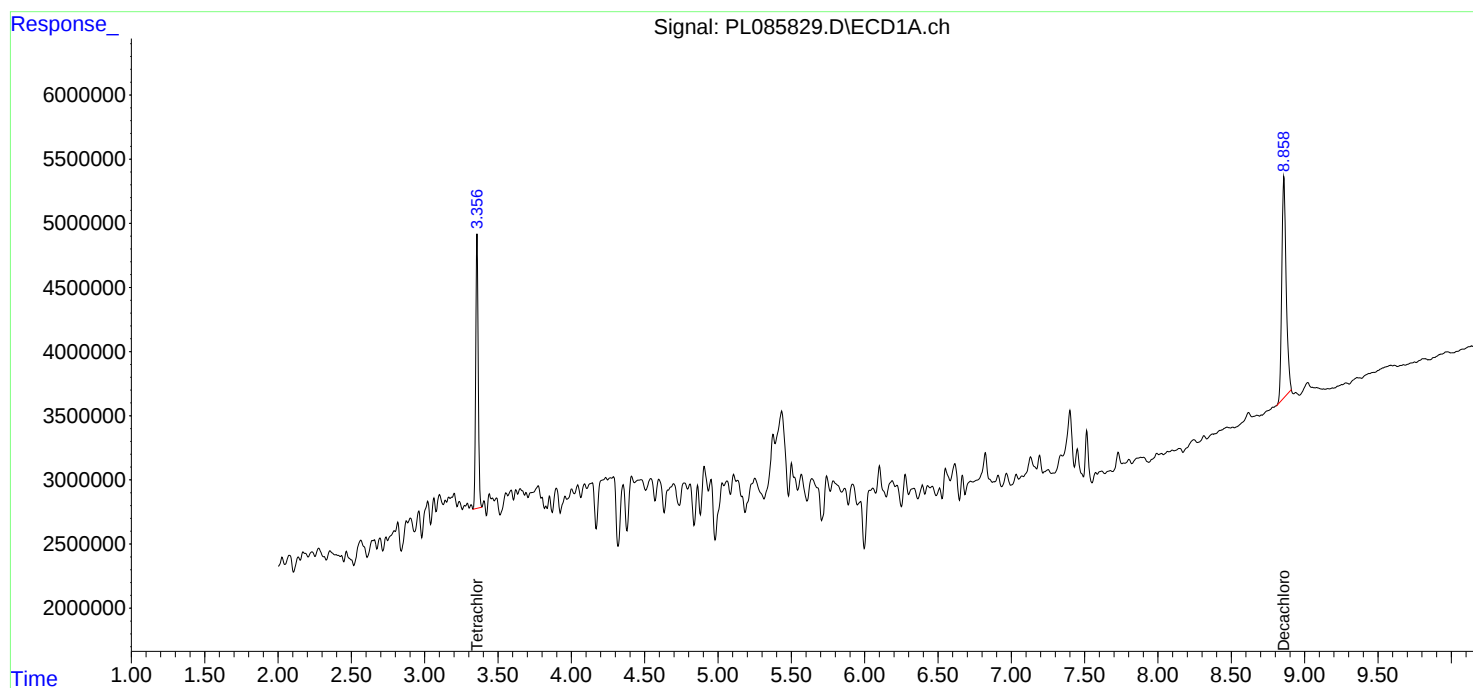

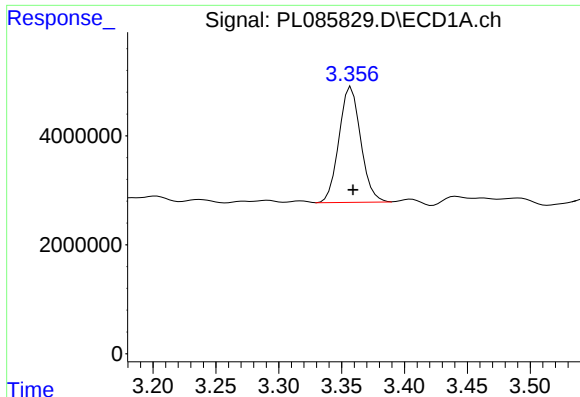


#1 Tetrachloro-m-xylene

R.T.: 3.356 min
Delta R.T.: -0.003 min
Response: 25515307
Conc: 8.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
H-1(0-5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/11/2023
Supervised By :Ankita Jodhani 10/11/2023

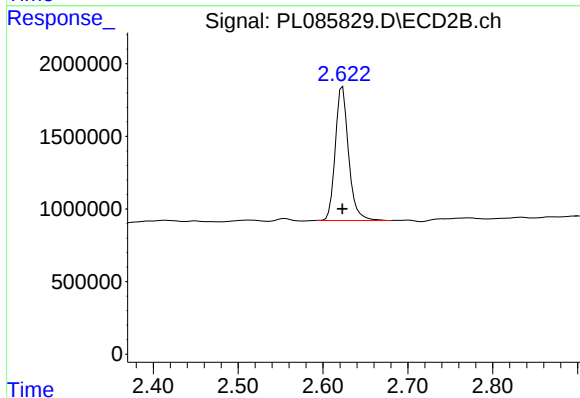


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 10031682
Conc: 10.74 ng/ml

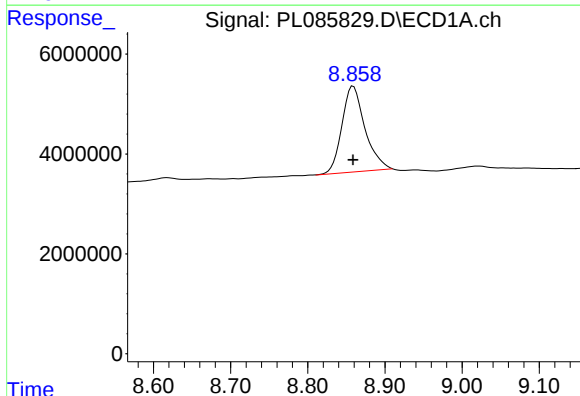

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 35711110
Conc: 16.40 ng/ml

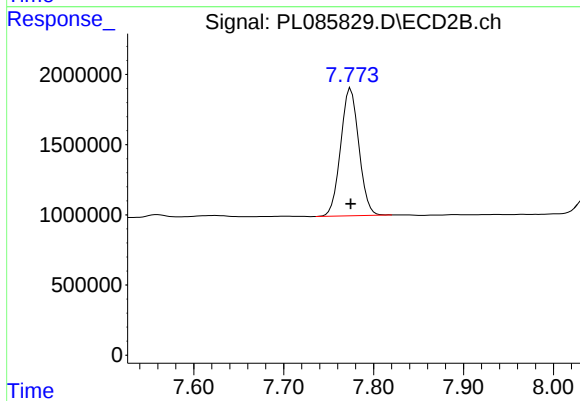

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 12798190
Conc: 13.87 ng/ml