

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101118\
 Data File : PL040909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2018 13:00
 Operator : AJ\SJ
 Sample : J5326-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 13:13:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.480	4.105	112.7E6	58481841	20.564	20.974
28)	SA Decachlor...	8.233	9.237	99722516	48982517	19.179	18.943
Target Compounds							
6)	B beta-BHC	4.421f	4.995f	6096960	8775614	1.922	5.475 #
7)	B delta-BHC	0.000	5.151f	0	316293	N.D.	0.096 #
8)	B Heptachlo...	0.000	5.992	0	16660065	N.D.	5.809 #
14)	MA Endrin	6.044	0.000	37925097	0	6.603	N.D. #
15)	B Endosulfa...	6.240f	0.000	17902946	0	3.194	N.D. #
16)	A 4,4'-DDD	0.000	6.917f	0	12355181	N.D.	5.898 #
23)	Chlordane-1	4.421	5.151	6096960	316293	23.889	2.561 #
24)	Chlordane-2	0.000	5.515	0	1382154	N.D.	11.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101118\
Data File : PL040909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2018 13:00
Operator : AJ\SJ
Sample : J5326-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 13:13:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

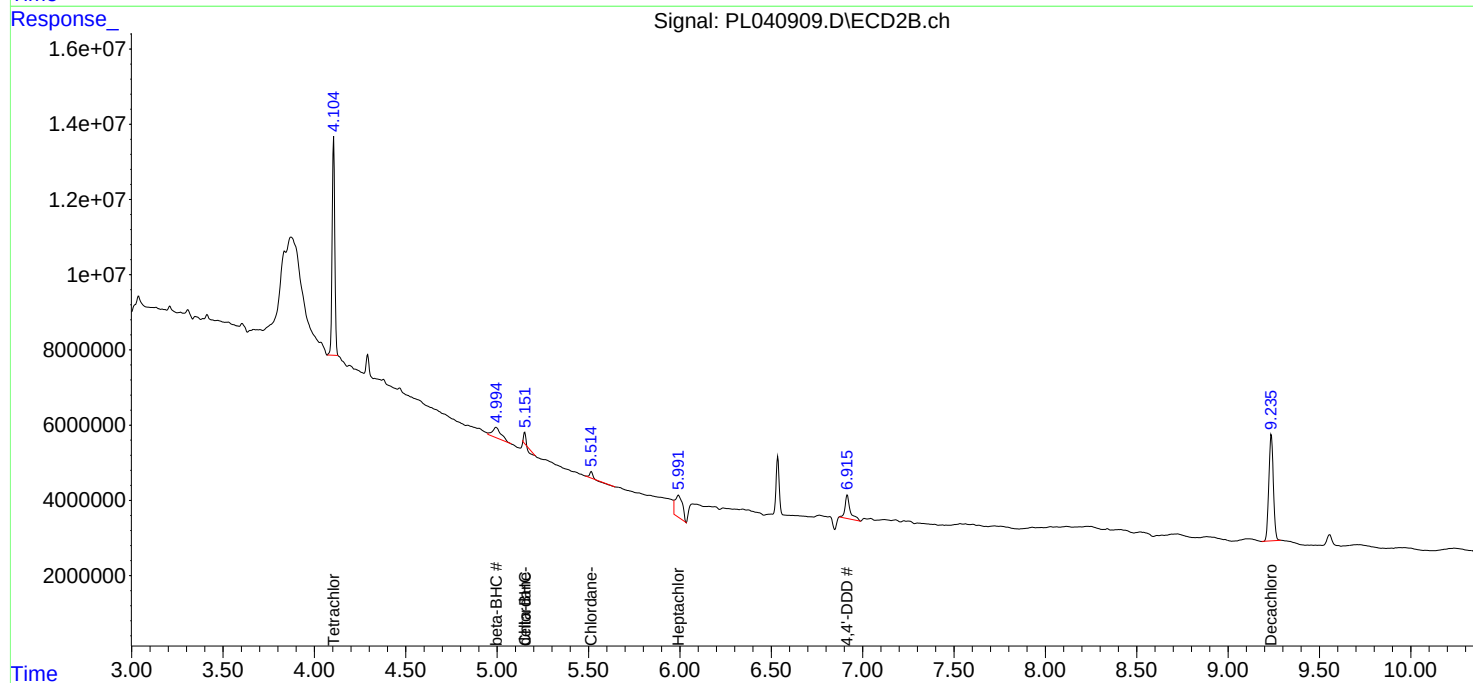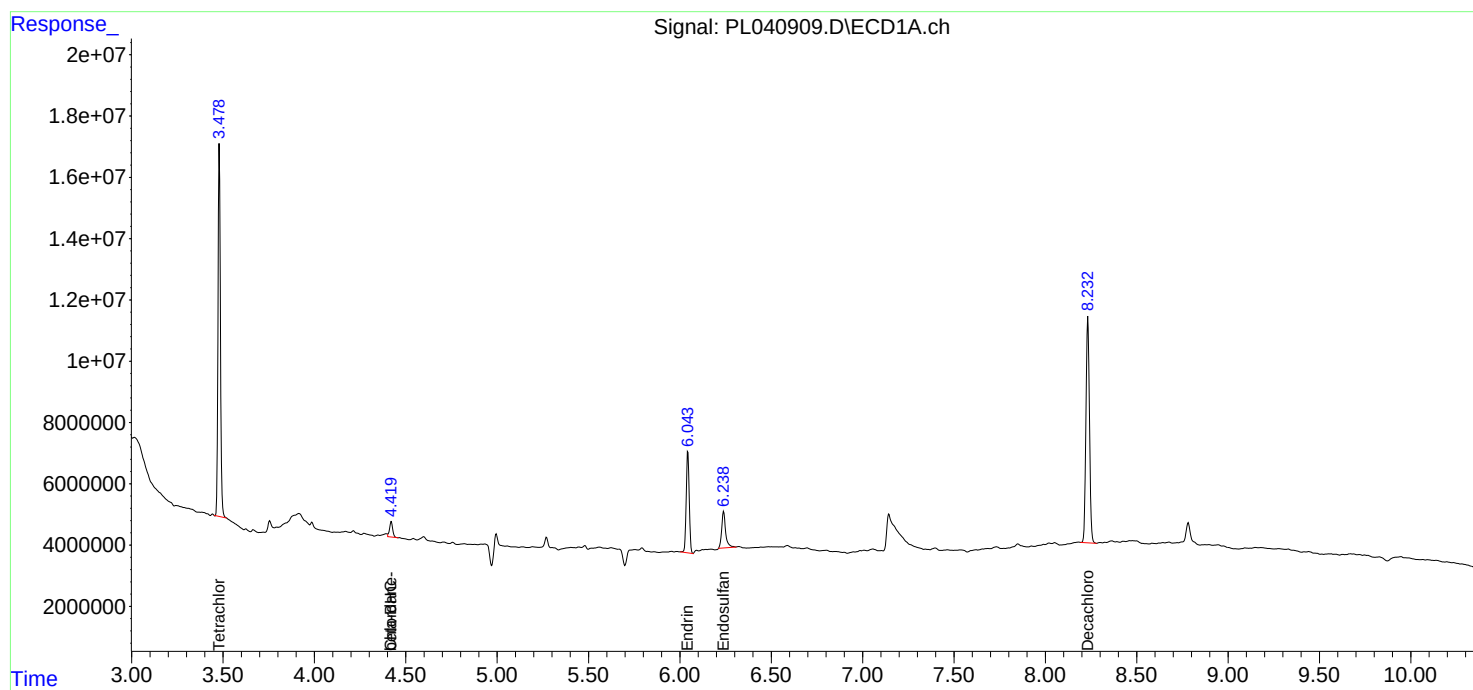


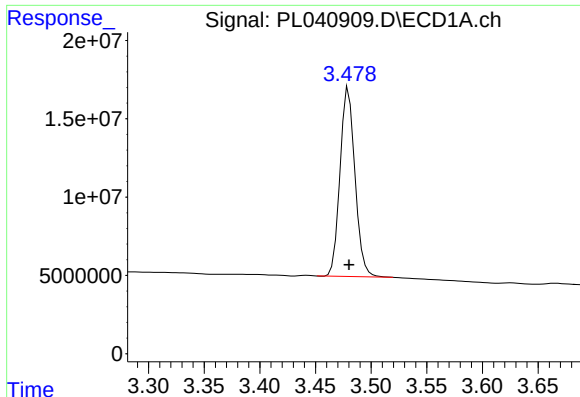

#1 Tetrachloro-m-xylene


R.T.: 3.480 min
Delta R.T.: 0.000 min
Response: 112705262
Conc: 20.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

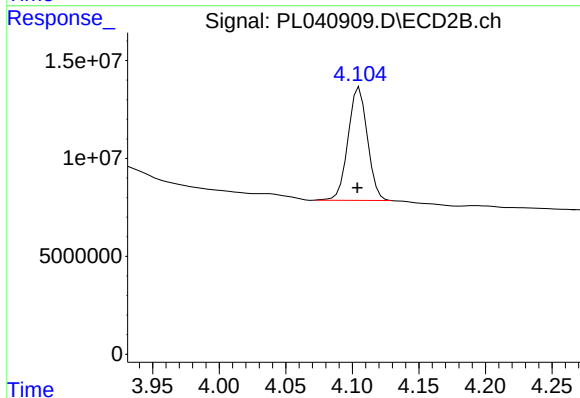


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.002 min
Response: 58481841
Conc: 20.97 ng/ml

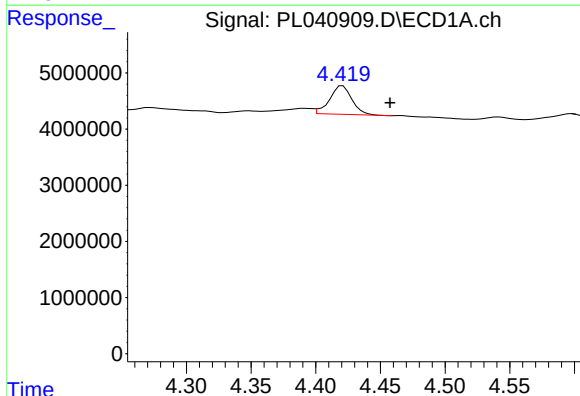


#6 beta-BHC

R.T.: 4.421 min
Delta R.T.: -0.037 min
Response: 6096960
Conc: 1.92 ng/ml

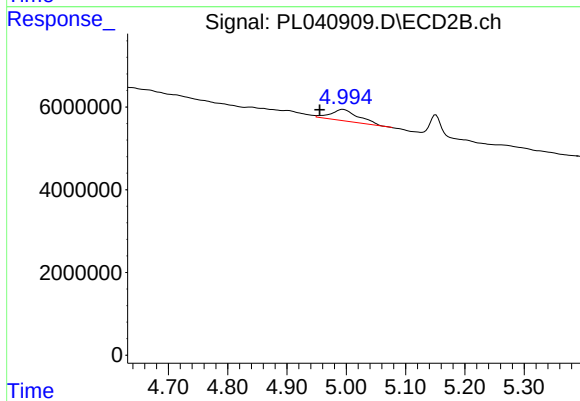

#6 beta-BHC


R.T.: 4.995 min
Delta R.T.: 0.040 min
Response: 8775614
Conc: 5.48 ng/ml

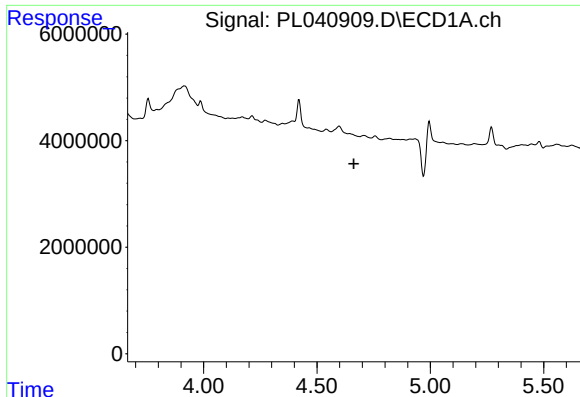

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

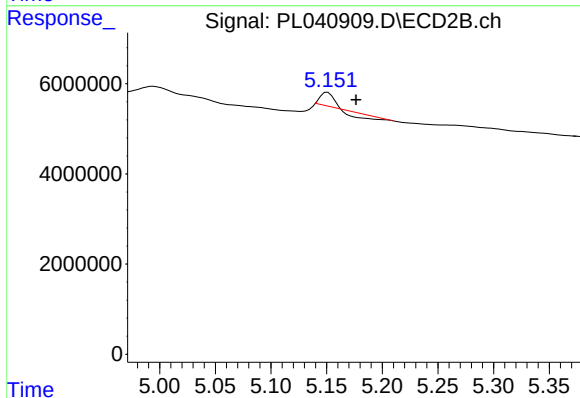


#7 delta-BHC

R.T.: 5.151 min
Delta R.T.: -0.025 min
Response: 316293
Conc: 0.10 ng/ml

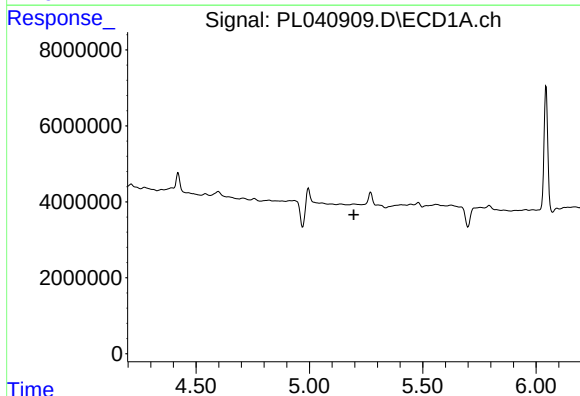


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.196 min
Response: 0
Conc: N.D.

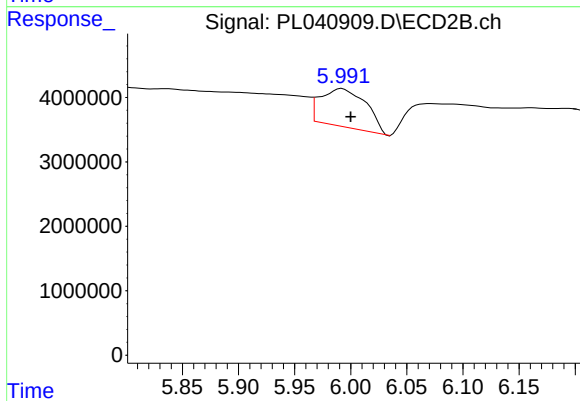

#8 Heptachlor epoxide


R.T.: 5.992 min
Delta R.T.: -0.008 min
Response: 16660065
Conc: 5.81 ng/ml

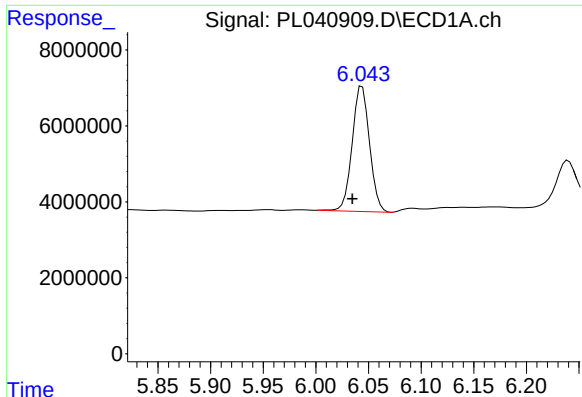

#14 Endrin


R.T.: 6.044 min
Delta R.T.: 0.009 min
Response: 37925097
Conc: 6.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

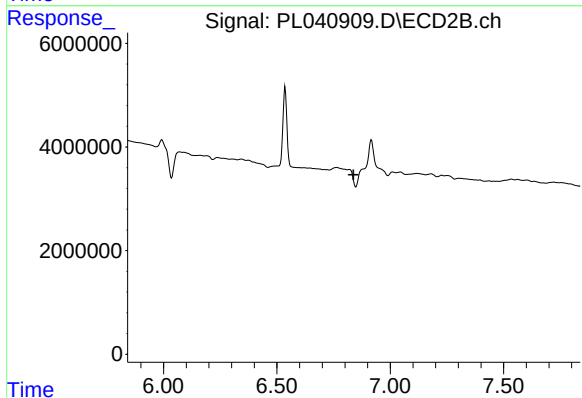


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

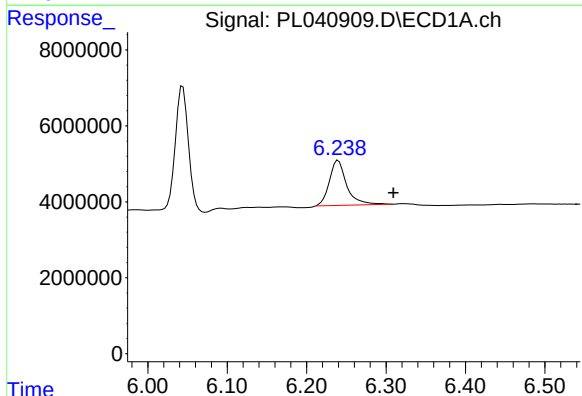


#15 Endosulfan II

R.T.: 6.240 min
Delta R.T.: -0.069 min
Response: 17902946
Conc: 3.19 ng/ml

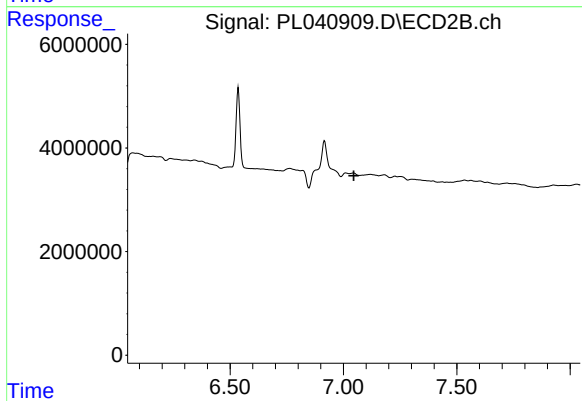

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

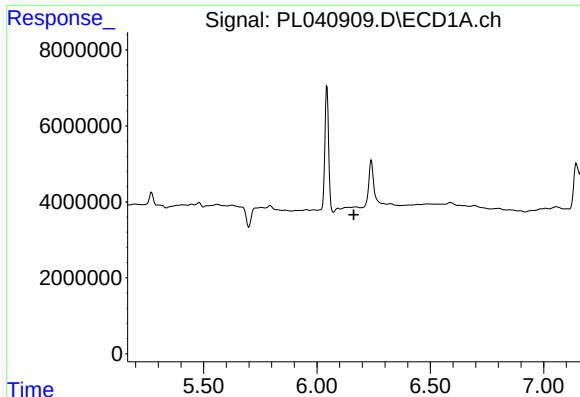

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

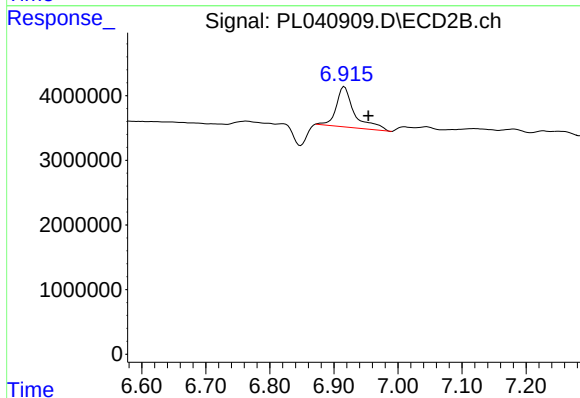


#16 4,4'-DDD

R.T.: 6.917 min
Delta R.T.: -0.037 min
Response: 12355181
Conc: 5.90 ng/ml

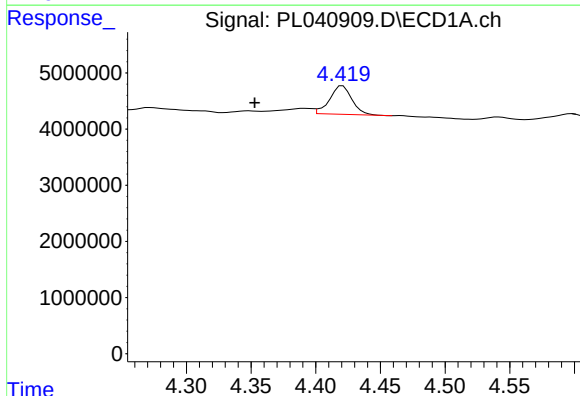


#23 Chlordane-1

R.T.: 4.421 min
Delta R.T.: 0.068 min
Response: 6096960
Conc: 23.89 ng/ml

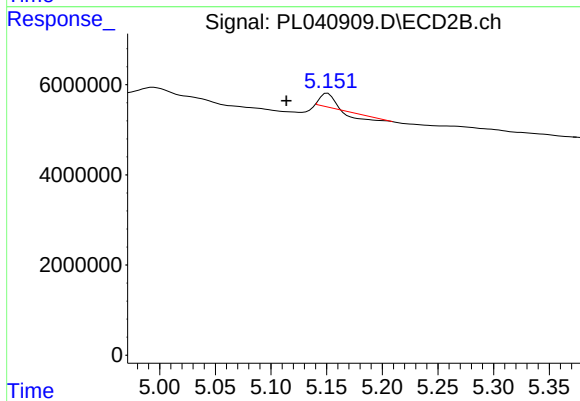

#23 Chlordane-1


R.T.: 5.151 min
Delta R.T.: 0.037 min
Response: 316293
Conc: 2.56 ng/ml

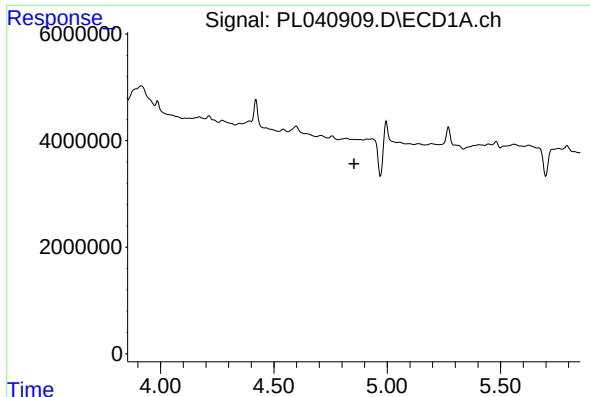

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.854 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

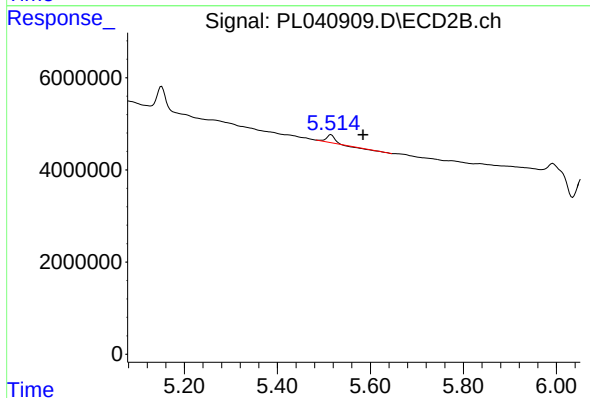


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: -0.069 min
Response: 1382154
Conc: 11.18 ng/ml

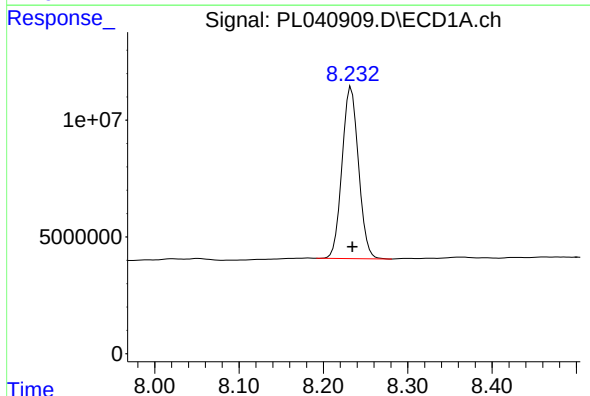

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: -0.001 min
Response: 99722516
Conc: 19.18 ng/ml

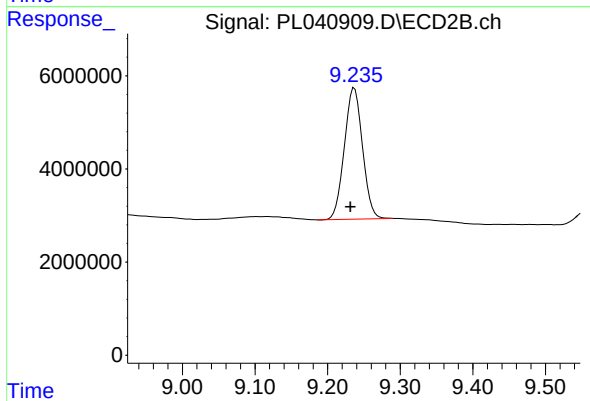

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.005 min
Response: 48982517
Conc: 18.94 ng/ml