

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101118\
 Data File : PL040912.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2018 13:42
 Operator : AJ\SJ
 Sample : J5326-24
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 14:10:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.480	4.105	105.6E6	55459167	19.263	19.890
28)	SA Decachlor...	8.234	9.237	100.1E6	49748134	19.254	19.239
Target Compounds							
6)	B beta-BHC	4.421f	4.995f	6291738	8825017	1.983	5.506 #
7)	B delta-BHC	0.000	5.151f	0	96816	N.D.	0.029 #
8)	B Heptachlo...	5.136f	0.000	2409251	0	0.367	N.D. #
14)	MA Endrin	6.044	0.000	43898096	0	7.642	N.D. #
15)	B Endosulfa...	6.240f	0.000	20101076	0	3.586	N.D. #
16)	A 4,4'-DDD	0.000	6.916f	0	12484858	N.D.	5.960 #
23)	Chlordane-1	4.421	5.151	6291738	96816	24.653	0.784 #
24)	Chlordane-2	0.000	5.516	0	1454520	N.D.	11.761 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101118\
Data File : PL040912.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2018 13:42
Operator : AJ\SJ
Sample : J5326-24
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 14:10:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

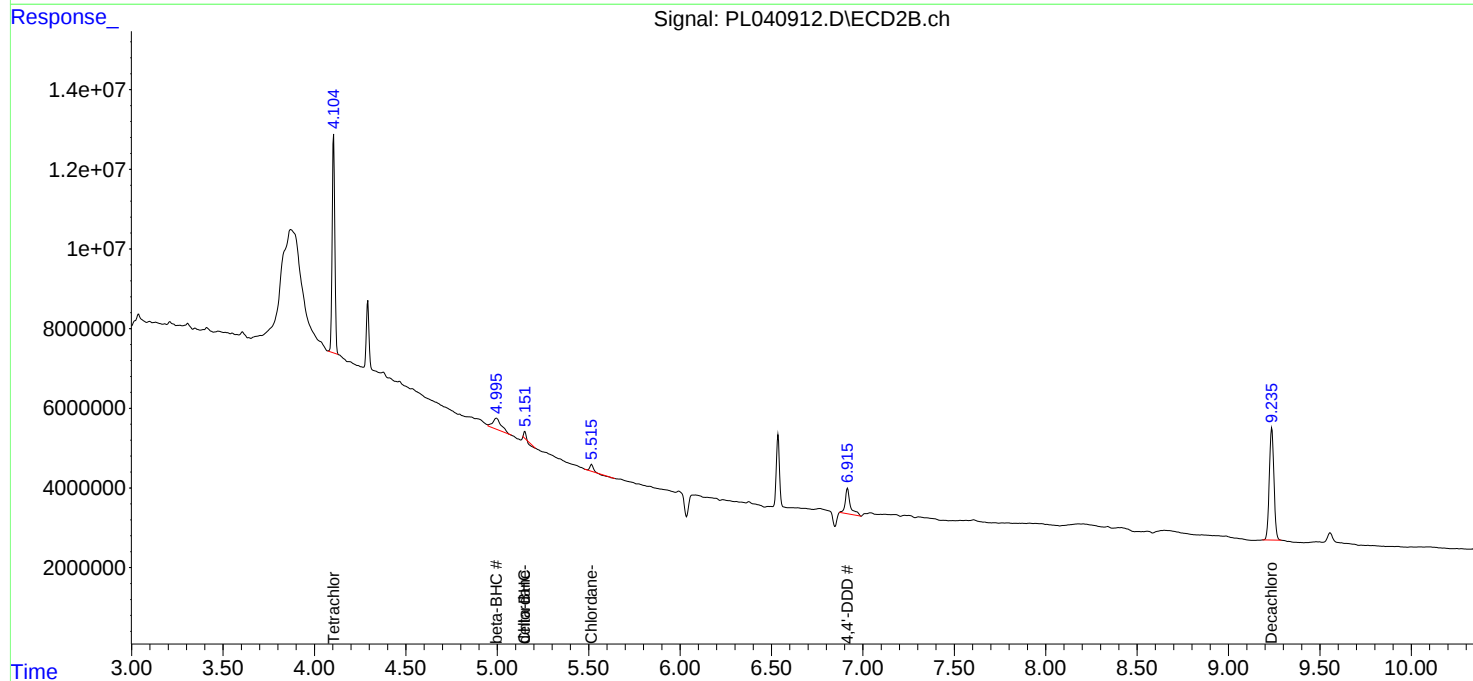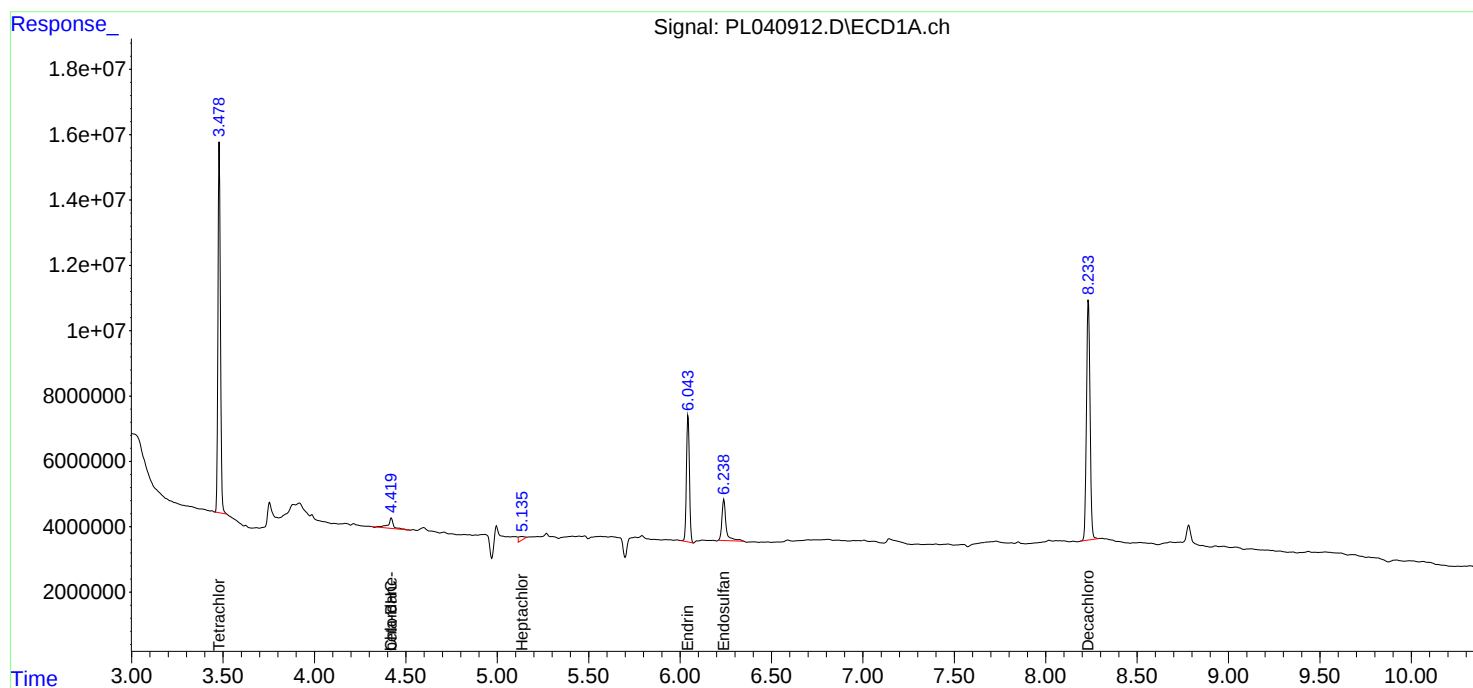


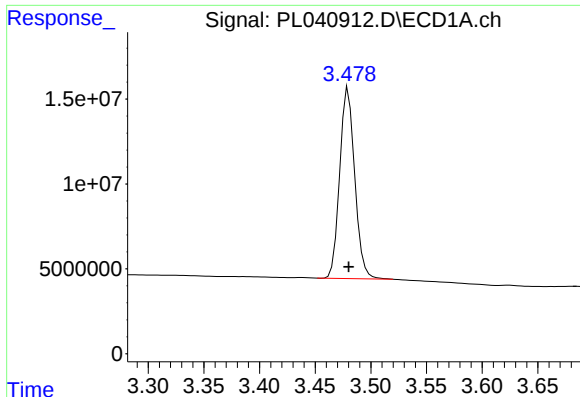

#1 Tetrachloro-m-xylene


R.T.: 3.480 min
Delta R.T.: 0.000 min
Response: 105577685
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

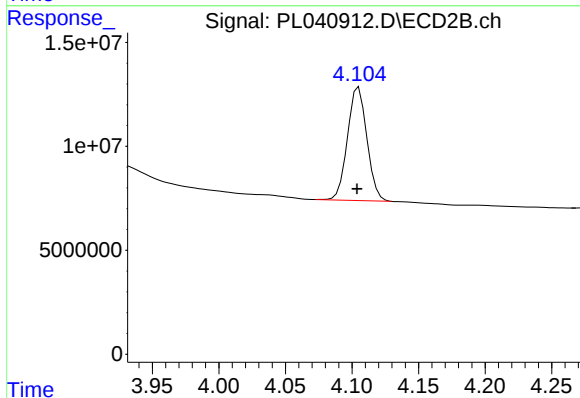


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.001 min
Response: 55459167
Conc: 19.89 ng/ml

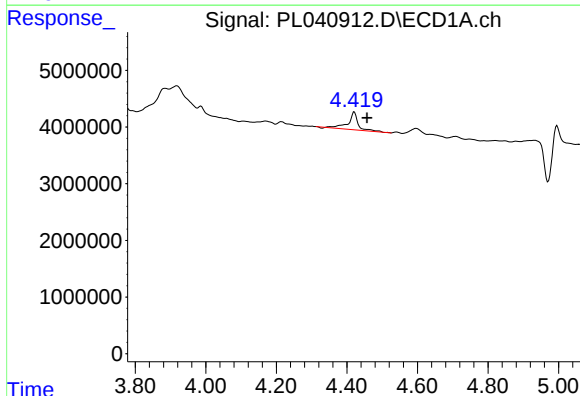


#6 beta-BHC

R.T.: 4.421 min
Delta R.T.: -0.037 min
Response: 6291738
Conc: 1.98 ng/ml

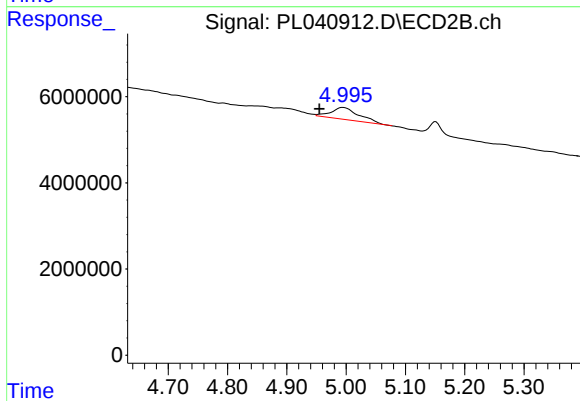

#6 beta-BHC


R.T.: 4.995 min
Delta R.T.: 0.040 min
Response: 8825017
Conc: 5.51 ng/ml

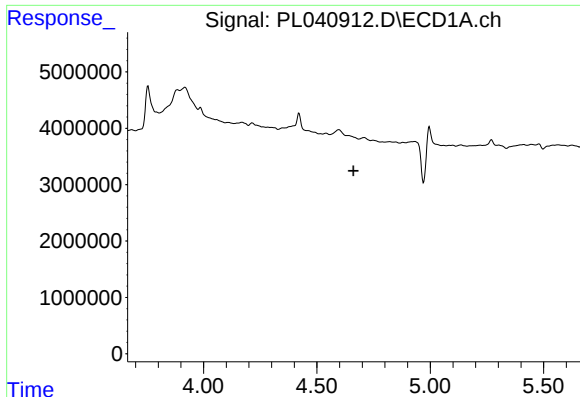

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

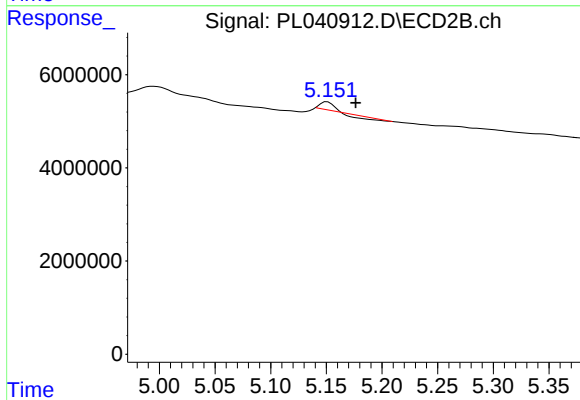


#7 delta-BHC

R.T.: 5.151 min
Delta R.T.: -0.026 min
Response: 96816
Conc: 0.03 ng/ml

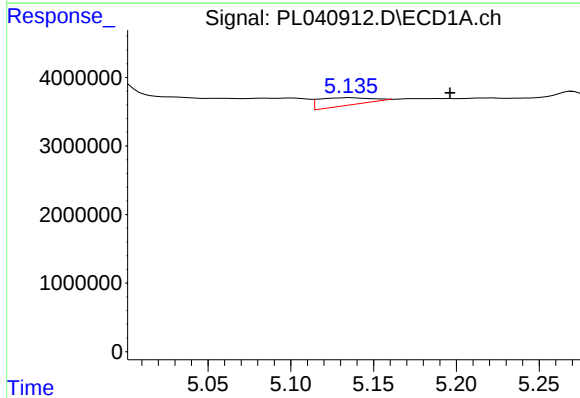


#8 Heptachlor epoxide

R.T.: 5.136 min
Delta R.T.: -0.060 min
Response: 2409251
Conc: 0.37 ng/ml

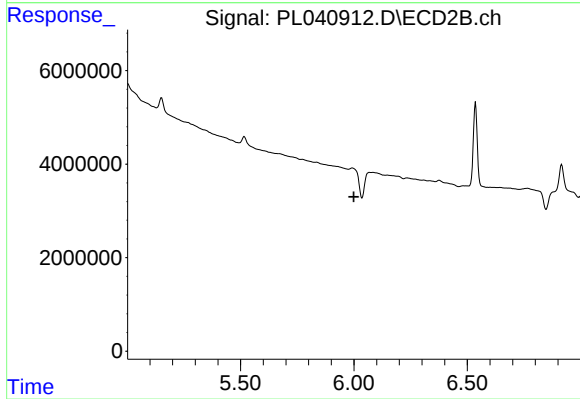

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.000 min
Response: 0
Conc: N.D.

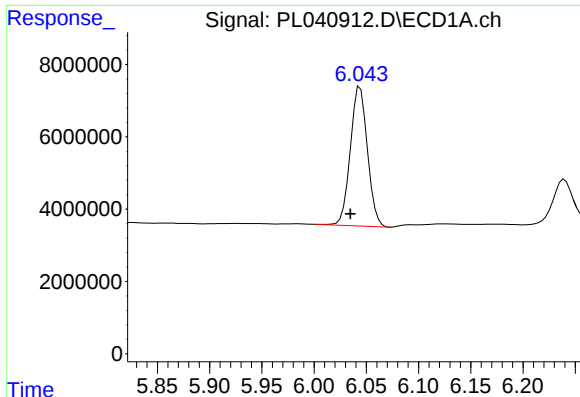

#14 Endrin


R.T.: 6.044 min
Delta R.T.: 0.009 min
Response: 43898096
Conc: 7.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

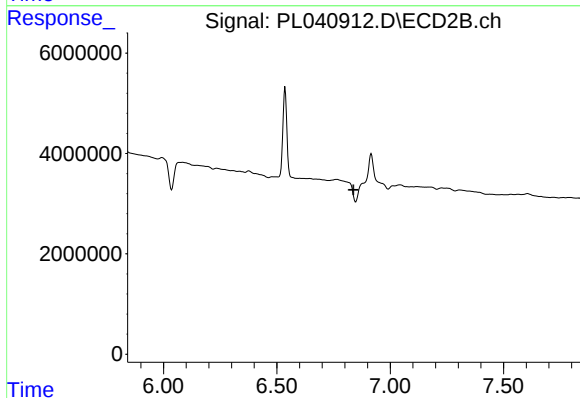


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

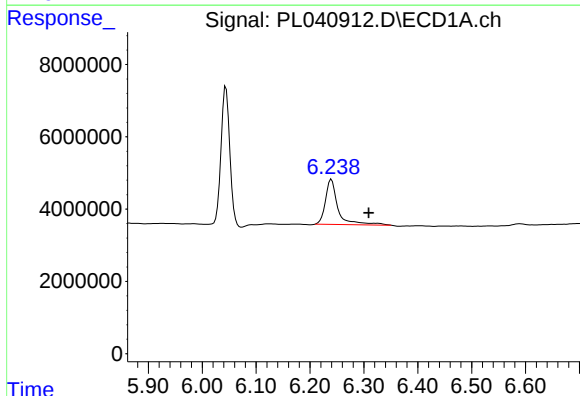


#15 Endosulfan II

R.T.: 6.240 min
Delta R.T.: -0.069 min
Response: 20101076
Conc: 3.59 ng/ml

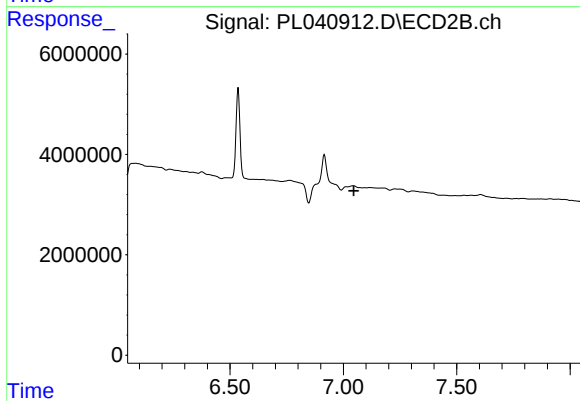

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

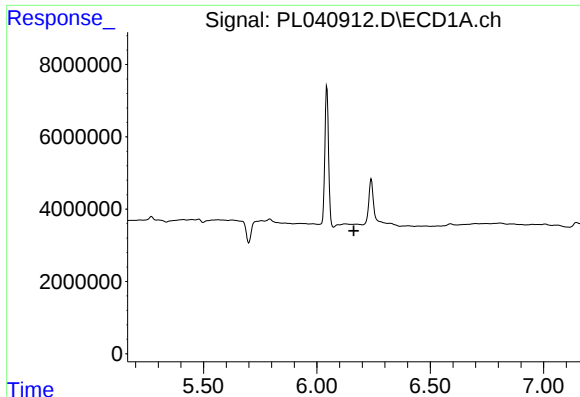

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

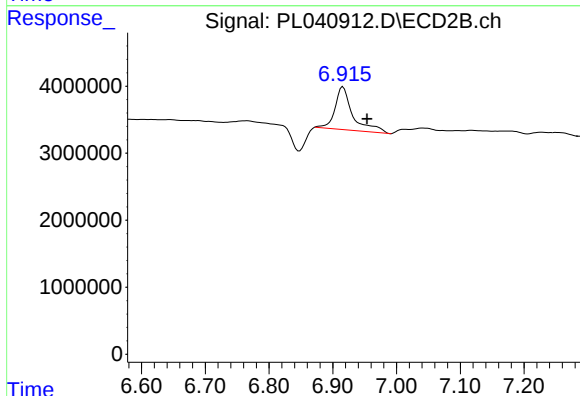


#16 4,4'-DDD

R.T.: 6.916 min
Delta R.T.: -0.038 min
Response: 12484858
Conc: 5.96 ng/ml

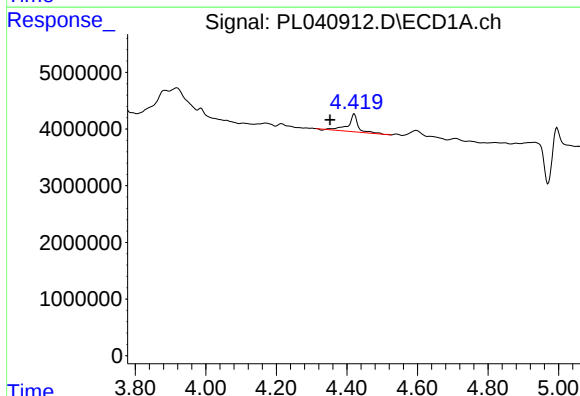


#23 Chlordane-1

R.T.: 4.421 min
Delta R.T.: 0.068 min
Response: 6291738
Conc: 24.65 ng/ml

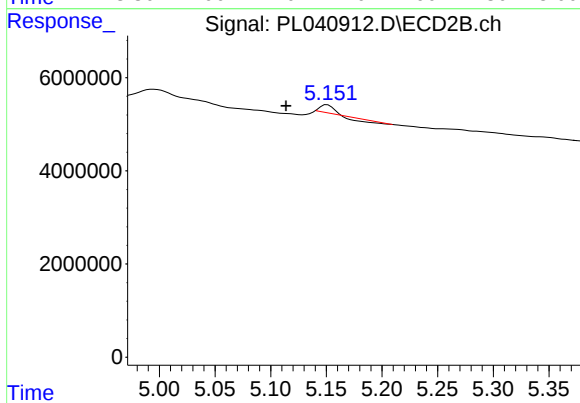

#23 Chlordane-1


R.T.: 5.151 min
Delta R.T.: 0.037 min
Response: 96816
Conc: 0.78 ng/ml

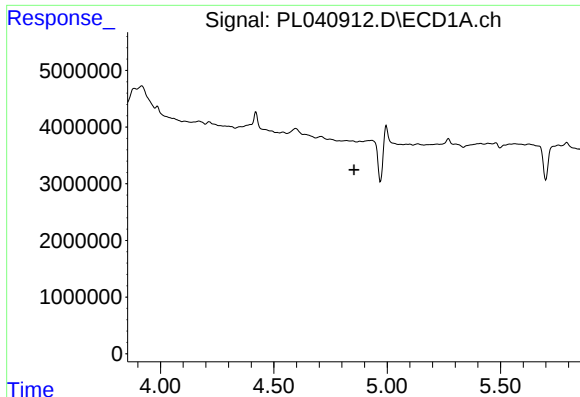

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.854 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

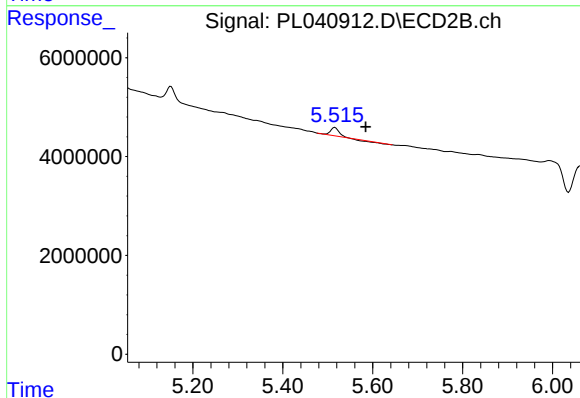


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: -0.068 min
Response: 1454520
Conc: 11.76 ng/ml

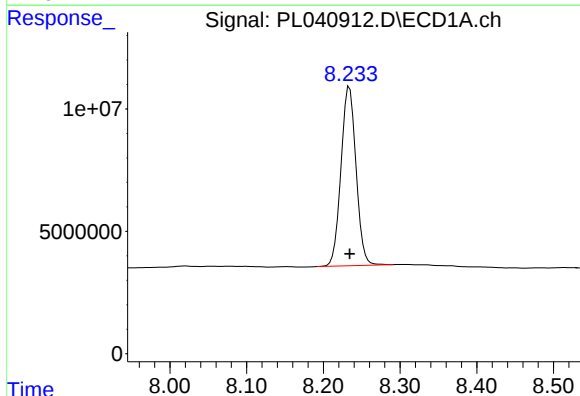

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 100112337
Conc: 19.25 ng/ml

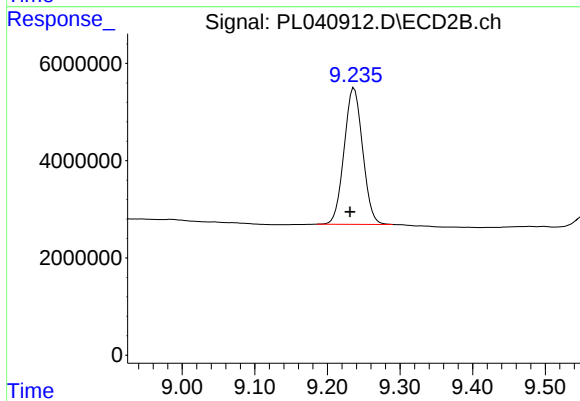

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.005 min
Response: 49748134
Conc: 19.24 ng/ml