

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101118\
 Data File : PL040943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2018 21:00
 Operator : AJ\SJ
 Sample : J5373-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:42:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.106	114.8E6	60741922	20.953	21.785
28)	SA Decachlor...	8.233	9.238	109.7E6	49880710	21.099	19.290
Target Compounds							
3)	MA gamma-BHC...	4.214	0.000	89208	0	0.012	N.D. #
6)	B beta-BHC	4.421f	4.998f	3503143	7681706	1.104	4.793 #
13)	MA Dieldrin	5.724f	0.000	41019	0	0.006	N.D. #
14)	MA Endrin	6.044	6.866	13182650	1458827	2.295	0.654 #
15)	B Endosulfa...	6.324	7.046	1742399	2076629	0.311	0.874 #
16)	A 4,4'-DDD	6.116f	6.917f	1259504	9089369	0.279	4.339 #
19)	B Endosulfa...	6.694	0.000	663132	0	0.130	N.D. #
20)	A Methoxychlor	6.953	0.000	885139	0	0.340	N.D. #
23)	Chlordane-1	4.421	0.000	3503143	0	13.726	N.D. #
27)	Chlordane-5	6.324	0.000	1742399	0	8.040	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101118\
Data File : PL040943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2018 21:00
Operator : AJ\SJ
Sample : J5373-02
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:42:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

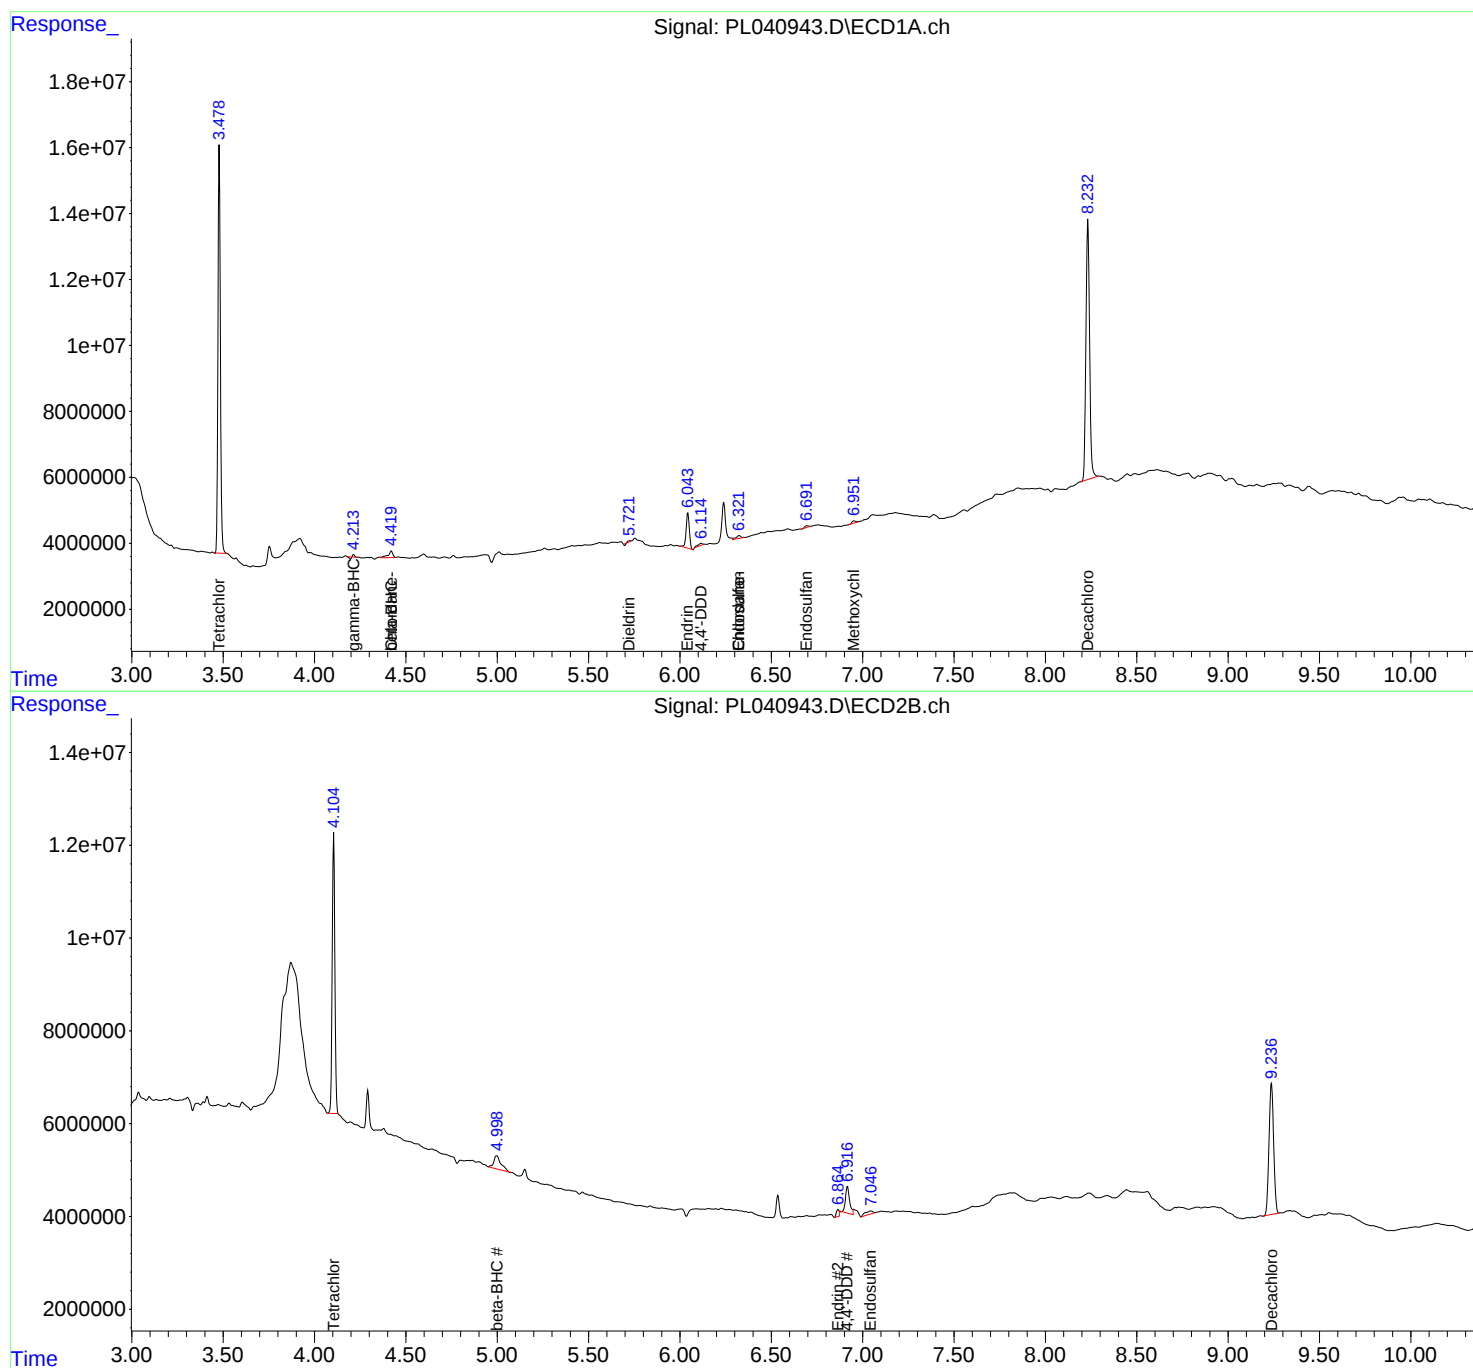


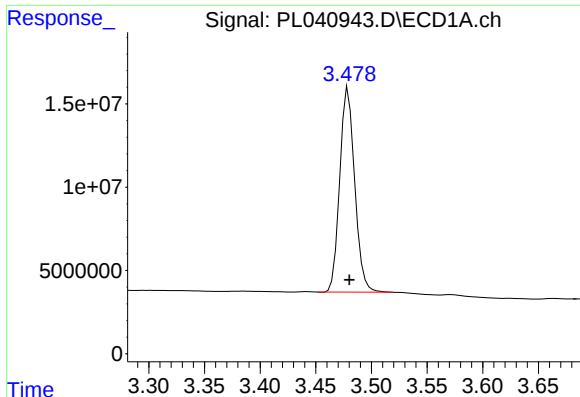

#1 Tetrachloro-m-xylene


R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 114839653
Conc: 20.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

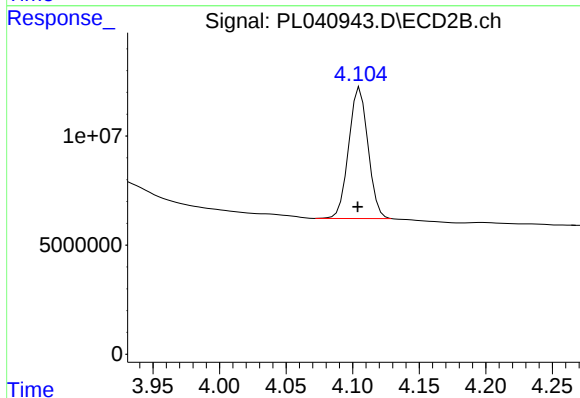


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.002 min
Response: 60741922
Conc: 21.78 ng/ml

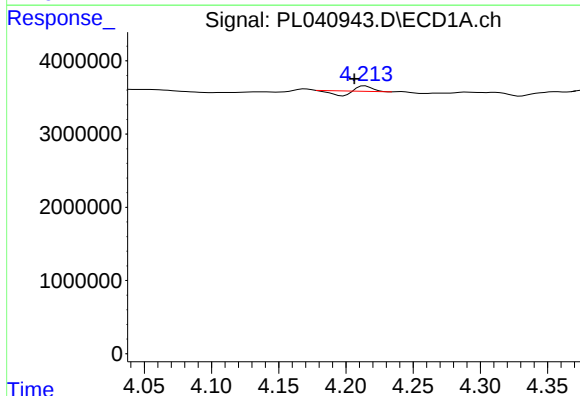


#3 gamma-BHC (Lindane)

R.T.: 4.214 min
Delta R.T.: 0.008 min
Response: 89208
Conc: 0.01 ng/ml

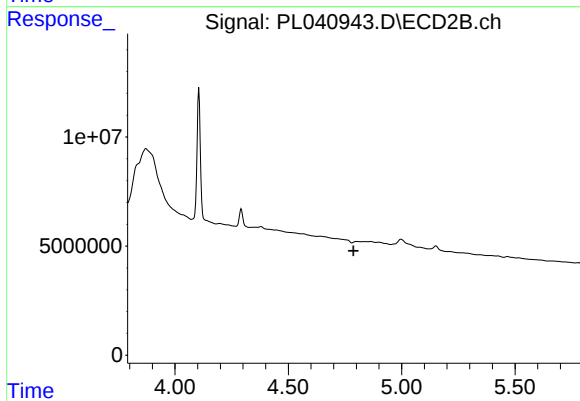

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

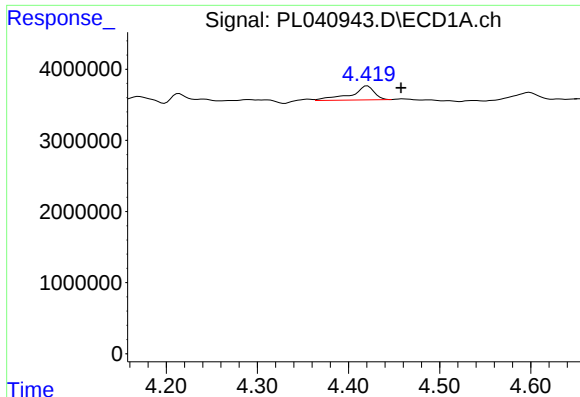

#6 beta-BHC


R.T.: 4.421 min
Delta R.T.: -0.037 min
Response: 3503143
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

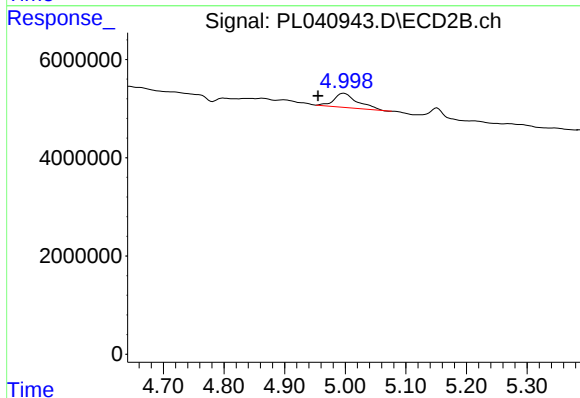


#6 beta-BHC

R.T.: 4.998 min
Delta R.T.: 0.043 min
Response: 7681706
Conc: 4.79 ng/ml

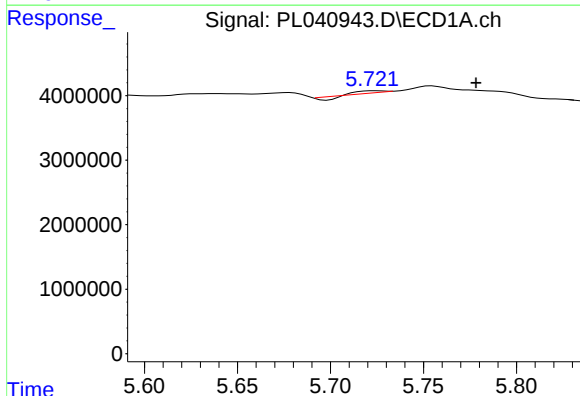


#13 Dieldrin

R.T.: 5.724 min
Delta R.T.: -0.054 min
Response: 41019
Conc: 0.01 ng/ml

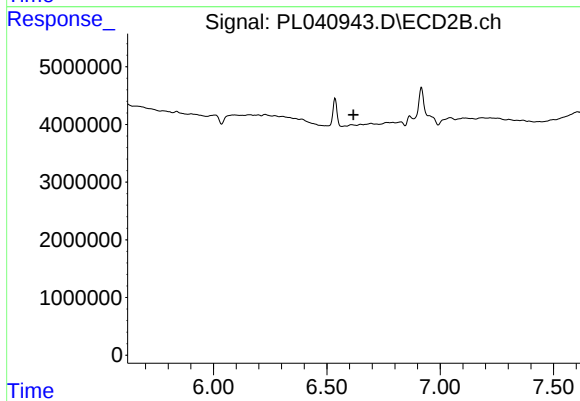

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.618 min
Response: 0
Conc: N.D.

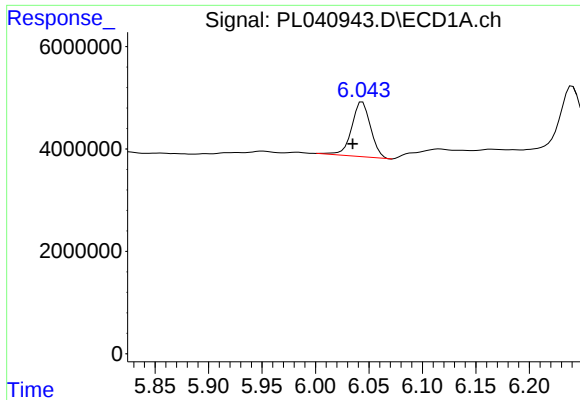

#14 Endrin


R.T.: 6.044 min
Delta R.T.: 0.009 min
Response: 13182650
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

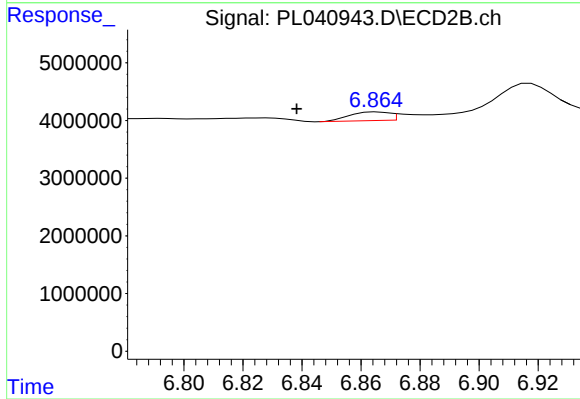


#14 Endrin

R.T.: 6.866 min
Delta R.T.: 0.027 min
Response: 1458827
Conc: 0.65 ng/ml

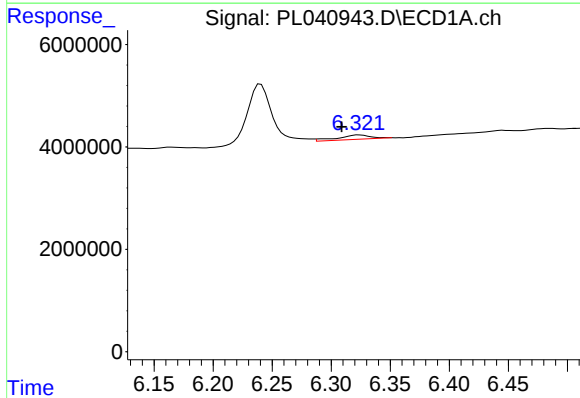


#15 Endosulfan II

R.T.: 6.324 min
Delta R.T.: 0.015 min
Response: 1742399
Conc: 0.31 ng/ml

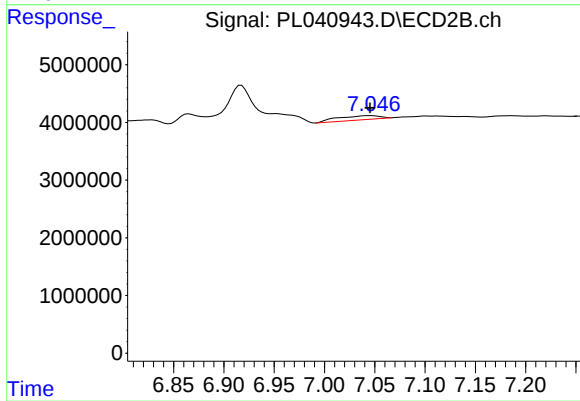

#15 Endosulfan II


R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 2076629
Conc: 0.87 ng/ml

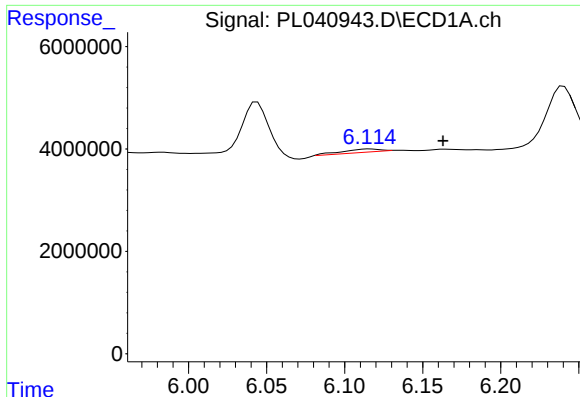

#16 4,4'-DDD


R.T.: 6.116 min
Delta R.T.: -0.047 min
Response: 1259504
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

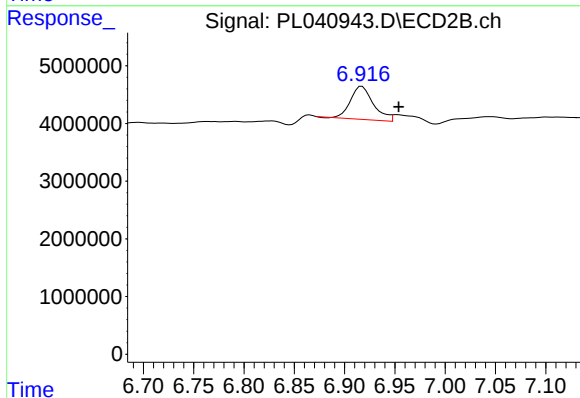


#16 4,4'-DDD

R.T.: 6.917 min
Delta R.T.: -0.037 min
Response: 9089369
Conc: 4.34 ng/ml

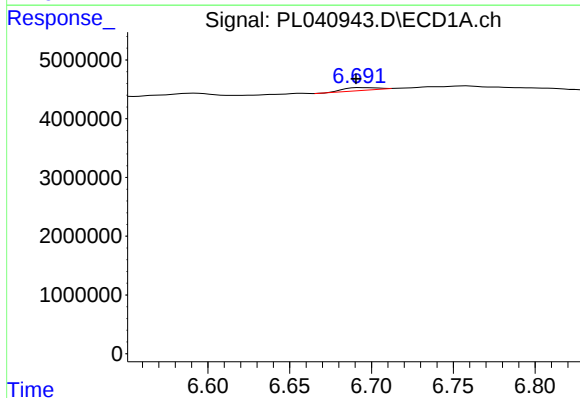


#19 Endosulfan Sulfate

R.T.: 6.694 min
Delta R.T.: 0.004 min
Response: 663132
Conc: 0.13 ng/ml

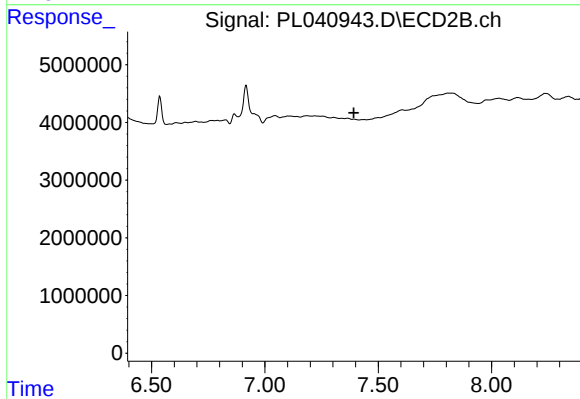

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.392 min
Response: 0
Conc: N.D.

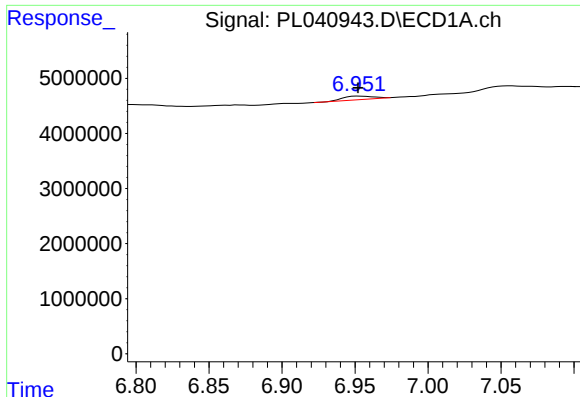

#20 Methoxychlor


R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 885139
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

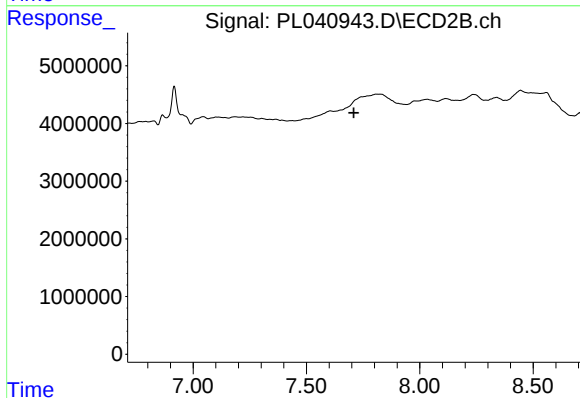


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

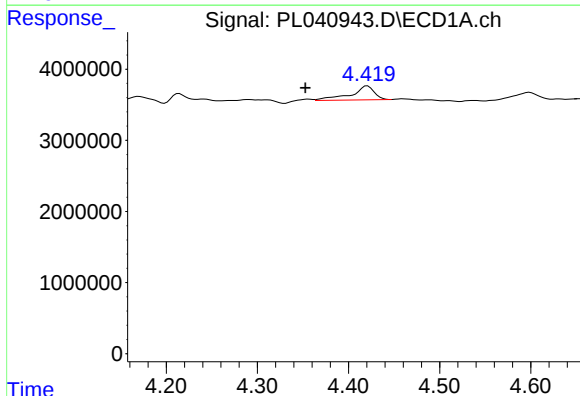


#23 Chlordane-1

R.T.: 4.421 min
Delta R.T.: 0.068 min
Response: 3503143
Conc: 13.73 ng/ml

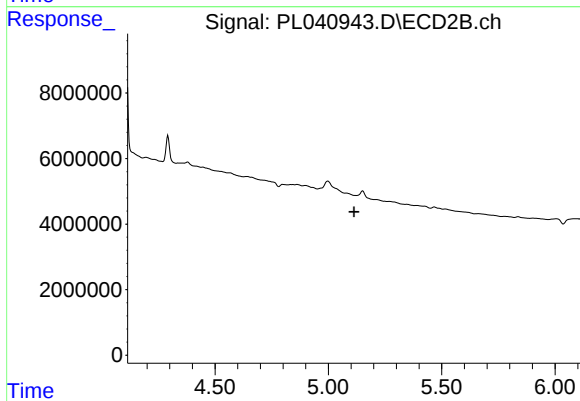

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

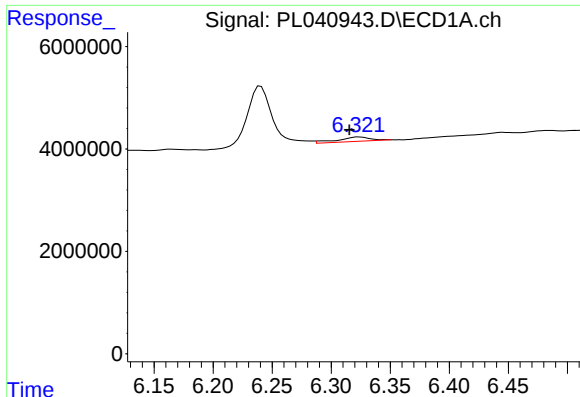

#27 Chlordane-5


R.T.: 6.324 min
Delta R.T.: 0.008 min
Response: 1742399
Conc: 8.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

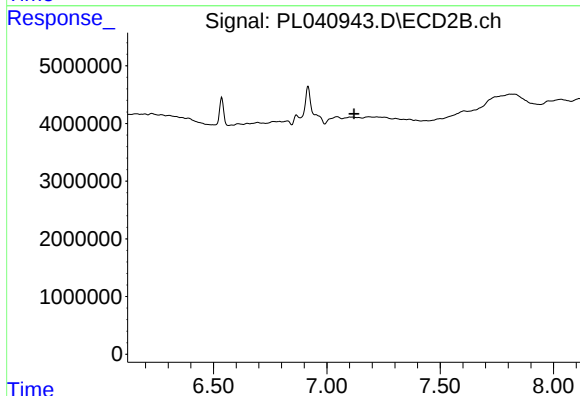


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

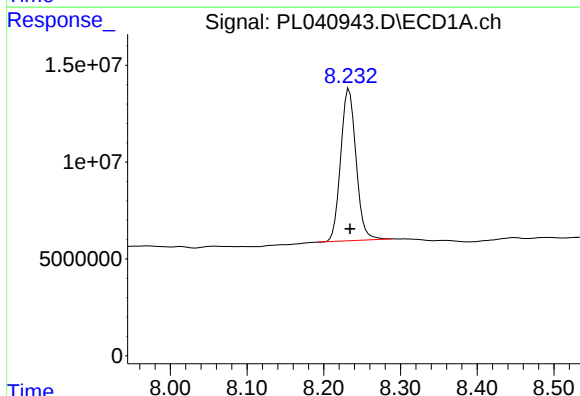

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: -0.001 min
Response: 109706064
Conc: 21.10 ng/ml

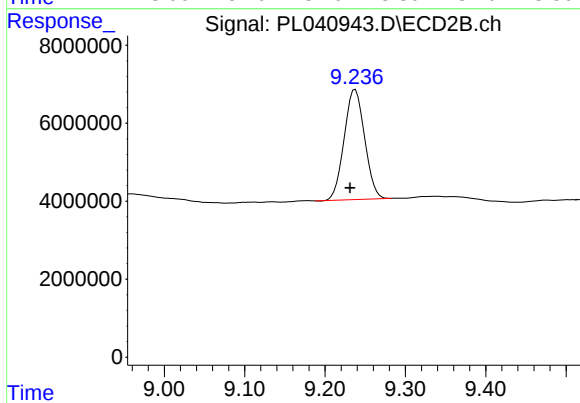

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.006 min
Response: 49880710
Conc: 19.29 ng/ml