

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101119\
 Data File : PL053231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2019 10:32
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 23:32:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.917	0	38046802	N.D.	11.352 #
12) B	4,4'-DDE	5.765f	6.367f	18339296	68068729	1.580	20.841 #
13) MA	Dieldrin	5.857f	0.000	16289267	0	1.262	N.D. #
14) MA	Endrin	0.000	6.751	0	13477890	N.D.	4.854 #
15) B	Endosulfa...	0.000	6.974	0	8268610	N.D.	2.787 #
17) MA	4,4'-DDT	0.000	7.188	0	3464783	N.D.	1.331 #
18) B	Endrin al...	0.000	7.087	0	6532775	N.D.	2.664 #
27)	Chlordane-5	0.000	7.034	0	9447425	N.D.	107.102 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101119\
Data File : PL053231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2019 10:32
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 23:32:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

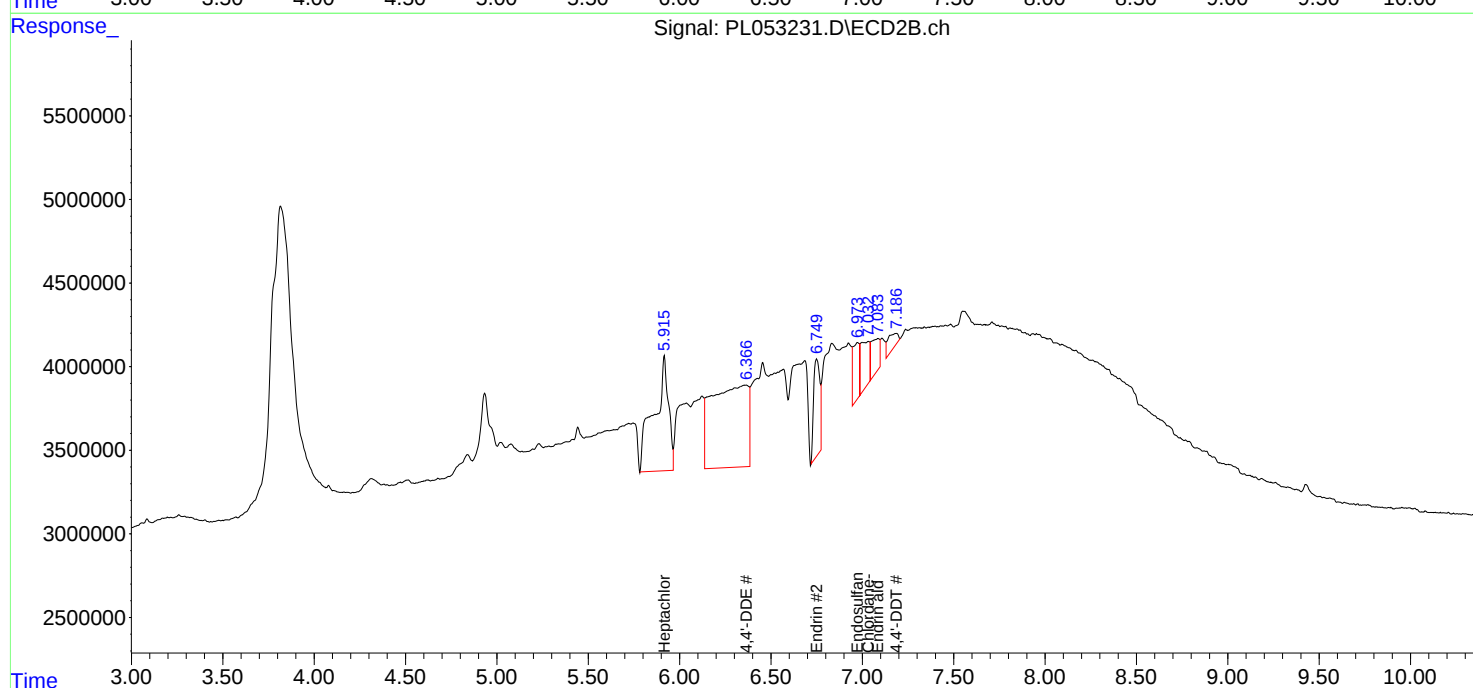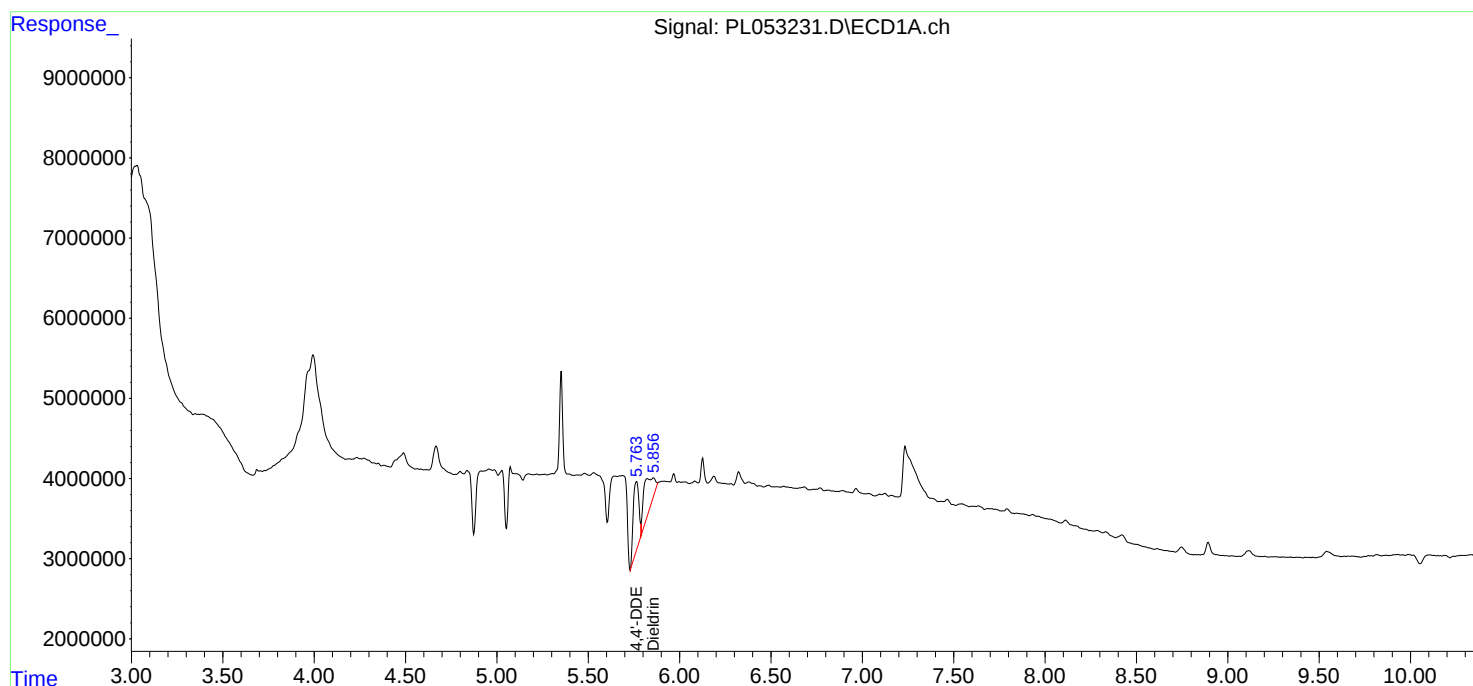


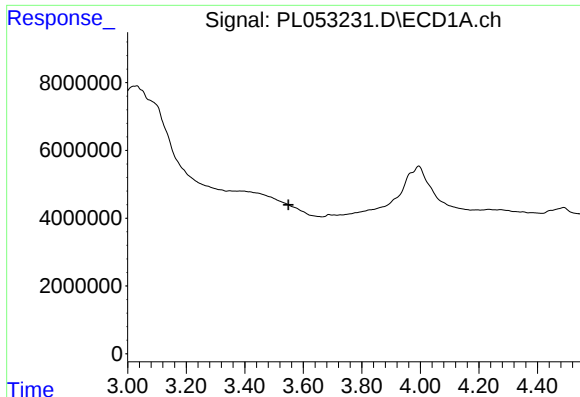

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

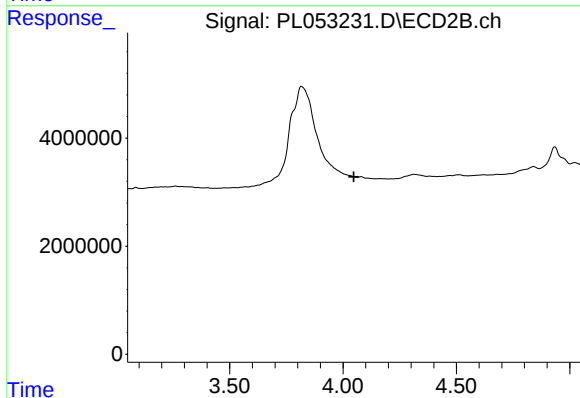


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.047 min
Response: 0
Conc: N.D.

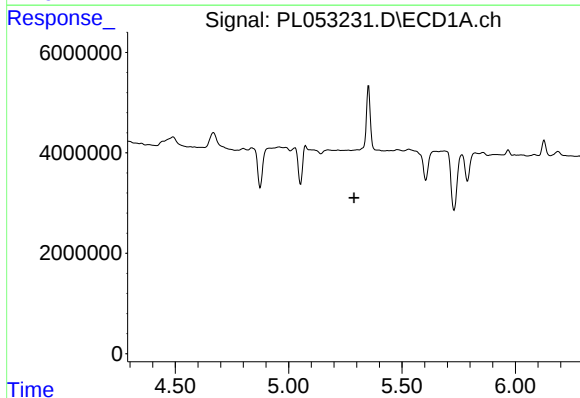


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

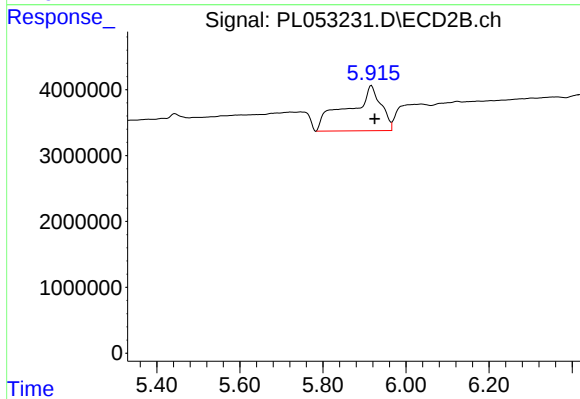

#8 Heptachlor epoxide


R.T.: 5.917 min
Delta R.T.: -0.008 min
Response: 38046802
Conc: 11.35 ng/ml

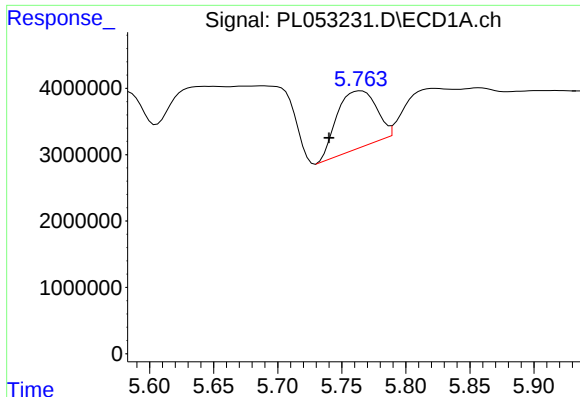

#12 4,4'-DDE


R.T.: 5.765 min
Delta R.T.: 0.025 min
Response: 18339296
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

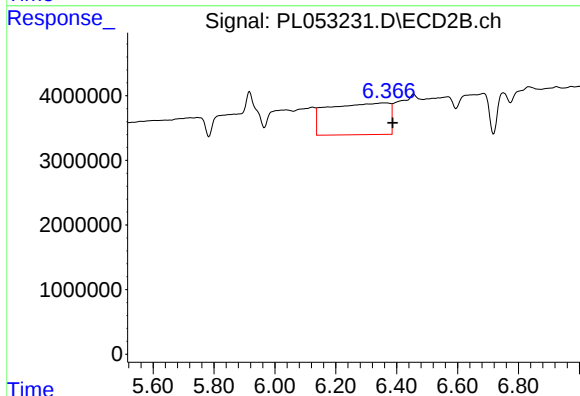


#12 4,4'-DDE

R.T.: 6.367 min
Delta R.T.: -0.020 min
Response: 68068729
Conc: 20.84 ng/ml

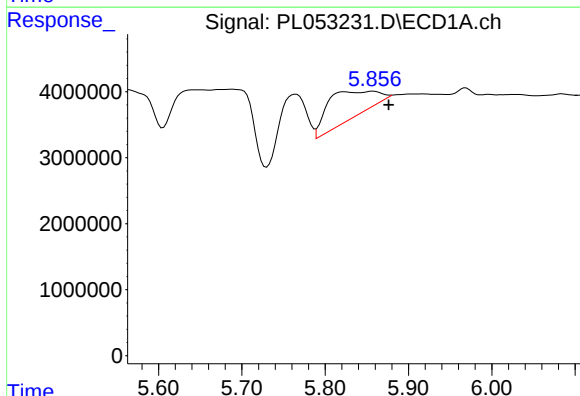


#13 Dieldrin

R.T.: 5.857 min
Delta R.T.: -0.019 min
Response: 16289267
Conc: 1.26 ng/ml

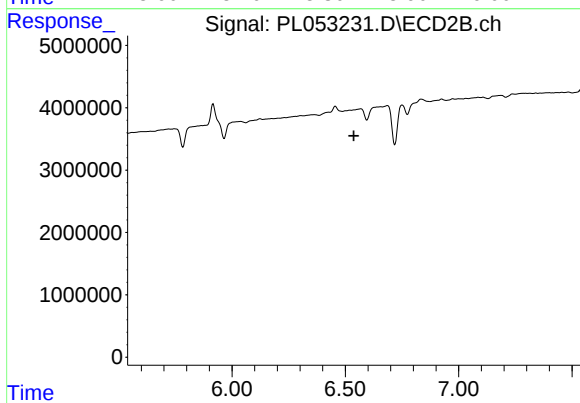

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.538 min
Response: 0
Conc: N.D.

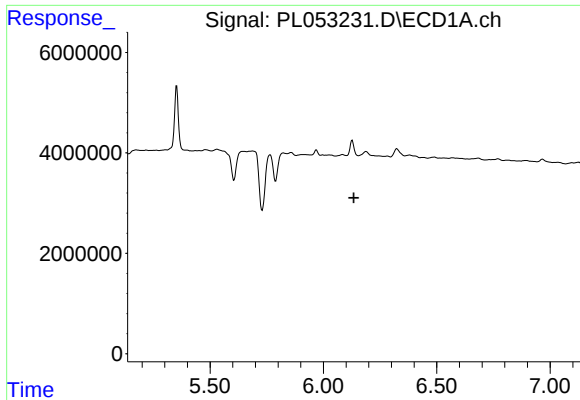

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

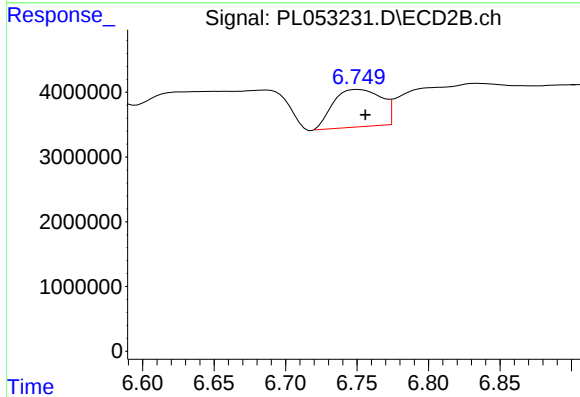


#14 Endrin

R.T.: 6.751 min
Delta R.T.: -0.005 min
Response: 13477890
Conc: 4.85 ng/ml

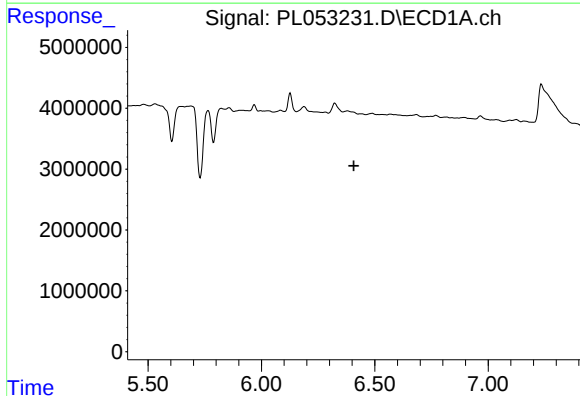


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

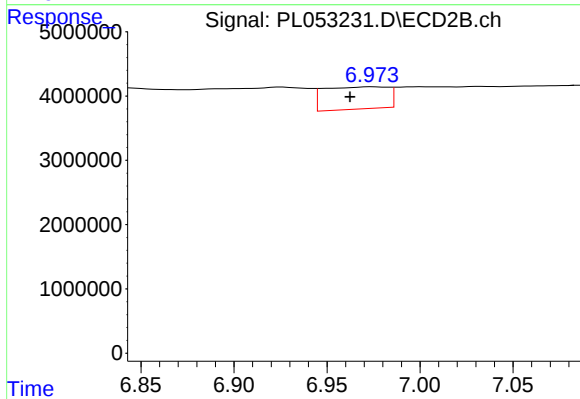

#15 Endosulfan II


R.T.: 6.974 min
Delta R.T.: 0.012 min
Response: 8268610
Conc: 2.79 ng/ml

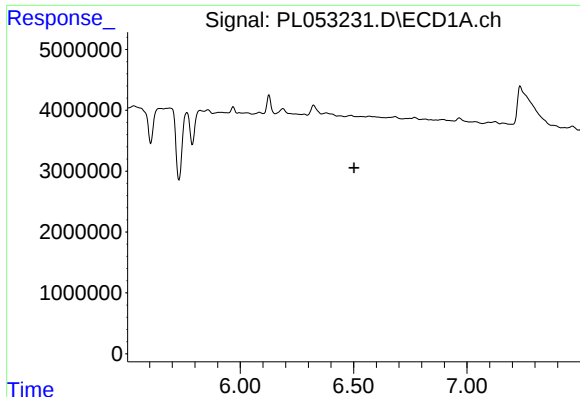

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

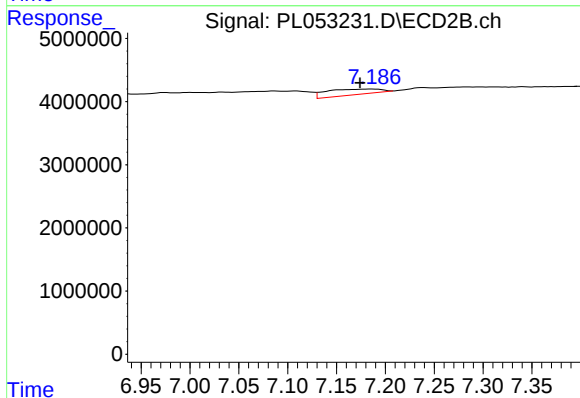


#17 4,4'-DDT

R.T.: 7.188 min
Delta R.T.: 0.013 min
Response: 3464783
Conc: 1.33 ng/ml

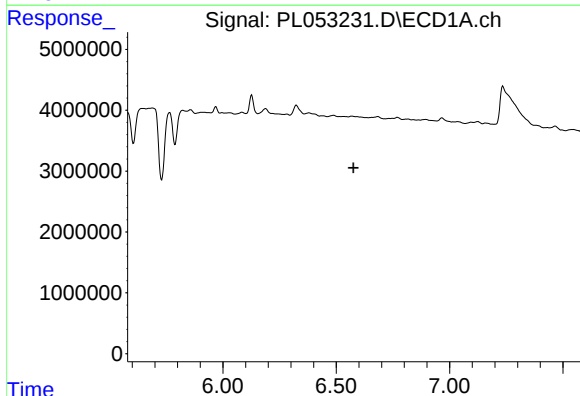


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.577 min
Response: 0
Conc: N.D.

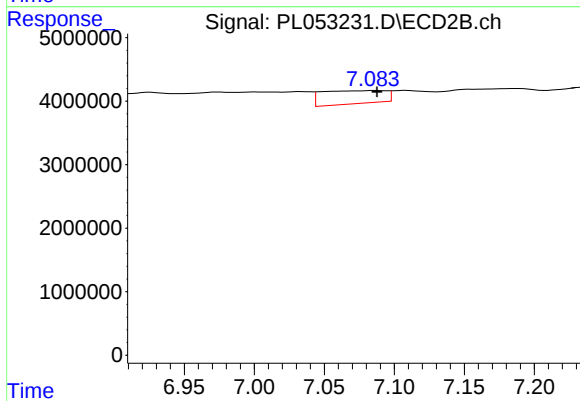

#18 Endrin aldehyde


R.T.: 7.087 min
Delta R.T.: -0.001 min
Response: 6532775
Conc: 2.66 ng/ml

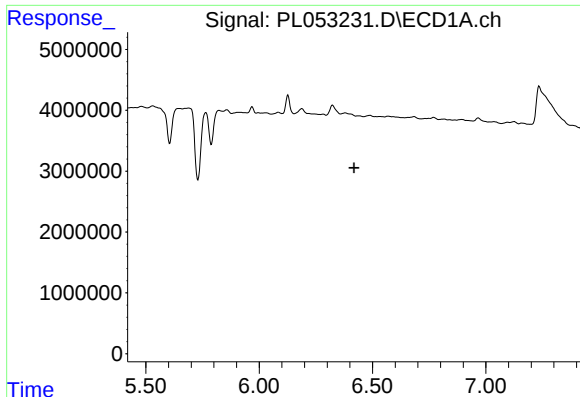

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

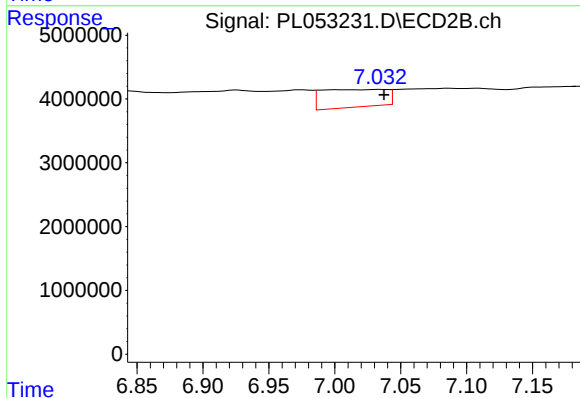


#27 Chlordane-5

R.T.: 7.034 min
Delta R.T.: -0.004 min
Response: 9447425
Conc: 107.10 ng/ml

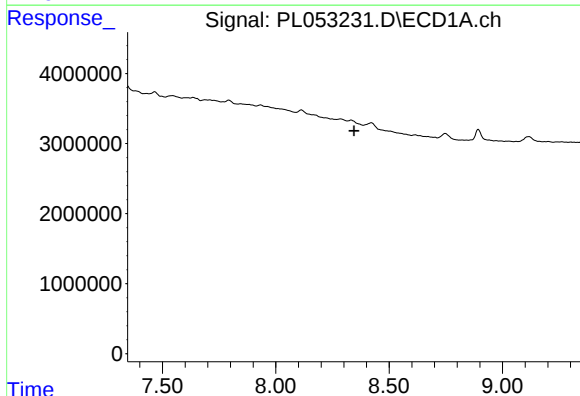

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.345 min
Response: 0
Conc: N.D.

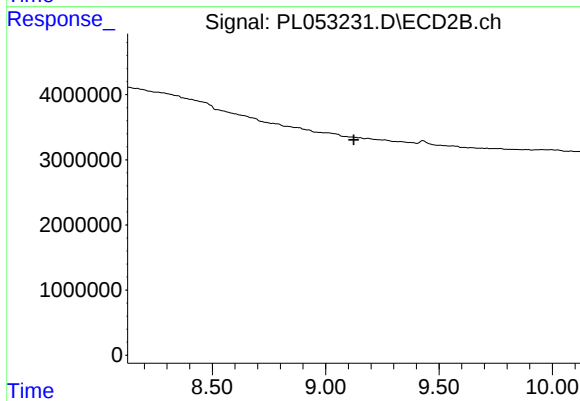

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.124 min
Response: 0
Conc: N.D.