

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101119\
 Data File : PL053248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2019 15:43
 Operator : SG\AJ
 Sample : K5300-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-18A-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 23:35:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	4.046	214.6E6	53634557	21.577	19.974
28)	SA Decachlor...	8.338	9.123	169.9E6	55126979	16.959	18.791
Target Compounds							
7)	B delta-BHC	0.000	5.085f	0	2702672	N.D.	0.747 #
8)	B Heptachlo...	0.000	5.931	0	2456012	N.D.	0.733 #
10)	B gamma-Chl...	0.000	6.169	0	766351	N.D.	0.227 #
15)	B Endosulfa...	0.000	6.972	0	399557	N.D.	0.135 #
18)	B Endrin al...	0.000	7.093	0	5928246	N.D.	2.417 #
25)	Chlordane-3	0.000	6.169	0	766351	N.D.	1.760 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101119\
Data File : PL053248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2019 15:43
Operator : SG\AJ
Sample : K5300-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-18A-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 23:35:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

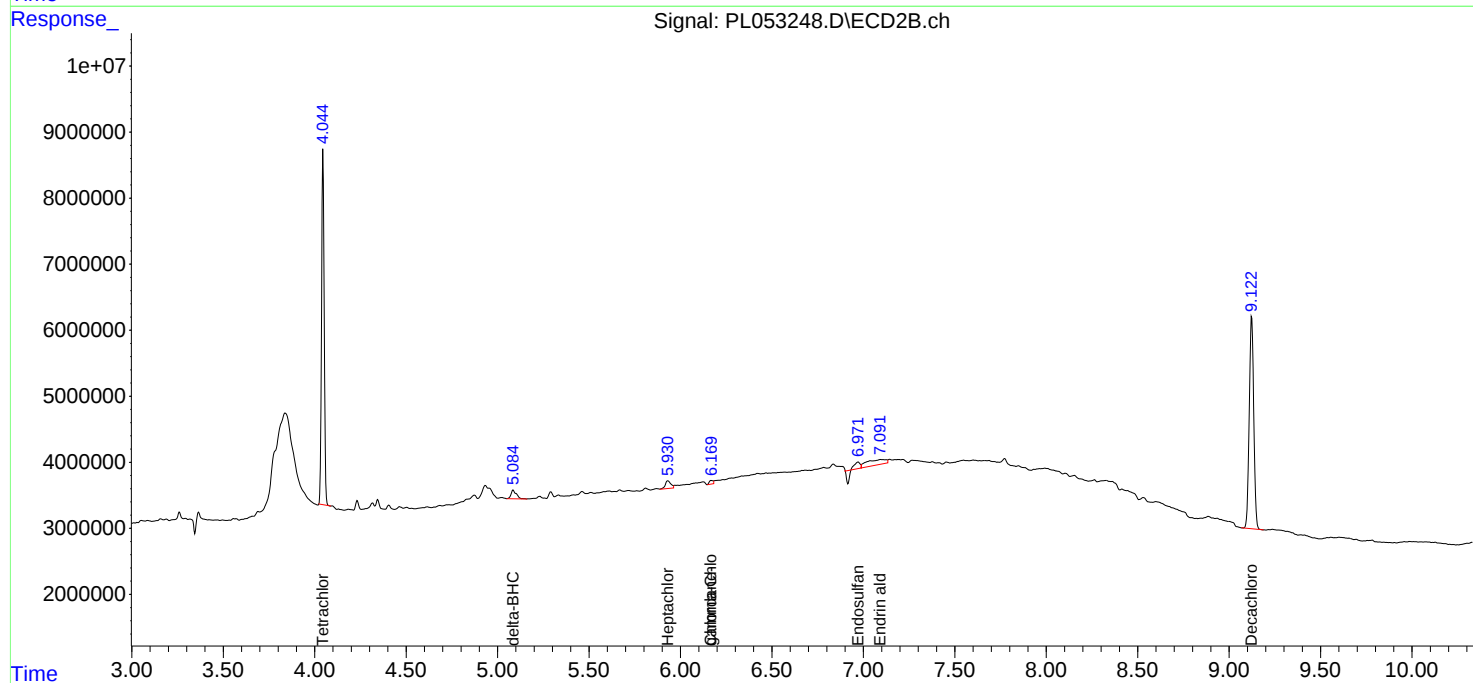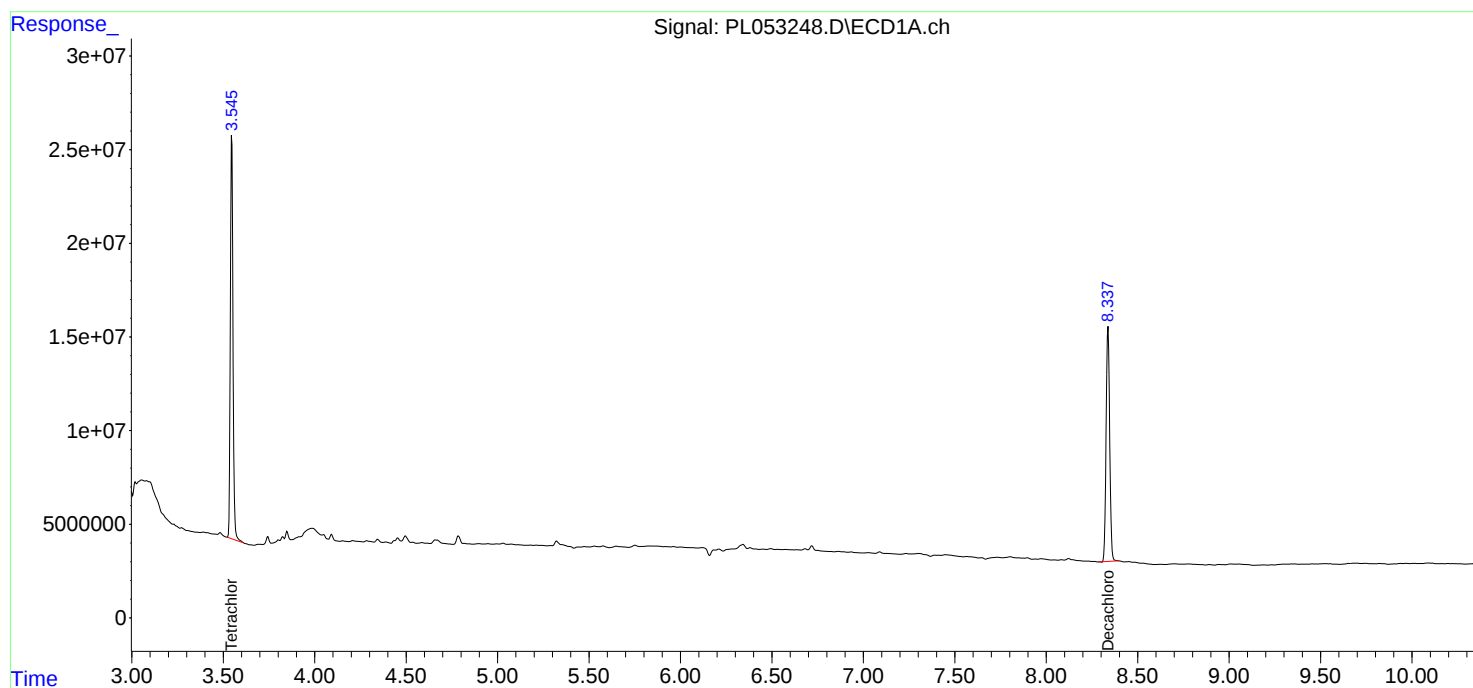


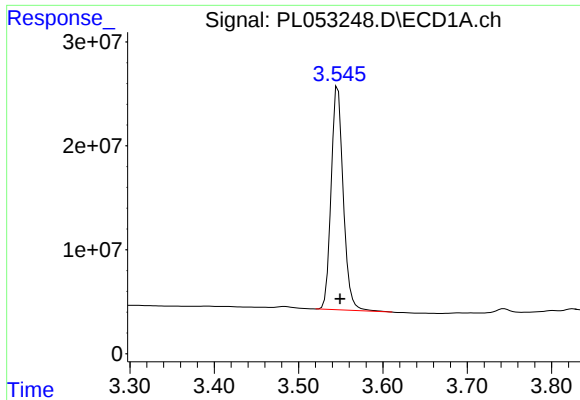

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: -0.002 min
Response: 214618448
Conc: 21.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-18A-D

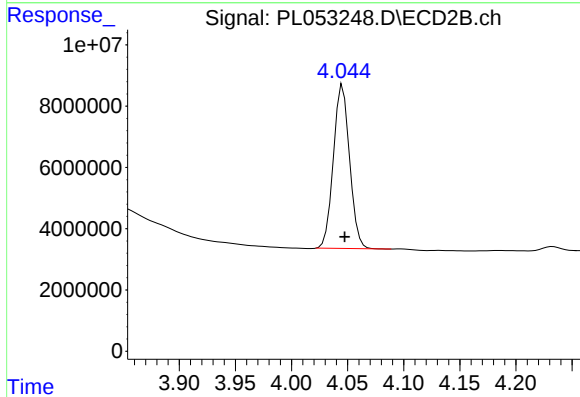


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.001 min
Response: 53634557
Conc: 19.97 ng/ml

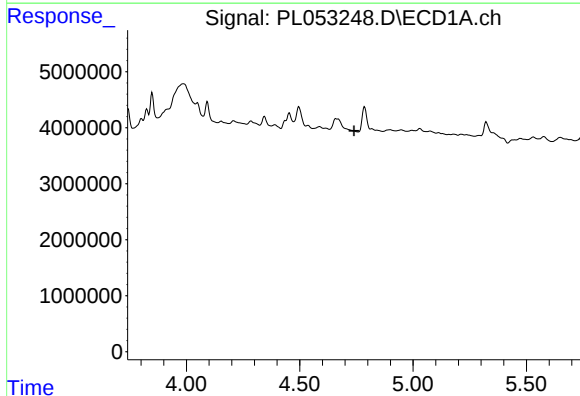


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

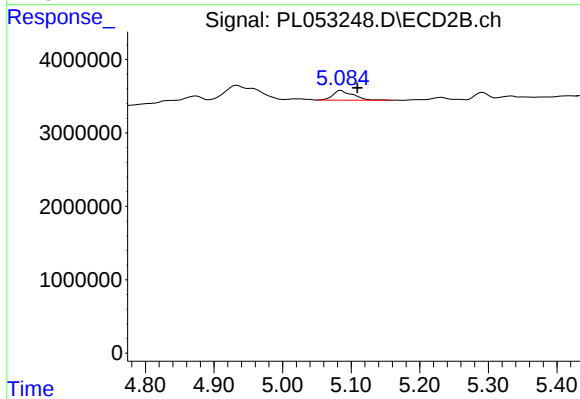

#7 delta-BHC


R.T.: 5.085 min
Delta R.T.: -0.024 min
Response: 2702672
Conc: 0.75 ng/ml

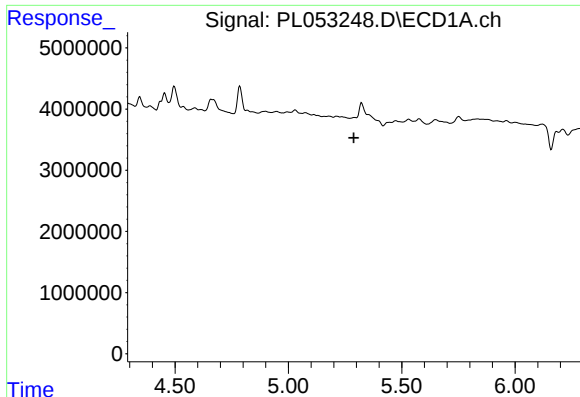

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-18A-D

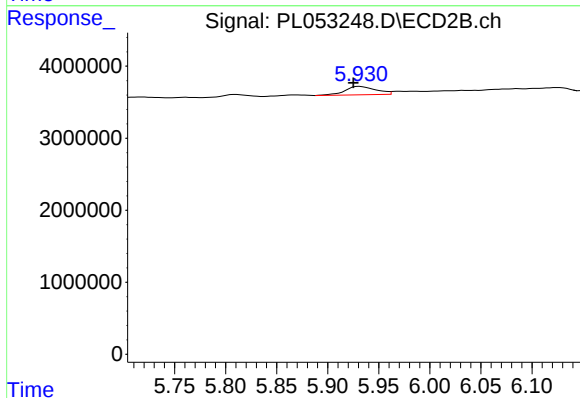


#8 Heptachlor epoxide

R.T.: 5.931 min
Delta R.T.: 0.006 min
Response: 2456012
Conc: 0.73 ng/ml

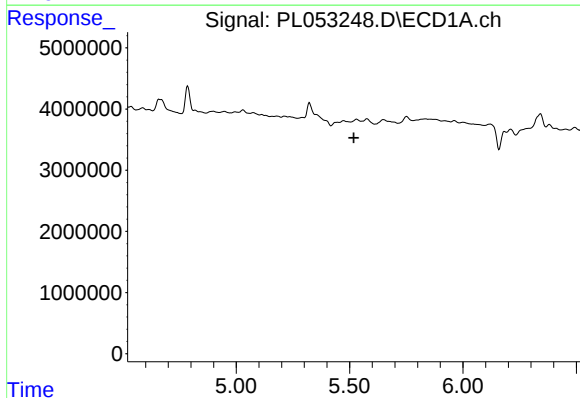


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

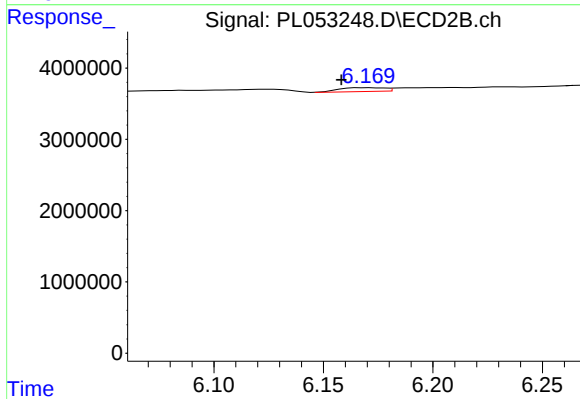

#10 gamma-Chlordane


R.T.: 6.169 min
Delta R.T.: 0.011 min
Response: 766351
Conc: 0.23 ng/ml

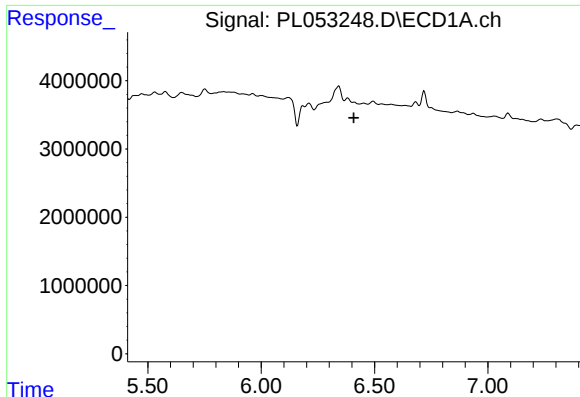

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-18A-D

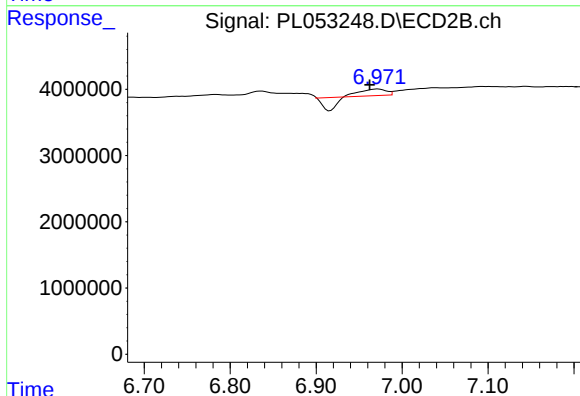


#15 Endosulfan II

R.T.: 6.972 min
Delta R.T.: 0.009 min
Response: 399557
Conc: 0.13 ng/ml

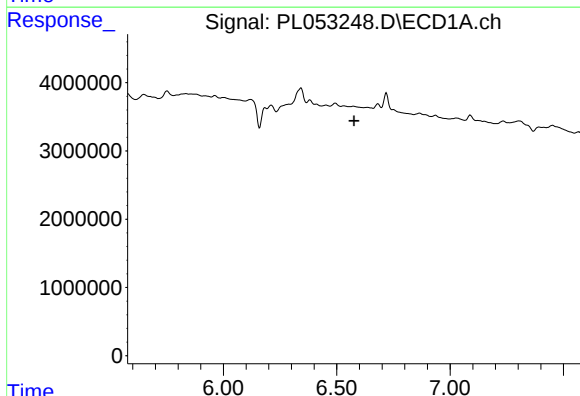


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.577 min
Response: 0
Conc: N.D.

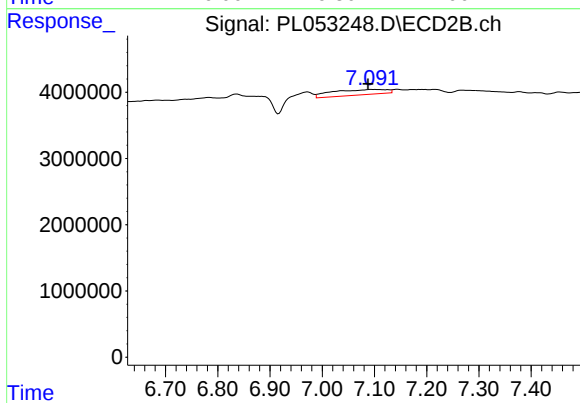

#18 Endrin aldehyde


R.T.: 7.093 min
Delta R.T.: 0.005 min
Response: 5928246
Conc: 2.42 ng/ml

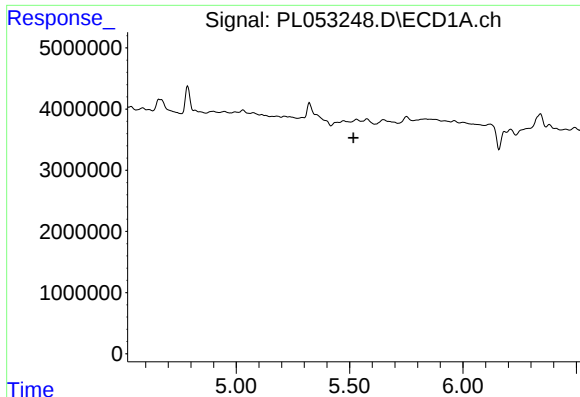

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-18A-D

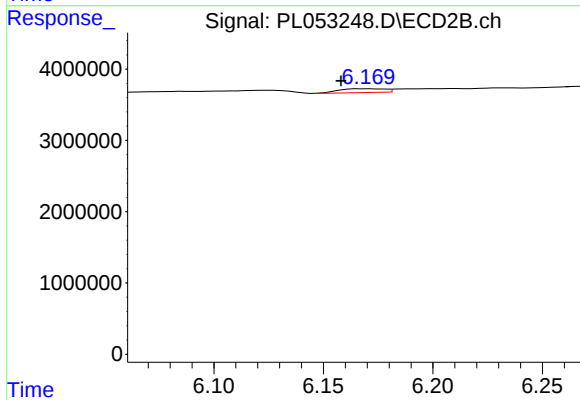


#25 Chlordane-3

R.T.: 6.169 min
Delta R.T.: 0.011 min
Response: 766351
Conc: 1.76 ng/ml

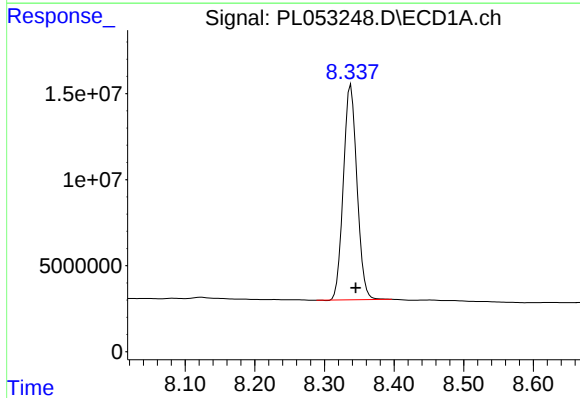

#28 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.007 min
Response: 169859483
Conc: 16.96 ng/ml

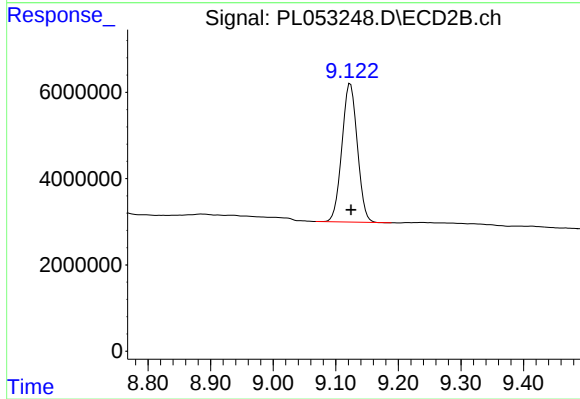

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 55126979
Conc: 18.79 ng/ml