

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101119\
 Data File : PL053245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2019 15:01
 Operator : SG\AJ
 Sample : K5266-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190854-AMENDED-COMP-A

Manual Integrations
 APPROVED

Ankita
 10/14/2019 12:33:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 23:35:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	4.046	103.3E6	27983082	10.382	10.421
28) SA Decachlor...	8.338	9.122	45572147	14169555	4.550	4.830
Target Compounds						
12) B 4,4'-DDE	5.733	6.386	6639329	3035940	0.572m	0.930 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101119\
Data File : PL053245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2019 15:01
Operator : SG\AJ
Sample : K5266-06
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20190854-AMENDED-COMP-A


Manual Integrations
APPROVED

Ankita
10/14/2019 12:33:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 23:35:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

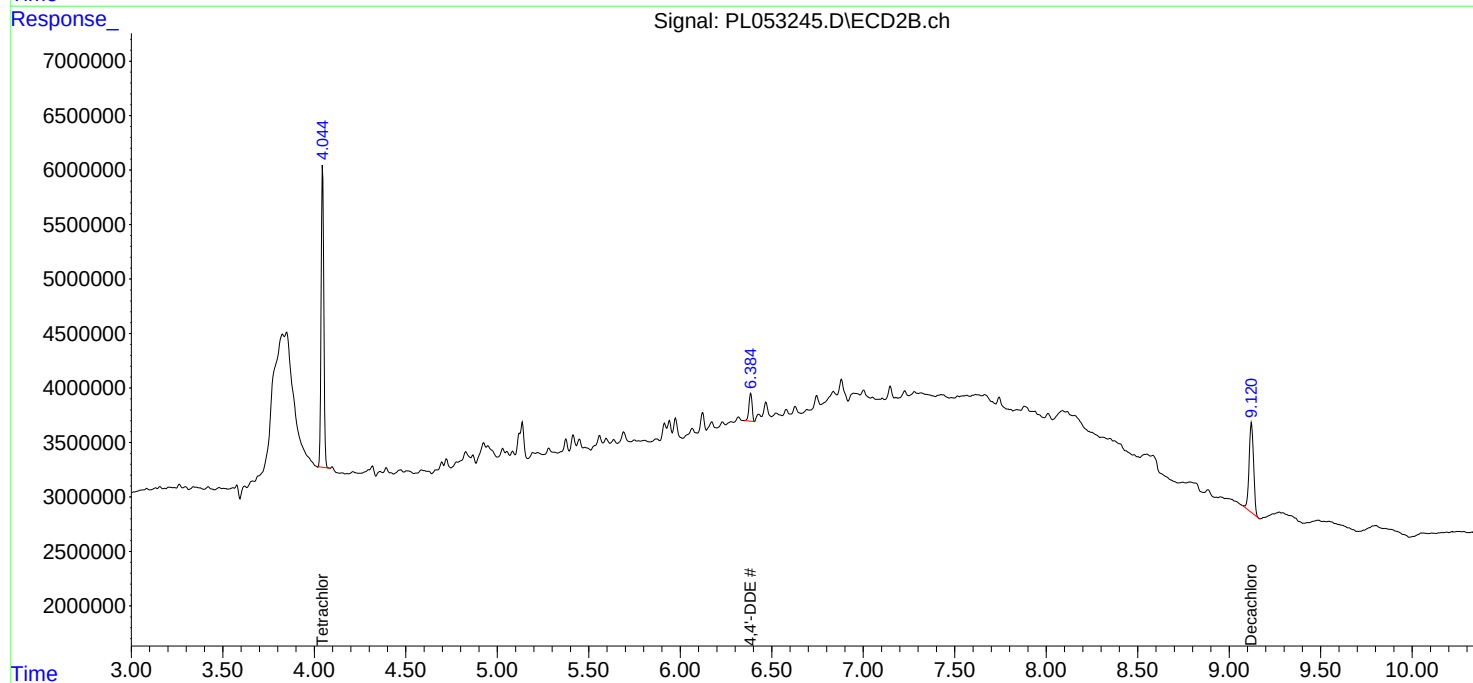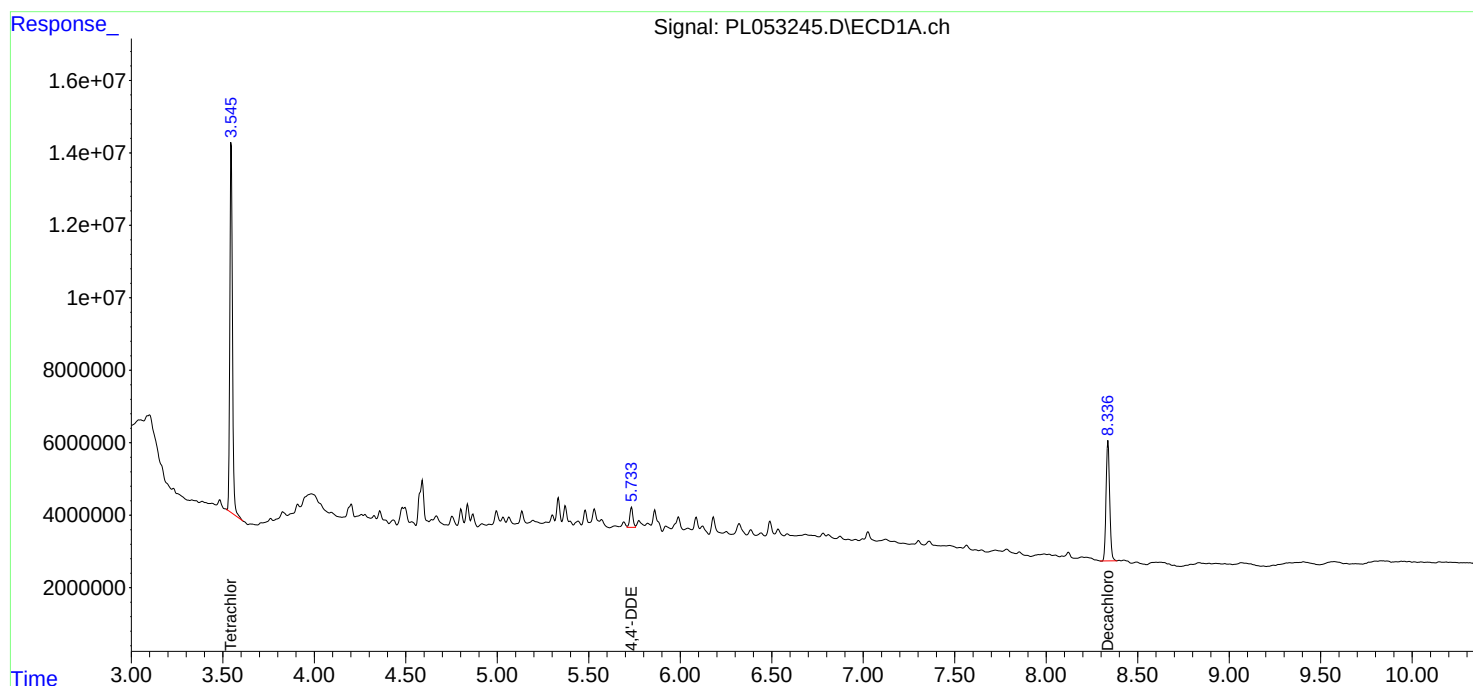

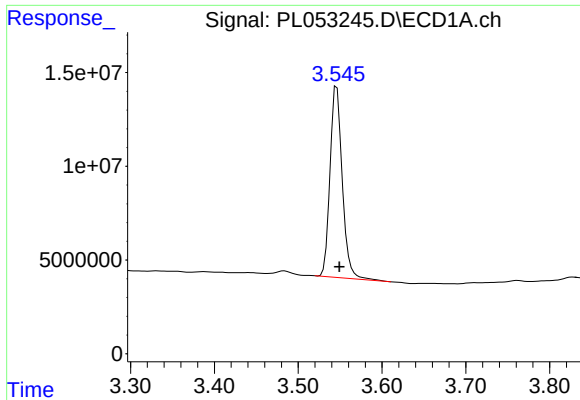


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 103268196
Conc: 10.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190854-AMENDED-COMP-A


Manual Integrations
APPROVED

Ankita
10/14/2019 12:33:03 PM

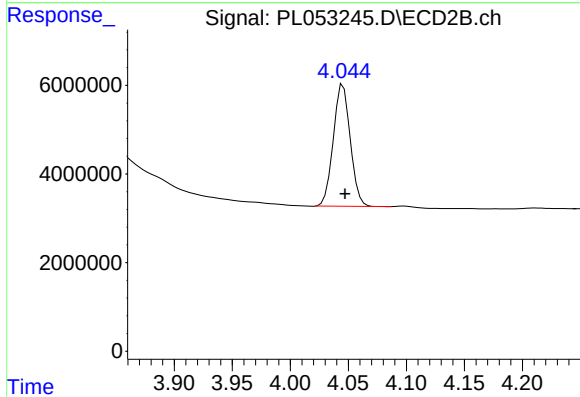


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.002 min
Response: 27983082
Conc: 10.42 ng/ml

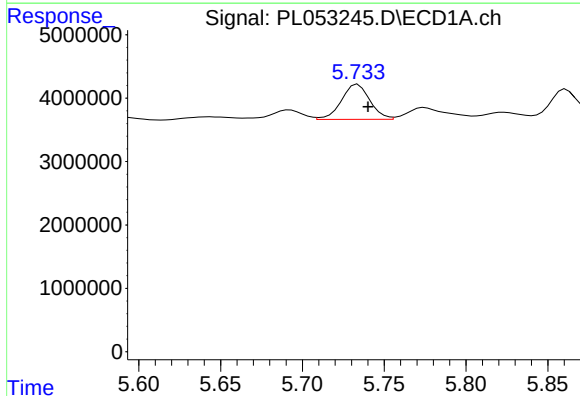


#12 4,4'-DDE

R.T.: 5.733 min
Delta R.T.: -0.008 min
Response: 6639329
Conc: 0.57 ng/ml m

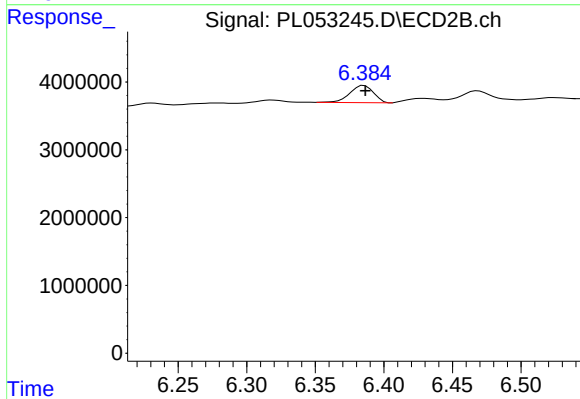

#12 4,4'-DDE

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 3035940
Conc: 0.93 ng/ml

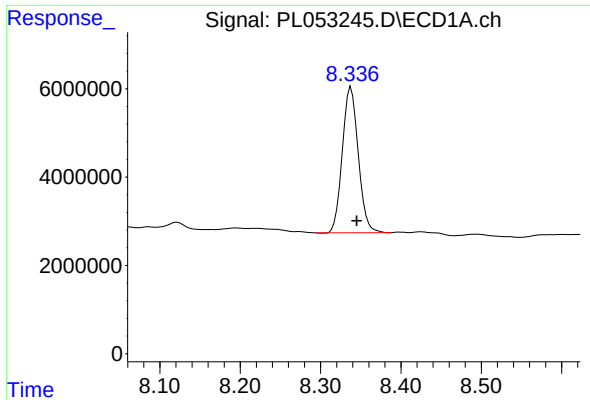


#28 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.007 min
Response: 45572147
Conc: 4.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190854-AMENDED-COMP-A

Manual Integrations
APPROVED

Ankita
10/14/2019 12:33:03 PM

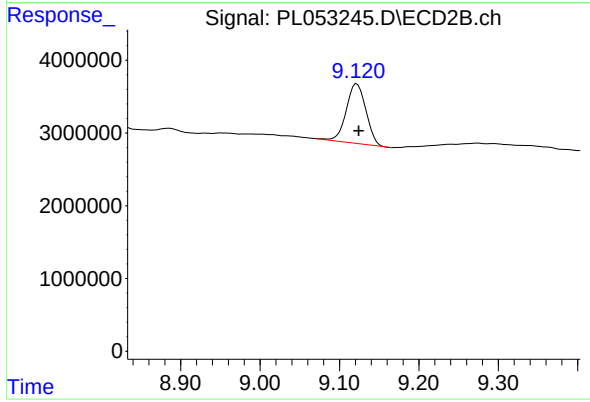

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.002 min
Response: 14169555
Conc: 4.83 ng/ml