

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101120\
 Data File : PL062186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2020 18:41
 Operator : DD\AJ
 Sample : L1955-11
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-04

Manual Integrations
 APPROVED

Ankita
 10/13/2020 3:55:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:46:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 10 05:27:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	30851180	49024391	17.302	17.201
27)	SA Decachlor...	8.125	8.993	66495695	97006744	34.980	34.905
Target Compounds							
2)	A alpha-BHC	3.844	4.338	2860262	3930207	1.171	0.982
3)	MA gamma-BHC...	4.123	4.621	1420982	3219304	0.628	0.863 #
4)	MA Heptachlor	4.421	5.127	1814422	4286878	0.901	1.148 #
5)	MB Aldrin	4.665	5.430	1852112	2636733	1.012	0.782
6)	B beta-BHC	4.372	4.793	838231	2036680	0.879	1.134 #
7)	B delta-BHC	4.573	5.005	1723890	2219984	0.817	0.827
8)	B Heptachlo...	5.102	5.813	1608463	2980890	0.921m	1.044m
9)	A Endosulfan I	5.438	6.172	1457003	3088053	0.901	1.042
10)	B trans-Chl...	5.329	6.050	1760362	2482853	1.013	0.813
11)	B cis-Chlor...	5.386	6.122	1709366	2750465	0.982	0.889
12)	B 4,4'-DDE	5.550	6.280	1433778	2630090	0.874	0.885
13)	MA Dieldrin	5.679	6.427	1615592	2631577	0.906	0.858
14)	MA Endrin	5.933	6.643	2050526	1830963	1.285	0.752 #
15)	B Endosulfa...	6.205	6.853	1462718	2883948	0.927	1.096m
16)	A 4,4'-DDD	6.062	6.768	1301282	1937958	0.932	0.827m
17)	MA 4,4'-DDT	6.301	7.068	779038	2190386	0.589	0.962 #
18)	B Endrin al...	6.372	6.978	1245962	2569595	0.917	1.150 #
19)	B Endosulfa...	6.584	7.200	1668554	2604944	1.000	0.977
20)	A Methoxychlor	6.844	7.527	603412	1144179	0.737	0.860
21)	B Endrin ke...	7.070	7.669	1339625	2507599	0.790	0.963

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101120\
Data File : PL062186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2020 18:41
Operator : DD\AJ
Sample : L1955-11
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:46:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 10 05:27:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

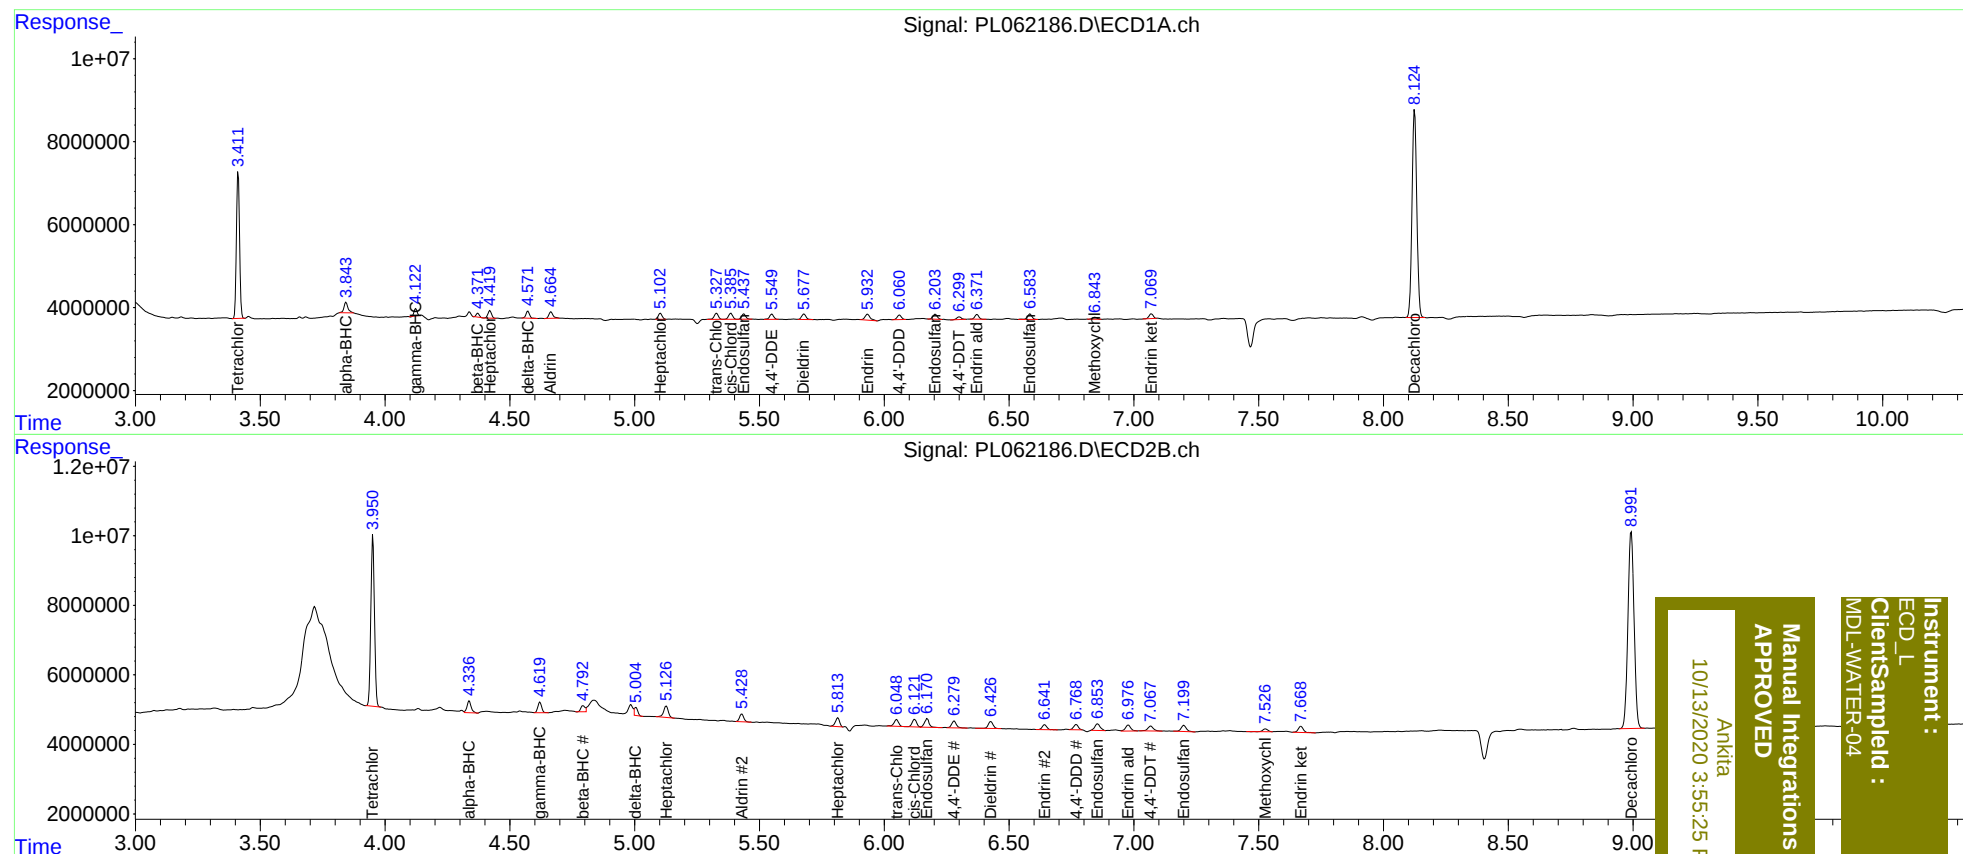

10/13/2020 3:55:25 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_L
Client Sample :
MDL-WATER-04