

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101121\
 Data File : PL070250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2021 18:44
 Operator : AR\AJ
 Sample : M4150-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FDR-20211007-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 03:15:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	5.562	10855193	31221974	21.694	23.606
28)	SA Decachlor...	10.390	11.482	13062532	23233739	18.877	19.199

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101121\
Data File : PL070250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2021 18:44
Operator : AR\AJ
Sample : M4150-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FDR-20211007-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 03:15:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

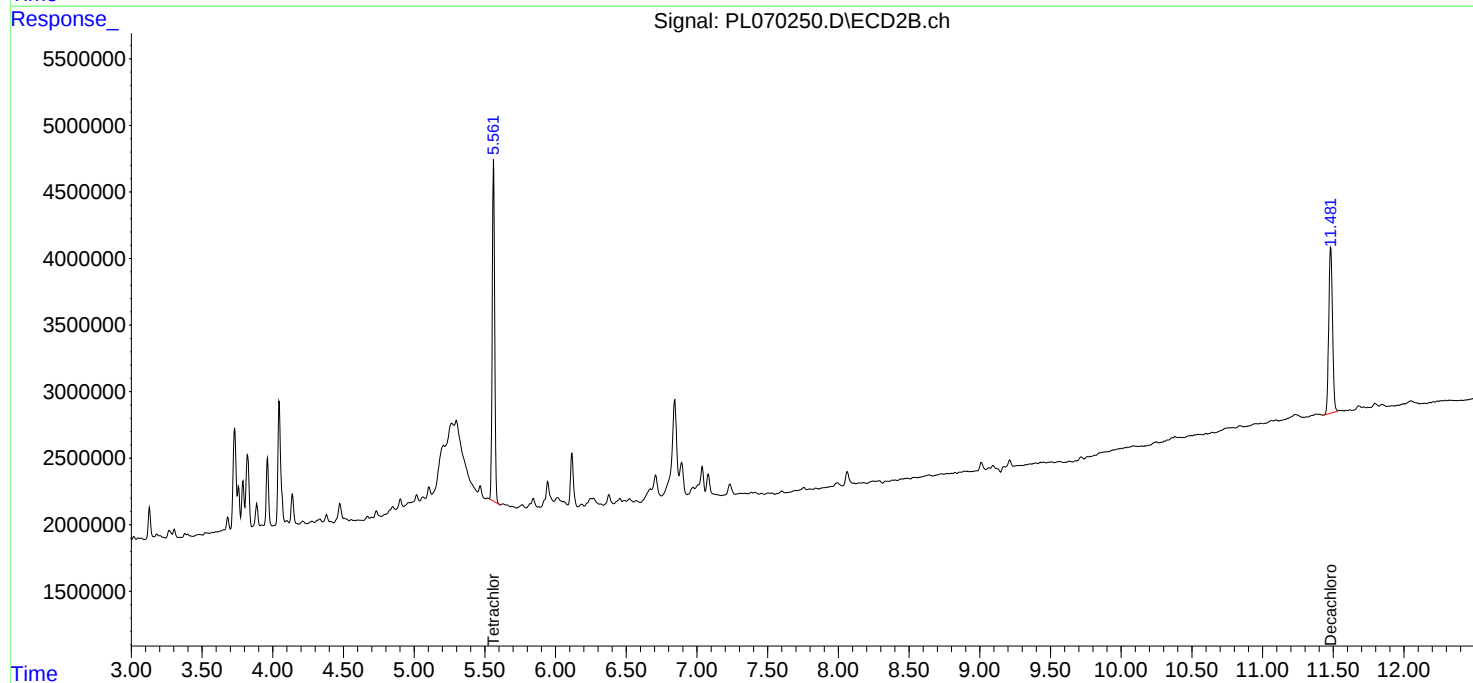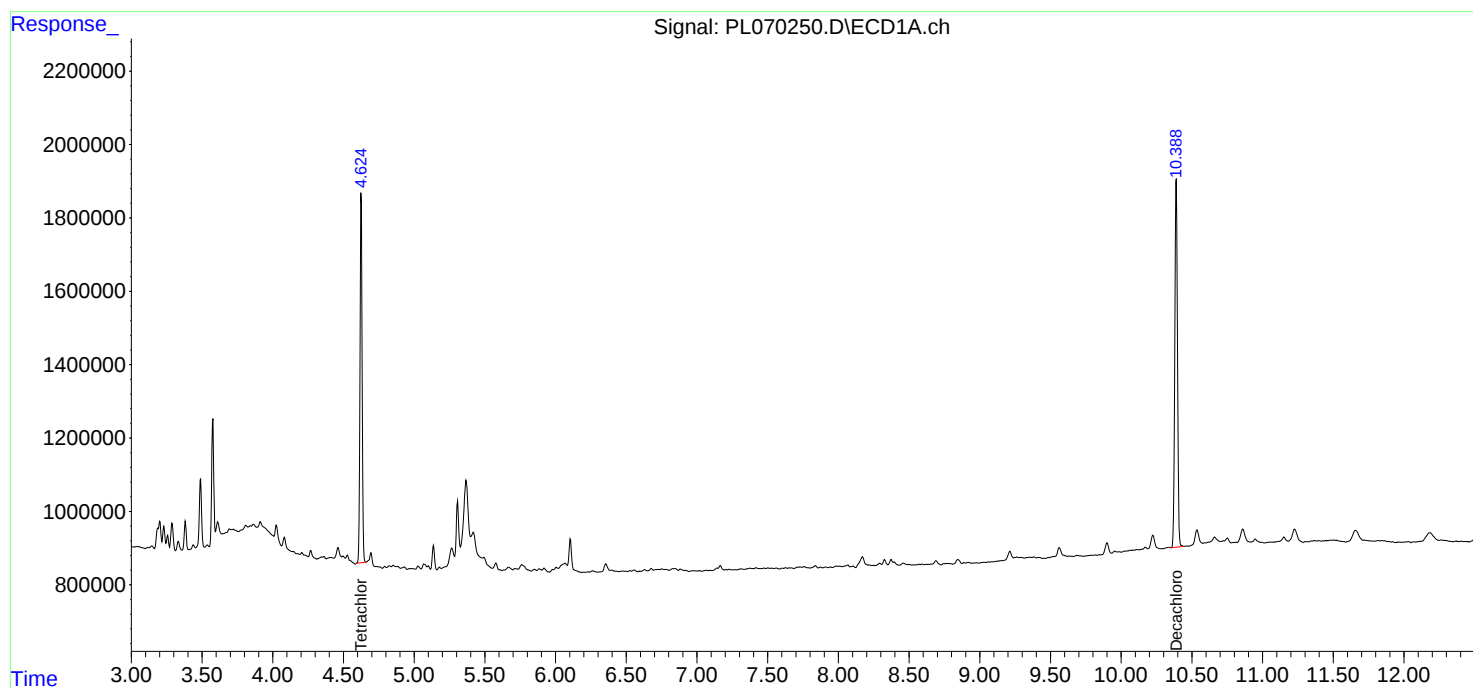


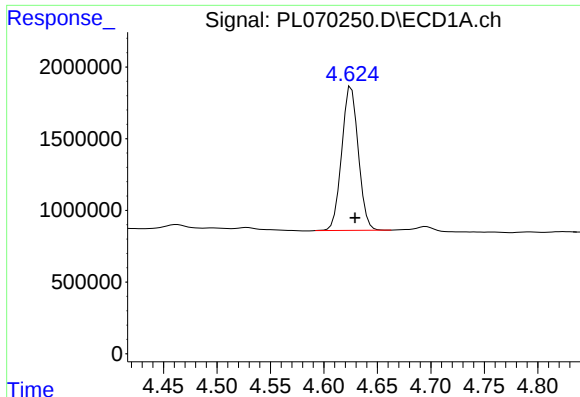

#1 Tetrachloro-m-xylene


R.T.: 4.626 min
Delta R.T.: -0.003 min
Response: 10855193
Conc: 21.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
FDR-20211007-WC

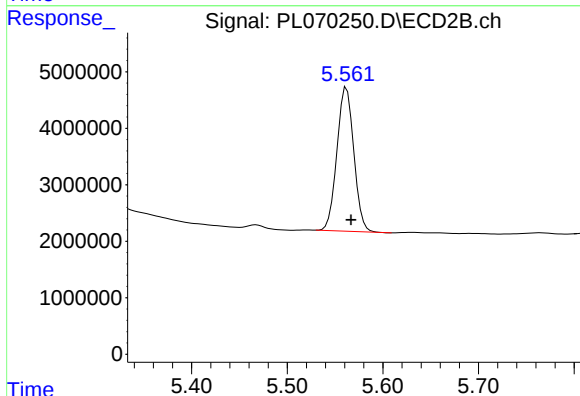


#1 Tetrachloro-m-xylene

R.T.: 5.562 min
Delta R.T.: -0.005 min
Response: 31221974
Conc: 23.61 ng/ml

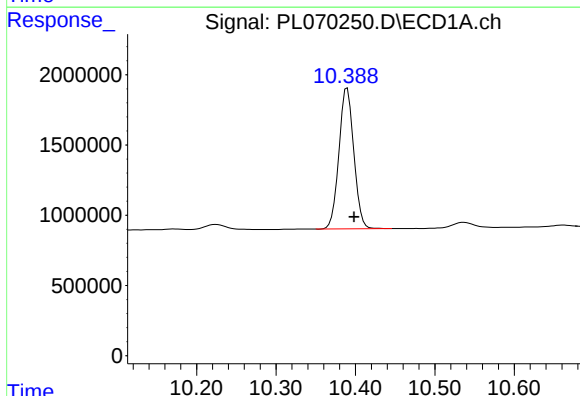

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.009 min
Response: 13062532
Conc: 18.88 ng/ml

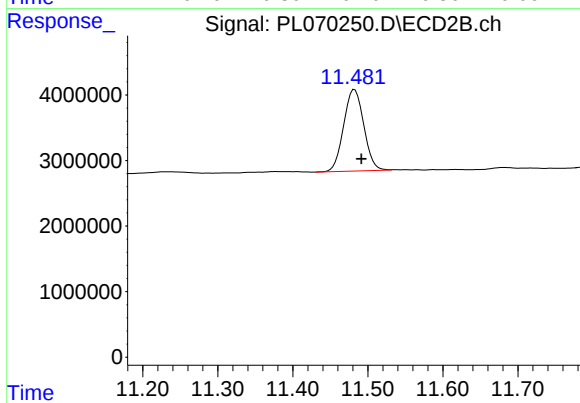

#28 Decachlorobiphenyl

R.T.: 11.482 min
Delta R.T.: -0.009 min
Response: 23233739
Conc: 19.20 ng/ml