

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101123\
 Data File : PL085850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 14:07
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 21:47:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	2.621	137.2E6	51091037	46.127	54.695
28)	SA Decachlor...	8.860	7.775	121.4E6	52096625	55.759	56.444
Target Compounds							
23)	Chlordane-1	4.515	3.611	60912160	15335731	506.697	470.437
24)	Chlordane-2	5.046	4.189	64794845	20189175	498.254	518.818
25)	Chlordane-3	5.758	4.818	251.5E6	53314548	492.888	527.618
26)	Chlordane-4	5.841	4.880	309.9E6	57293695	488.500	494.832
27)	Chlordane-5	6.688	5.550	48559079	14665461	473.338	526.183


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101123\
Data File : PL085850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 14:07
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 21:47:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

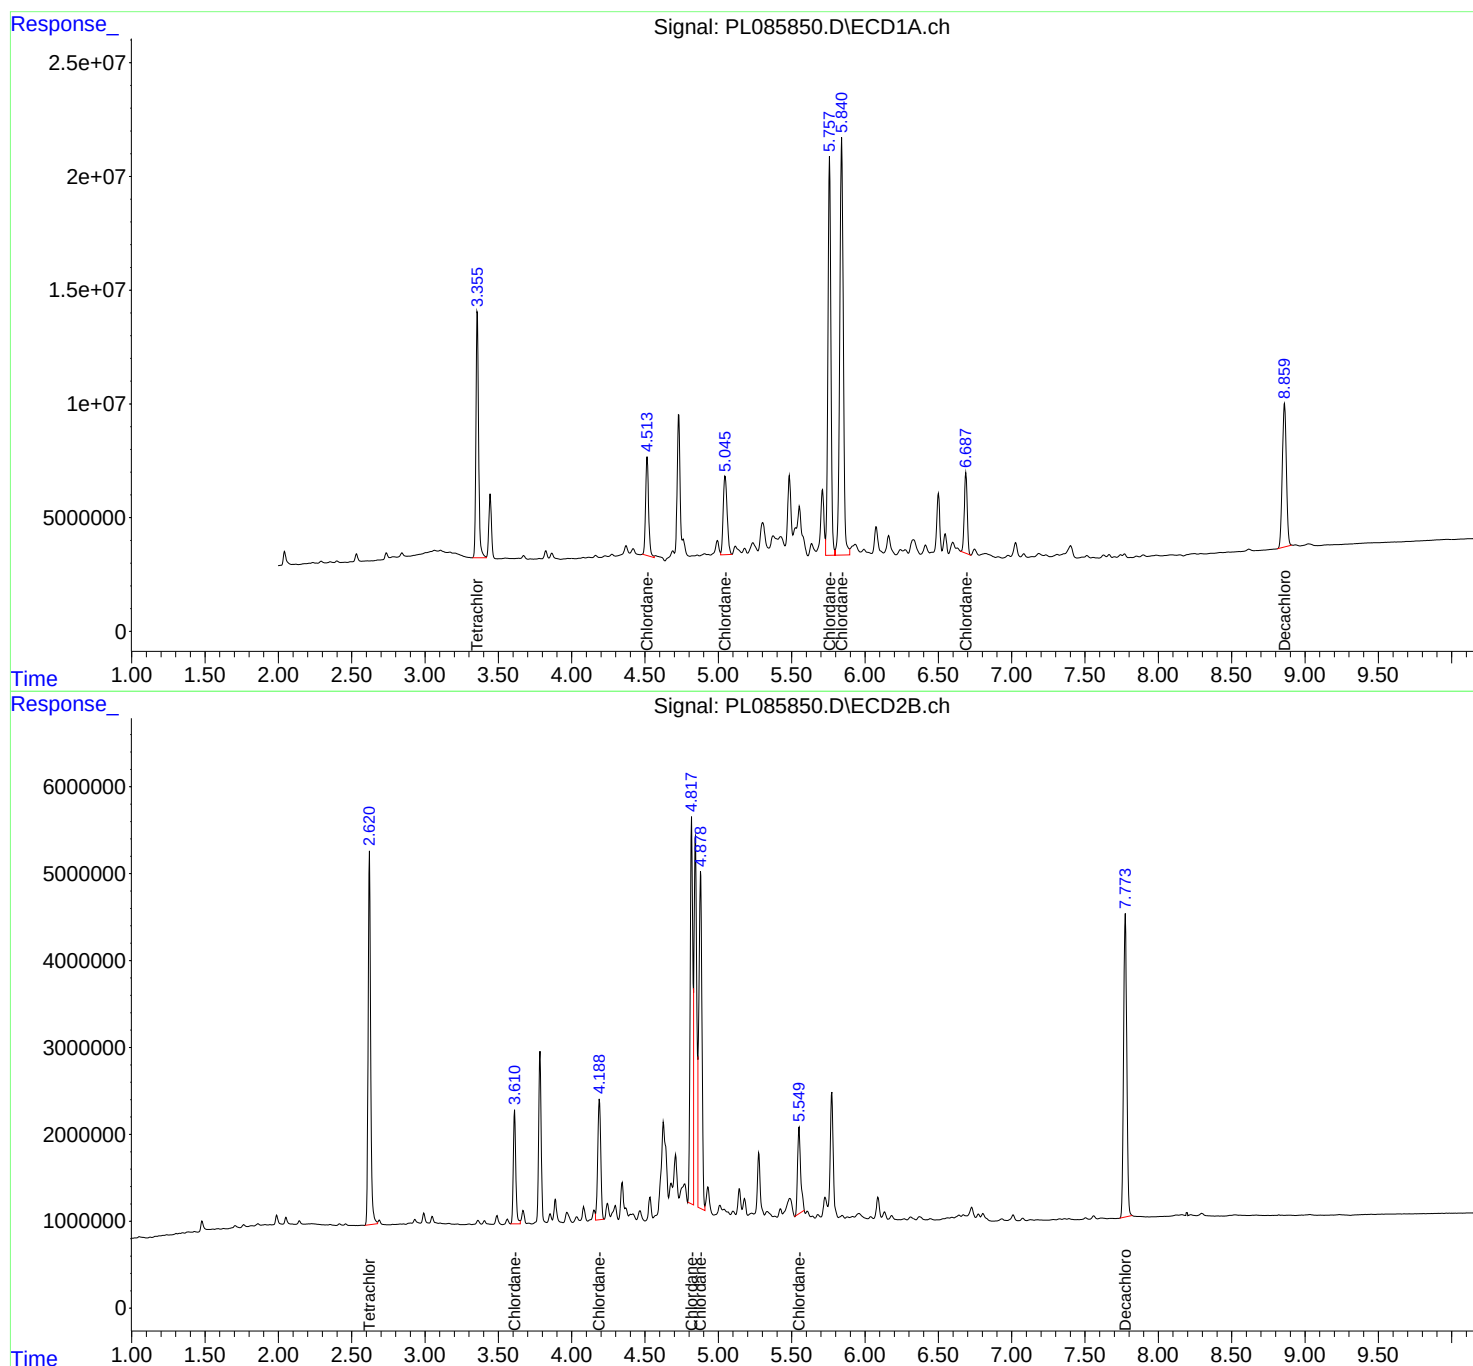


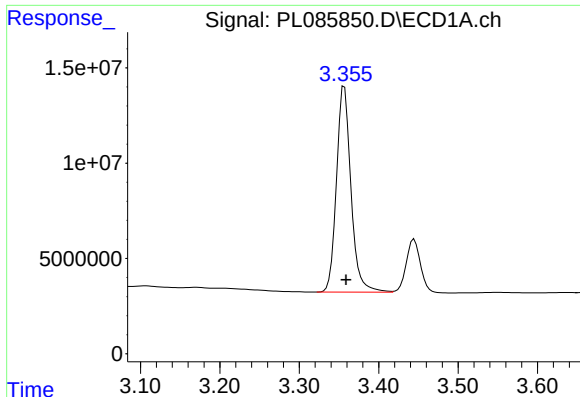

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.002 min
Response: 137188107
Conc: 46.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

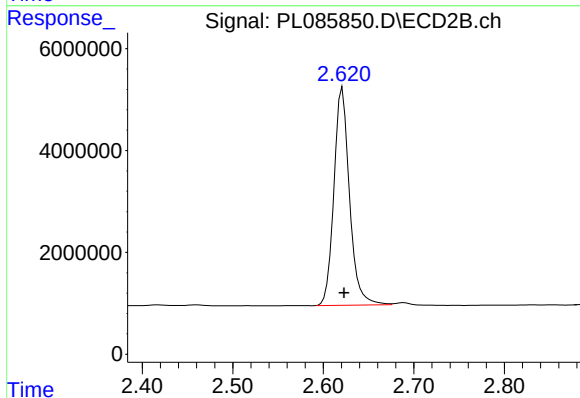


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 51091037
Conc: 54.69 ng/ml

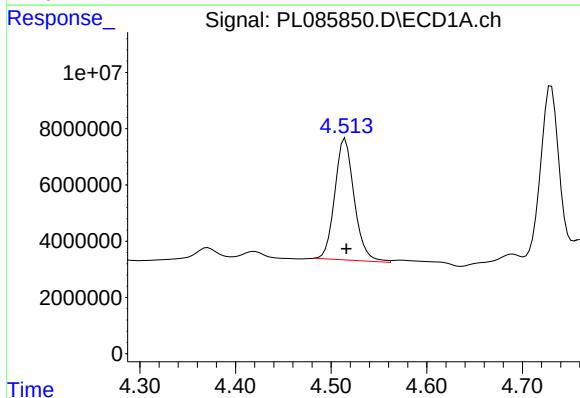


#23 Chlordane-1

R.T.: 4.515 min
Delta R.T.: -0.001 min
Response: 60912160
Conc: 506.70 ng/ml

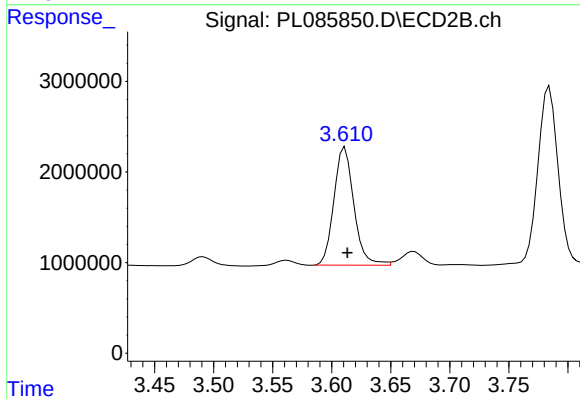

#23 Chlordane-1


R.T.: 3.611 min
Delta R.T.: -0.002 min
Response: 15335731
Conc: 470.44 ng/ml

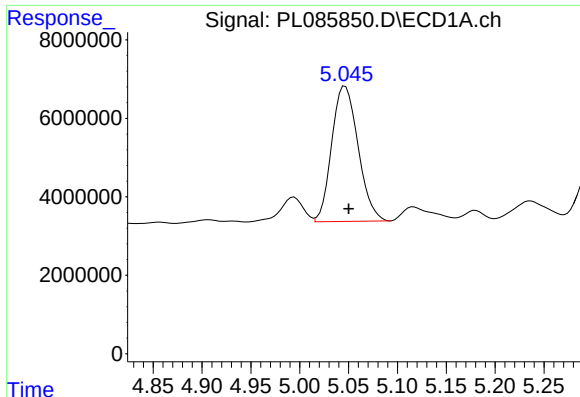

#24 Chlordane-2


R.T.: 5.046 min
Delta R.T.: -0.004 min
Response: 64794845
Conc: 498.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

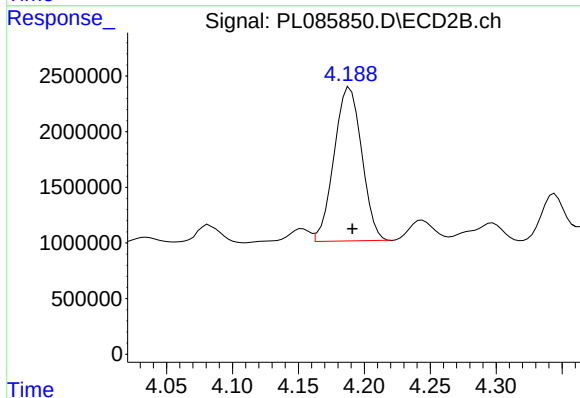


#24 Chlordane-2

R.T.: 4.189 min
Delta R.T.: -0.002 min
Response: 20189175
Conc: 518.82 ng/ml

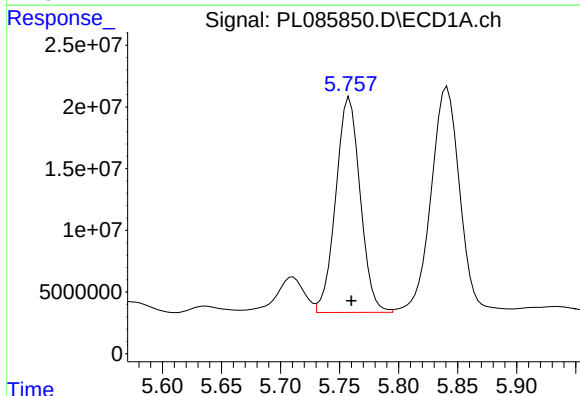


#25 Chlordane-3

R.T.: 5.758 min
Delta R.T.: -0.002 min
Response: 251471678
Conc: 492.89 ng/ml

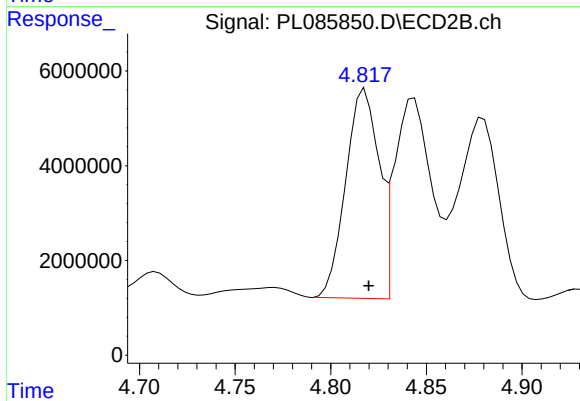

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: -0.002 min
Response: 53314548
Conc: 527.62 ng/ml

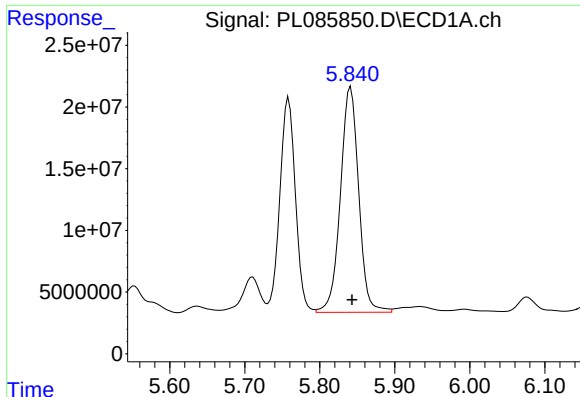

#26 Chlordane-4


R.T.: 5.841 min
Delta R.T.: -0.002 min
Response: 309924587
Conc: 488.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

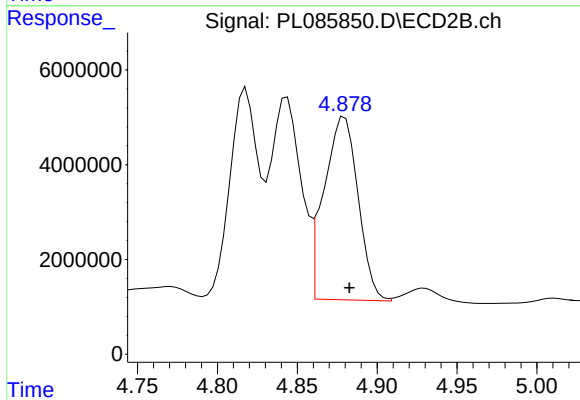


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: -0.003 min
Response: 57293695
Conc: 494.83 ng/ml

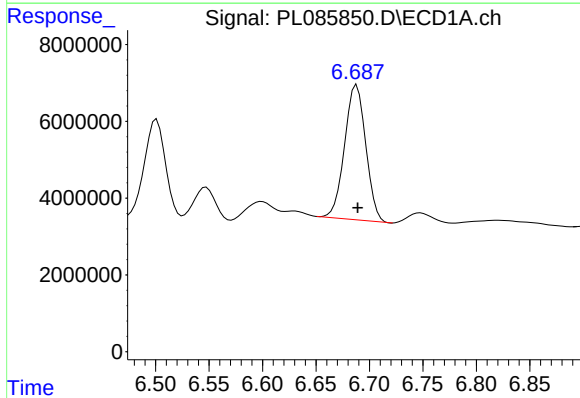


#27 Chlordane-5

R.T.: 6.688 min
Delta R.T.: 0.000 min
Response: 48559079
Conc: 473.34 ng/ml

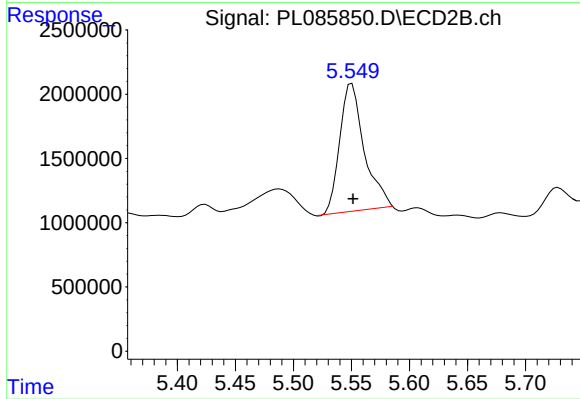

#27 Chlordane-5


R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 14665461
Conc: 526.18 ng/ml

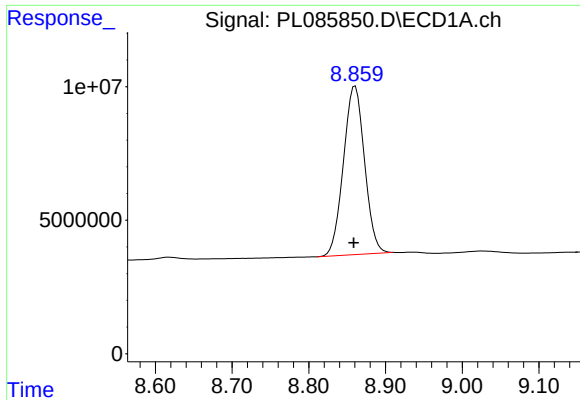

#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.002 min
Response: 121445665
Conc: 55.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

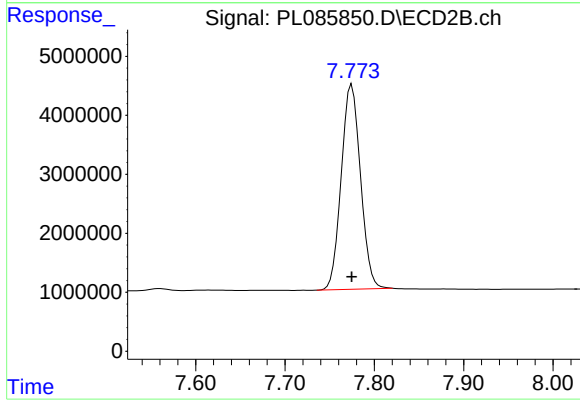

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 52096625
Conc: 56.44 ng/ml