

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101123\
 Data File : PL085865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 17:51
 Operator : AR\AJ
 Sample : 04805-01 20X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-1(0-5)

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/12/2023
 Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 02:06:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.354	2.621	1235865	1050373	0.416m	1.124 #
28) SA Decachlor...	8.884f	7.768	21595261	2544043	9.915	2.756m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101123\
Data File : PL085865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 17:51
Operator : AR\AJ
Sample : 04805-01 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B-1(0-5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 02:06:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

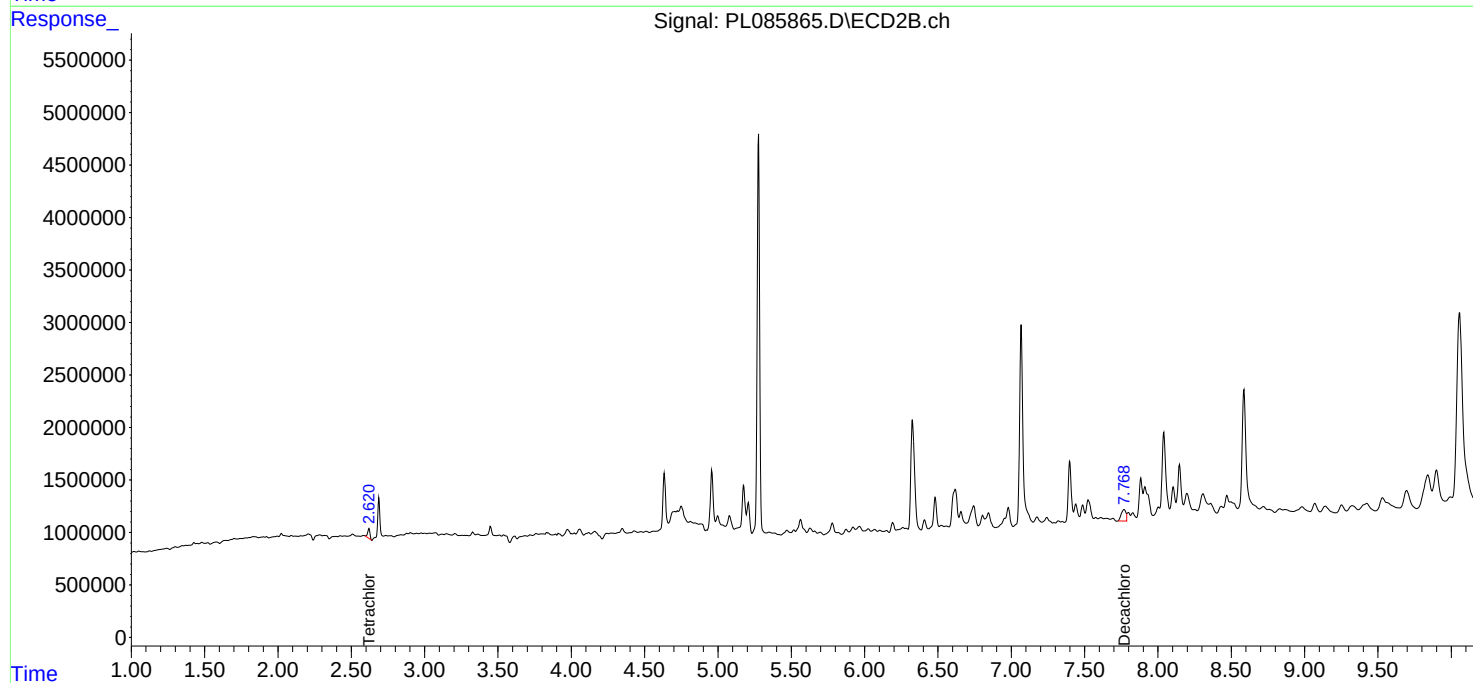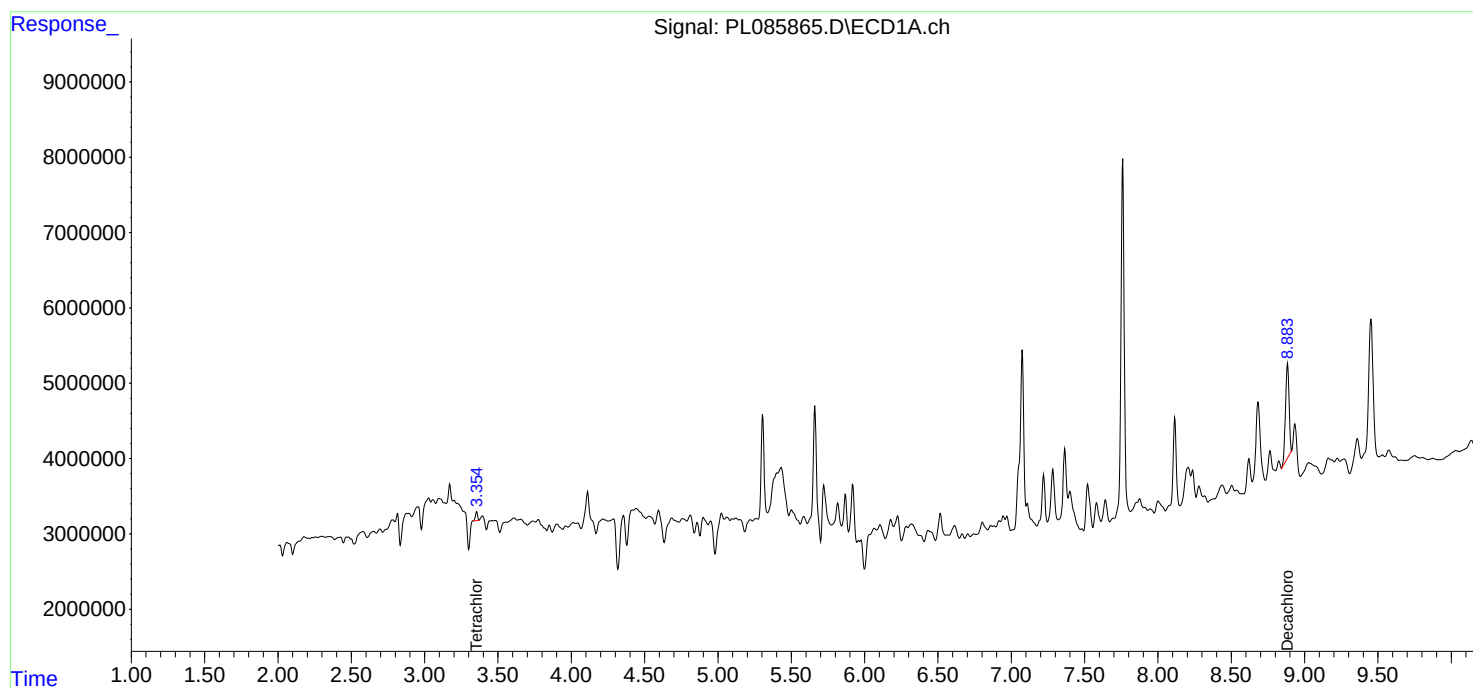

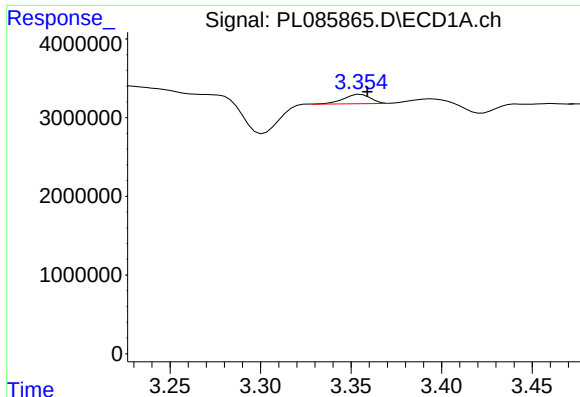


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: -0.005 min
Response: 1235865
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-1(0-5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

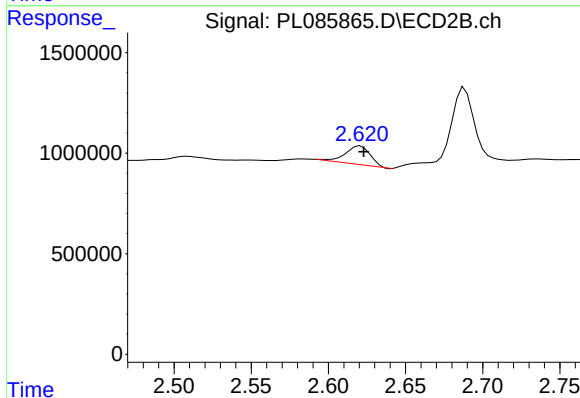


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 1050373
Conc: 1.12 ng/ml

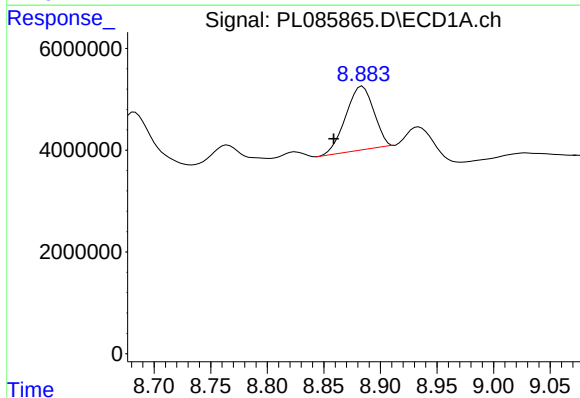

#28 Decachlorobiphenyl

R.T.: 8.884 min
Delta R.T.: 0.025 min
Response: 21595261
Conc: 9.91 ng/ml

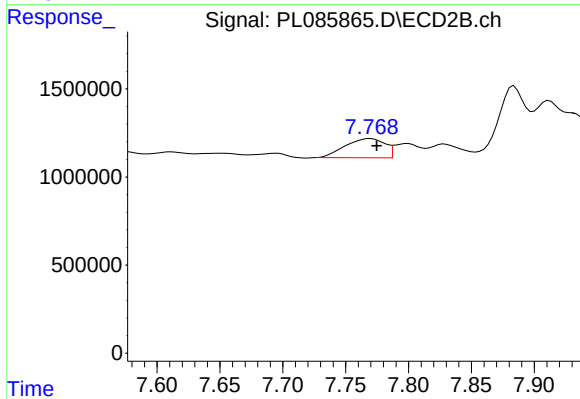

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.006 min
Response: 2544043
Conc: 2.76 ng/ml m