

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101218\
 Data File : PL040981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2018 18:26
 Operator : AJ\SJ
 Sample : J5450-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 23:55:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.106	115.0E6	59635817	20.991	21.388
28)	SA Decachlor...	8.230	9.237	109.1E6	52900318	20.992	20.458
Target Compounds							
3)	MA gamma-BHC...	4.212	0.000	1802931	0	0.247	N.D. #
5)	MB Aldrin	4.756	0.000	1122301	0	0.163	N.D. #
6)	B beta-BHC	4.419f	4.996f	11500591	6890222	3.624	4.299
7)	B delta-BHC	0.000	5.152	0	2614886	N.D.	0.797 #
8)	B Heptachlo...	5.256f	0.000	1984441	0	0.303	N.D. #
9)	A Endosulfan I	5.558	0.000	2752497	0	0.459	N.D. #
16)	A 4,4'-DDD	0.000	6.918f	0	9618294	N.D.	4.592 #
23)	Chlordane-1	4.419	5.152	11500591	2614886	45.062	21.171 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101218\
Data File : PL040981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2018 18:26
Operator : AJ\SJ
Sample : J5450-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 23:55:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

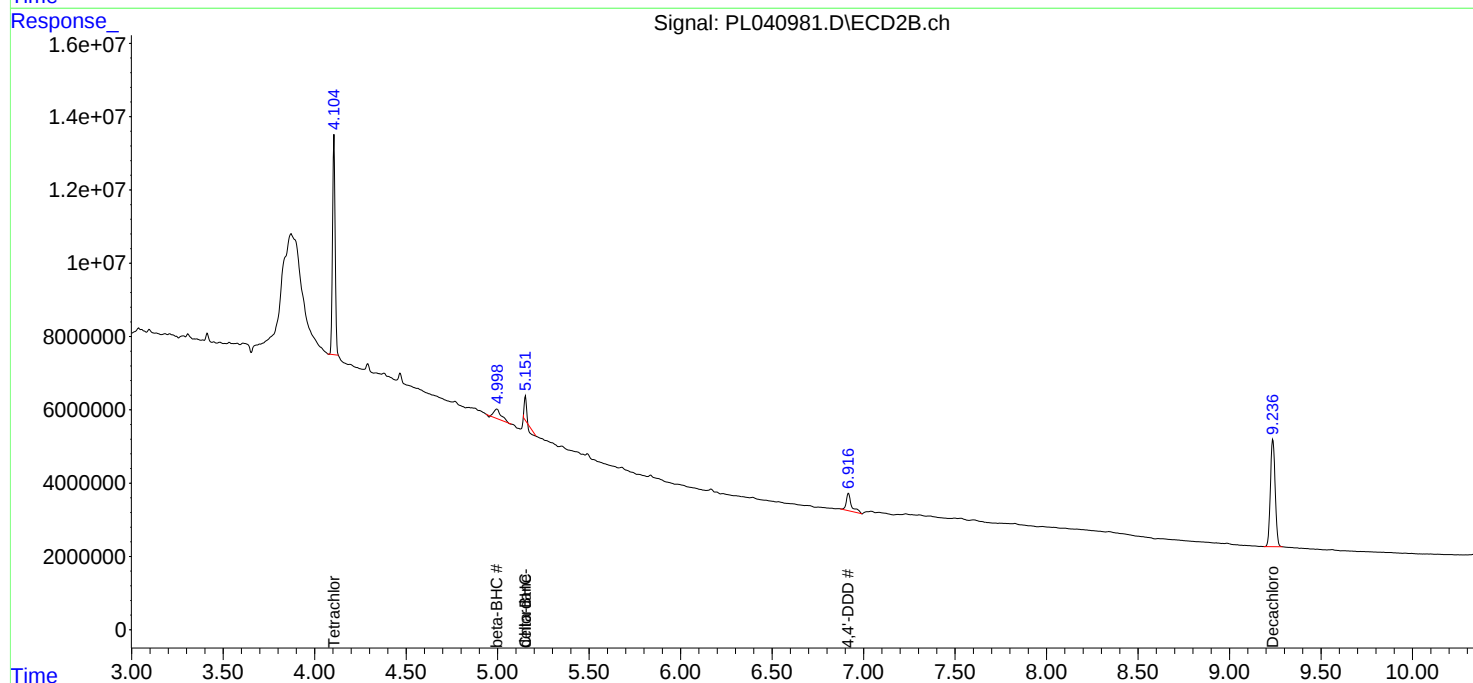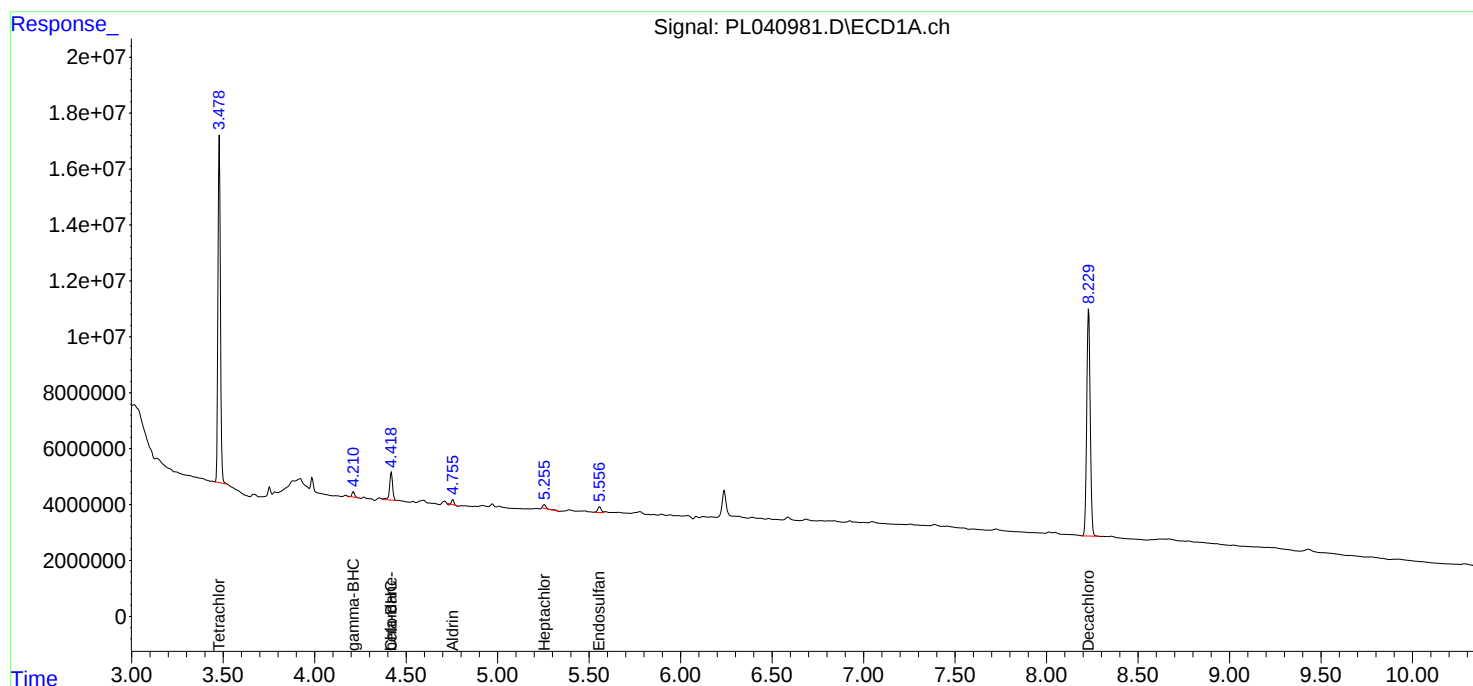


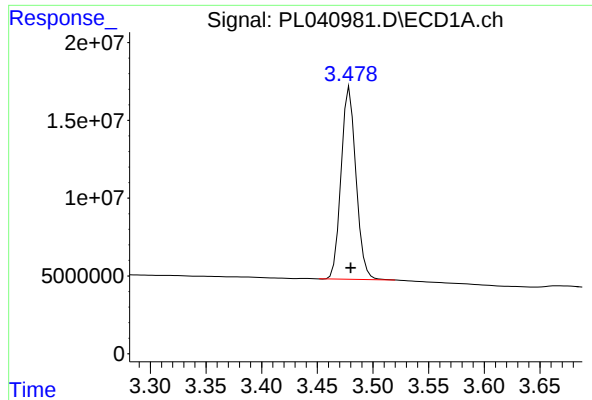

#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 115043838
Conc: 20.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

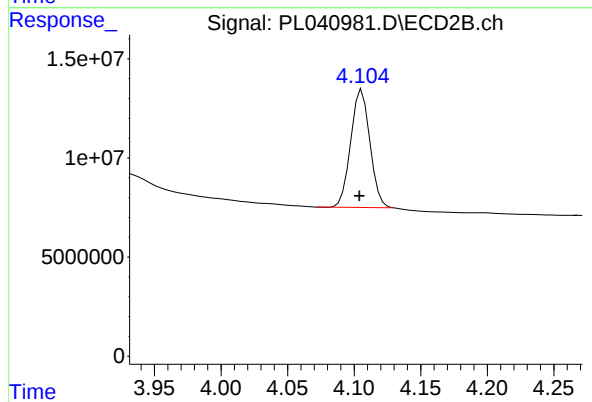

#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.002 min
Response: 59635817
Conc: 21.39 ng/ml